




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

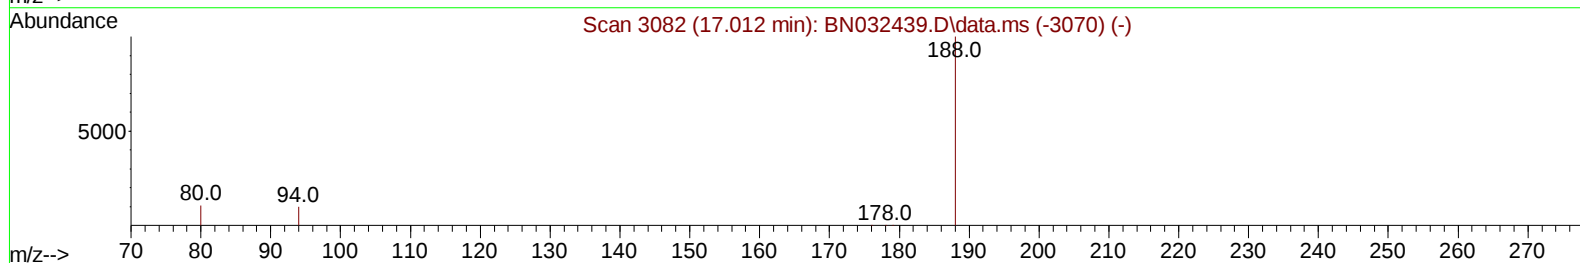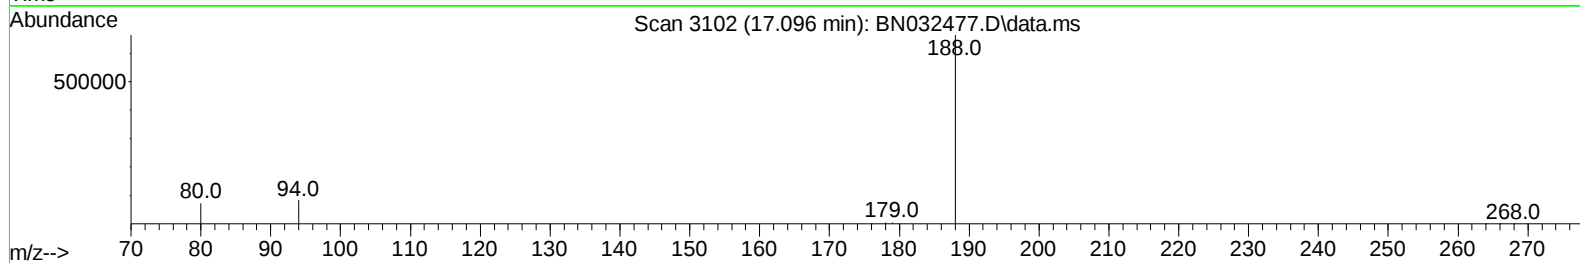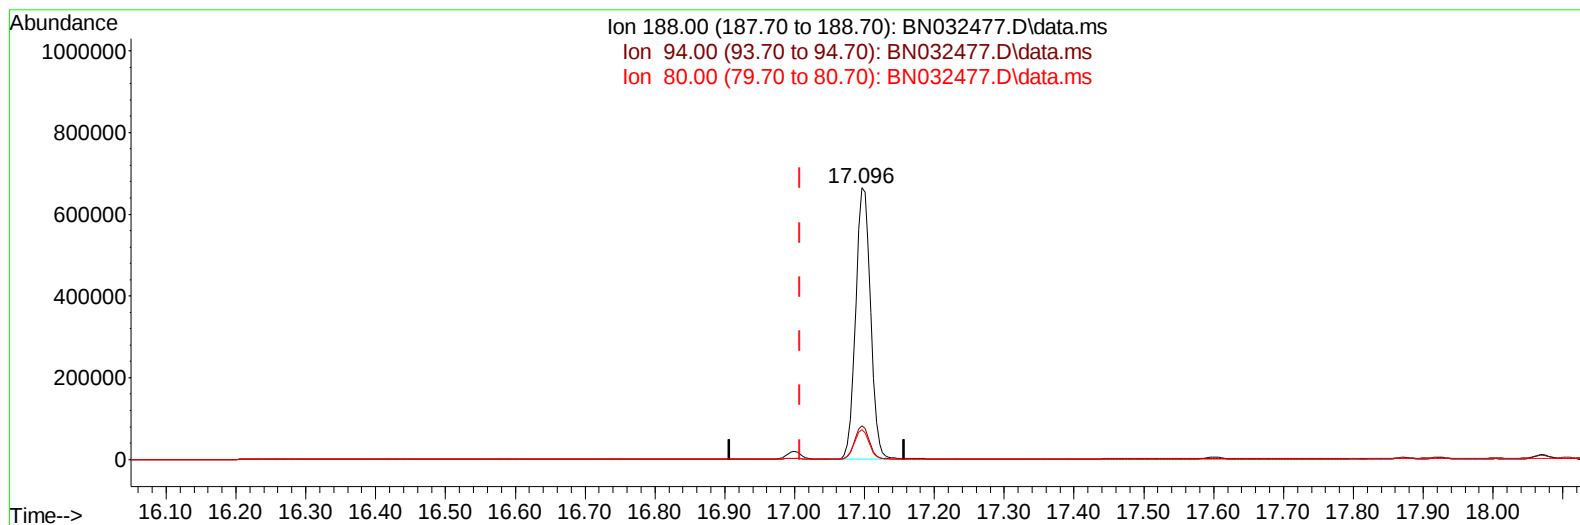

TIC: BN032477.D\data.ms

(13) Phenanthrene-d10 (I)

17.096min (+ 0.089) 0.40 ng/u1

response 980819

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	12.43#
80.00	10.50	10.99
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

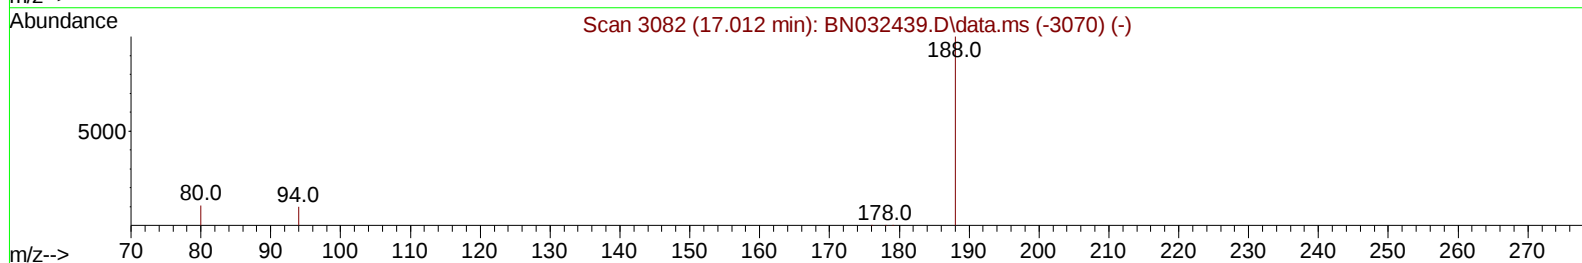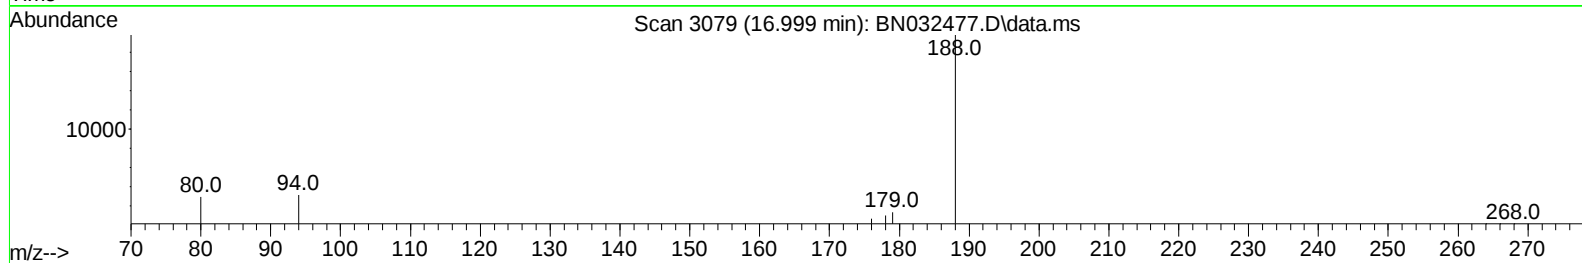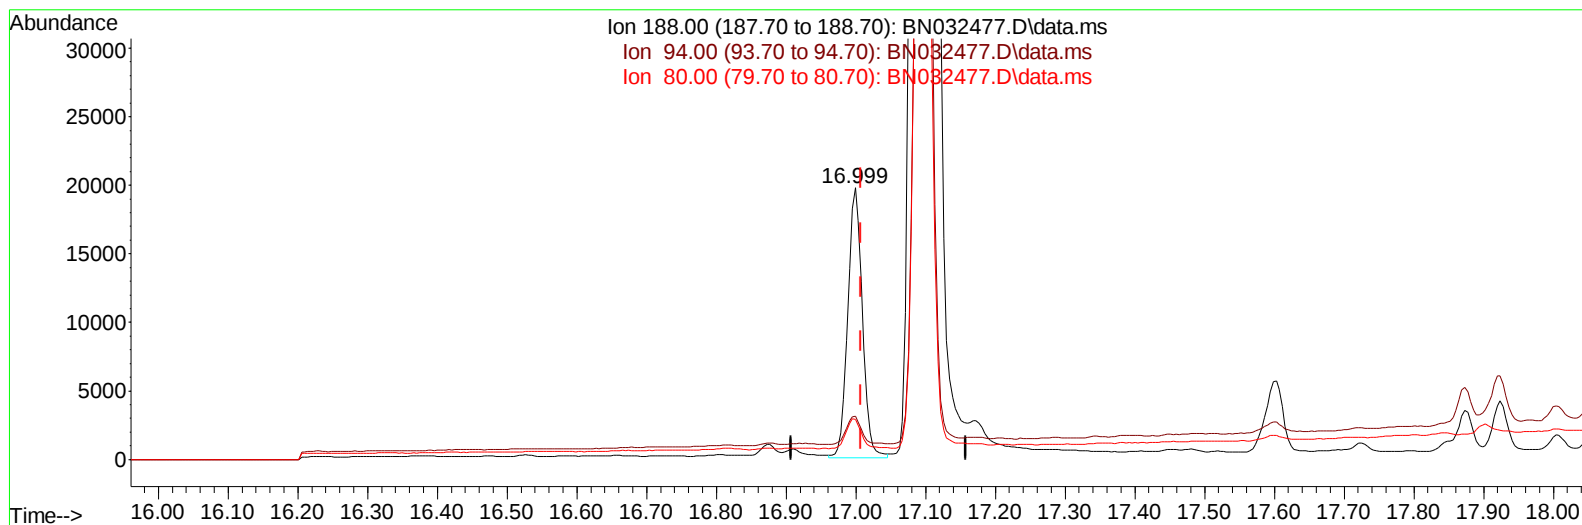

TIC: BN032477.D\data.ms

(13) Phenanthrene-d10 (I)

16.999min (-0.008) 0.40 ng/u1 m

response 28833

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	15.84#
80.00	10.50	14.77#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

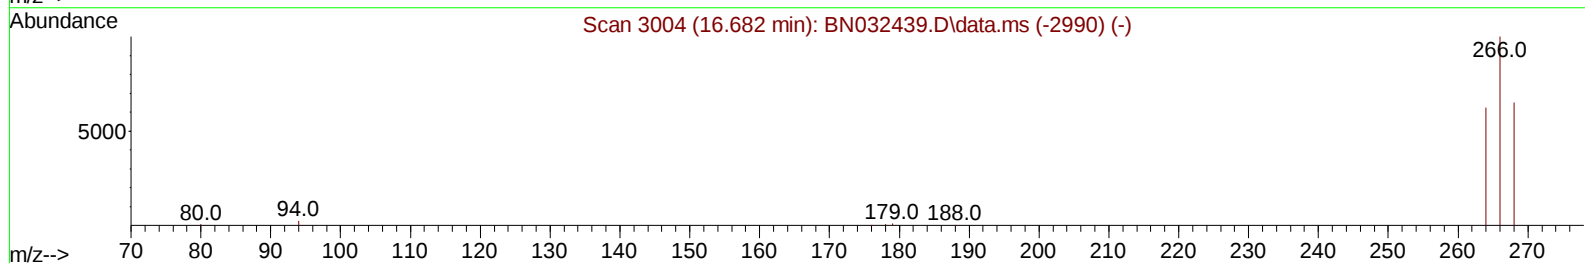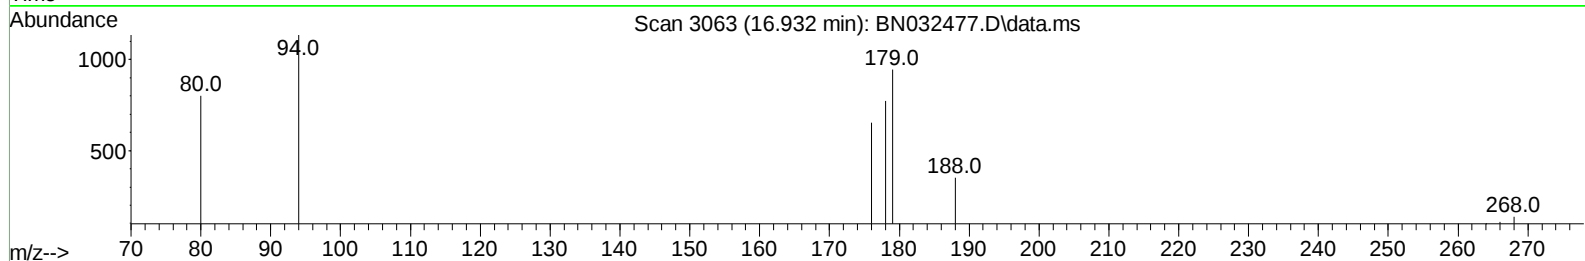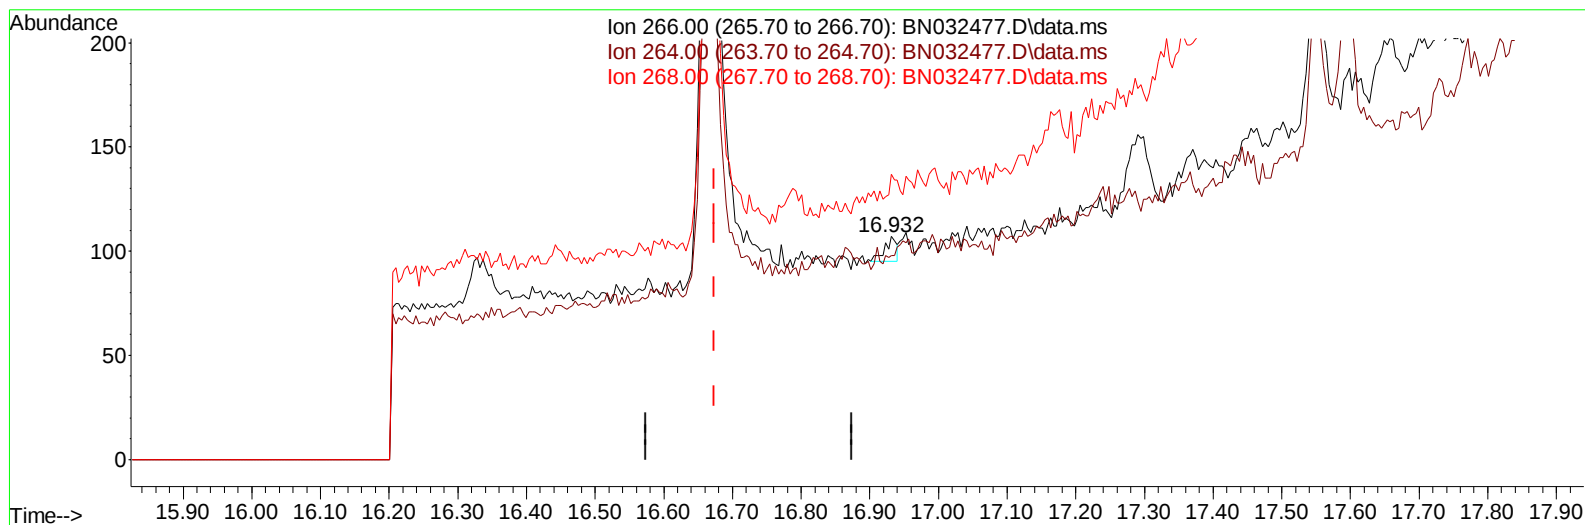

TIC: BN032477.D\data.ms

(14) Pentachloropheno1

16.932min (+ 0.258) 0.00 ng/u1

response

14

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.40	0.00#
268.00	65.50	64.29
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

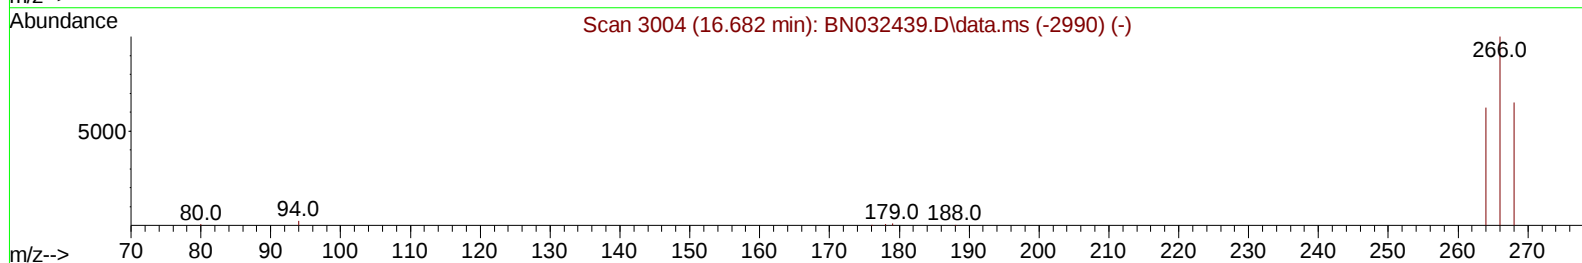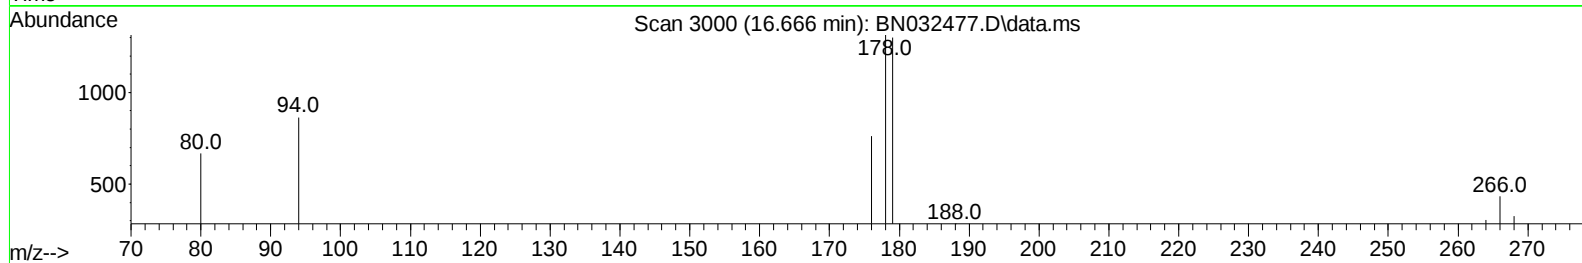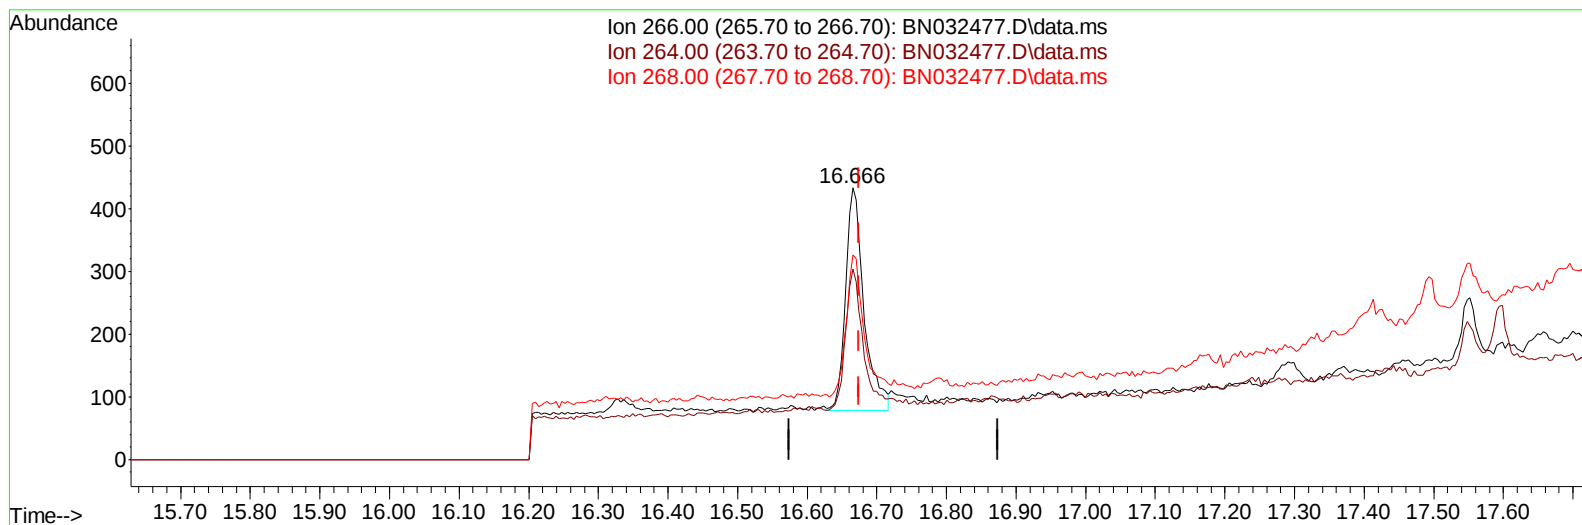

TIC: BN032477.D\data.ms

(14) Pentachlorophenol

16.666min (-0.008) 0.10 ng/ul m

response 654

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.40	0.00#
268.00	65.50	1.38#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

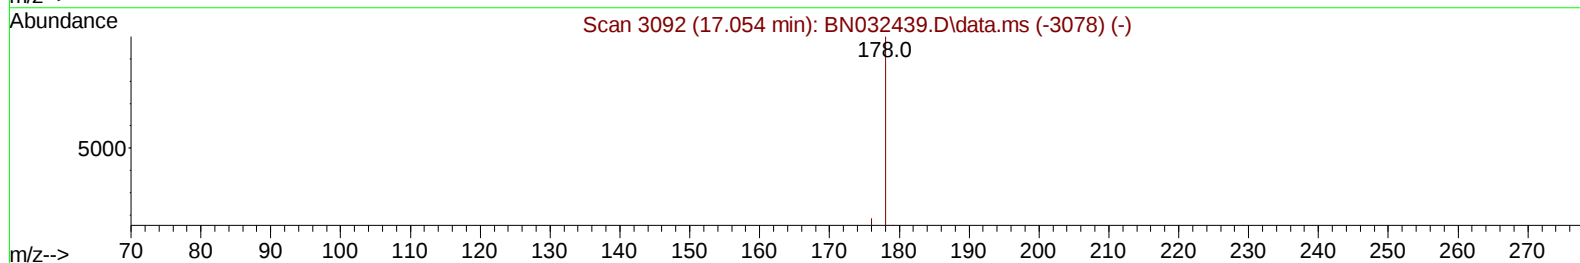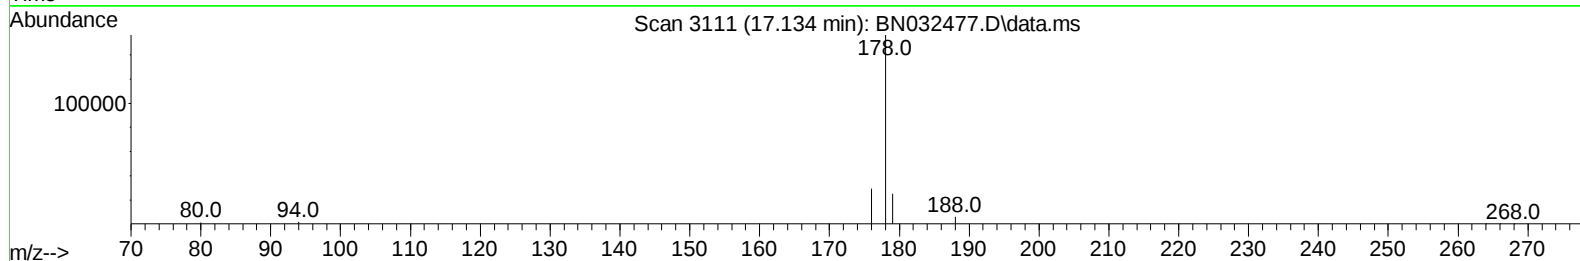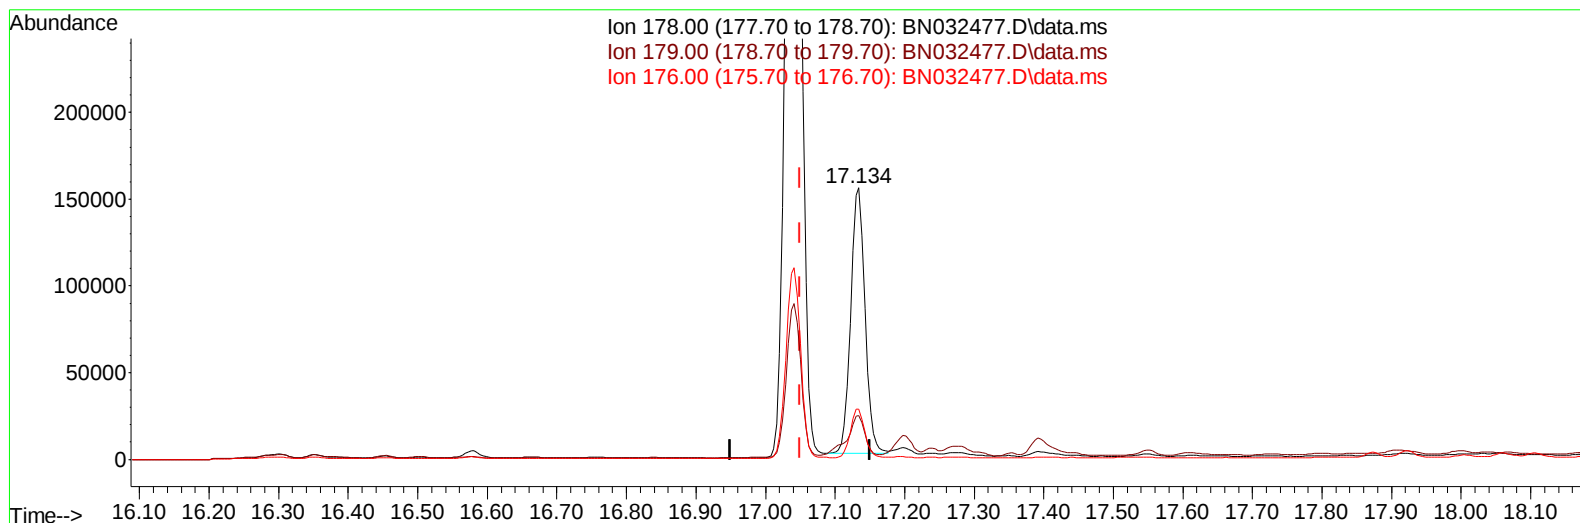

TIC: BN032477.D\data.ms

(15) Phenanthrene

17.134min (+ 0.084) 2.75 ng/u1

response 217096

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.70	16.17
176.00	19.50	18.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

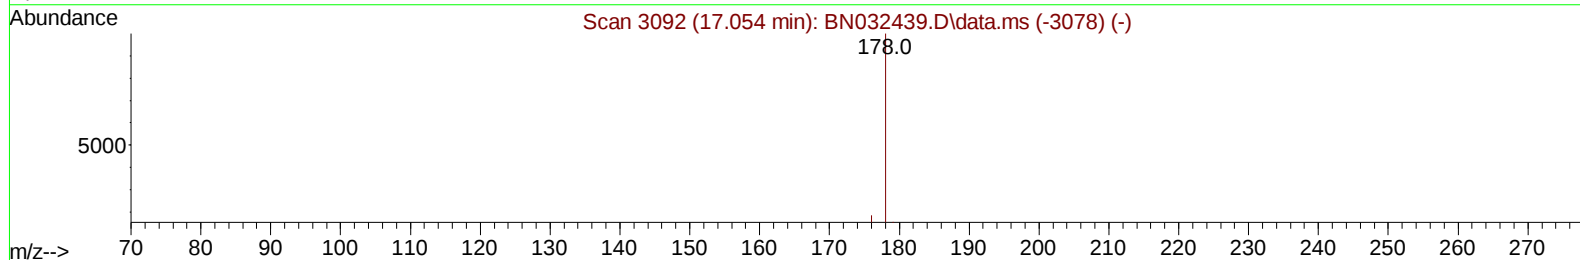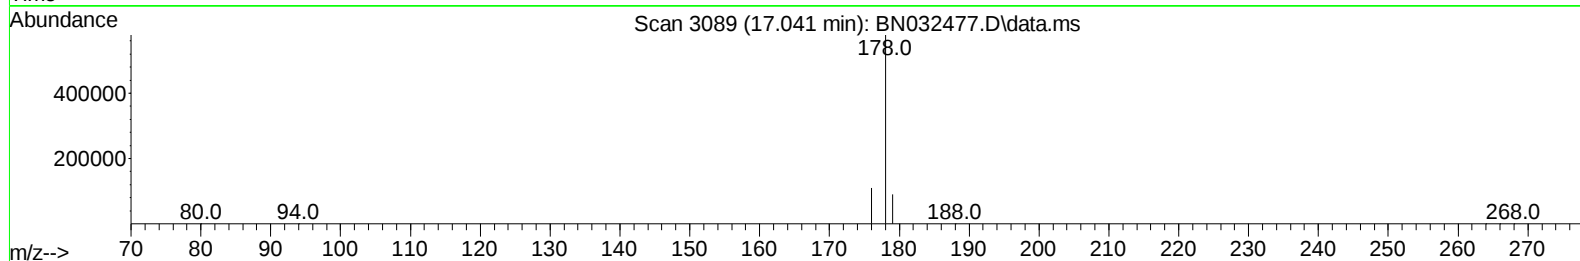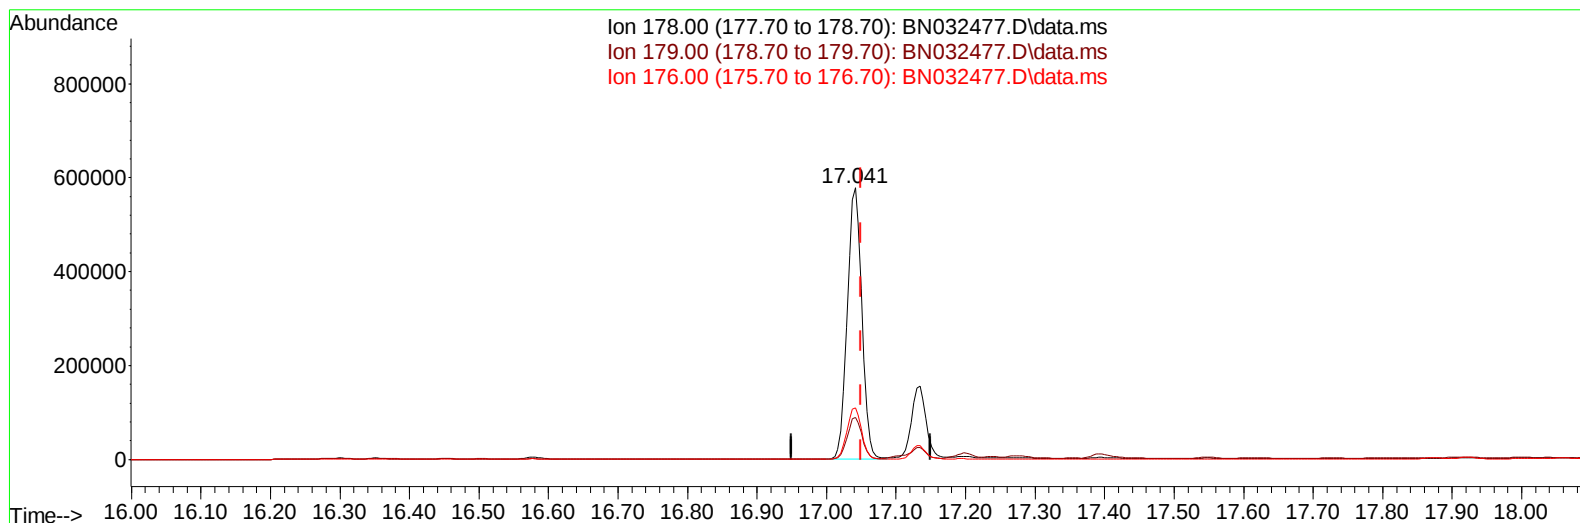

TIC: BN032477.D\data.ms

(15) Phenanthrene

17.041min (-0.008) 10.68 ng/ul m

response 844516

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.70	15.56
176.00	19.50	19.09
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

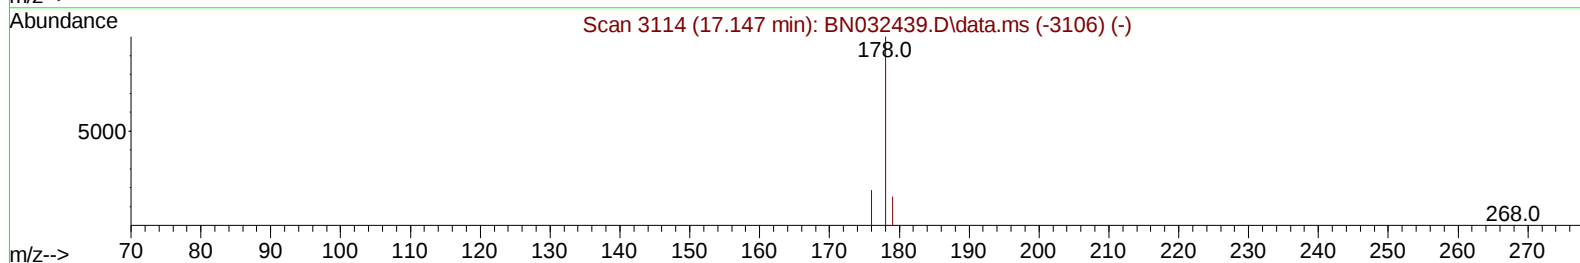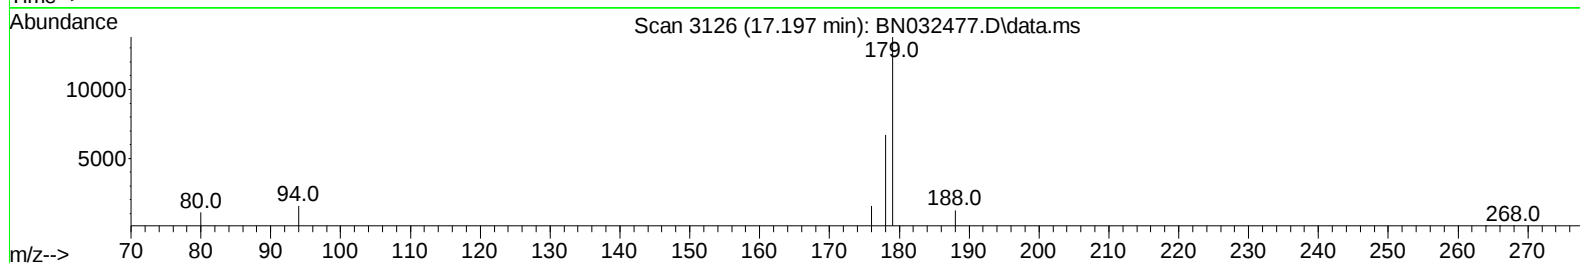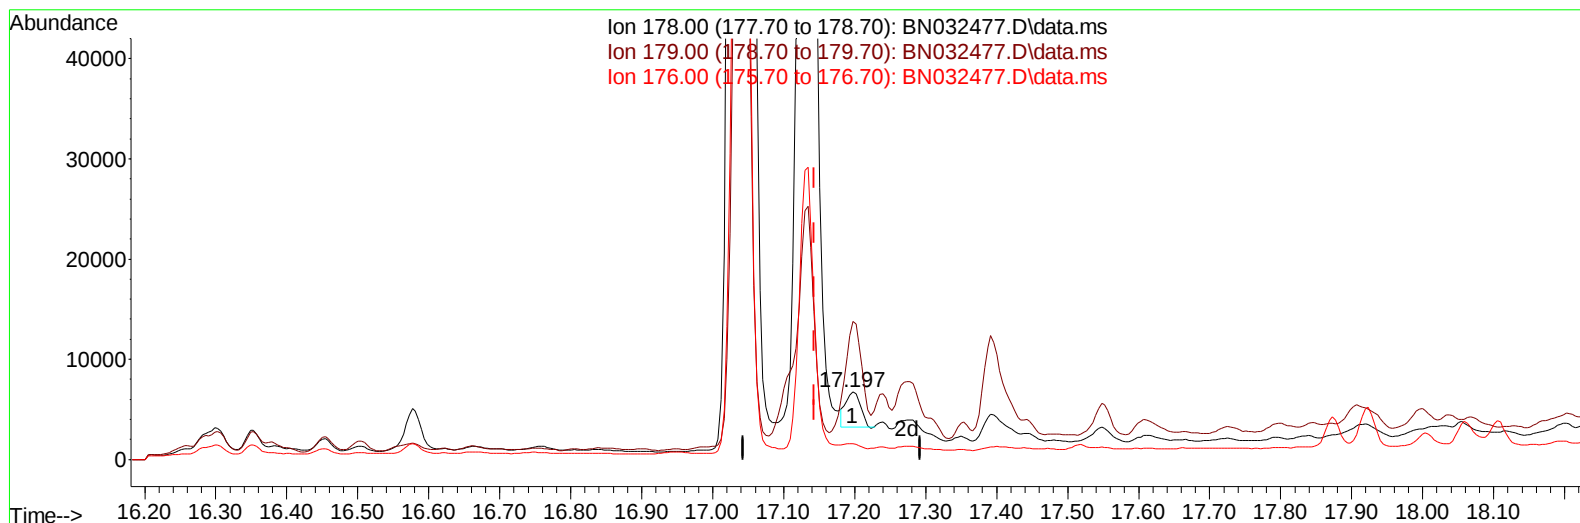

TIC: BN032477.D\data.ms

(16) Anthracene

17.197min (+ 0.055) 0.07 ng/u1

response 5126

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.60	205.46#
176.00	18.80	23.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

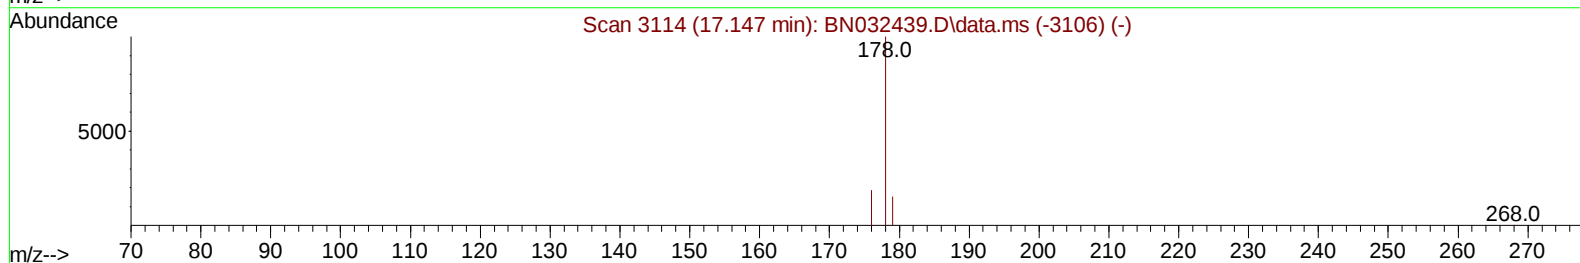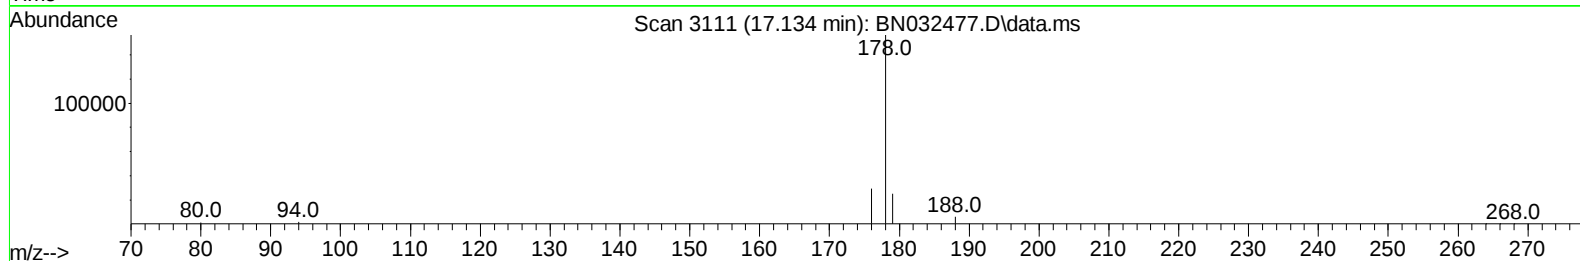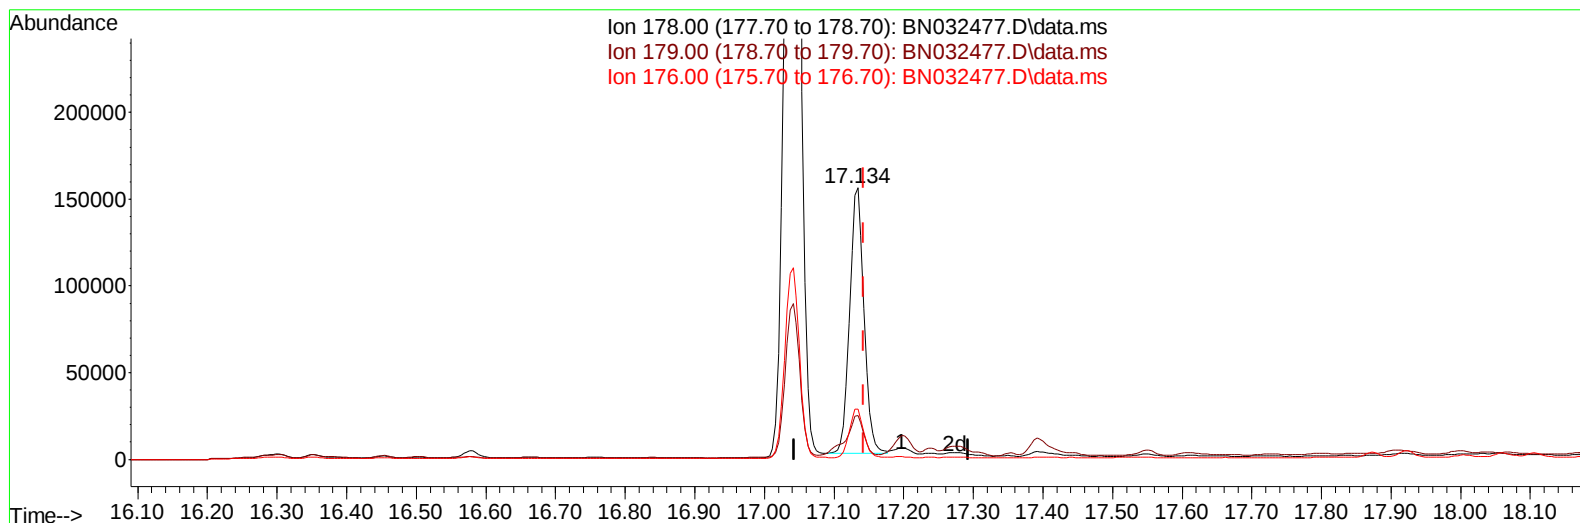

TIC: BN032477.D\data.ms

(16) Anthracene

17.134min (-0.008) 3.09 ng/u1 m

response 217638

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	15.60	16.17
176.00	18.80	18.62
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

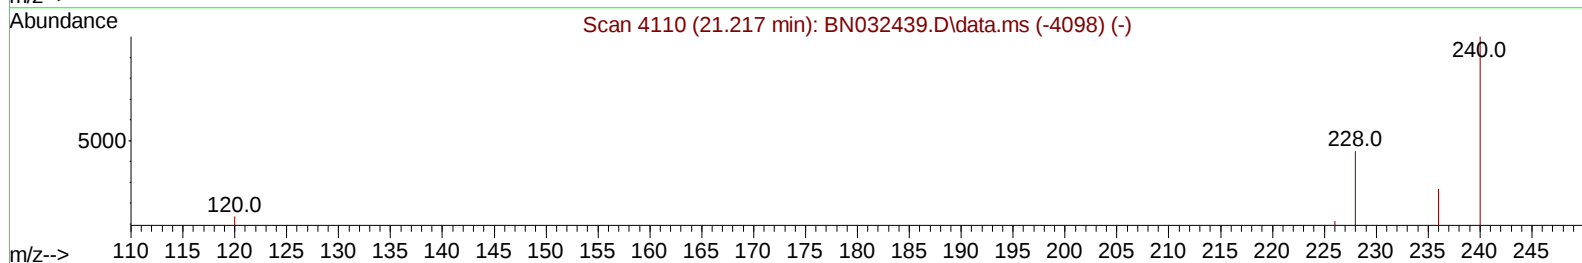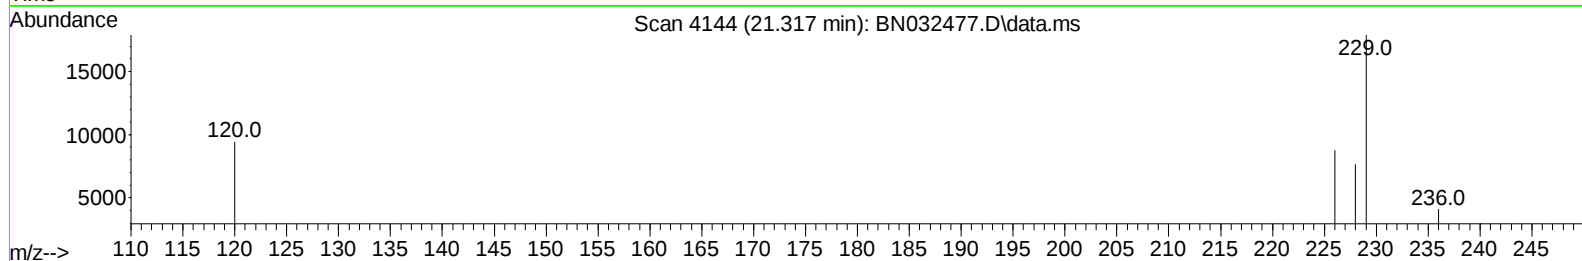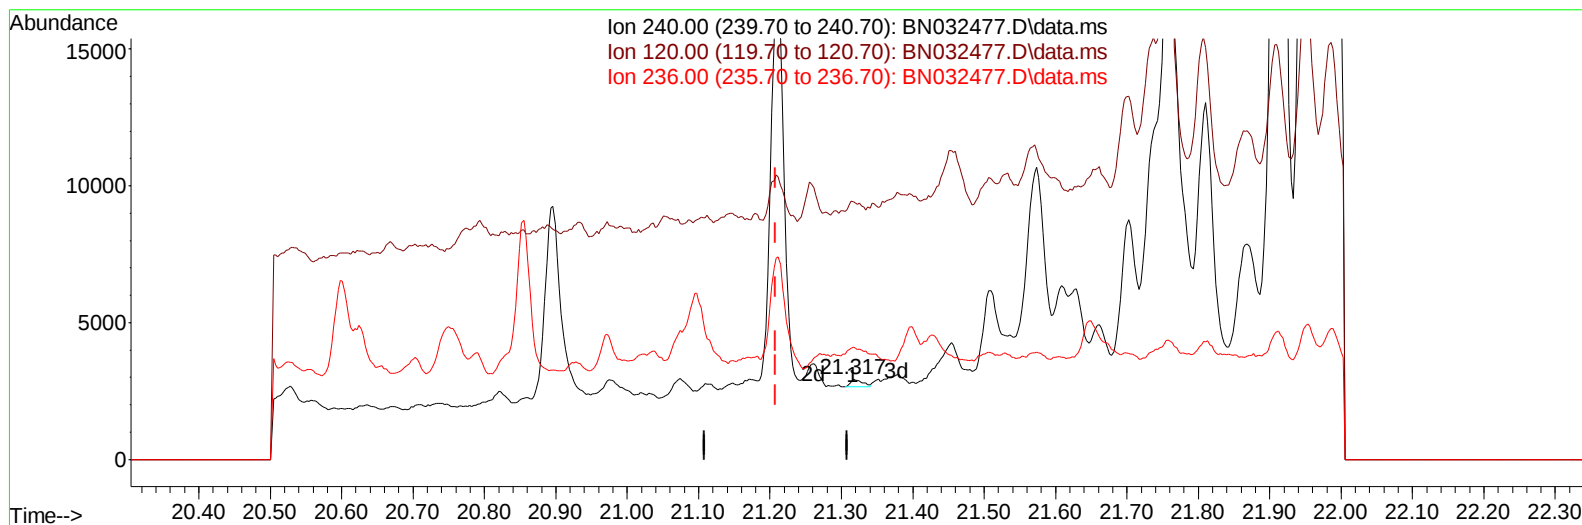

TIC: BN032477.D\data.ms

(17) Chrysene-d12

21.317min (+ 0.108) 0.40 ng/u1

response 307

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	319.87#
236.00	28.40	139.47#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

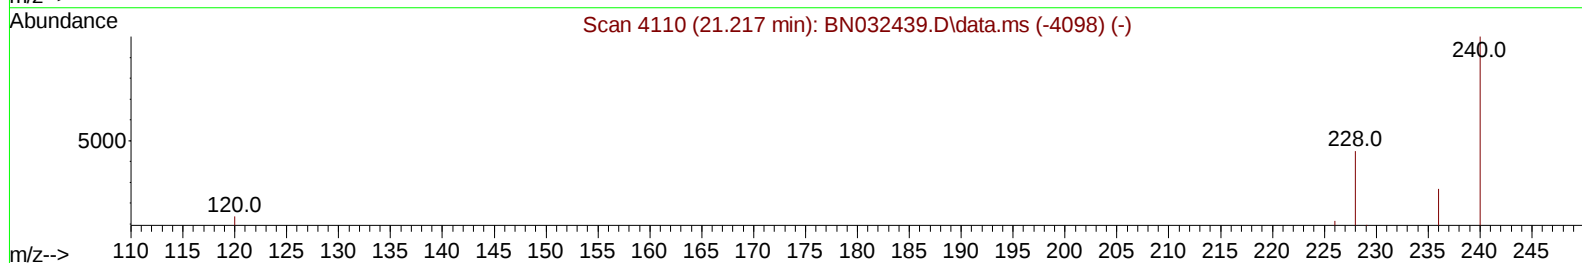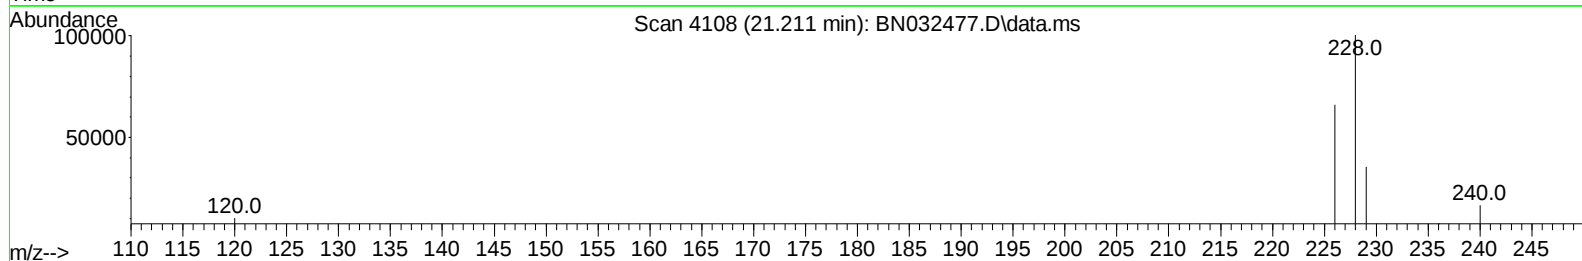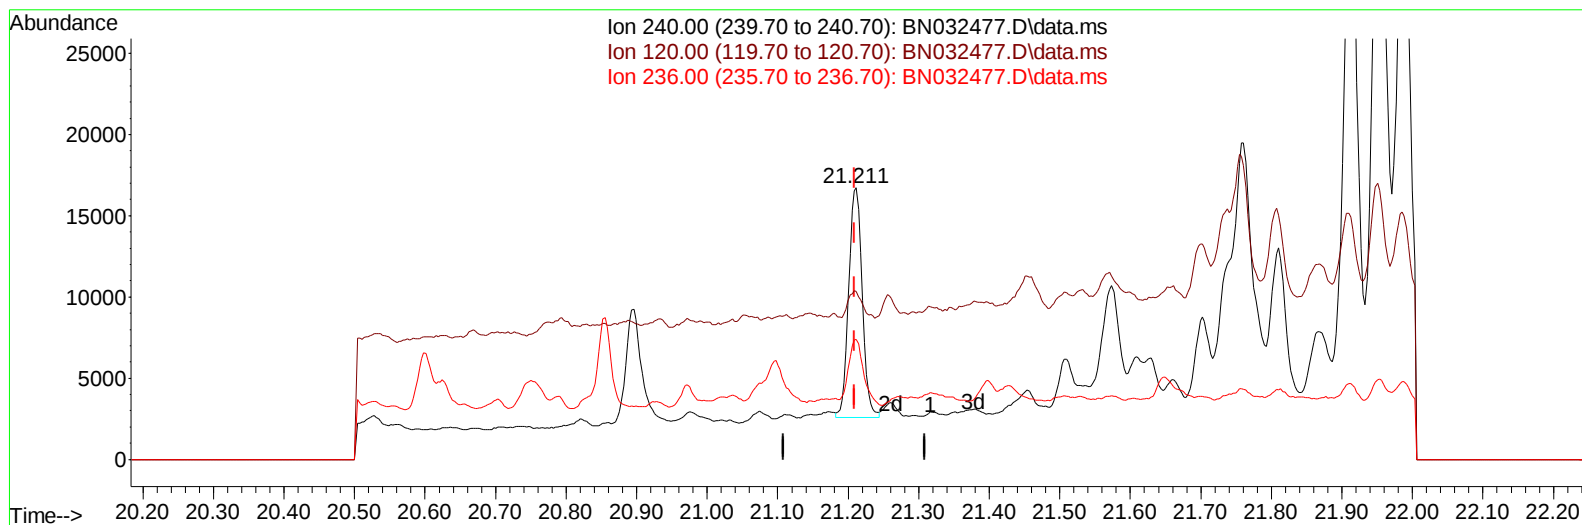

TIC: BN032477.D\data.ms

(17) Chrysene-d12

21.211min (+ 0.003) 0.40 ng/ul m

response 18711

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	61.82#
236.00	28.40	44.28#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

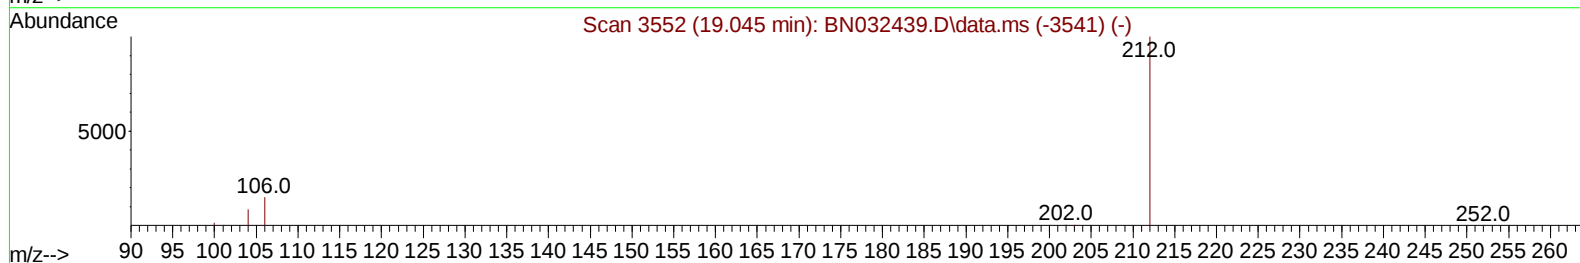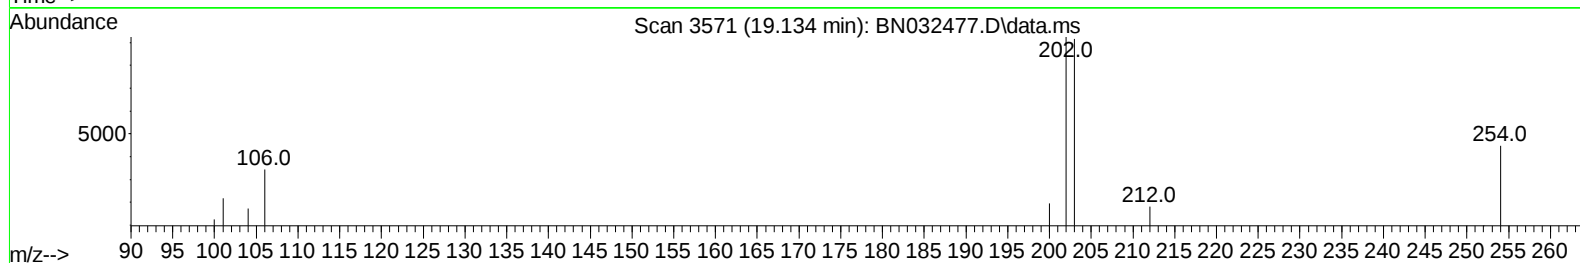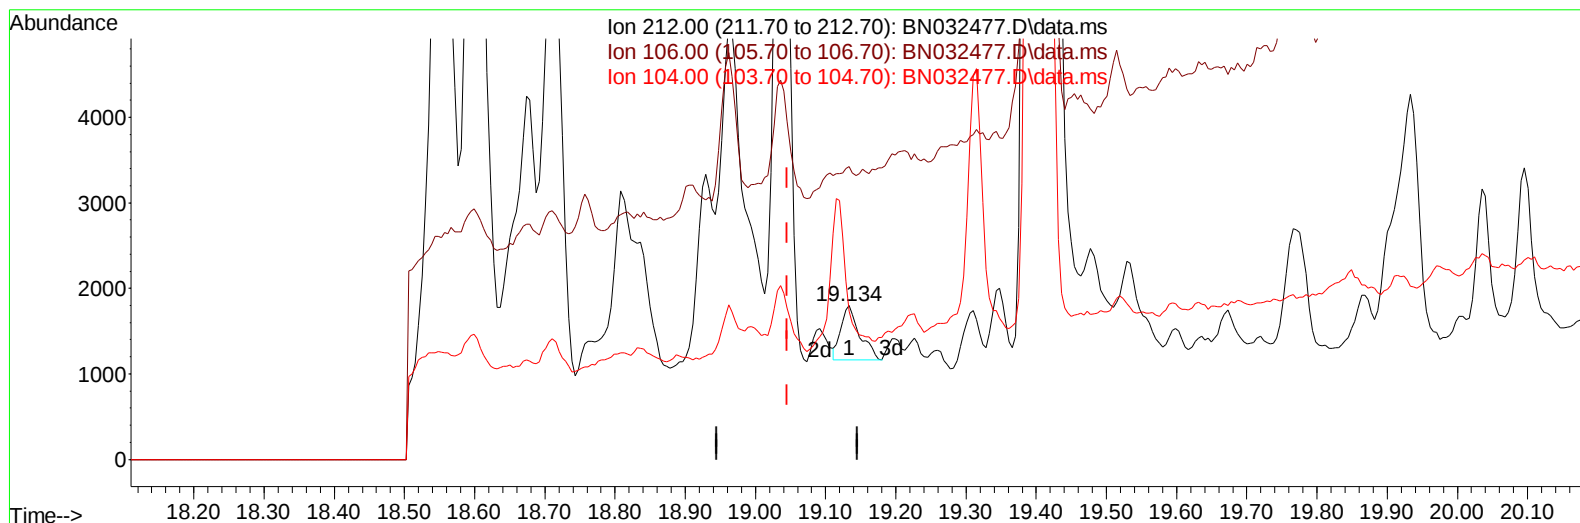

TIC: BN032477.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.134min (+ 0.088) 0.02 ng/u1

response 1181

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	14.70	147.50#
104.00	8.40	259.44#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

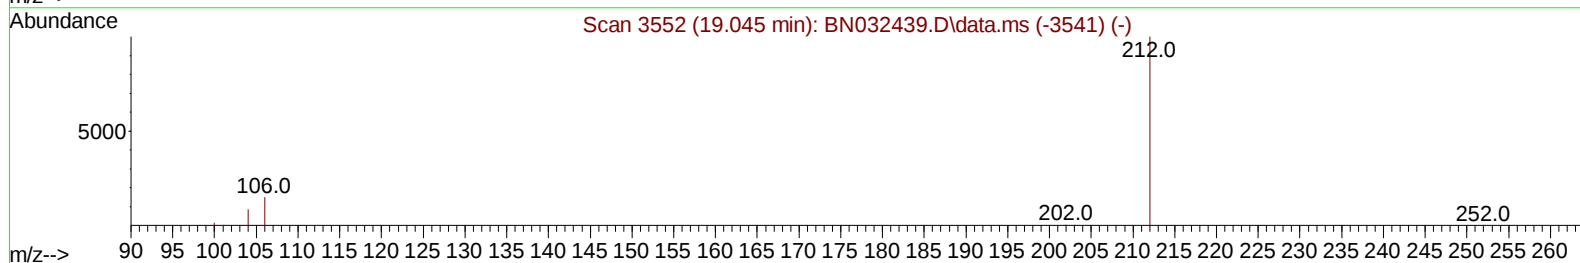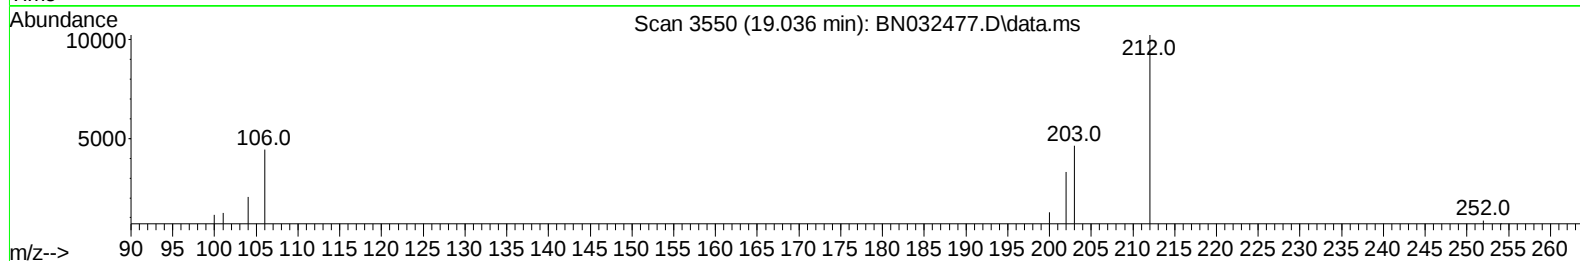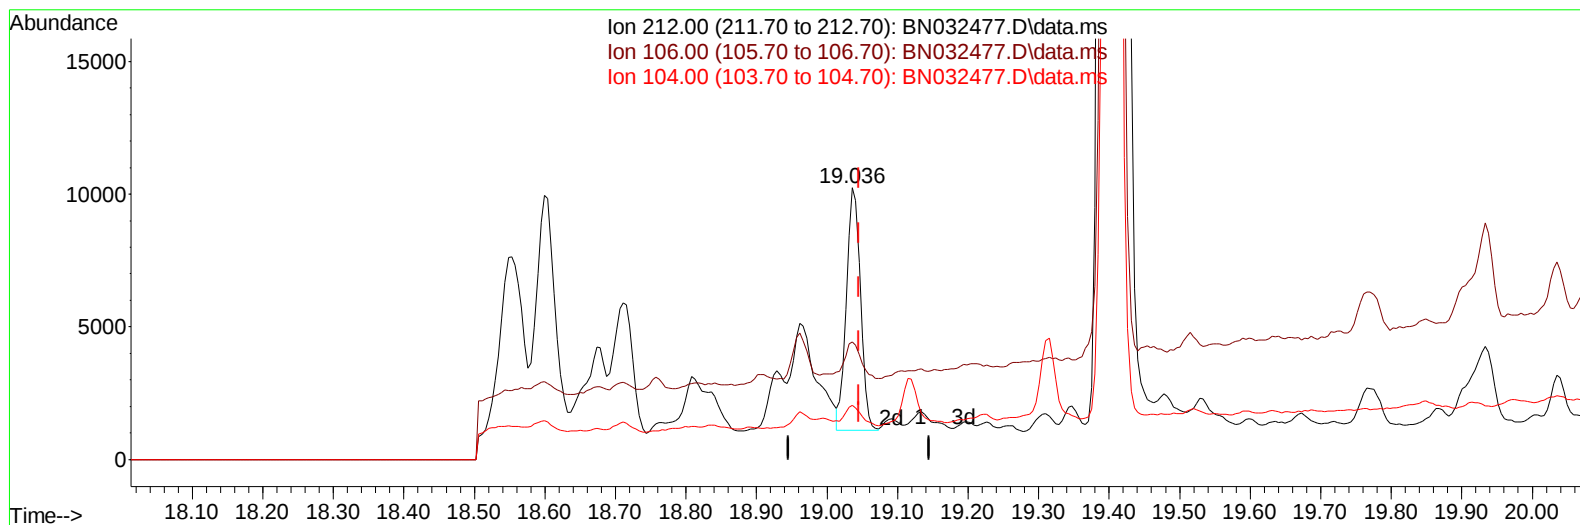

TIC: BN032477.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.036min (-0.009) 0.22 ng/u1 m

response 12609

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	14.70	13.82
104.00	8.40	24.30#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

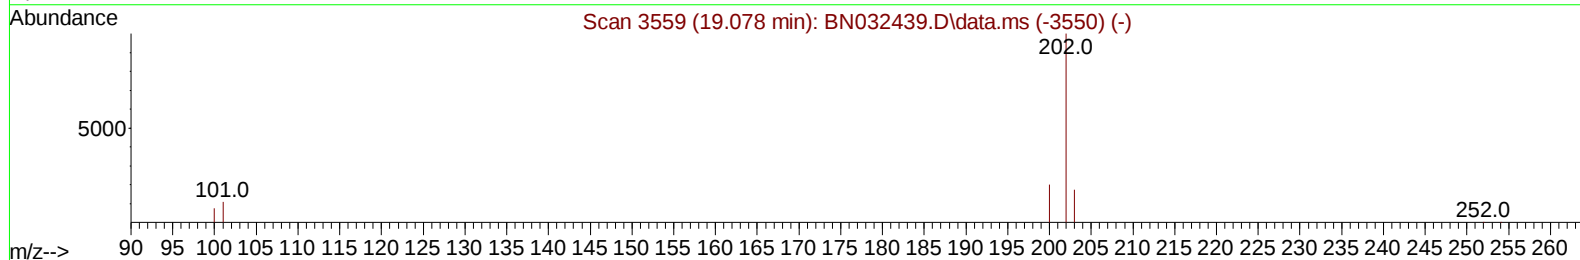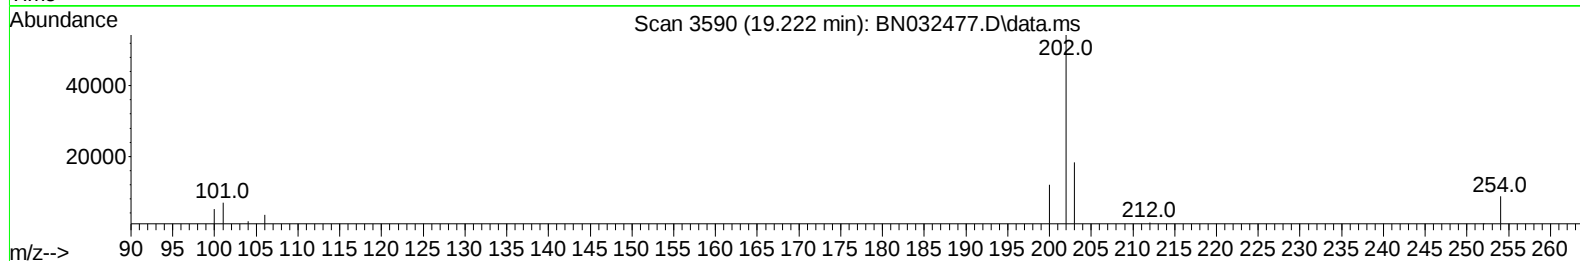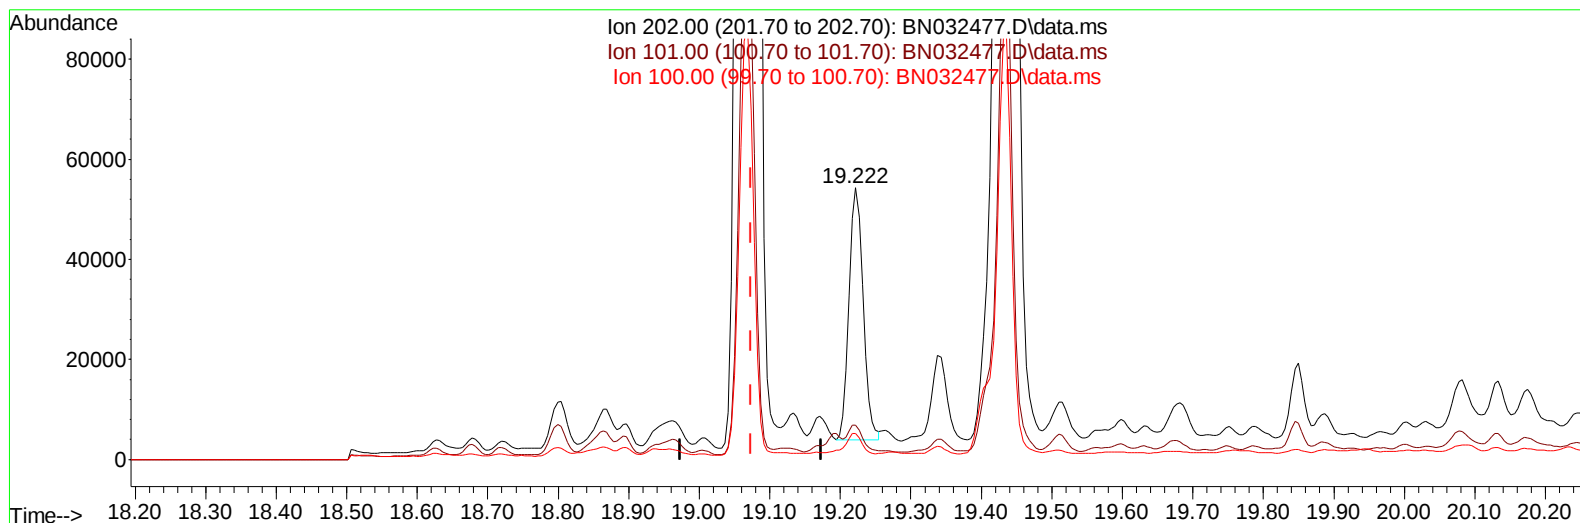

TIC: BN032477.D\data.ms

(19) Fluoranthene (C)

19.222min (+ 0.149) 0.98 ng/u1

response 69666

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.00	12.73
100.00	8.00	9.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

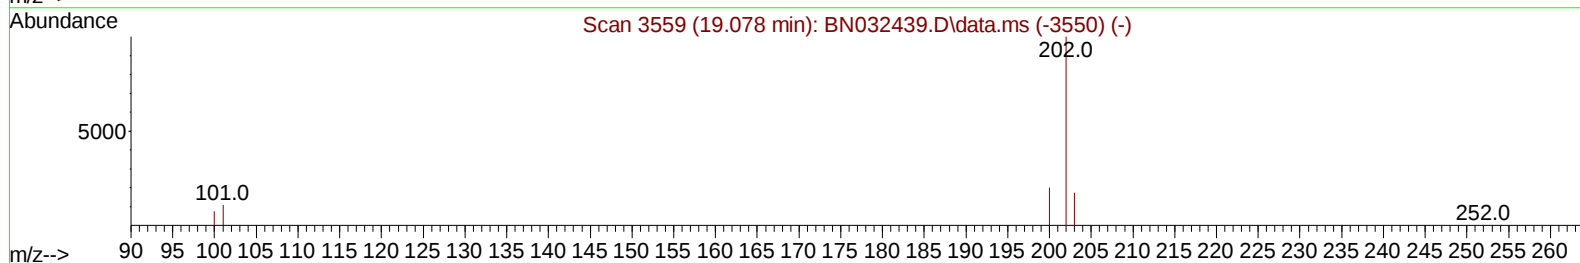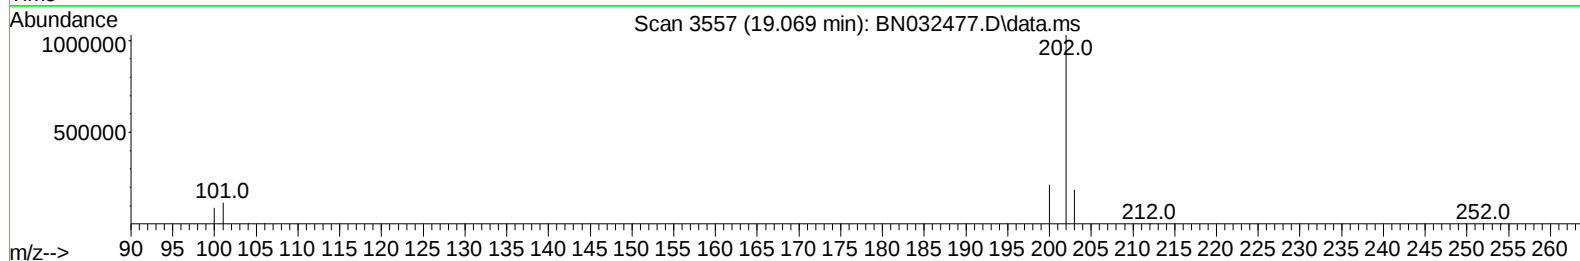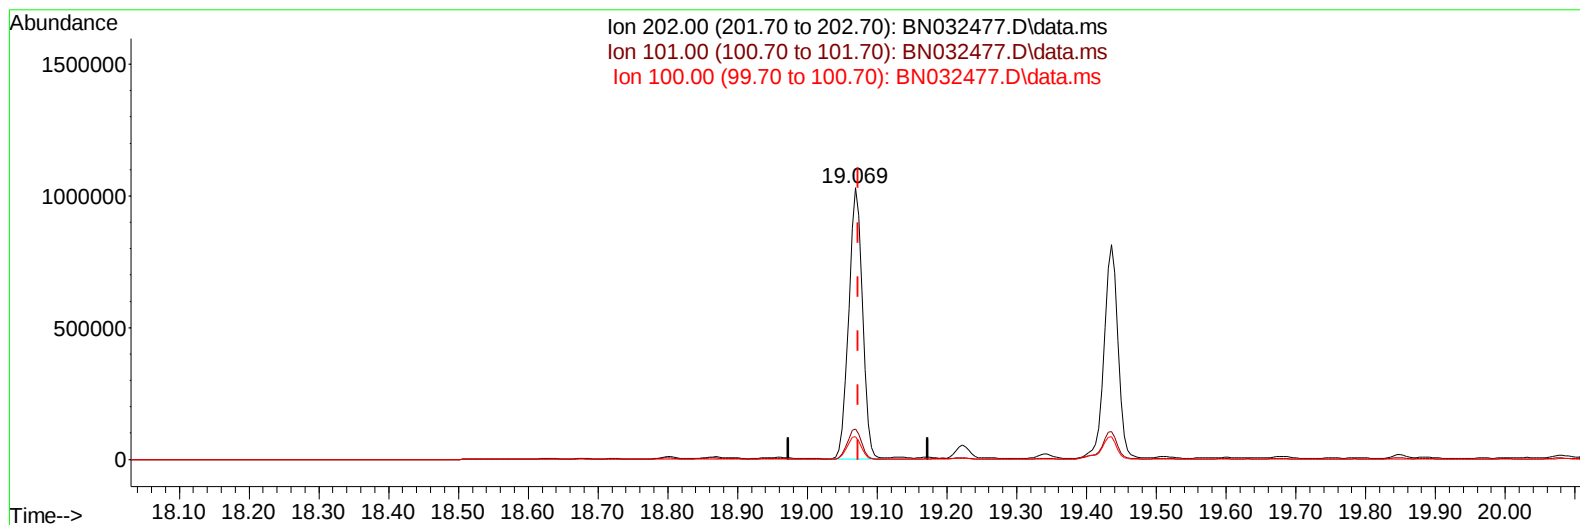

TIC: BN032477.D\data.ms

(19) Fluoranthene (C)

19.069min (-0.005) 19.73 ng/ul m

response 1405923

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.00	11.32
100.00	8.00	8.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

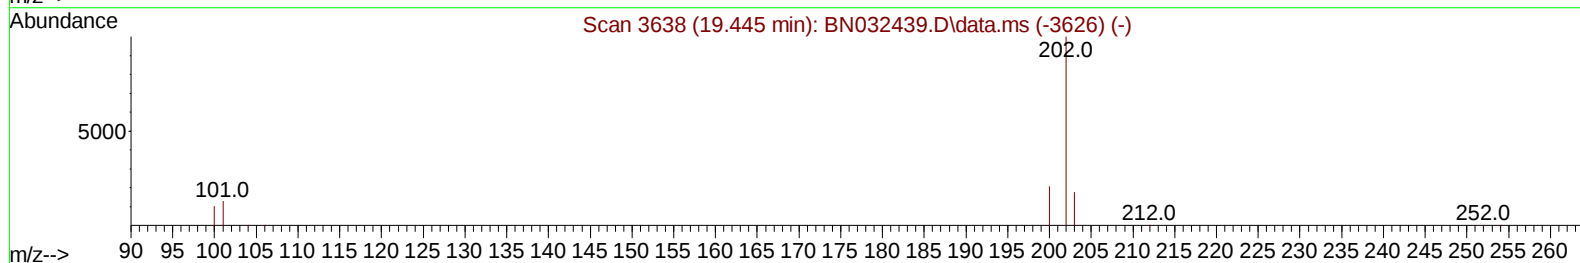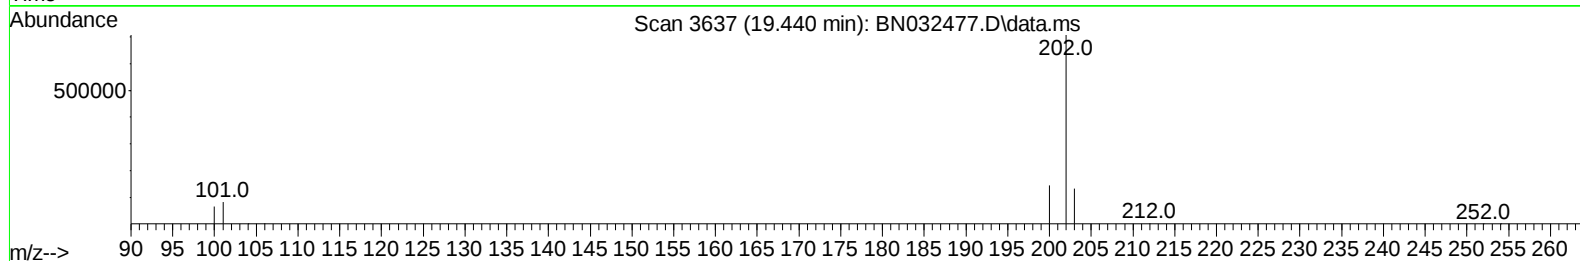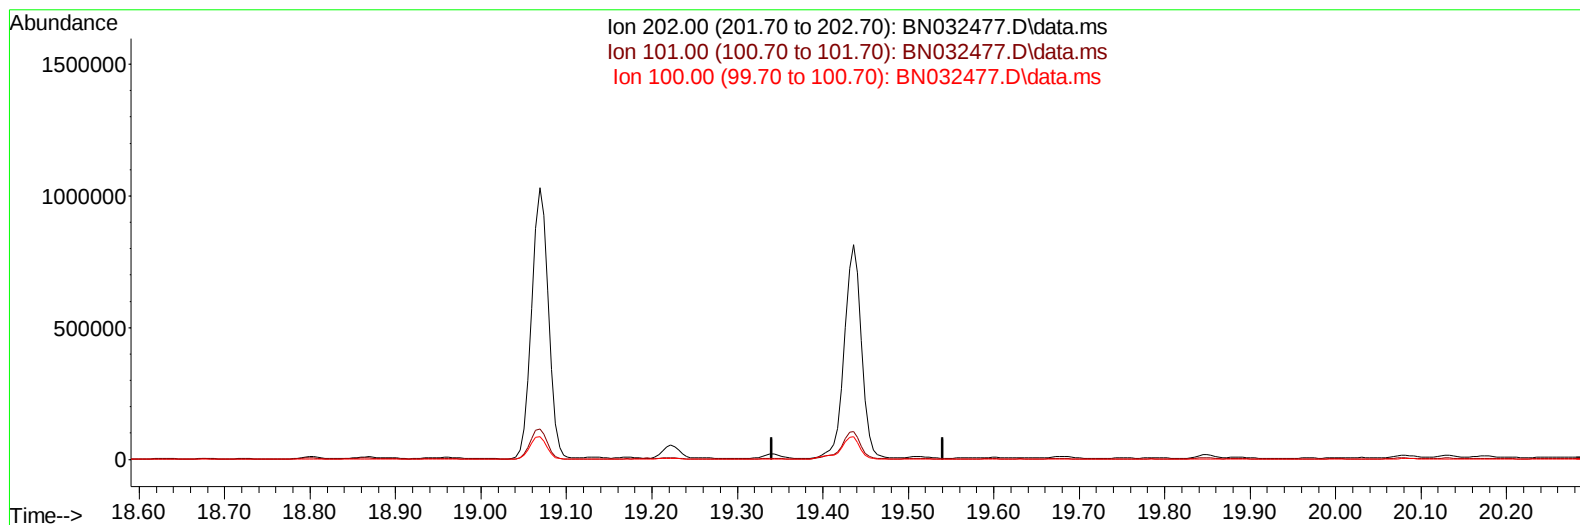

TIC: BN032477.D\data.ms

(20) Pyrene

19.440min (-19.440) 0.00 ng/u1

response 0

Ion	Exp%	Act%
202.00	100.00	0.00
101.00	13.70	0.00#
100.00	10.90	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

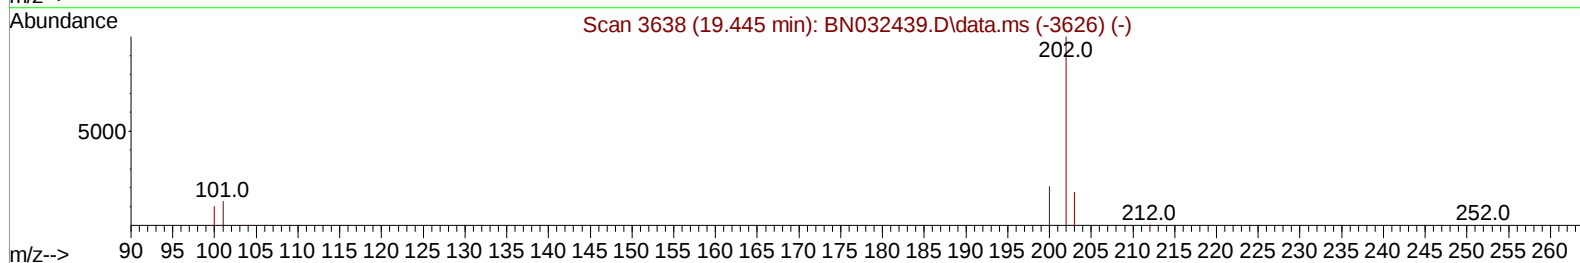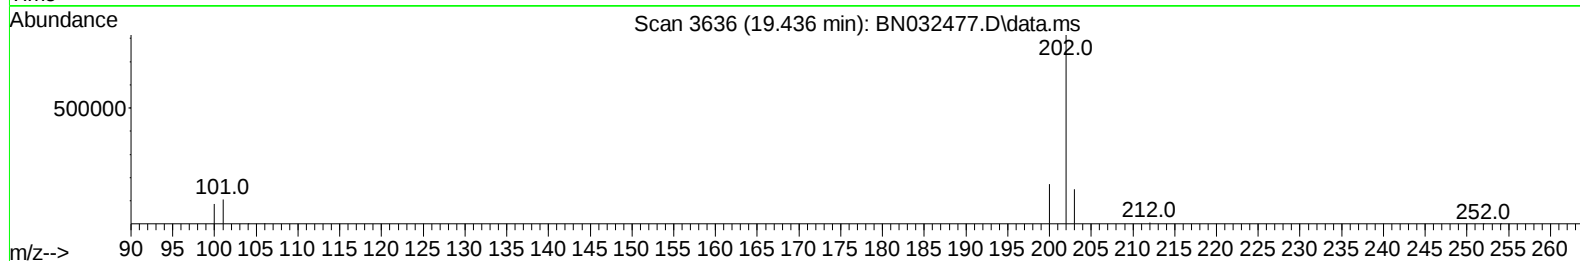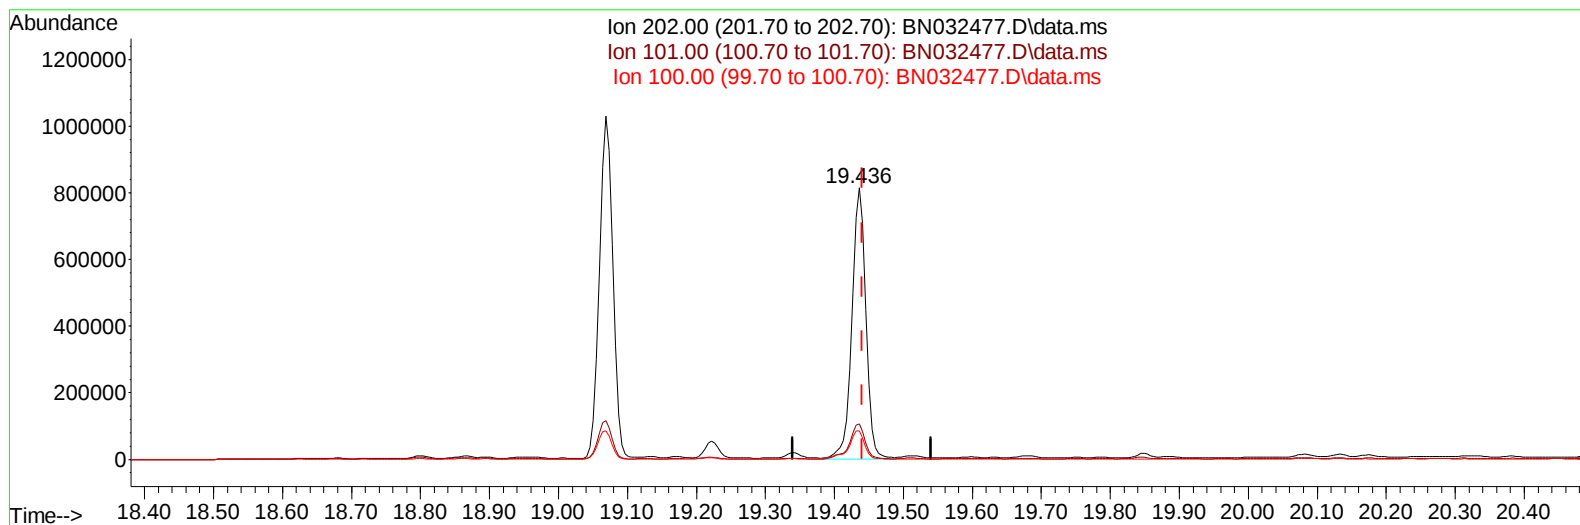

TIC: BN032477.D\data.ms

(20) Pyrene

19.436min (-0.005) 15.40 ng/ul m

response 1147006

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.70	13.09
100.00	10.90	10.52
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

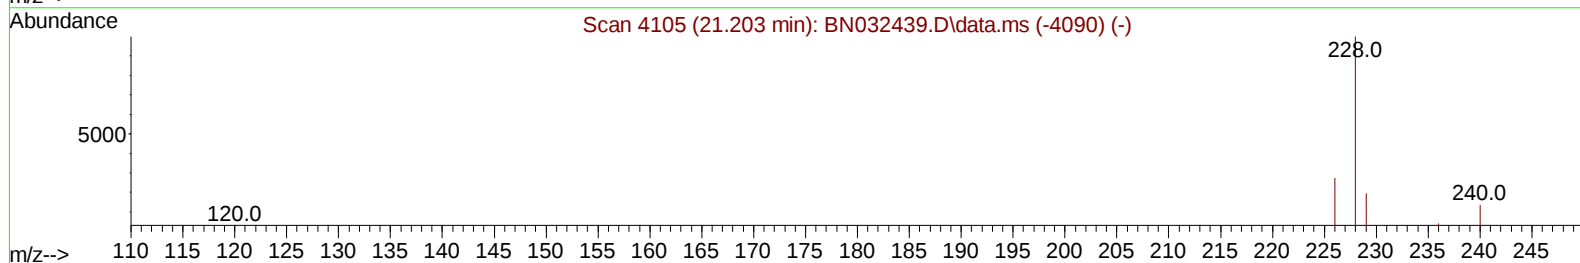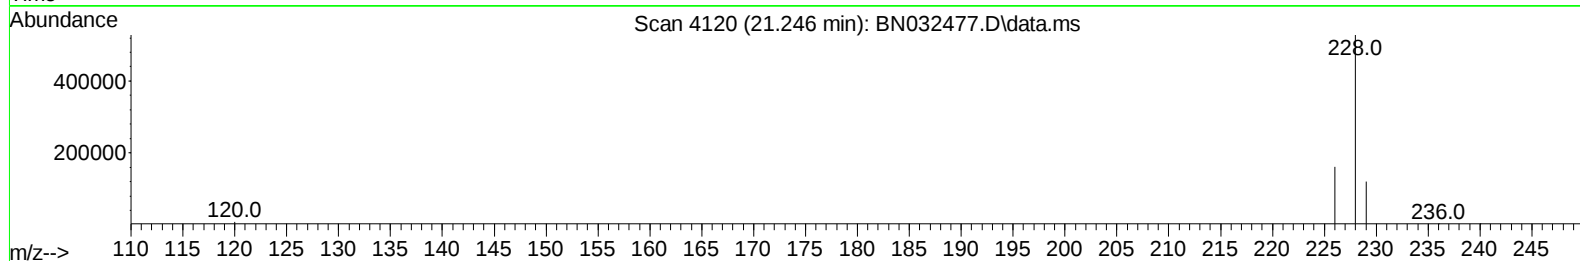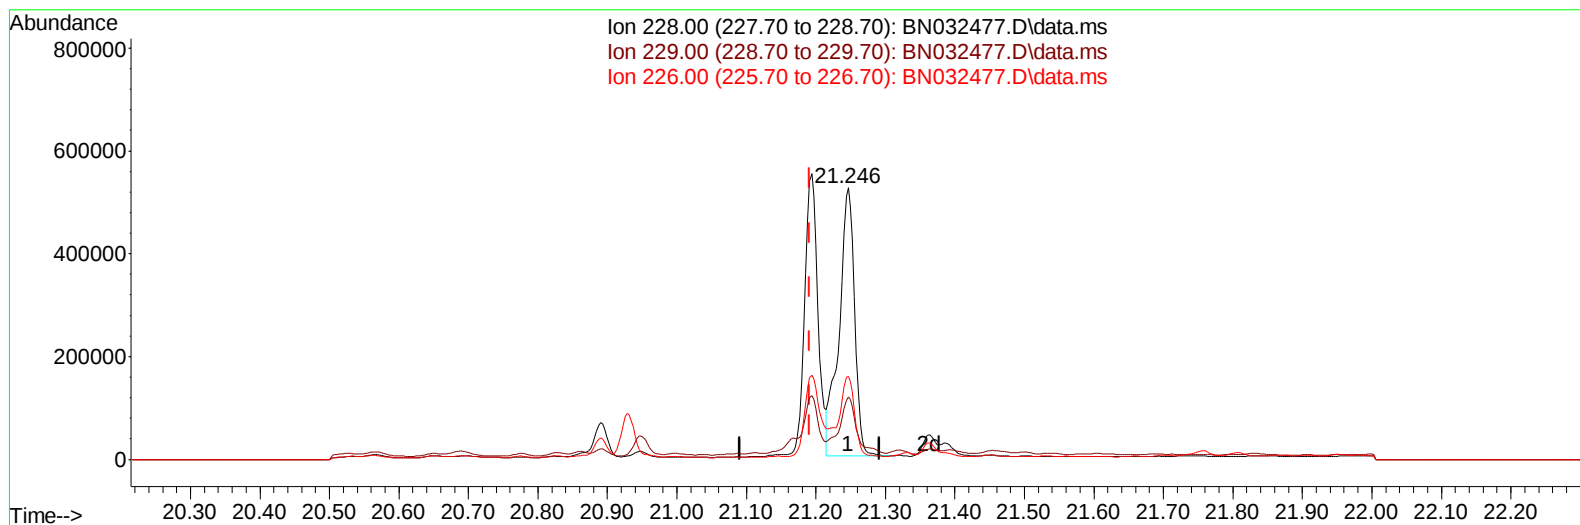

TIC: BN032477.D\data.ms

(21) Benzo(a)anthracene

21.246min (+ 0.055) 12.02 ng/u1

response 811831

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.60	22.98
226.00	27.30	30.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

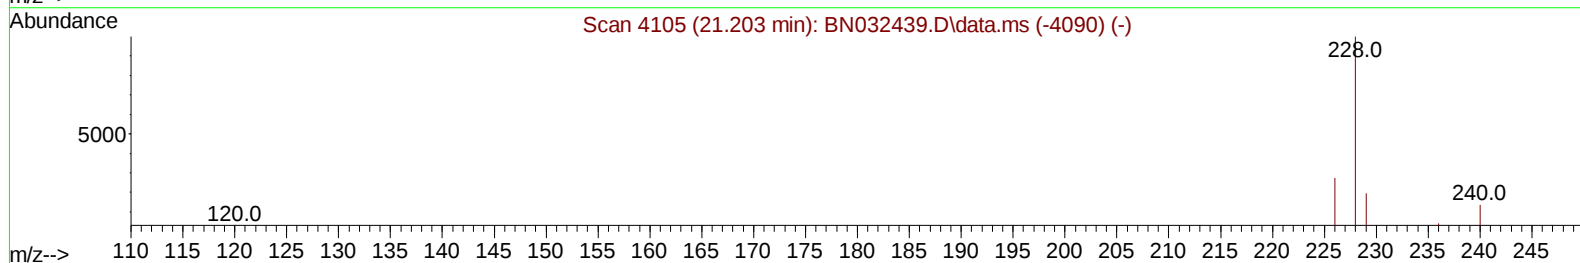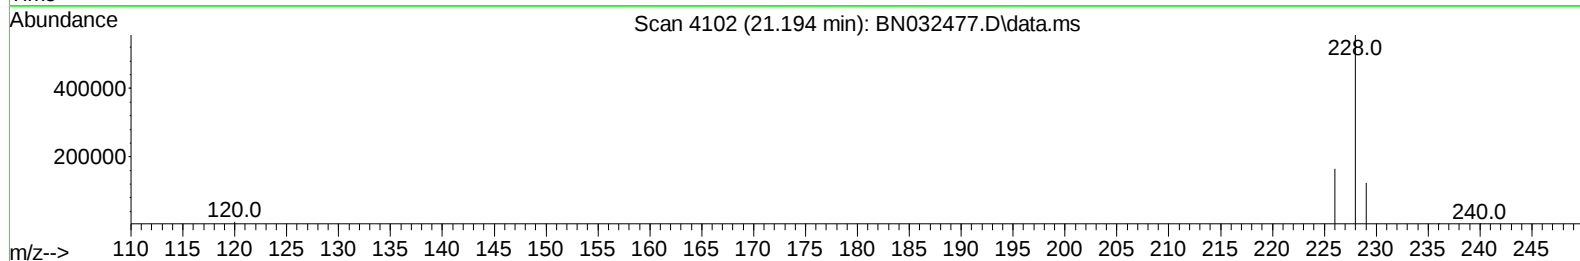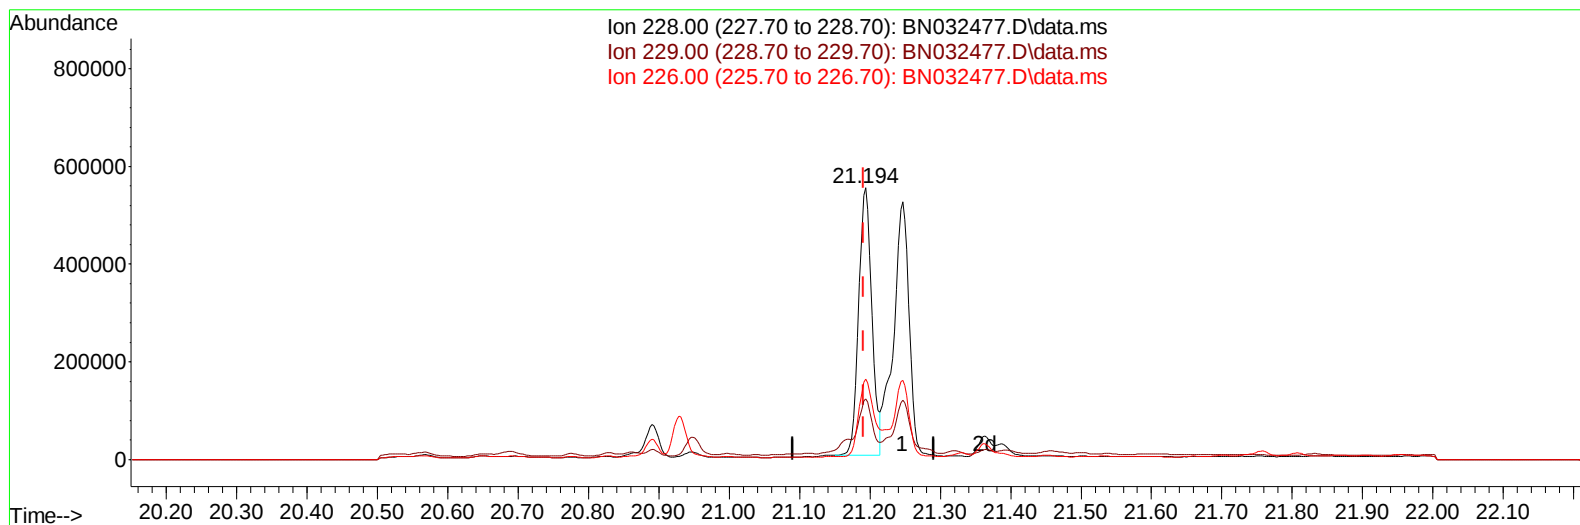

TIC: BN032477.D\data.ms

(21) Benzo(a)anthracene

21.194min (+ 0.003) 10.66 ng/ul m

response 720081

Ion	Exp%	Act%
228.00	100.00	100.00
229.00	19.60	22.34
226.00	27.30	29.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

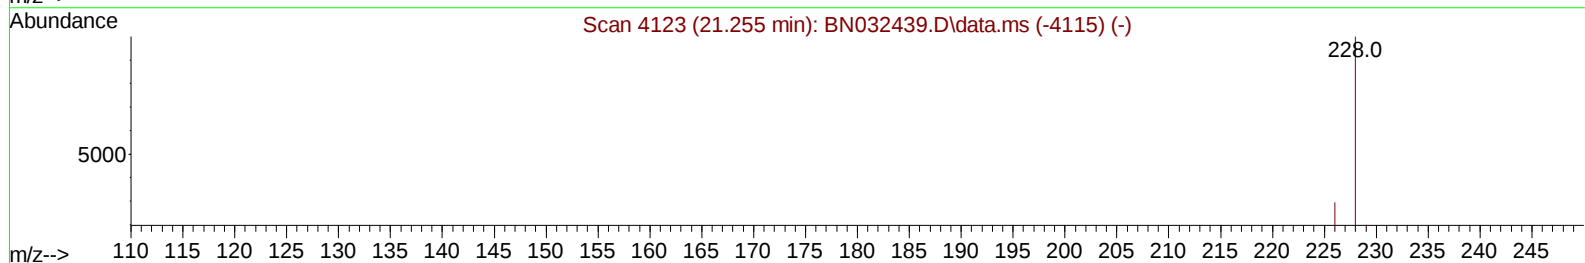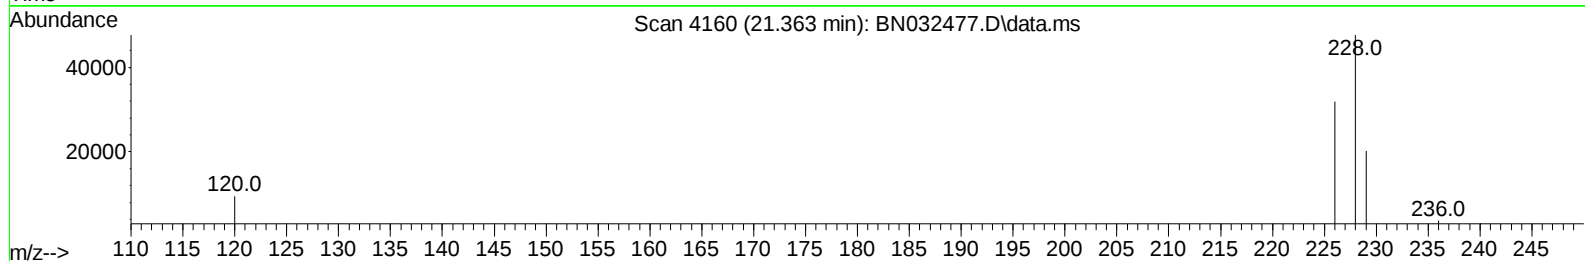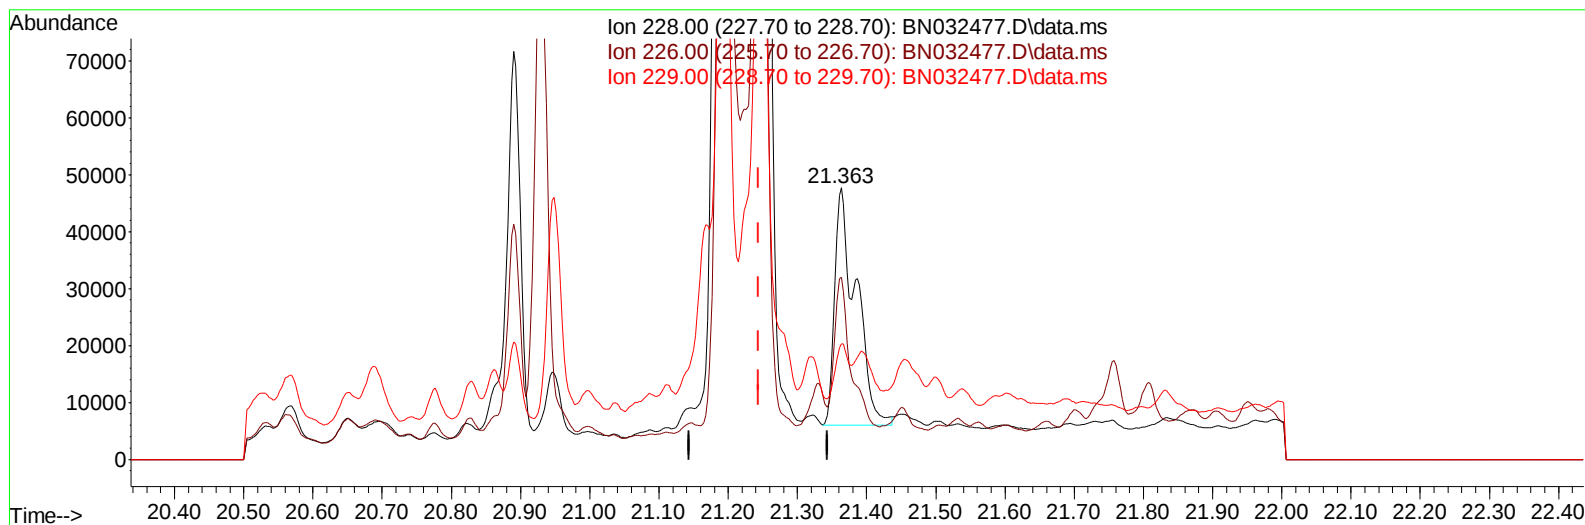

TIC: BN032477.D\data.ms

(22) Chrysene

21.363min (+ 0.120) 1.20 ng/u1

response 88867

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.50	67.02#
229.00	19.60	42.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

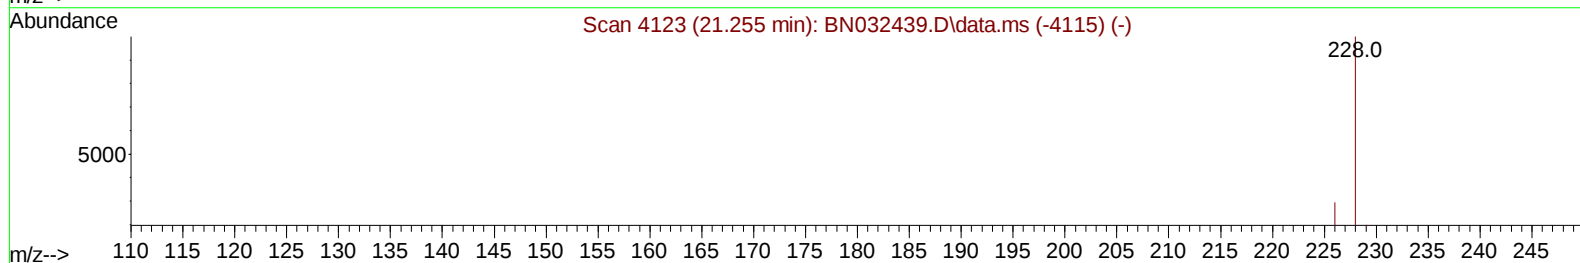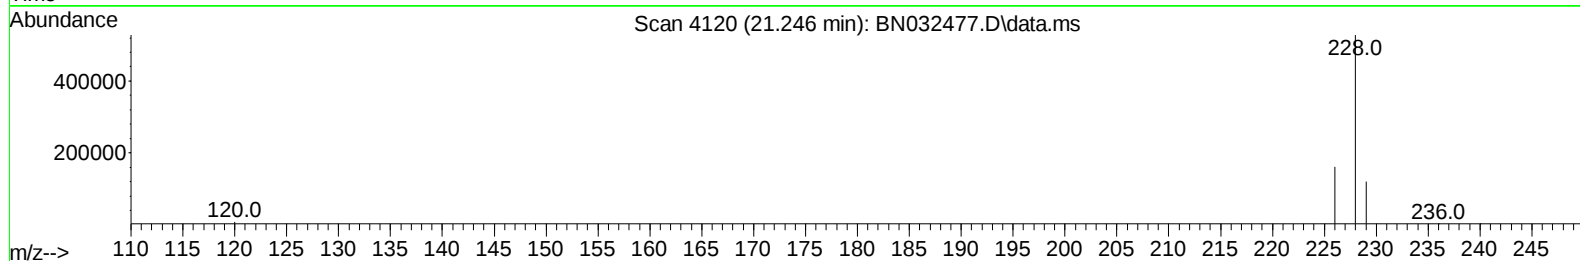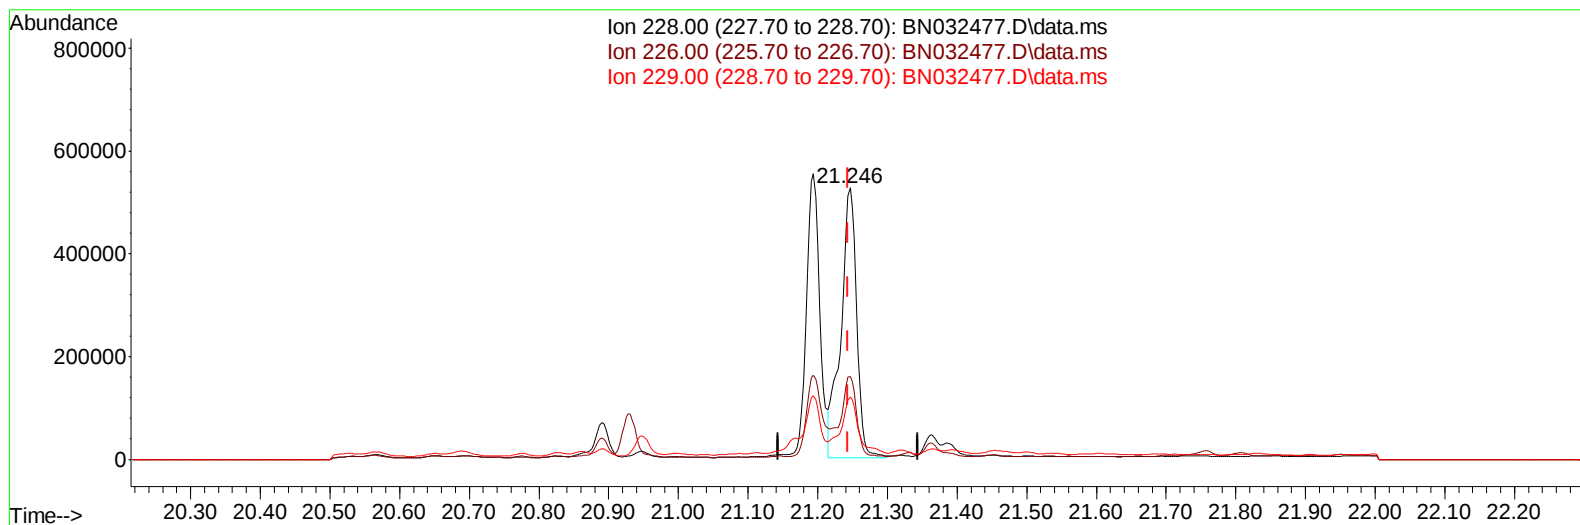

TIC: BN032477.D\data.ms

(22) Chrysene

21.246min (+ 0.003) 11.16 ng/ul m

response 827128

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.50	30.63
229.00	19.60	22.98
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

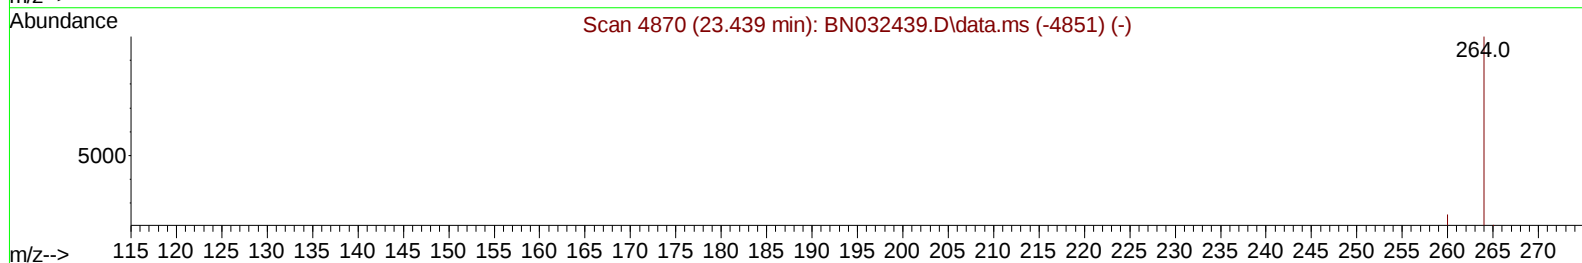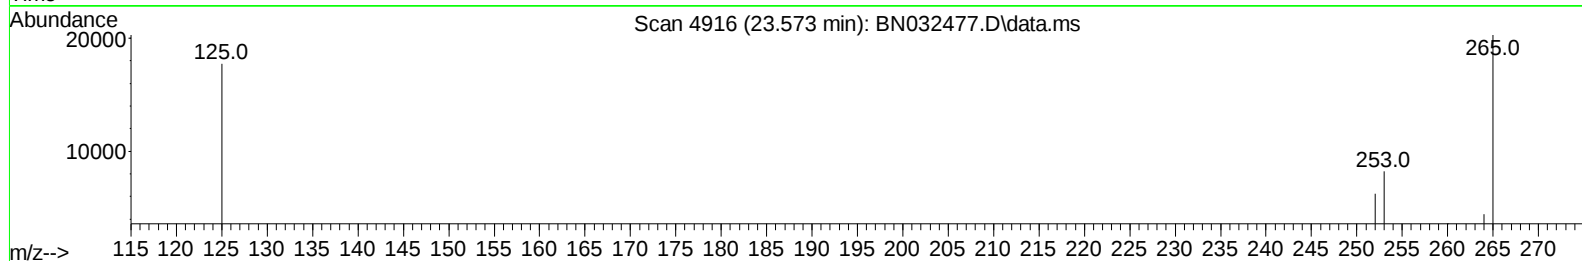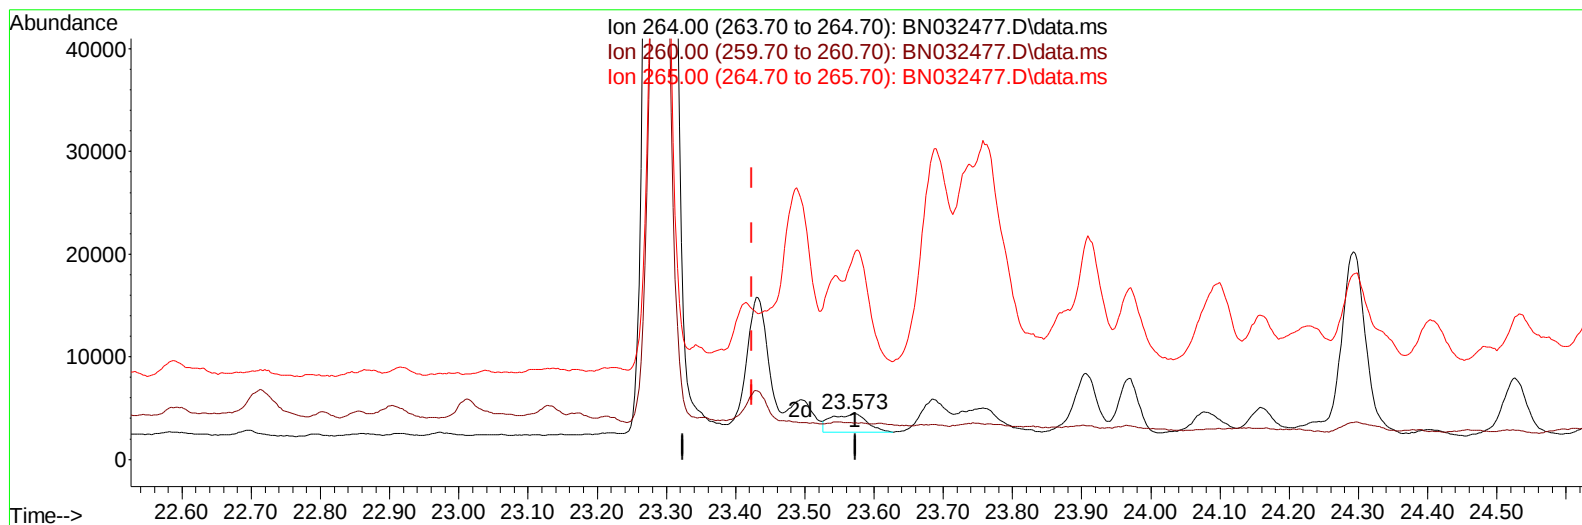

TIC: BN032477.D\data.ms

(23) Perylene-d12 (I)

23.573min (+ 0.149) 0.40 ng/u1

response 6312

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	80.98#
265.00	67.20	457.07#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

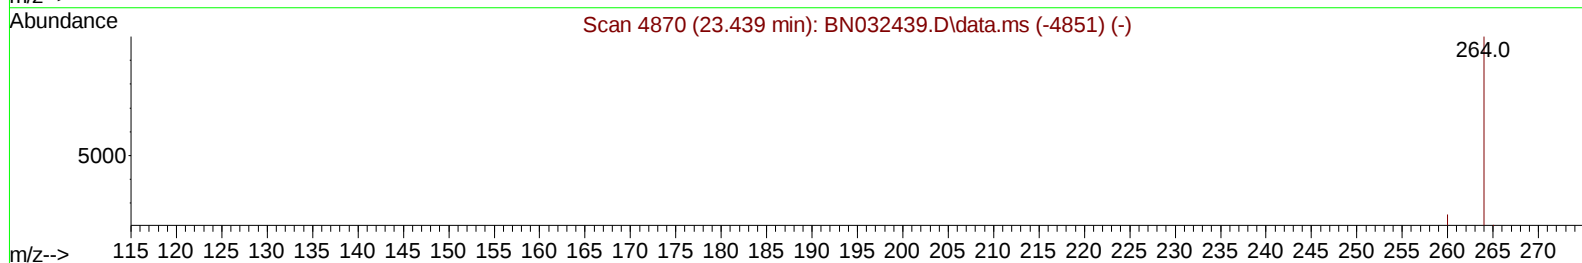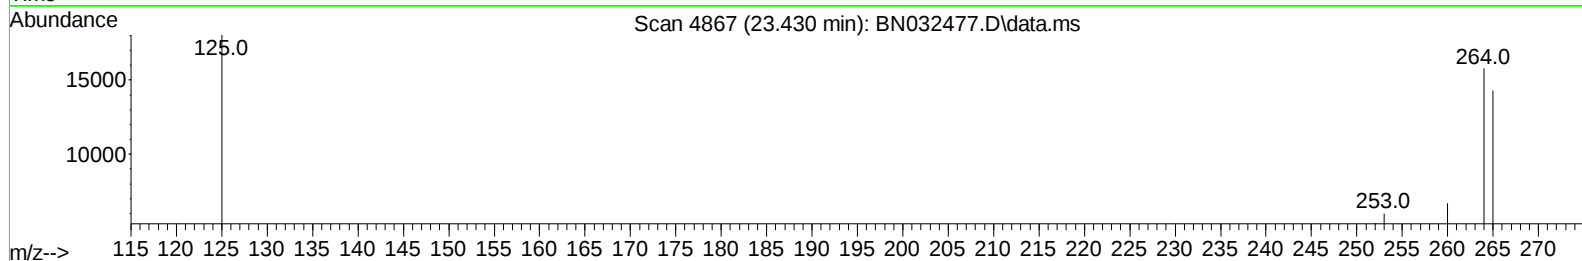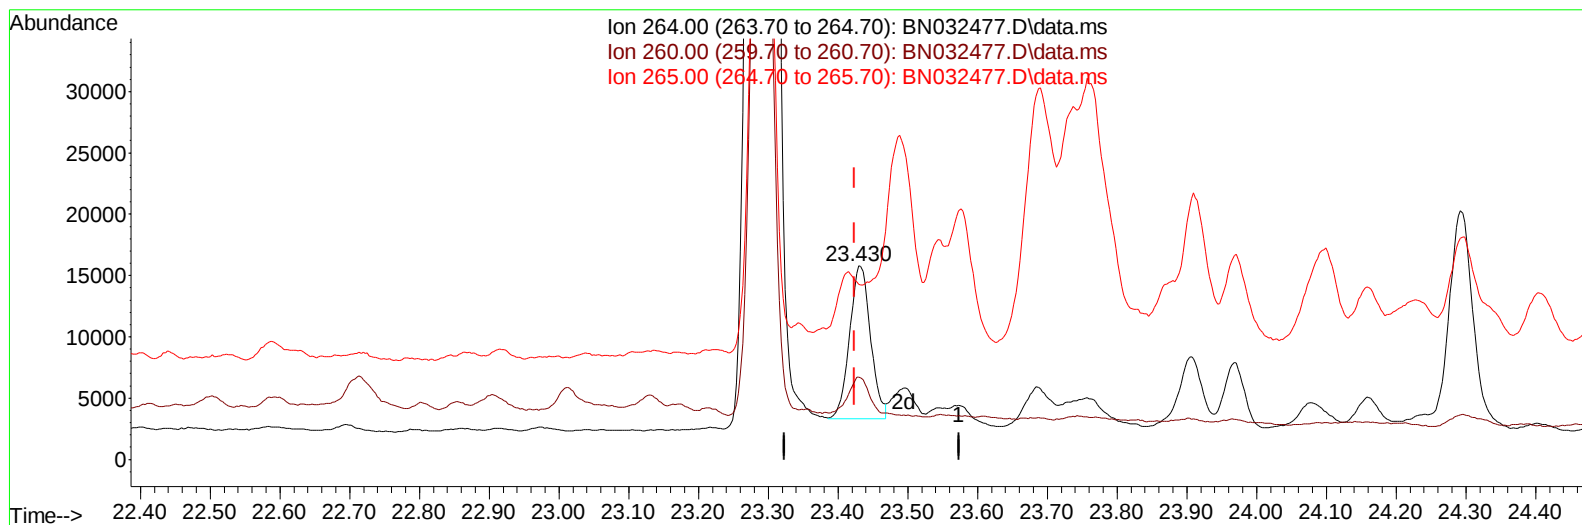

TIC: BN032477.D\data.ms

(23) Perylene-d12 (I)

23.430min (+ 0.006) 0.40 ng/ul m

response 26086

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	42.43#
265.00	67.20	90.60#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

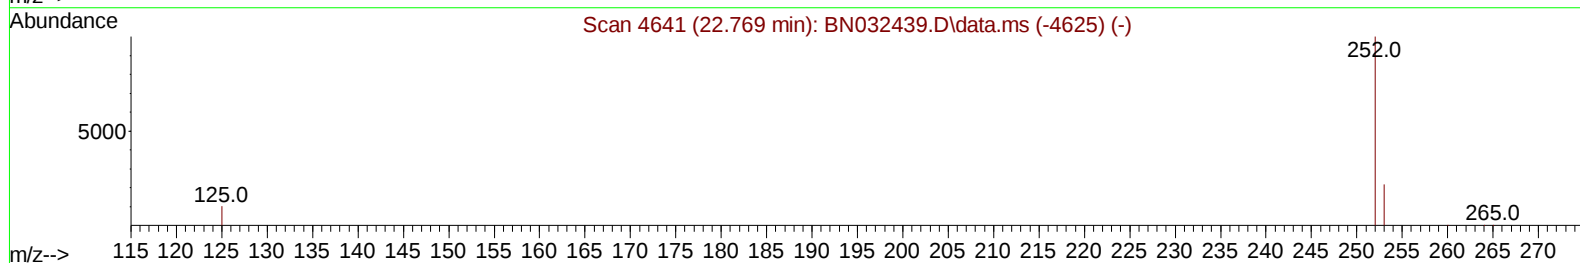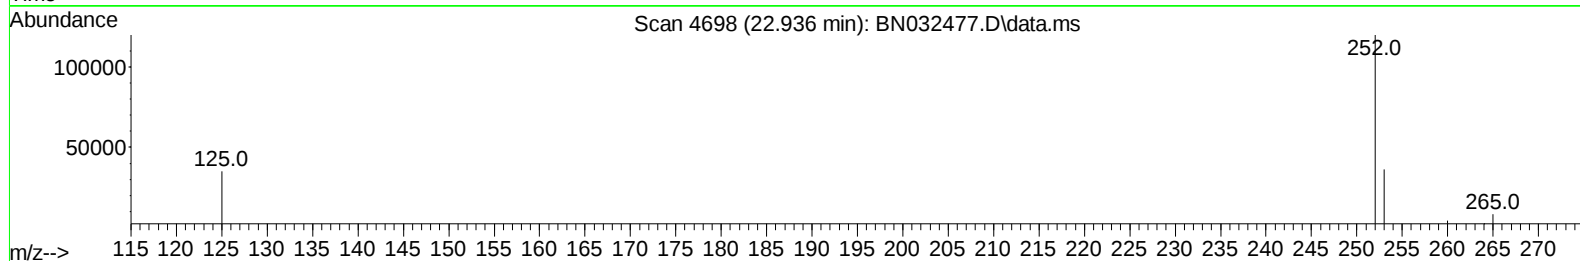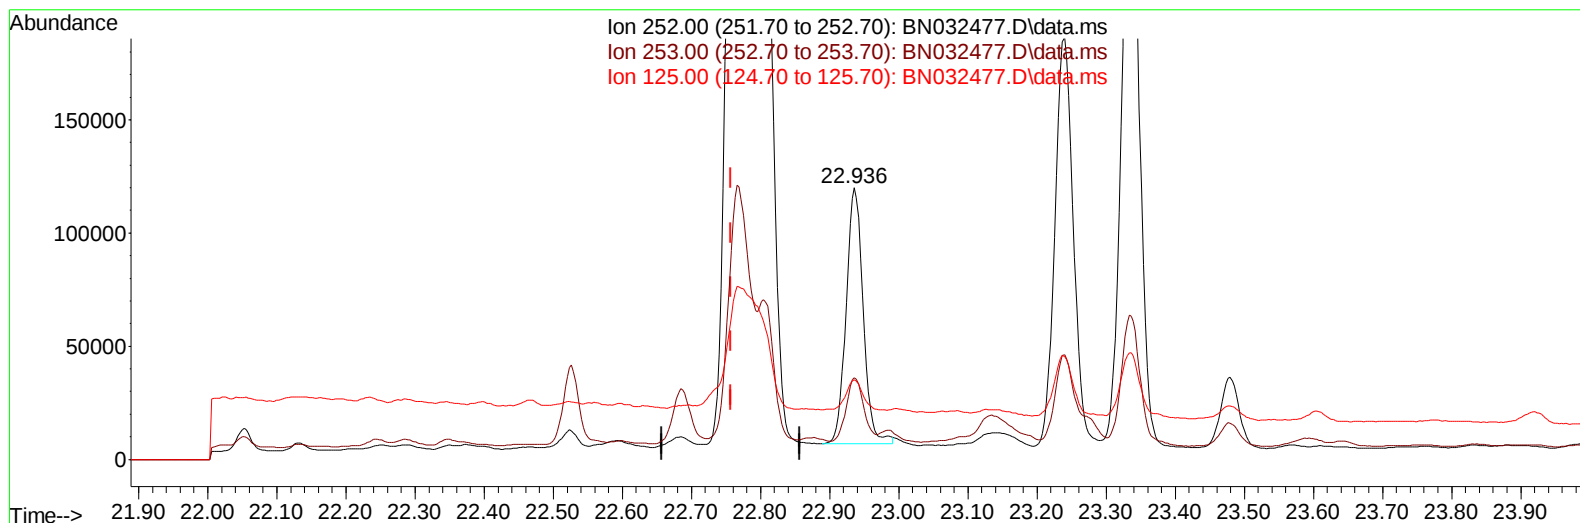

TIC: BN032477.D\data.ms

(24) Benzo(b)fluoranthene

22.936min (+ 0.178) 1.71 ng/u1

response 194206

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.10	30.19
125.00	16.00	29.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

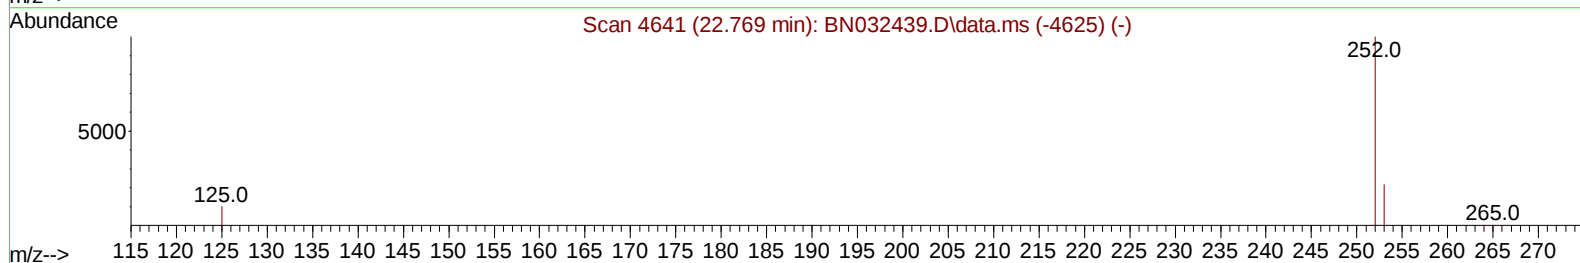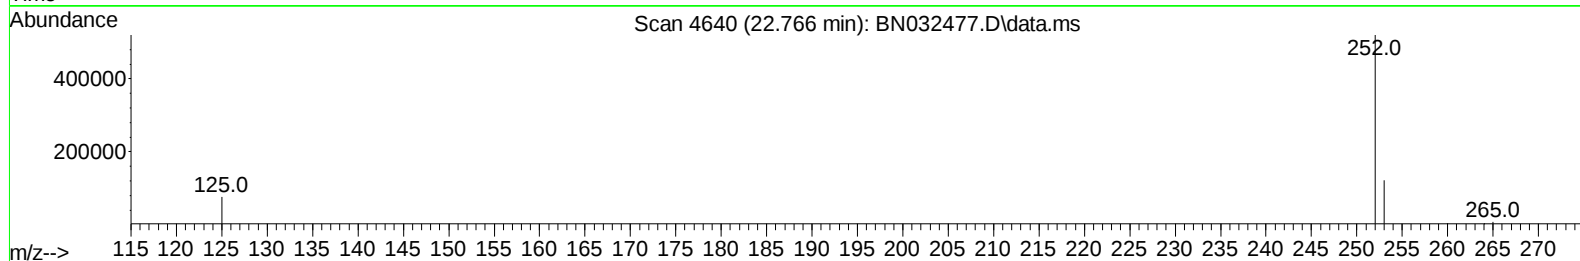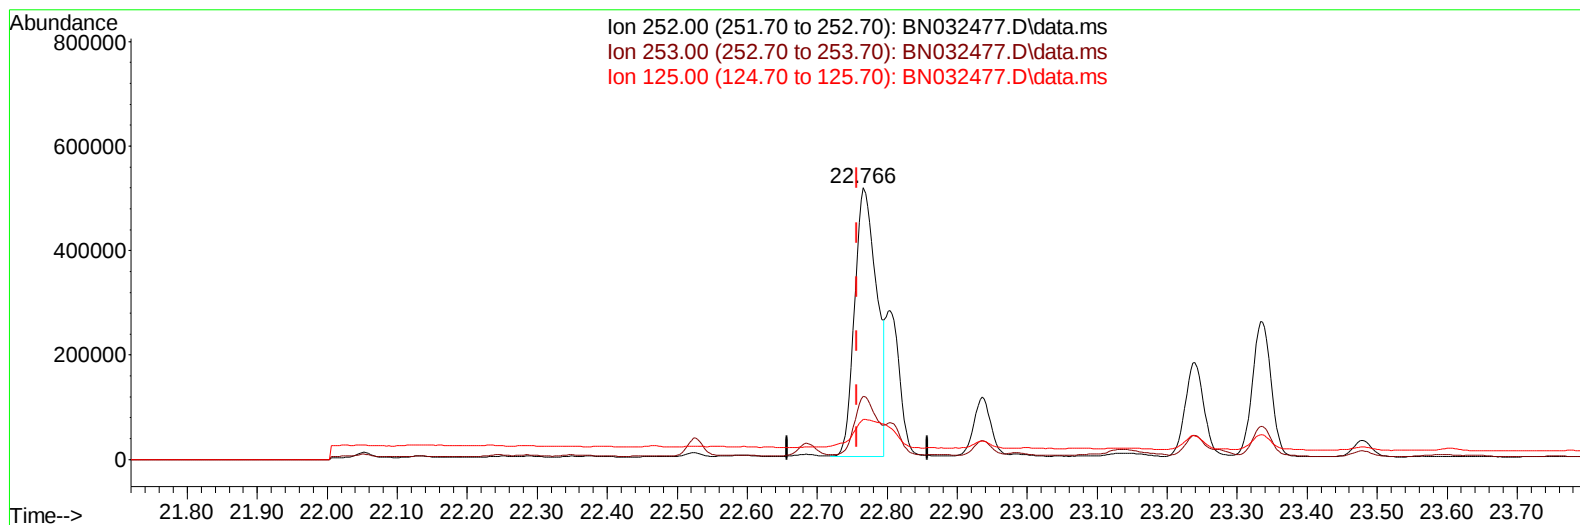

TIC: BN032477.D\data.ms

(24) Benzo(b)fluoranthene

22.766min (+ 0.009) 10.04 ng/ul m

response 1137959

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.10	23.30
125.00	16.00	14.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

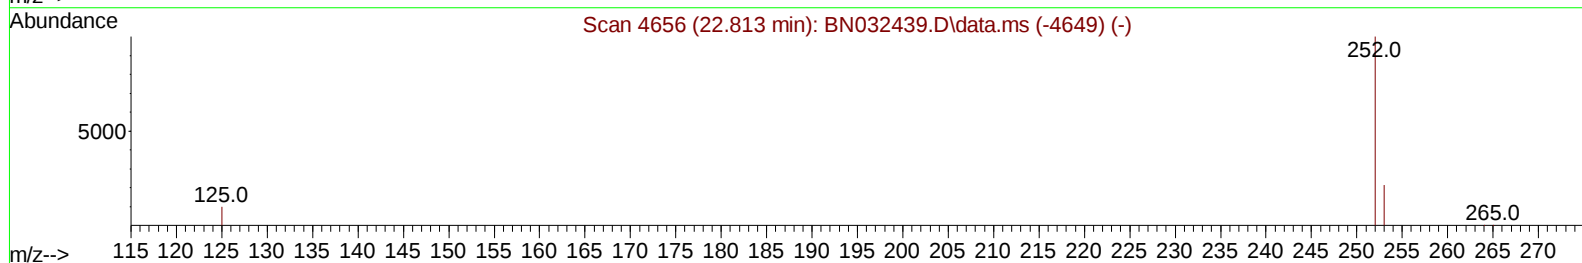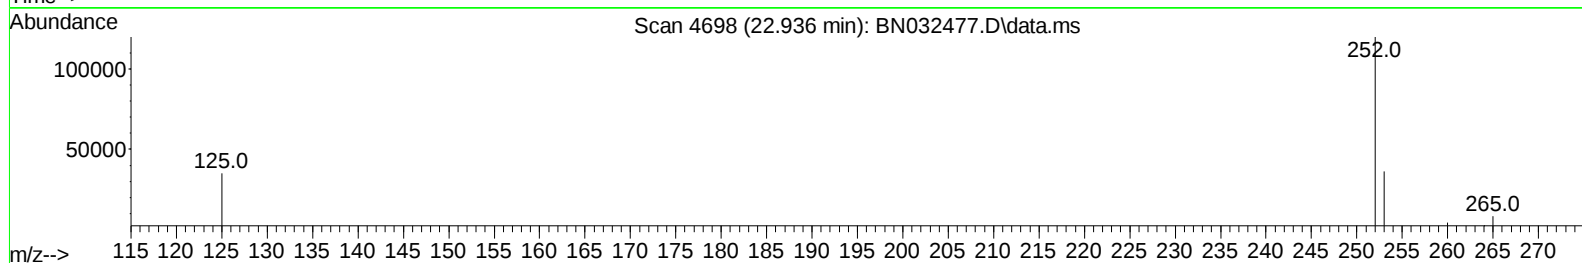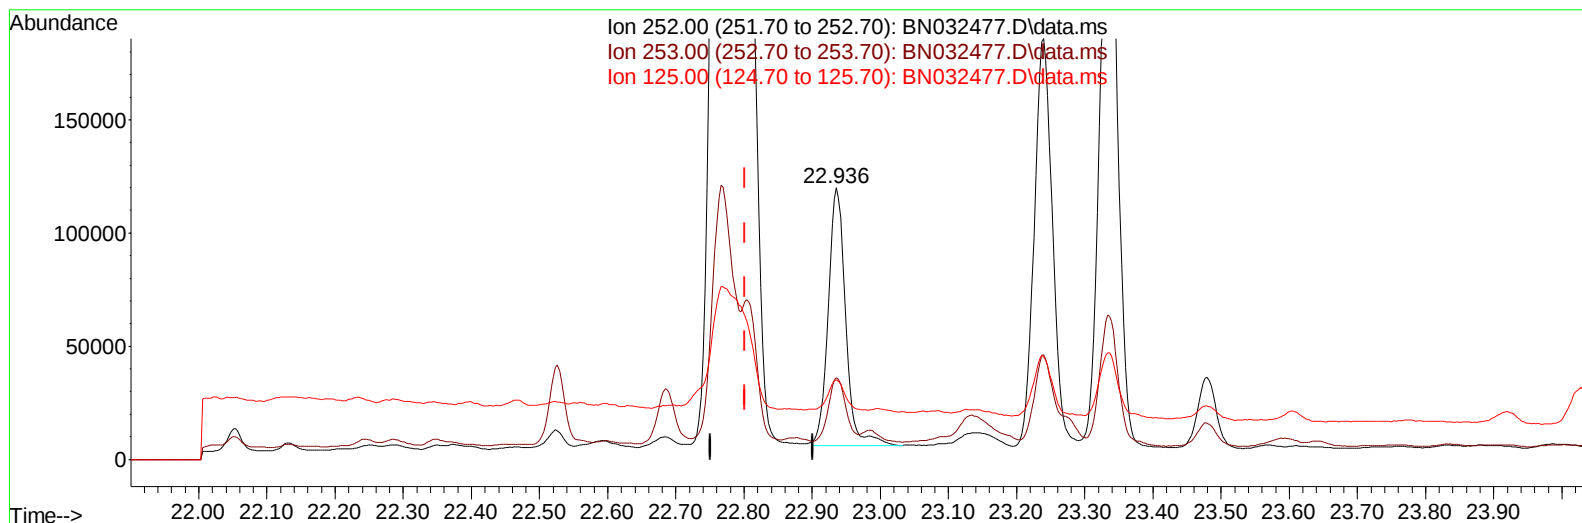

TIC: BN032477.D\data.ms

(25) Benzo(k)fluoranthene

22.936min (+ 0.134) 1.82 ng/u1

response 200697

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.40	30.19
125.00	16.00	29.33#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

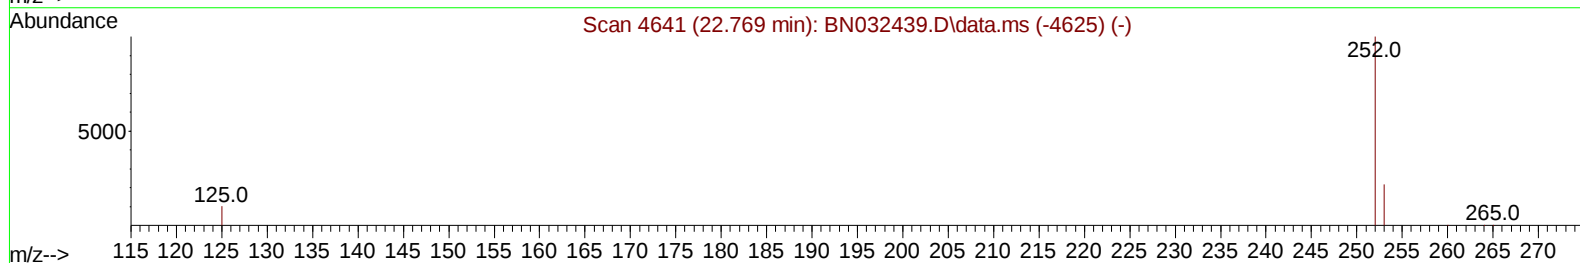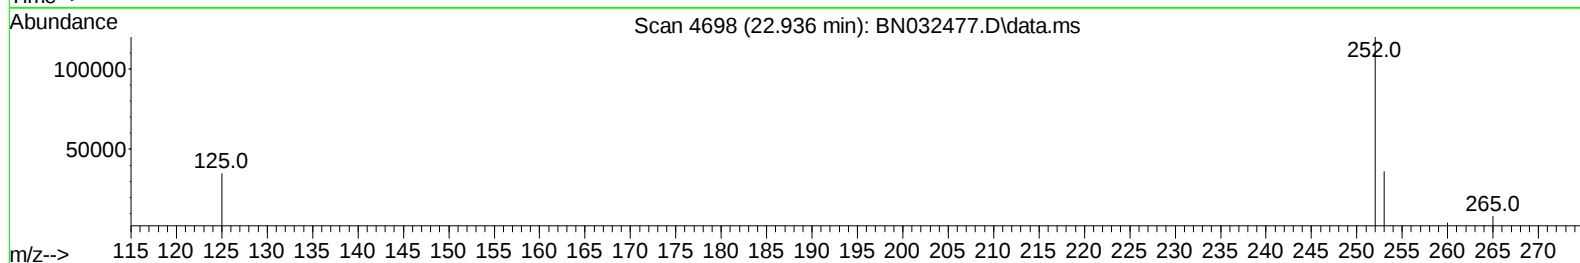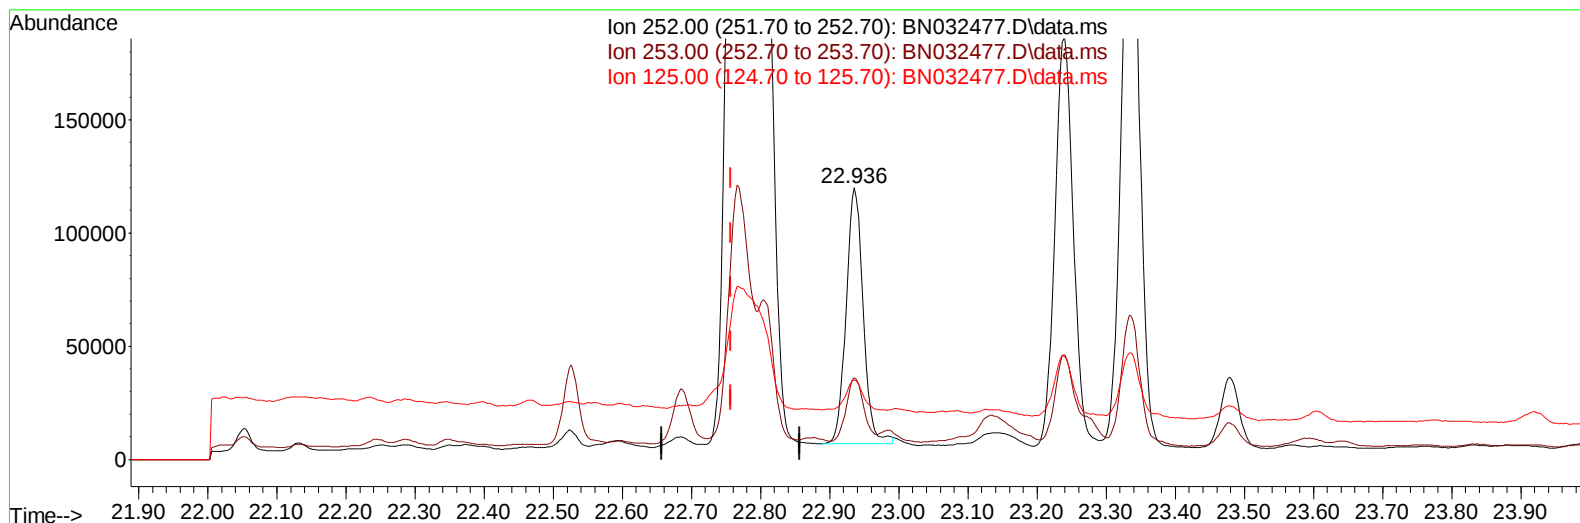

TIC: BN032477.D\data.ms

(24) Benzo(b)fluoranthene

22.936min (+ 0.178) 1.71 ng/u1

response 194206

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.10	30.19
125.00	16.00	29.33
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

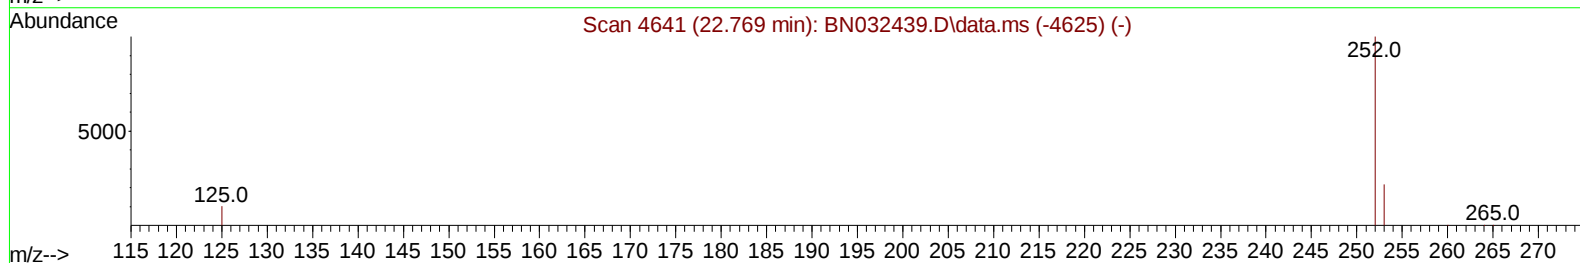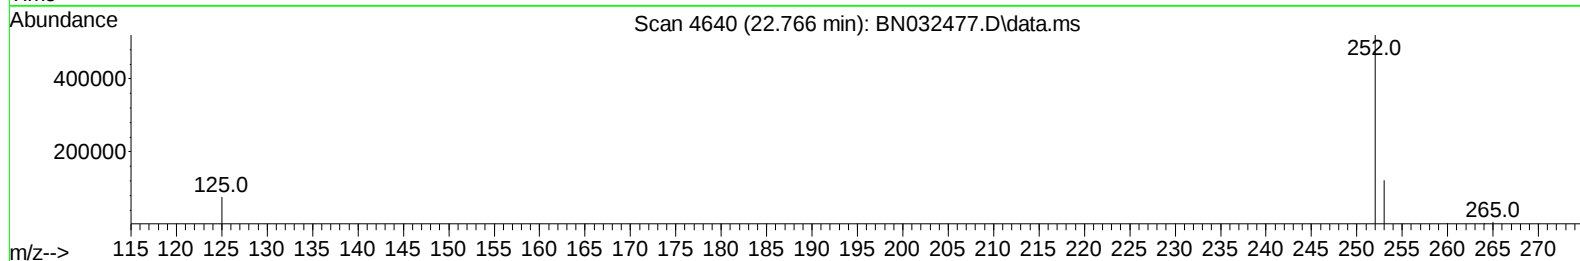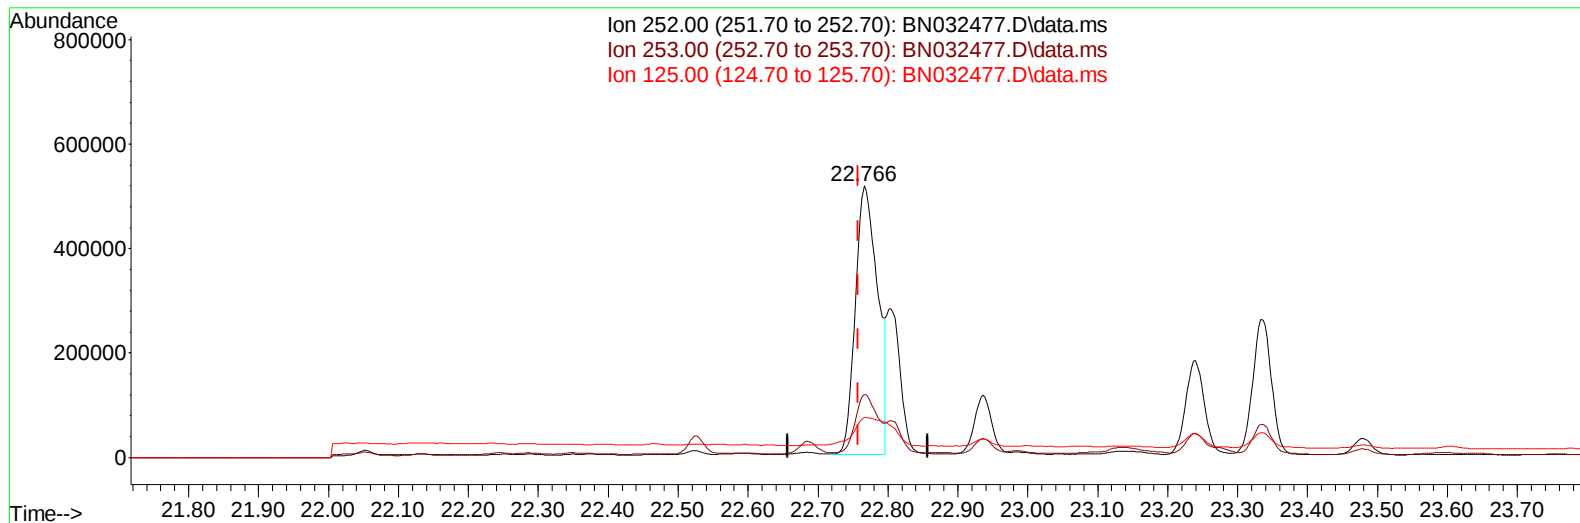

TIC: BN032477.D\data.ms

(24) Benzo(b)fluoranthene

22.766min (+ 0.009) 10.04 ng/ul m

response 1138036

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.10	23.30
125.00	16.00	14.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

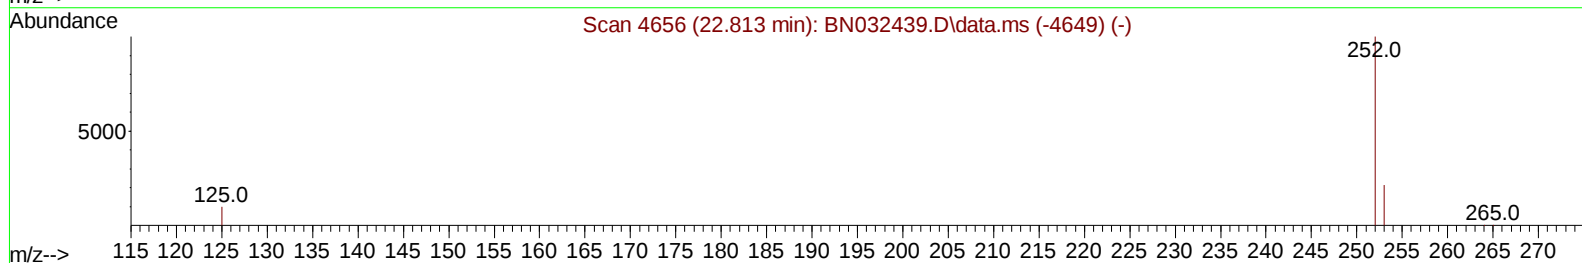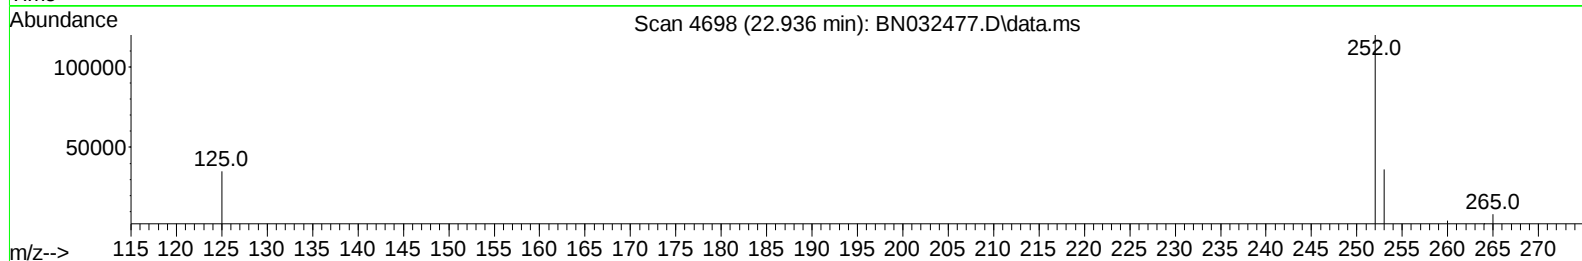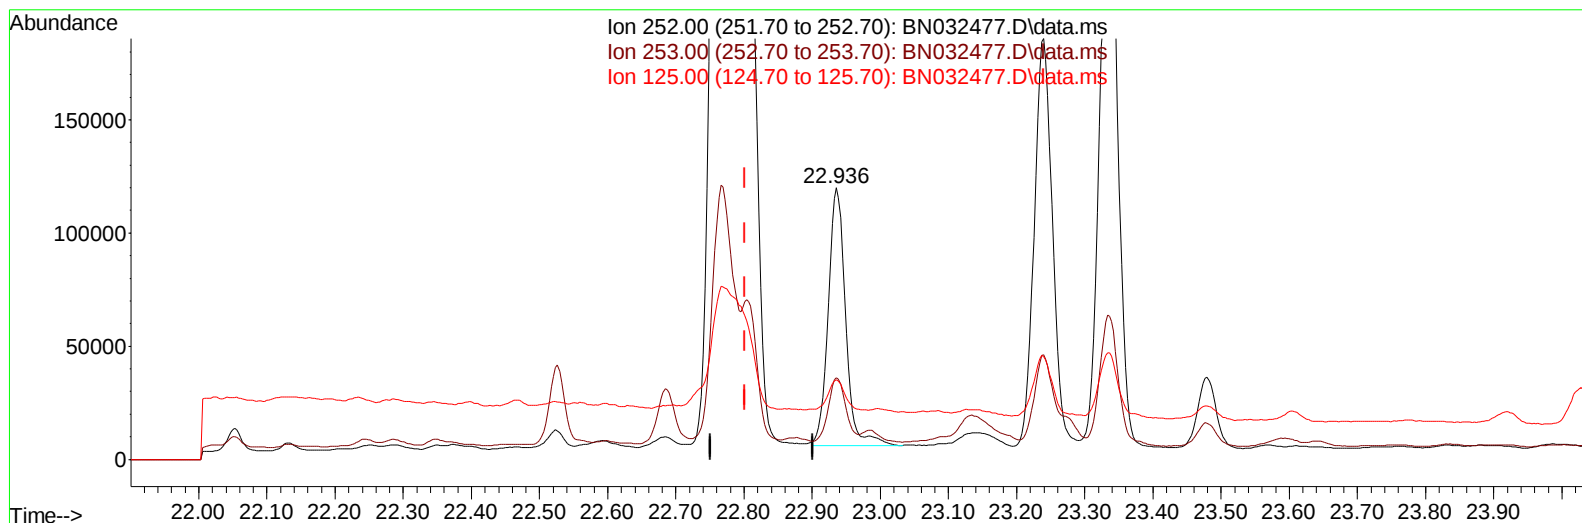

TIC: BN032477.D\data.ms

(25) Benzo(k)fluoranthene

22.936min (+ 0.134) 1.82 ng/u1

response 200697

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.40	30.19
125.00	16.00	29.33#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

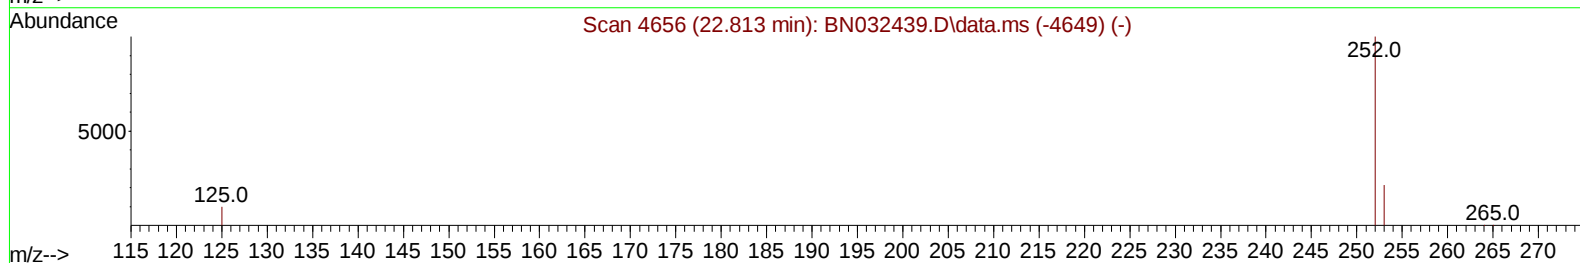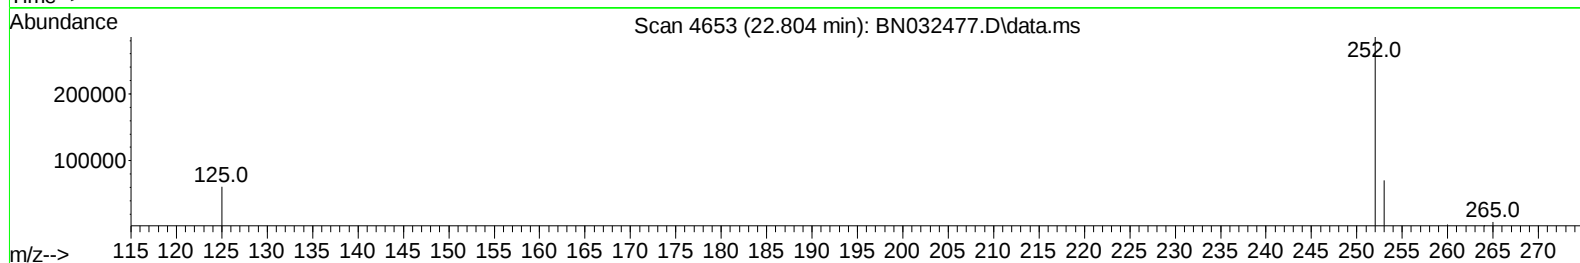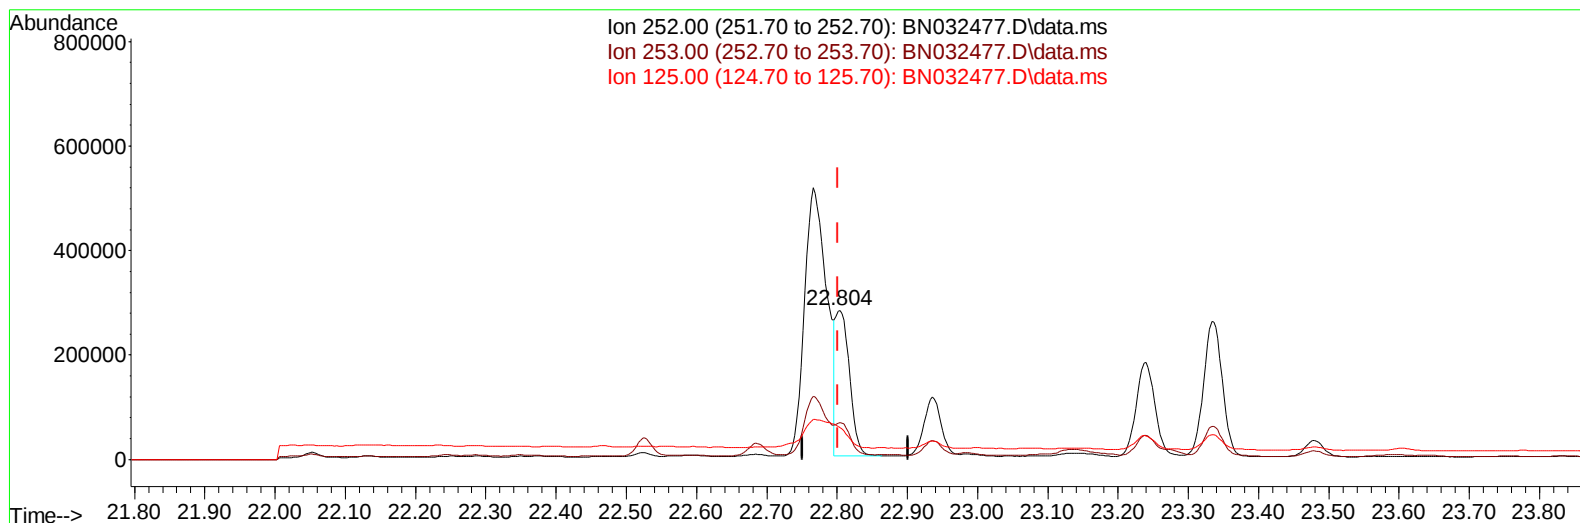

TIC: BN032477.D\data.ms

(25) Benzo(k)fluoranthene

22.804min (+ 0.003) 3.50 ng/u1 m

response 385047

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	25.40	24.69
125.00	16.00	21.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

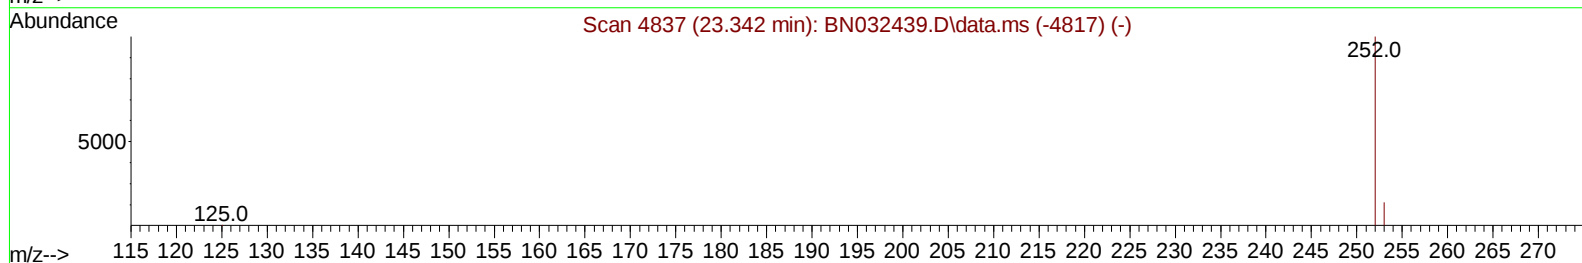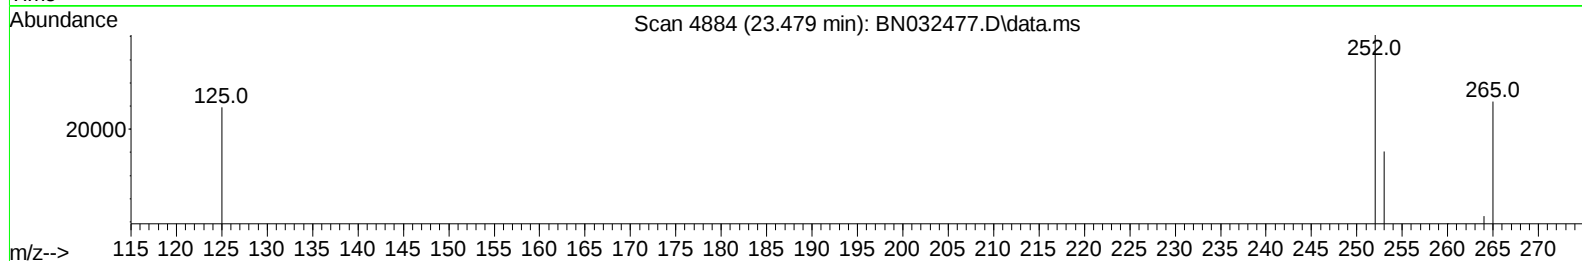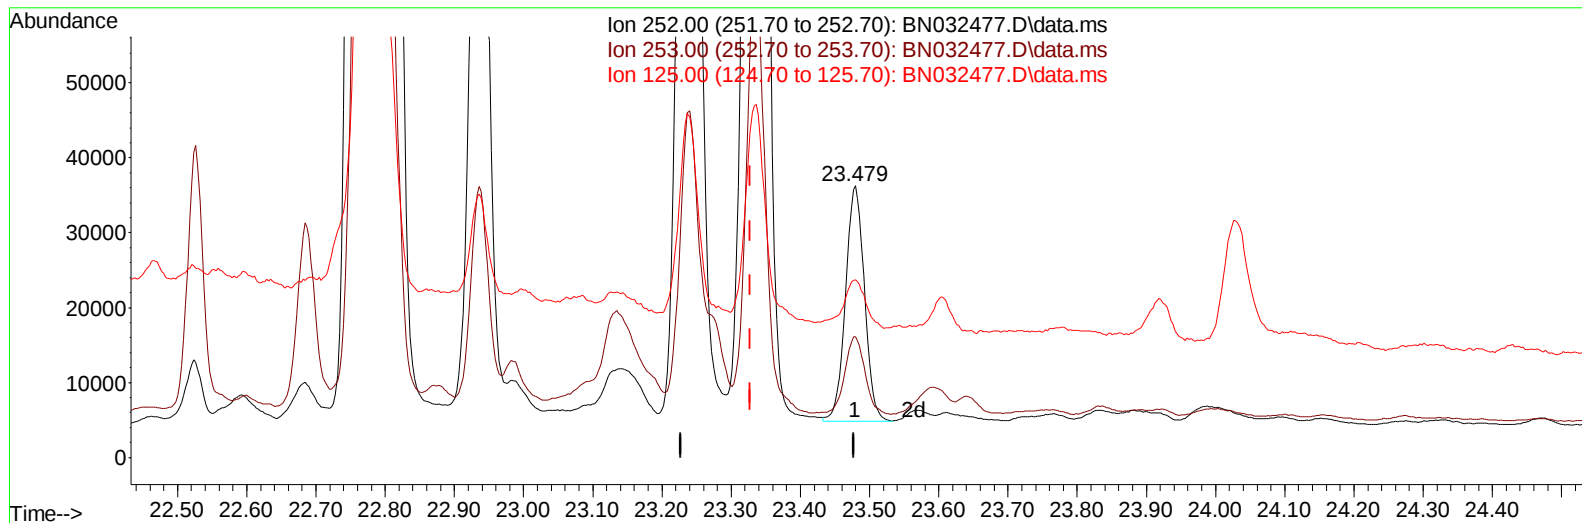

TIC: BN032477.D\data.ms

(26) Benzo(a)pyrene (C)

23.479min (+ 0.152) 0.76 ng/u1

response 59722

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.70	44.51#
125.00	20.50	65.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

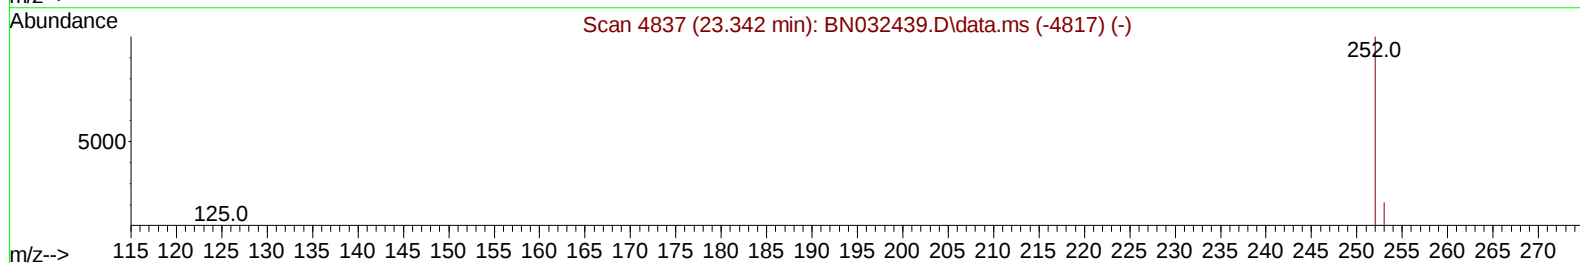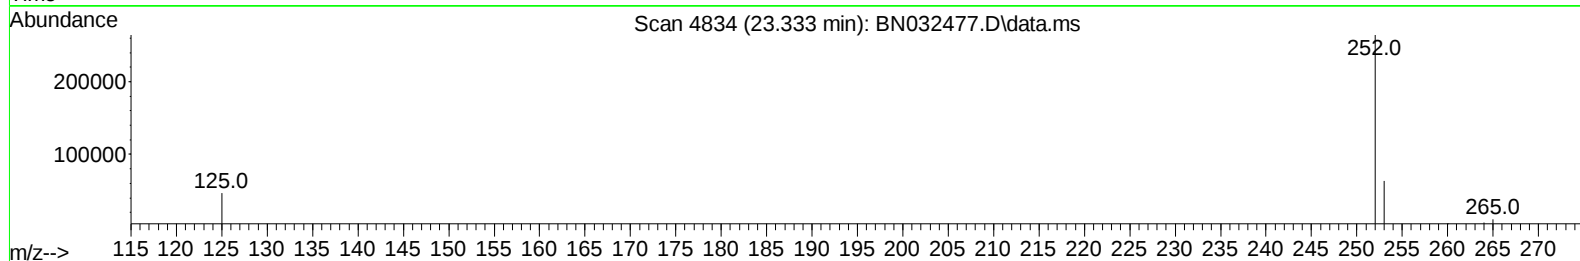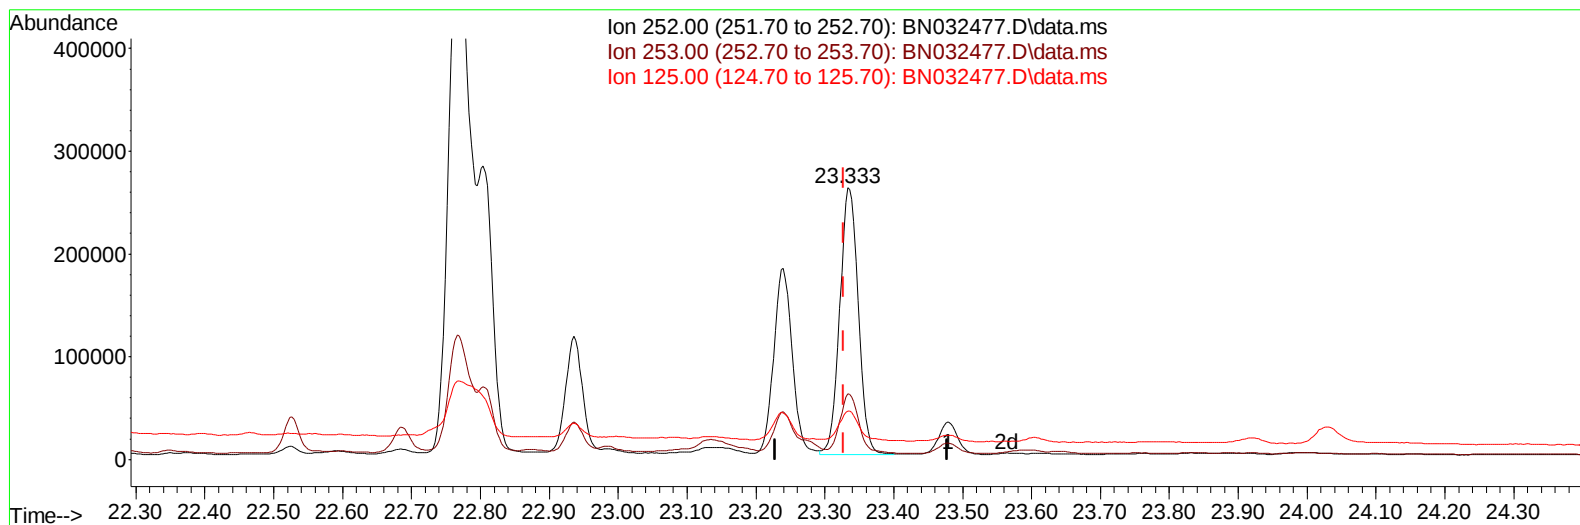

TIC: BN032477.D\data.ms

(26) Benzo(a)pyrene (C)

23.333min (+ 0.006) 6.15 ng/ul m

response 484924

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.70	24.11
125.00	20.50	17.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

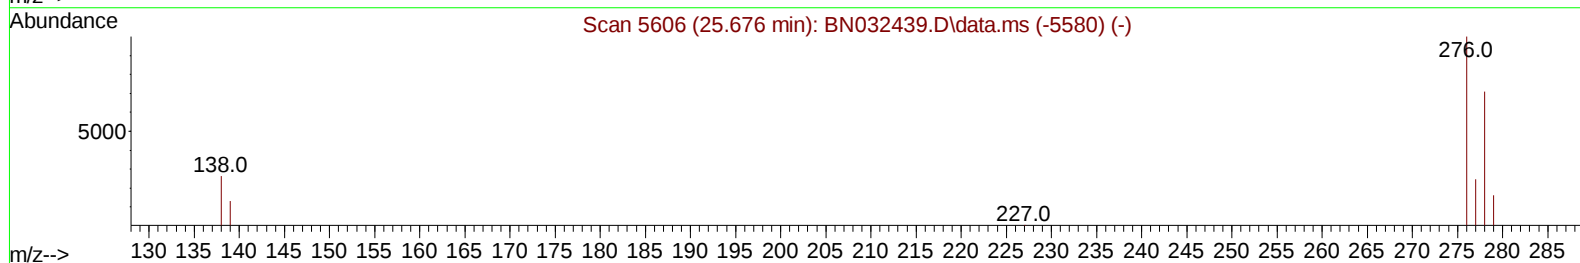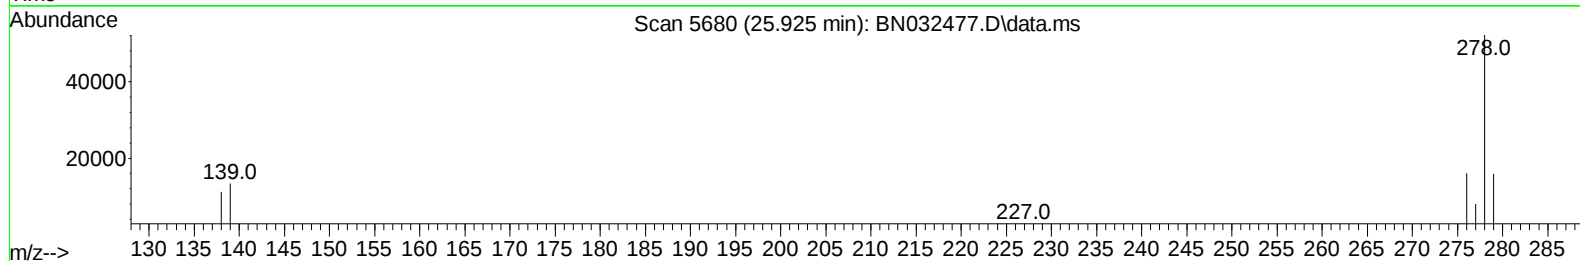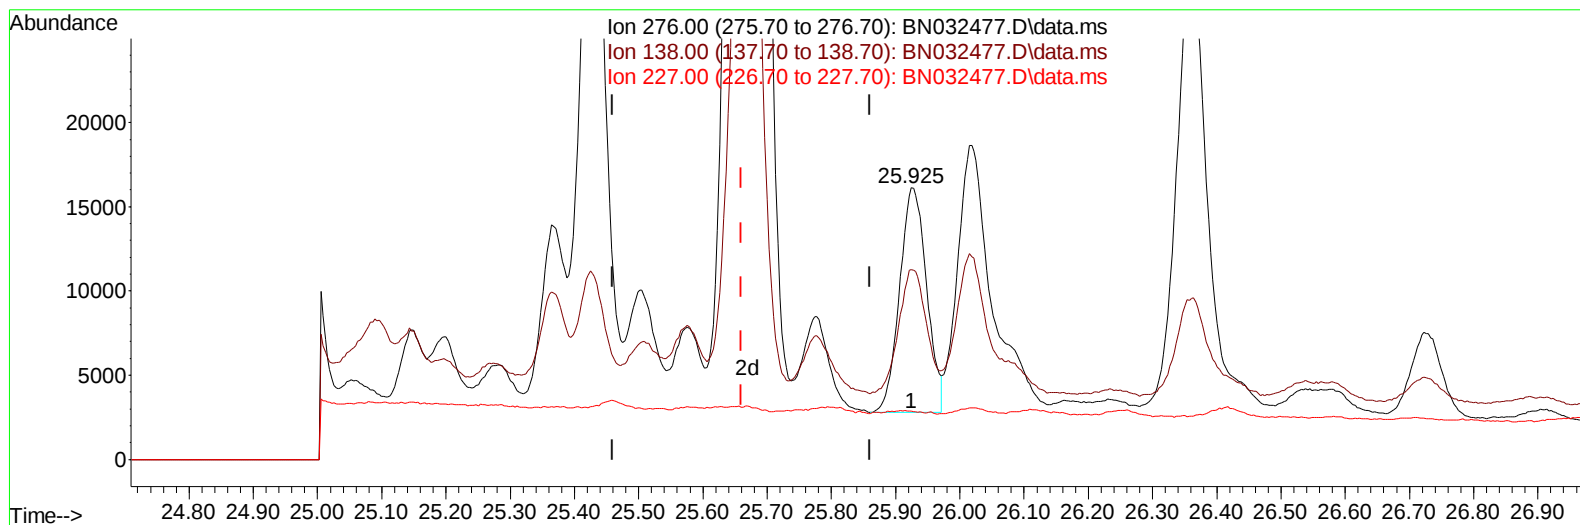

TIC: BN032477.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.925min (+ 0.265) 0.32 ng/u1

response 39103

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	26.60	57.06#
227.00	0.10	1.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

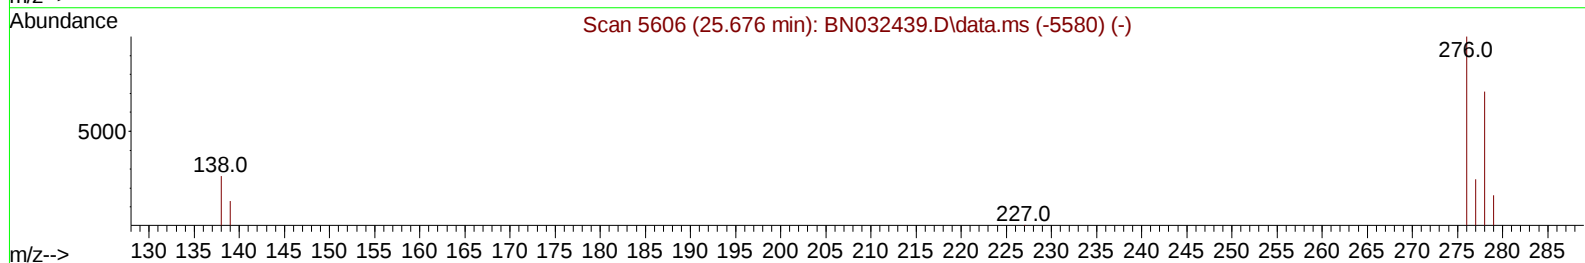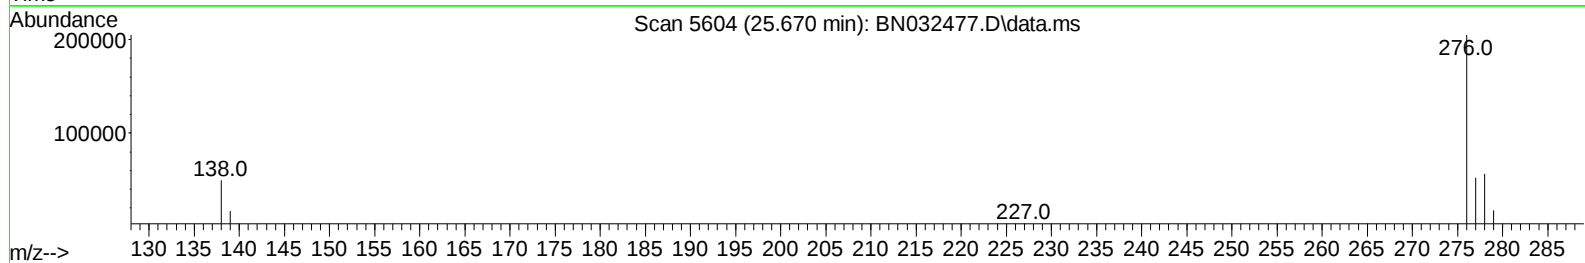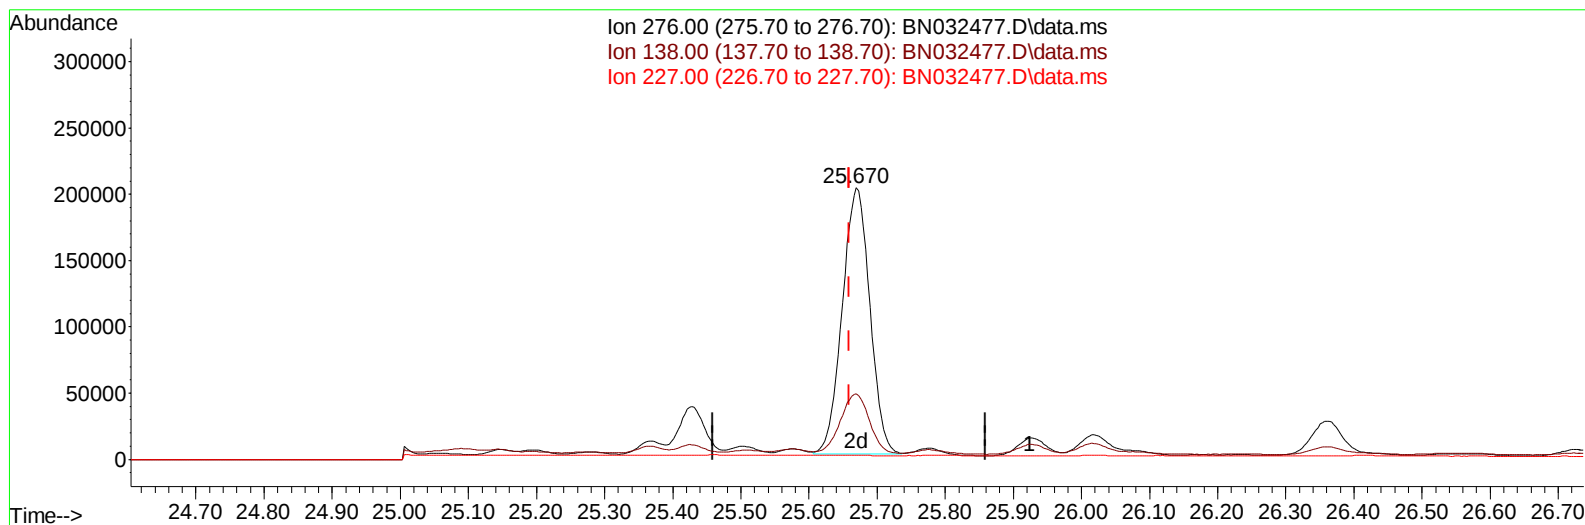

TIC: BN032477.D\data.ms

(27) Indeno(1,2,3-cd)pyrene

25.670min (+ 0.010) 4.56 ng/ul m

response 562709

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	26.60	3.97#
227.00	0.10	0.09
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

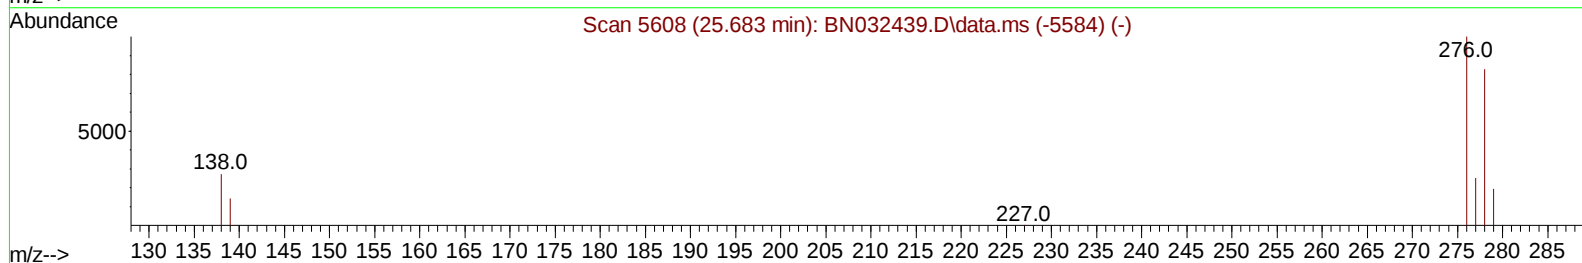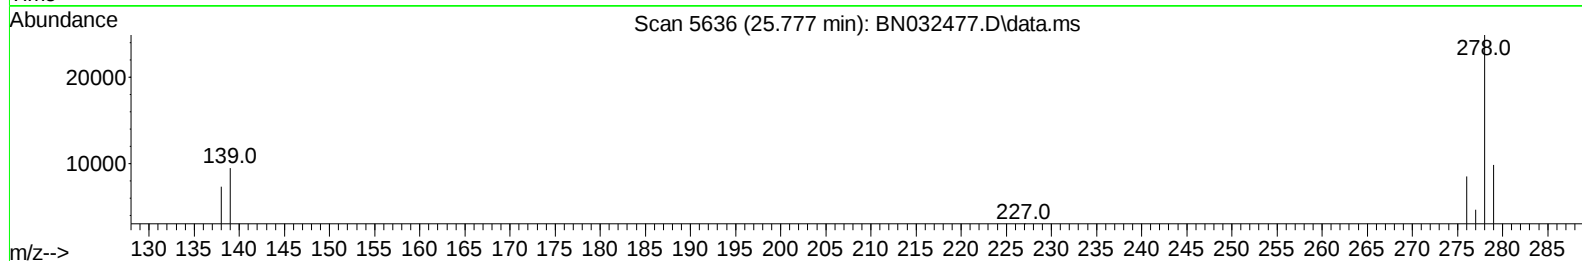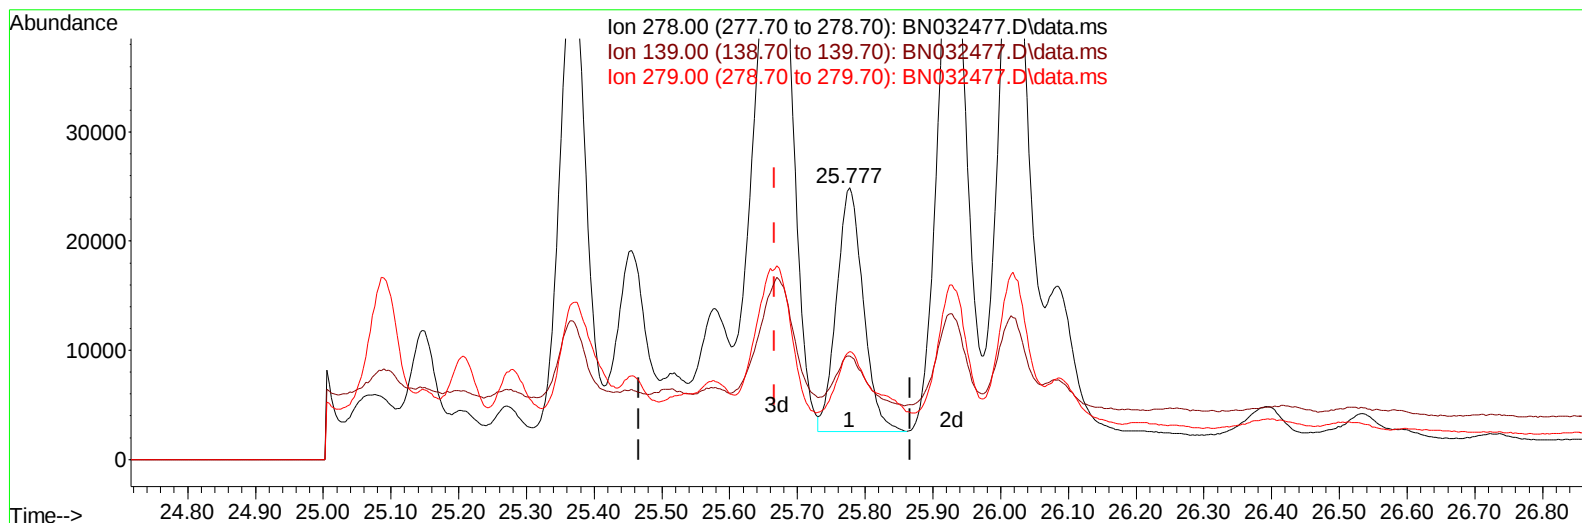

TIC: BN032477.D\data.ms

(28) Dibenzo(a,h)anthracene

25.777min (+ 0.111) 0.67 ng/u1

response 61223

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	19.90	38.14#
279.00	26.40	39.70#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

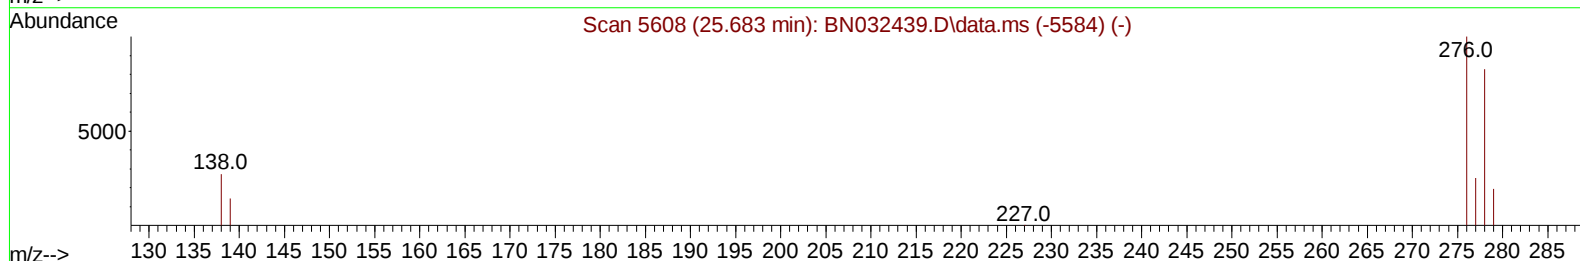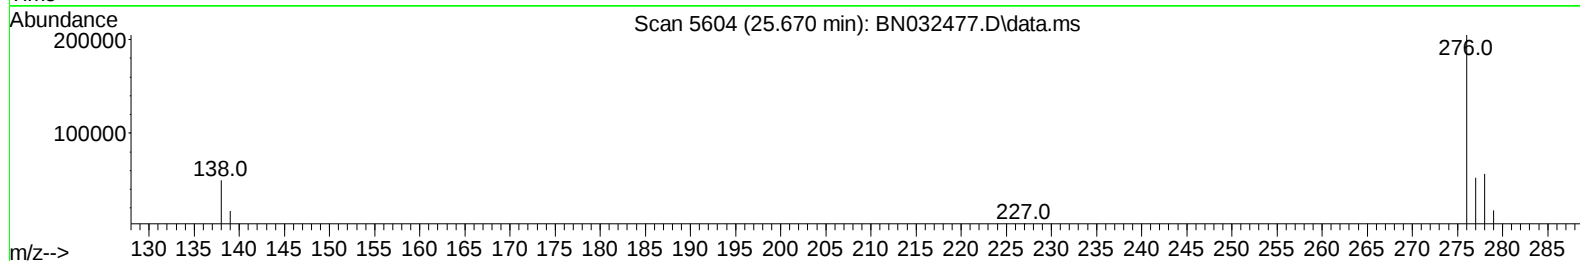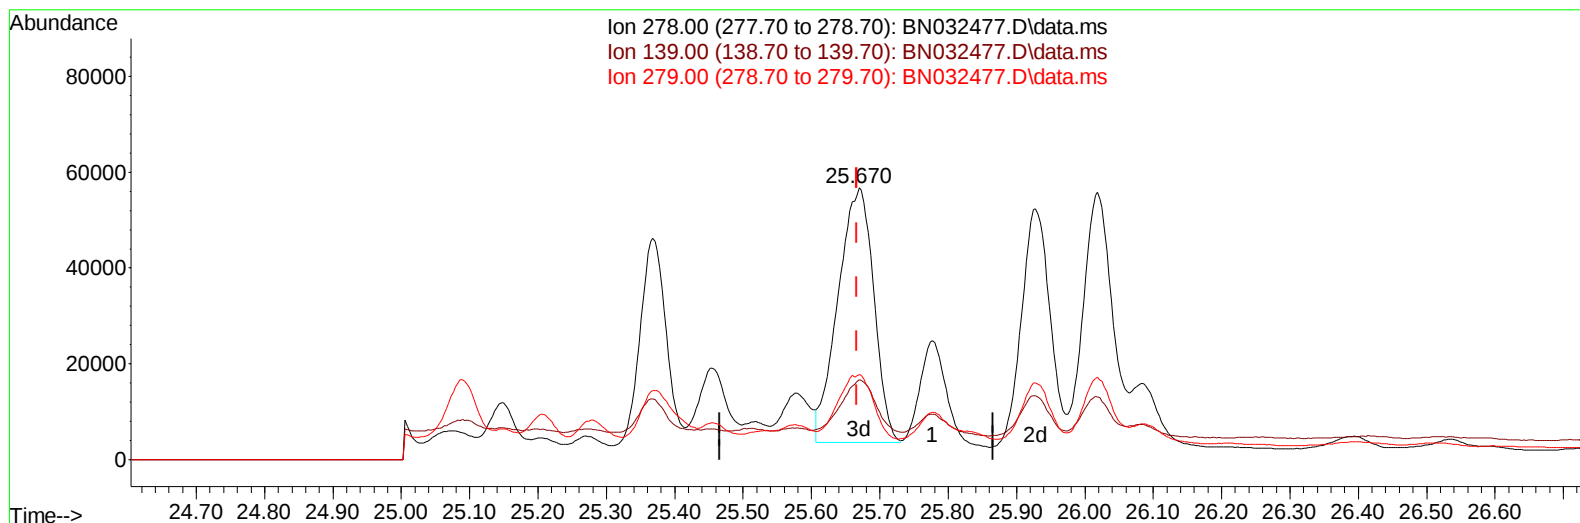

TIC: BN032477.D\data.ms

(28) Dibenzo(a,h)anthracene

25.670min (+ 0.003) 2.11 ng/ul m

response 193816

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	19.90	29.38#
279.00	26.40	31.25
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

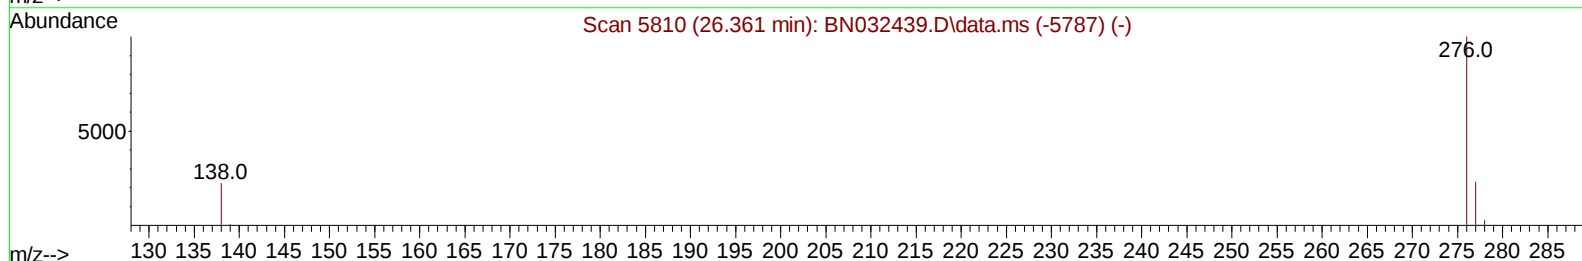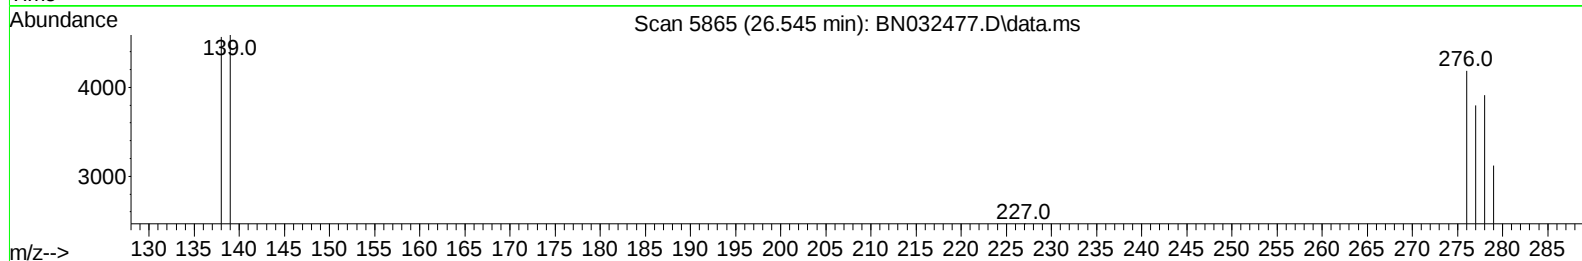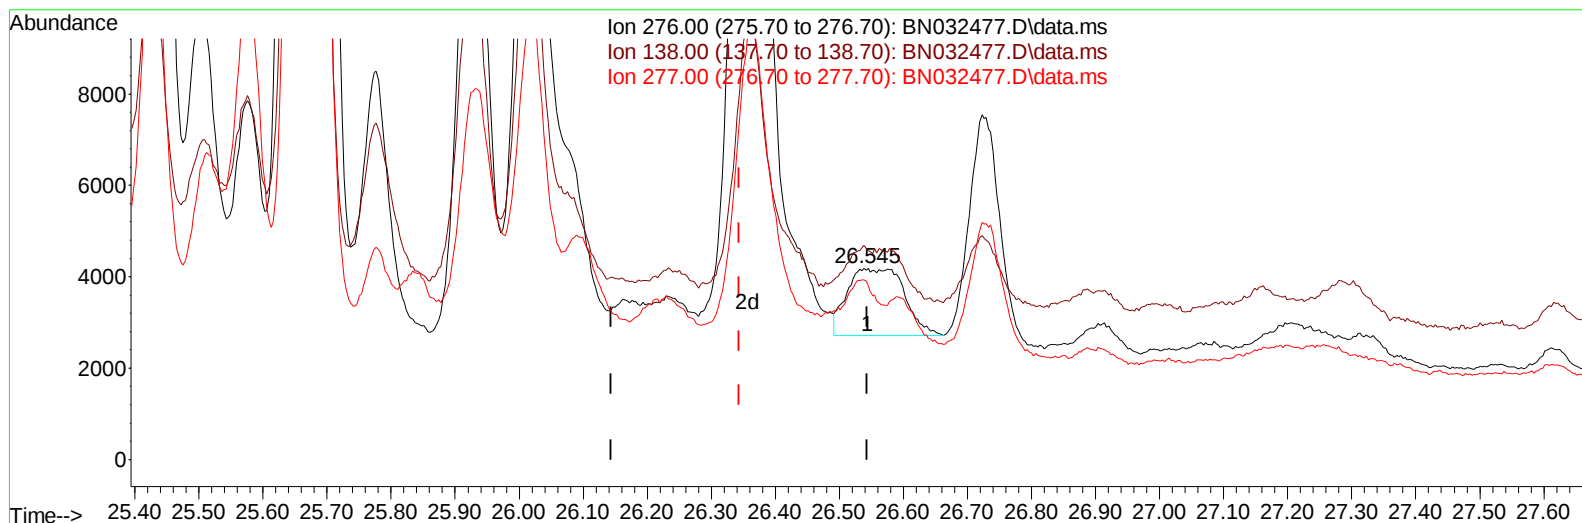

TIC: BN032477.D\data.ms

(29) Benzo(g,h,i)perylene

26.545min (+ 0.201) 0.09 ng/u1

response 9094

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	24.70	109.10#
277.00	24.70	90.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
 Data File : BN032477.D
 Acq On : 04 Jul 2024 16:57
 Operator : MA/JU
 Sample : P2964-11
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 03 03:26:42 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
 Supervised By :mohammad ahmed 07/05/2024

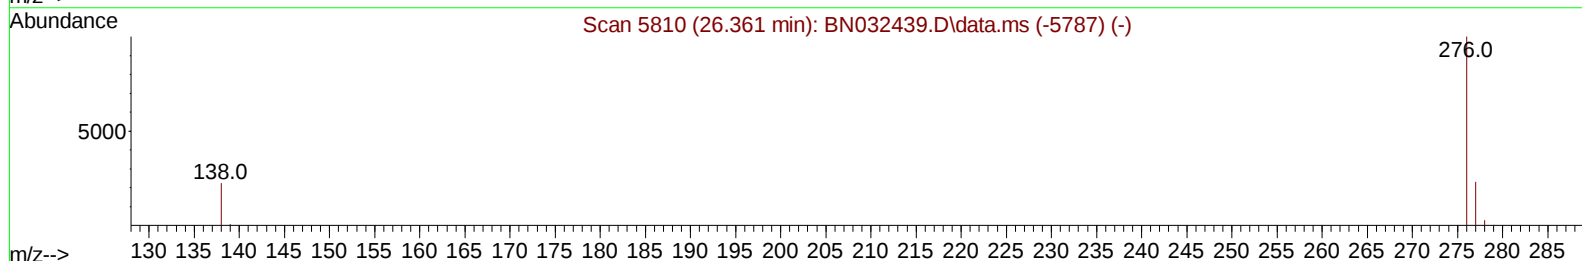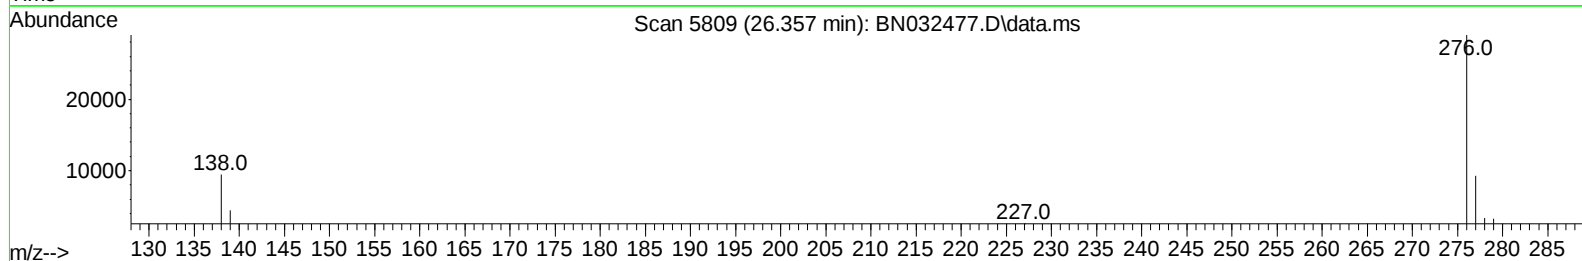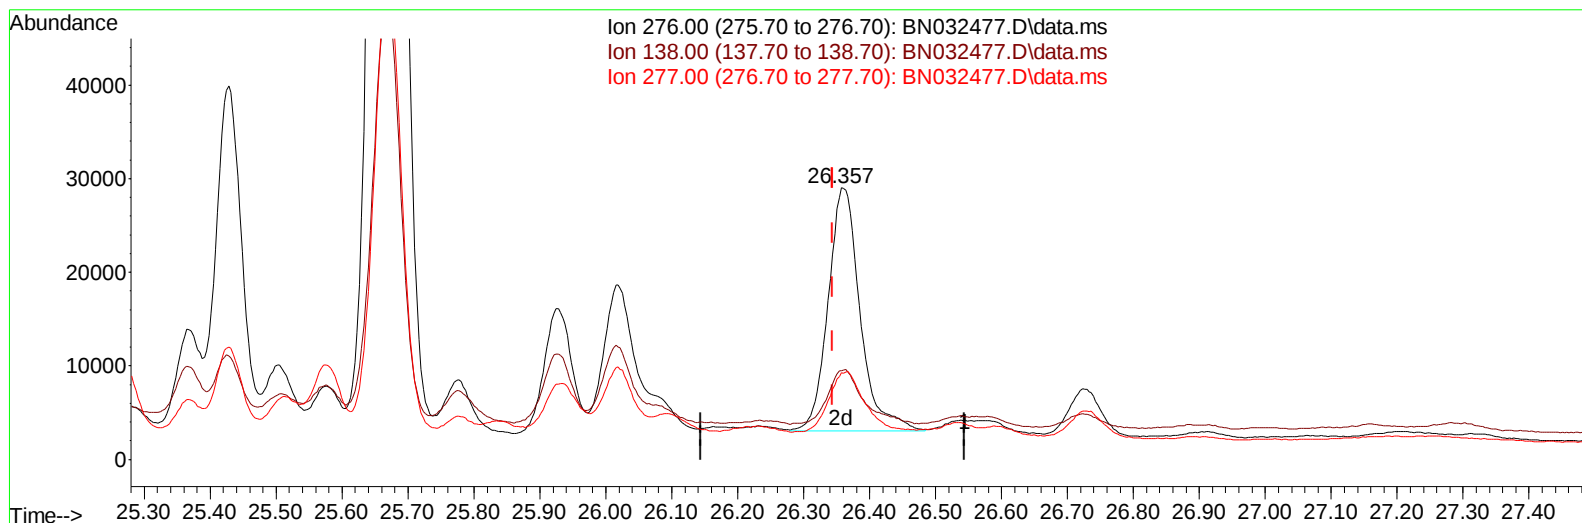

TIC: BN032477.D\data.ms

(29) Benzo(g,h,i)perylene

26.357min (+ 0.013) 0.89 ng/ul m

response 87804

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	24.70	32.56#
277.00	24.70	32.06#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
 Data File : BN032477.D
 Acq On : 04 Jul 2024 16:57
 Operator : MA/JU
 Sample : P2964-11
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4CS5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
 Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 04 23:07:05 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 03 03:26:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.595	152	8932	0.400	ng/ul	0.00
4) Naphthalene-d8	10.371	136	27324	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.244	164	16001	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.999	188	28833m	0.400	ng/ul	0.00
17) Chrysene-d12	21.211	240	18711m	0.400	ng/ul	0.00
23) Perylene-d12	23.430	264	26086m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	26461	2.665	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.966	152	7485	0.183	ng/ul	-0.01
18) Fluoranthene-d10	19.036	212	12609m	0.224	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.420	128	105760	1.463	ng/ul	99
7) 2-Methylnaphthalene	12.043	142	39812	0.831	ng/ul	98
8) 1-Methylnaphthalene	12.263	142	23579	0.474	ng/ul	99
10) Acenaphthylene	13.962	152	141716	2.129	ng/ul	99
11) Acenaphthene	14.304	153	31542	0.611	ng/ul	98
12) Fluorene	15.299	166	45779	0.744	ng/ul#	99
14) Pentachlorophenol	16.666	266	654m	0.100	ng/ul	
15) Phenanthrene	17.041	178	844516m	10.683	ng/ul	
16) Anthracene	17.134	178	217638m	3.087	ng/ul	
19) Fluoranthene	19.069	202	1405923m	19.732	ng/ul	
20) Pyrene	19.436	202	1147006m	15.405	ng/ul	
21) Benzo(a)anthracene	21.194	228	720081m	10.663	ng/ul	
22) Chrysene	21.246	228	827128m	11.159	ng/ul	
24) Benzo(b)fluoranthene	22.766	252	1138036m	10.041	ng/ul	
25) Benzo(k)fluoranthene	22.804	252	385047m	3.497	ng/ul	
26) Benzo(a)pyrene	23.333	252	484924m	6.150	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.670	276	562709m	4.558	ng/ul	
28) Dibenzo(a,h)anthracene	25.670	278	193816m	2.113	ng/ul	
29) Benzo(g,h,i)perylene	26.357	276	87804m	0.893	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032477.D
Acq On : 04 Jul 2024 16:57
Operator : MA/JU
Sample : P2964-11
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4CS5

Manual IntegrationsAPPROVED

Quant Time: Jul 04 23:07:05 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

