




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032490.D
Acq On : 05 Jul 2024 01:22
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 05 03:42:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

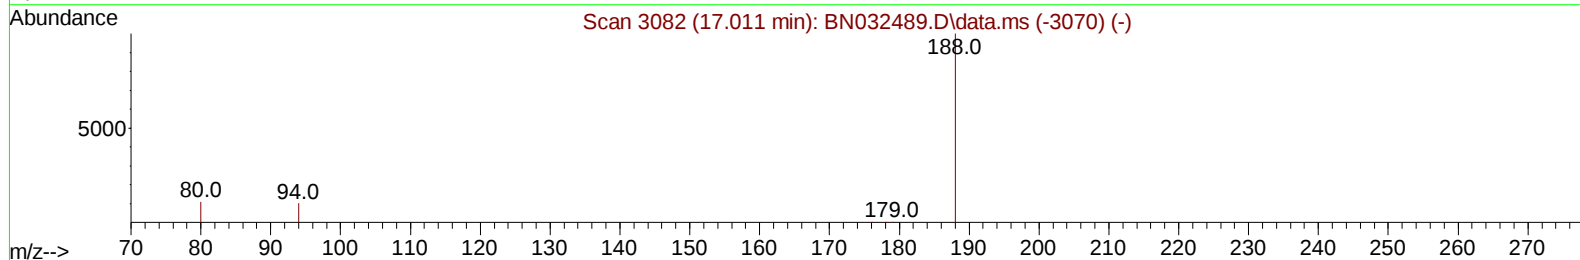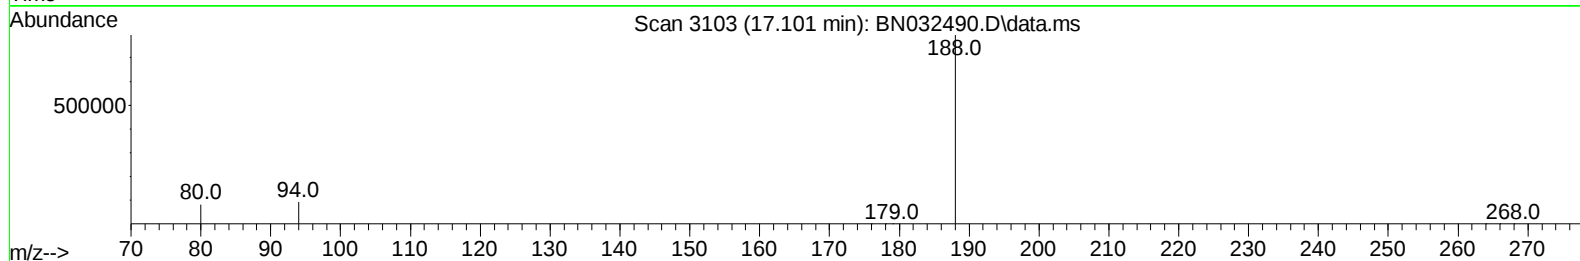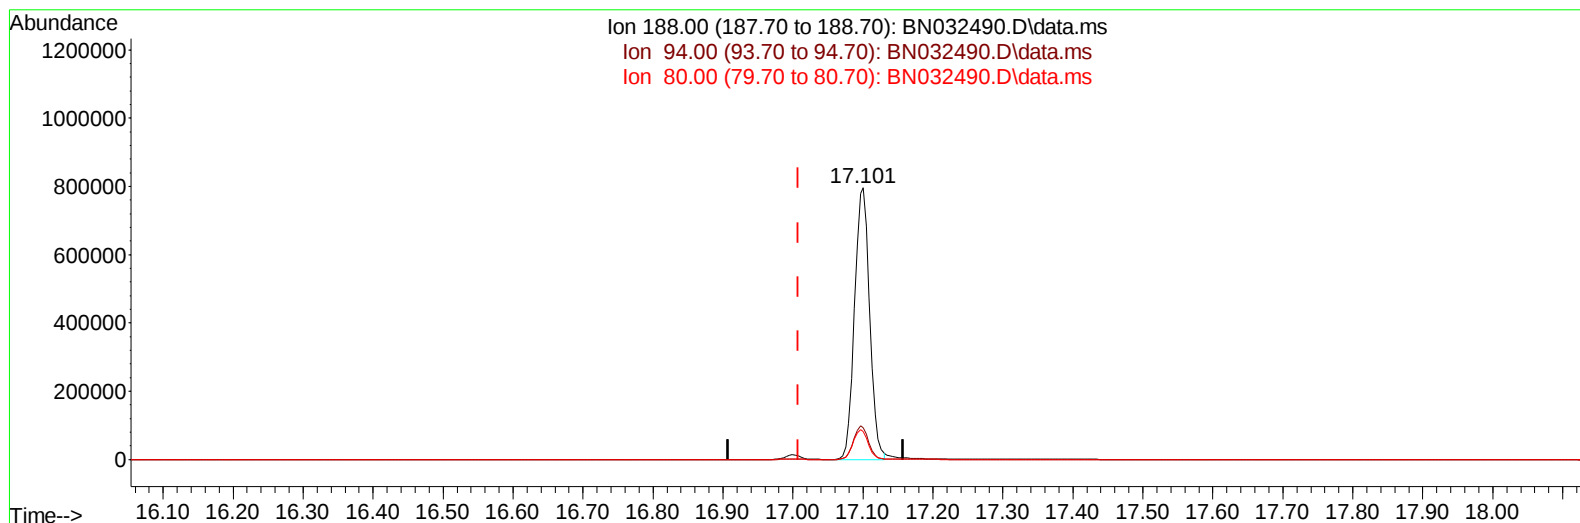

TIC: BN032490.D\data.ms

(13) Phenanthrene-d10 (I)**17.101min (+ 0.093) 0.40 ng/u1****response 1191587**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	11.62
80.00	10.50	10.22
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032490.D
Acq On : 05 Jul 2024 01:22
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Quant Time: Jul 05 03:42:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

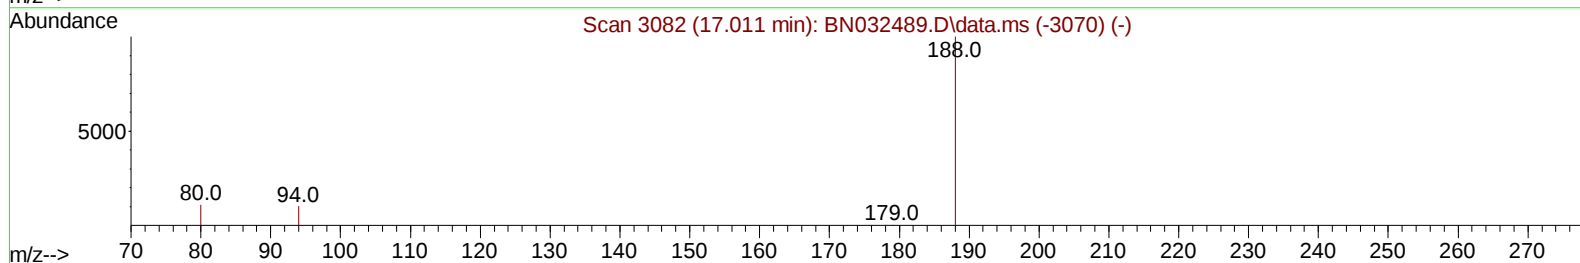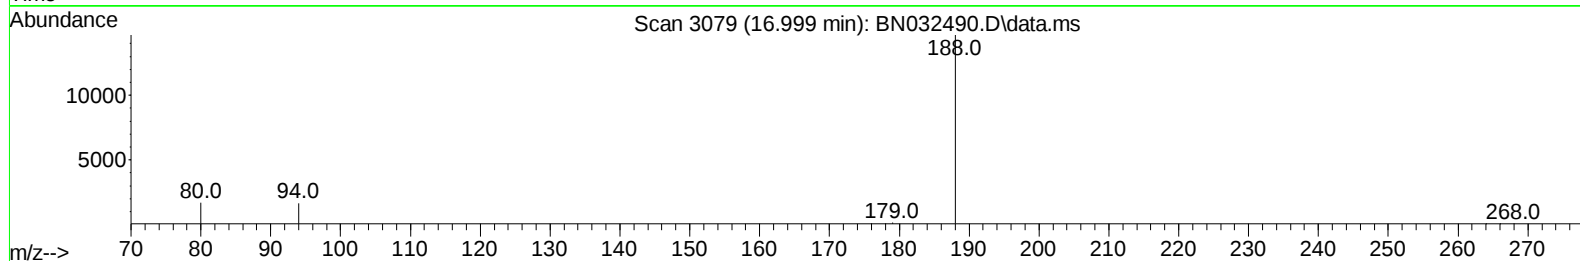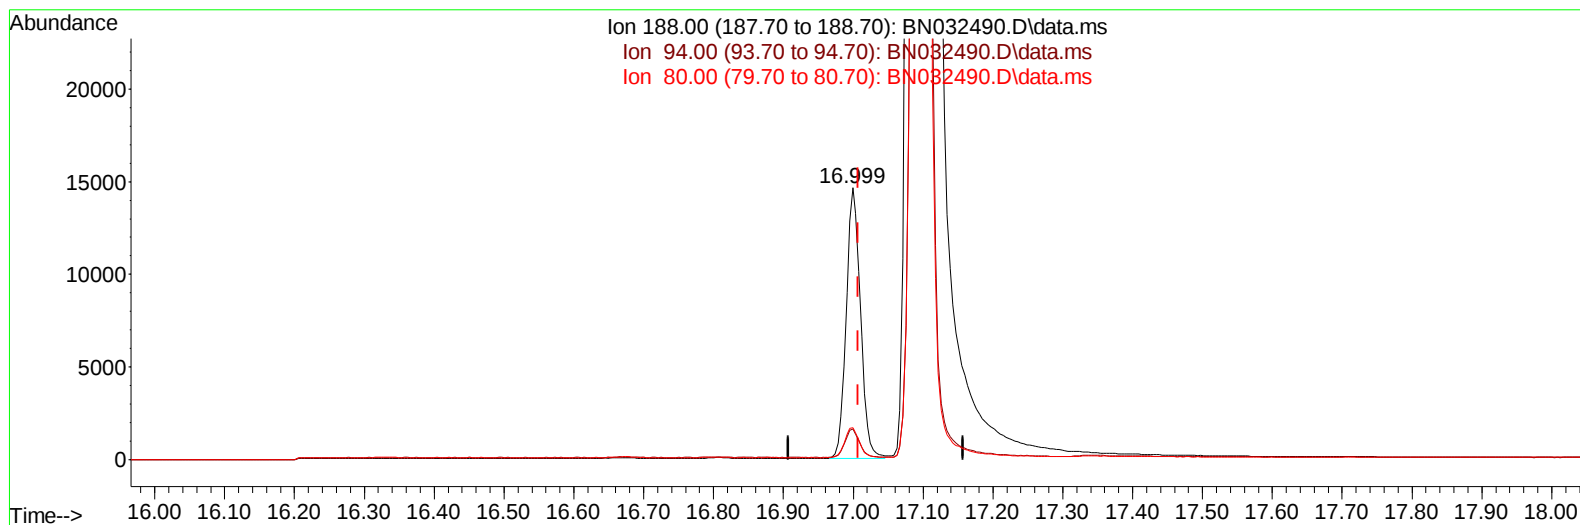

TIC: BN032490.D\data.ms

(13) Phenanthrene-d10 (I)

16.999min (-0.008) 0.40 ng/ul m

response 20782

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.20	11.25
80.00	10.50	11.64
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032490.D
Acq On : 05 Jul 2024 01:22
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Quant Time: Jul 05 03:42:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

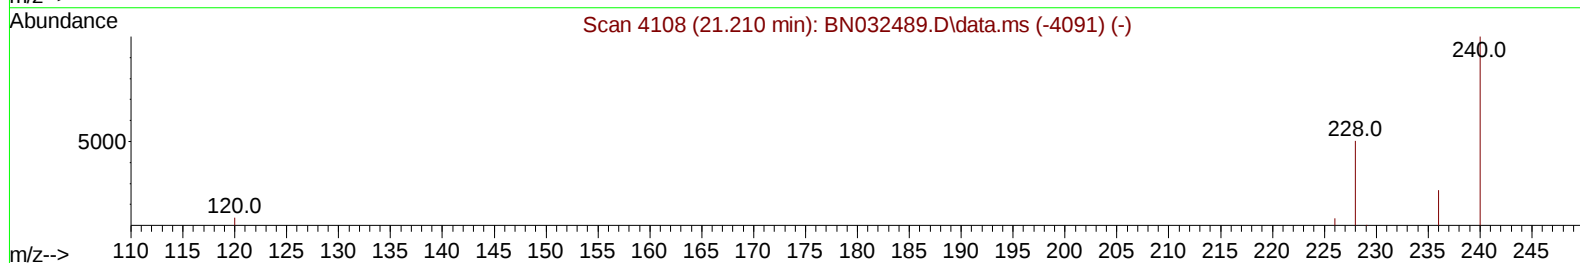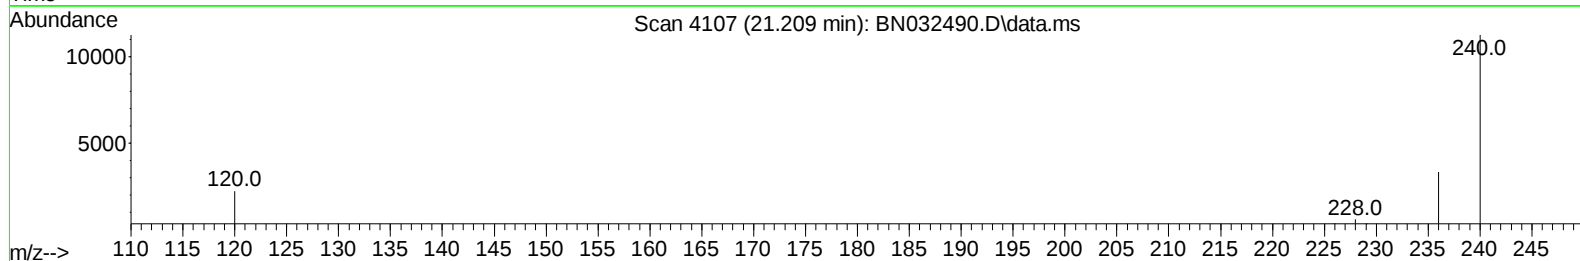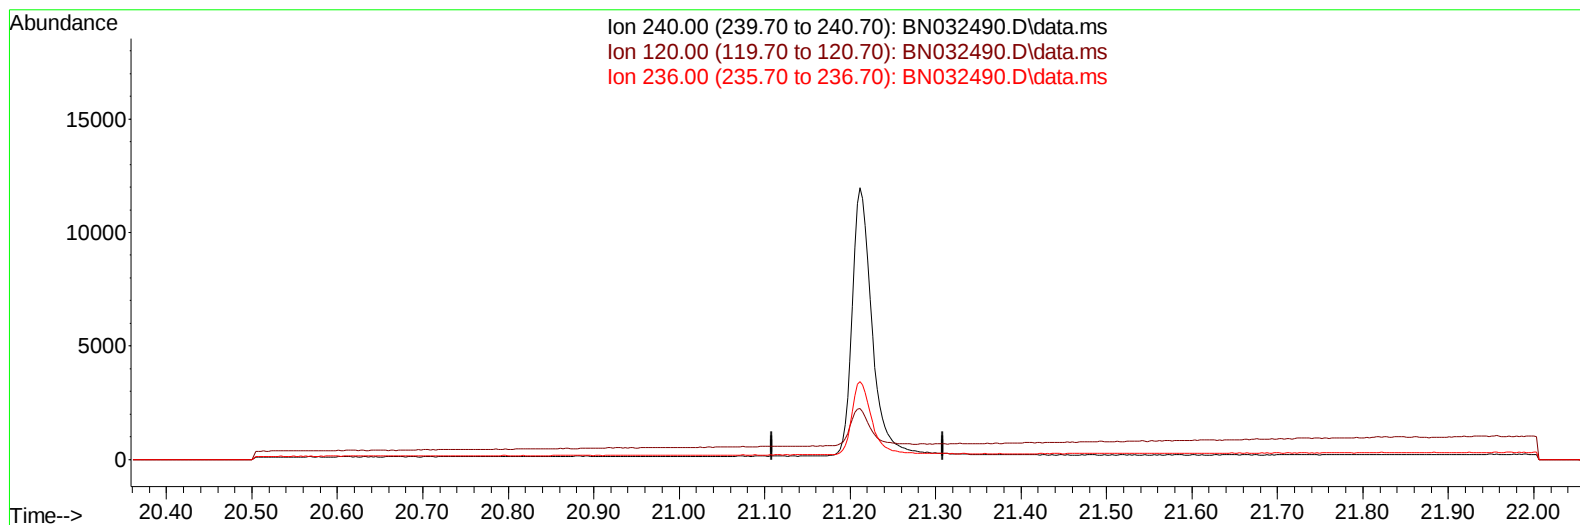

TIC: BN032490.D\data.ms

(17) Chrysene-d12

21.209min (-21.209) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.80	0.00#
236.00	28.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032490.D
Acq On : 05 Jul 2024 01:22
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Quant Time: Jul 05 03:42:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

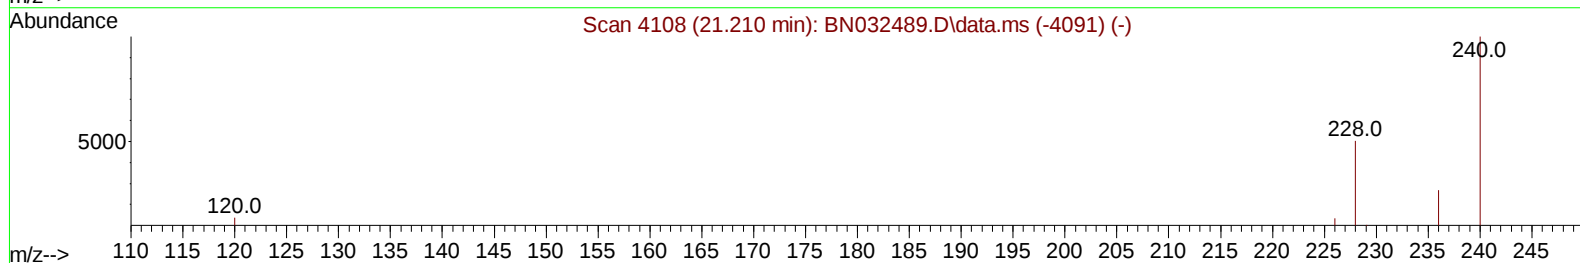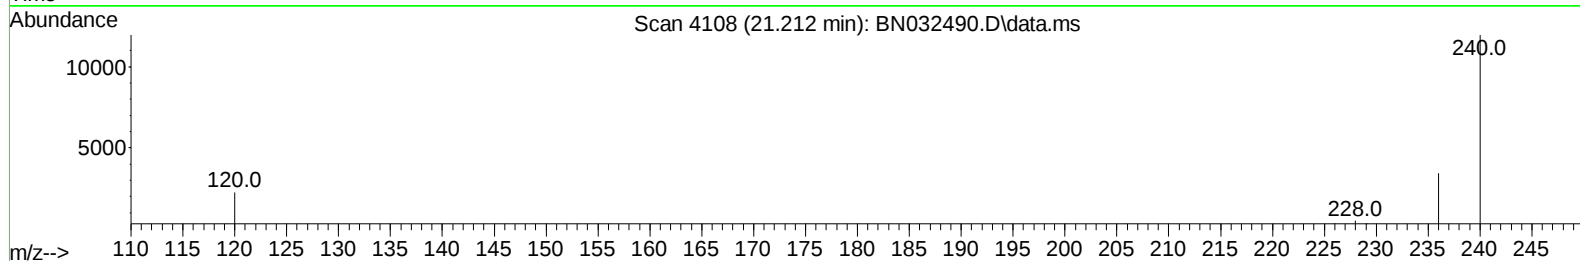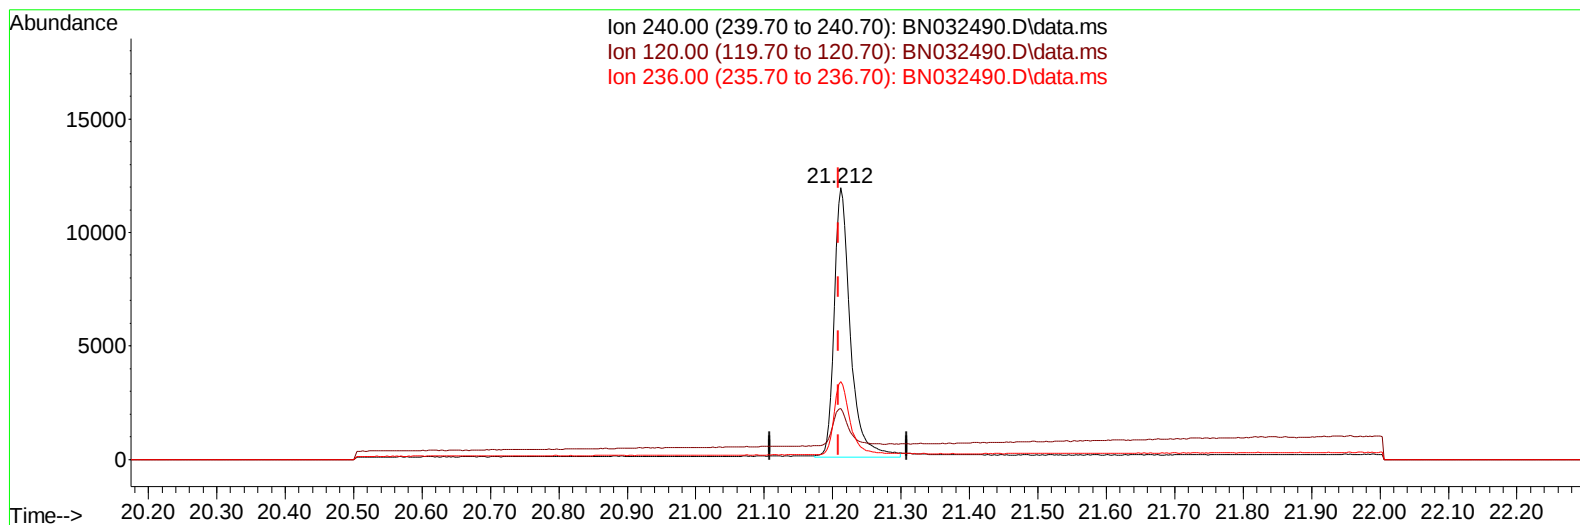

TIC: BN032490.D\data.ms

(17) Chrysene-d12

21.212min (+ 0.003) 0.40 ng/ul m

response 19455

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.80	18.79
236.00	28.40	28.67
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032490.D
Acq On : 05 Jul 2024 01:22
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Quant Time: Jul 05 03:42:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

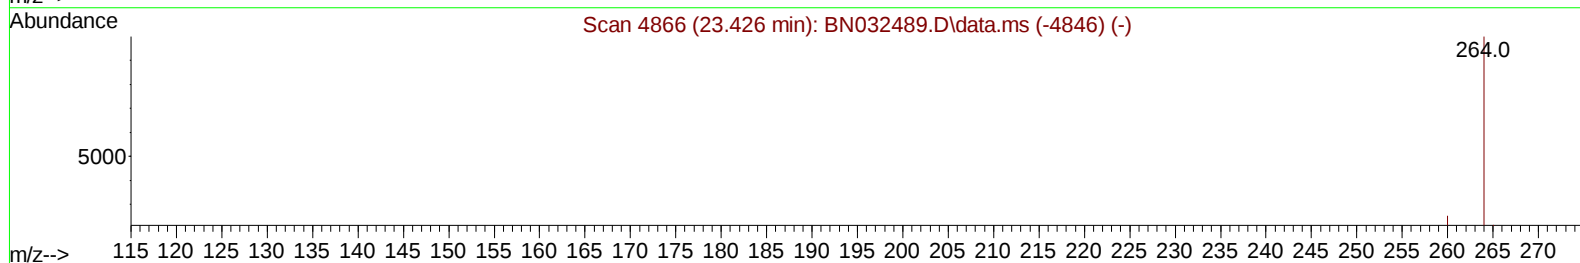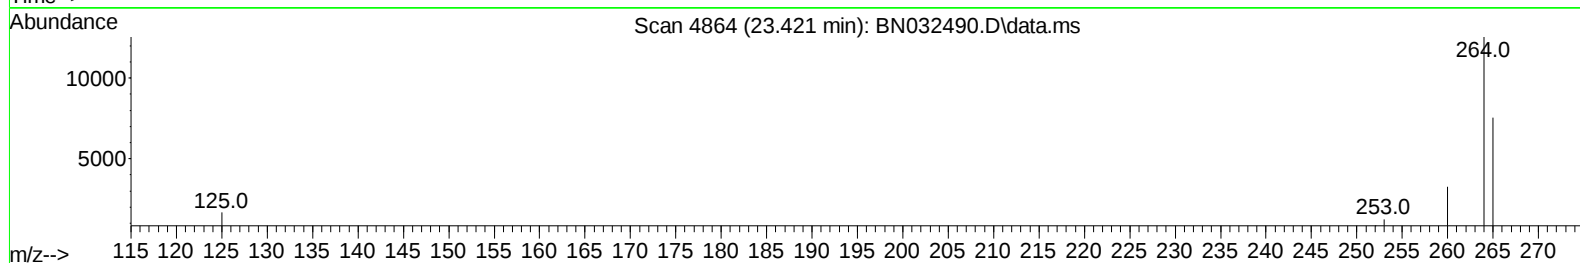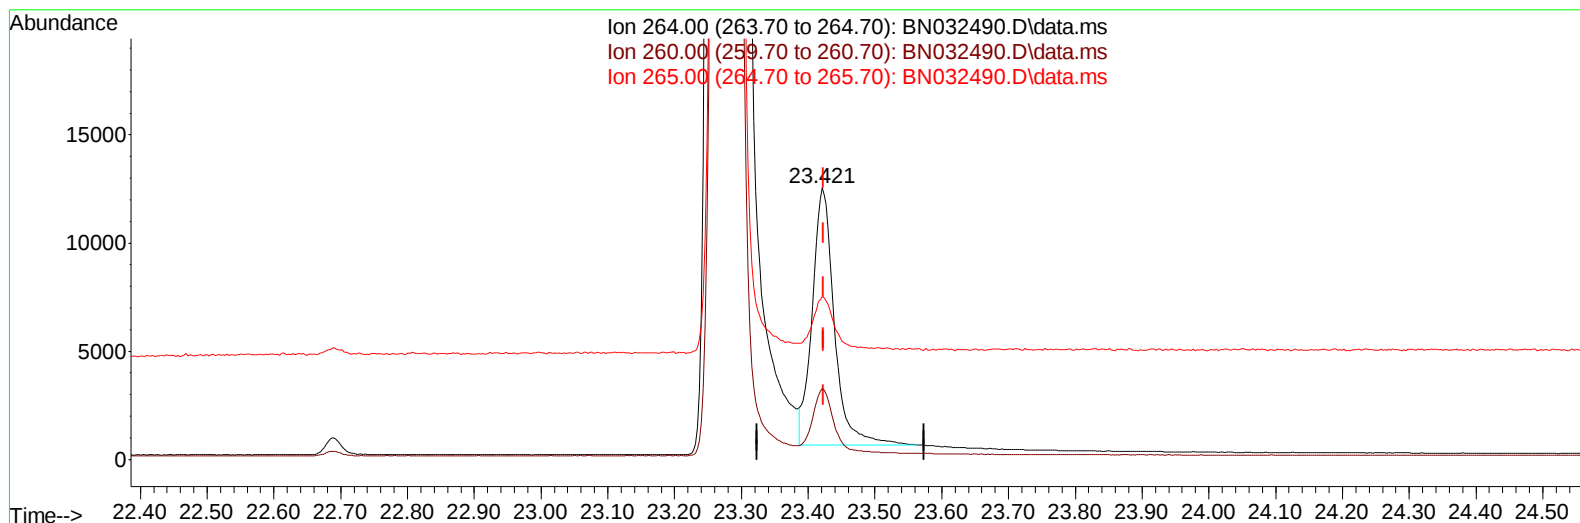

TIC: BN032490.D\data.ms

(23) Perylene-d12 (I)

23.421min (-0.003) 0.40 ng/u1

response 27687

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	25.96
265.00	67.20	60.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032490.D
Acq On : 05 Jul 2024 01:22
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Quant Time: Jul 05 03:42:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

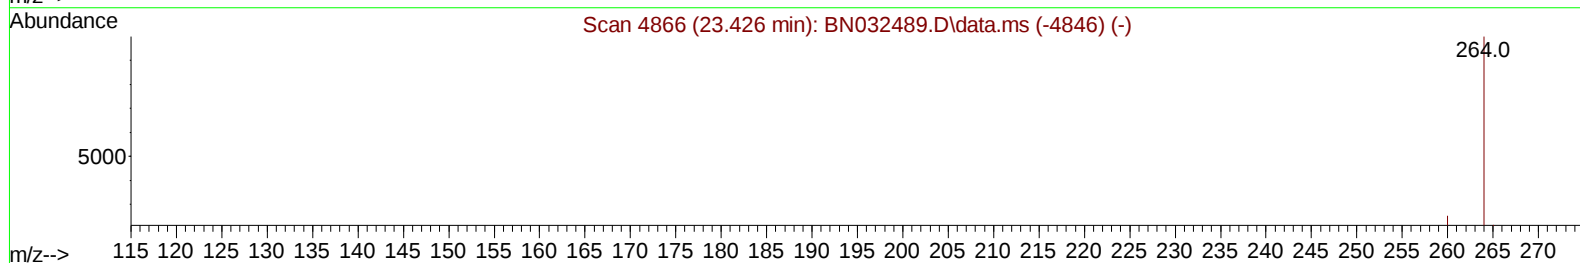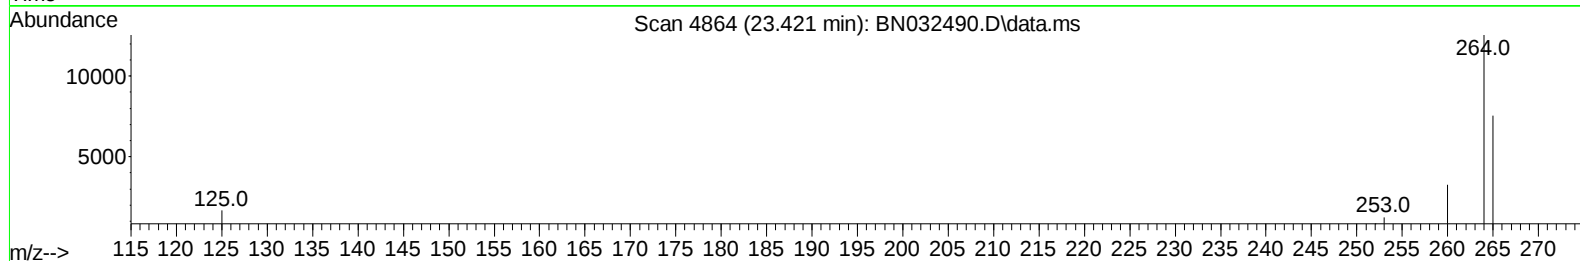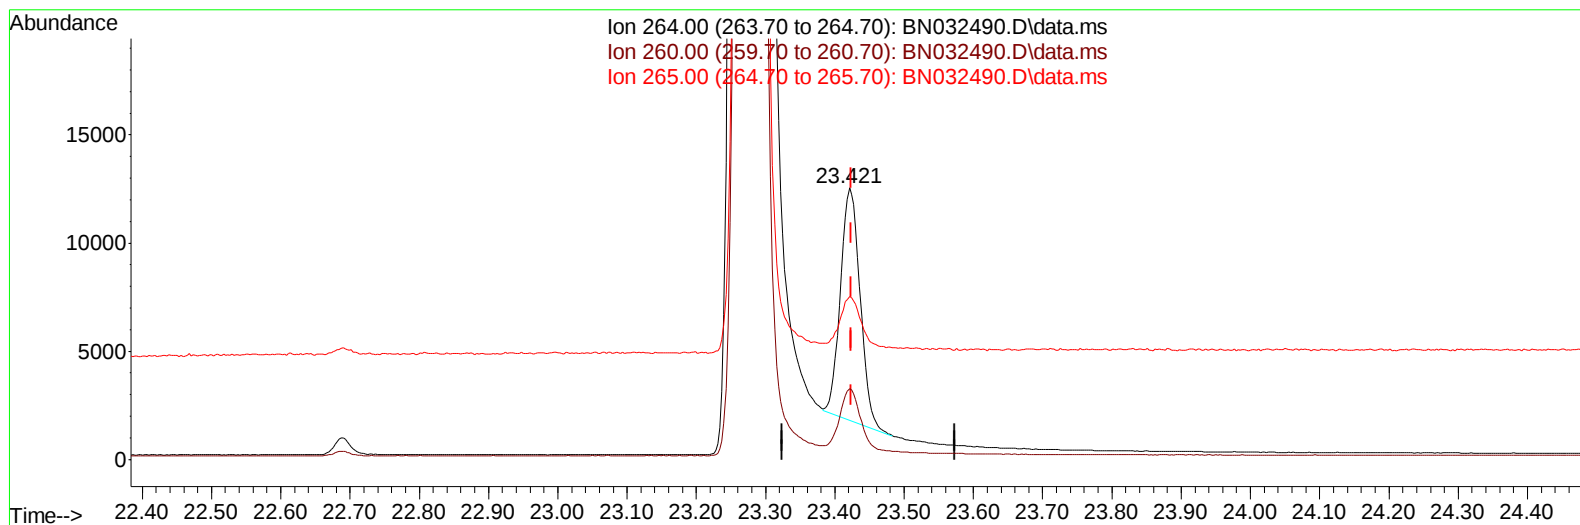

TIC: BN032490.D\data.ms

(23) Perylene-d12 (I)

23.421min (-0.003) 0.40 ng/ul m

response 21072

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.00	25.96
265.00	67.20	60.12
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
 Data File : BN032490.D
 Acq On : 05 Jul 2024 01:22
 Operator : MA/JU
 Sample : PB161629BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK629

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 07/05/2024
 Supervised By :mohammad ahmed 07/05/2024

Quant Time: Jul 05 03:42:06 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 03 03:26:42 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.595	152	6707	0.400	ng/ul	0.00
4) Naphthalene-d8	10.371	136	19348	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.244	164	10684	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.999	188	20782m	0.400	ng/ul	0.00
17) Chrysene-d12	21.212	240	19455m	0.400	ng/ul	0.00
23) Perylene-d12	23.421	264	21072m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	42355	5.681	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.977	152	7238	0.249	ng/ul	0.00
18) Fluoranthene-d10	19.041	212	15157	0.259	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070324\
Data File : BN032490.D
Acq On : 05 Jul 2024 01:22
Operator : MA/JU
Sample : PB161629BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK629

Manual IntegrationsAPPROVED

Quant Time: Jul 05 03:42:06 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 03 03:26:42 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 07/05/2024
Supervised By :mohammad ahmed 07/05/2024

