

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN070518\
 Data File : BN001970.D
 Acq On : 05 Jul 2018 16:44
 Operator : JU/SJ
 Sample : J3776-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DAZR1

Manual Integrations
 APPROVED

Sohil
 7/6/2018 5:19:34 PM

Quant Time: Jul 06 01:40:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 04 00:59:54 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	587513	20.00	ng/ul	0.00
18) Naphthalene-d8	10.48	136	2714329	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.34	164	1589213	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.08	188	3521625	20.00	ng/ul	0.00
75) Chrysene-d12	21.28	240	3059300	20.00	ng/ul	0.00
83) Perylene-d12	23.52	264	2668461	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	66434m	4.91	ng/uL	0.00
5) Phenol-d5	6.88	99	344471	6.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	1002073	30.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	1070974	25.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	703212	16.51	ng/ul	0.00
19) Nitrobenzene-d5	8.86	128	682094	33.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	762263	36.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	1408860	31.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	30600	0.66	ng/ul	0.00
43) Dimethylphthalate-d6	13.75	166	4622285	34.44	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	5243414	31.65	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	155920	6.31	ng/ul	0.00
57) Fluorene-d10	15.33	176	4004910	34.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	690747	36.01	ng/ul	0.00
70) Anthracene-d10	17.18	188	5900534	34.68	ng/ul	0.00
76) Pyrene-d10	19.48	212	6130699	39.75	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.37	264	5134130	35.38	ng/ul	0.00

Target Compounds

				Qvalue
81) Bis(2-ethylhexyl)phthalate	21.21	149	143256	1.176 ng/ul# 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN070518\
Data File : BN001970.D
Acq On : 05 Jul 2018 16:44
Operator : JU/SJ
Sample : J3776-05
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampled :
DAZR1

Quant Time: Jul 06 01:40:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 04 00:59:54 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
7/6/2018 5:19:34 PM

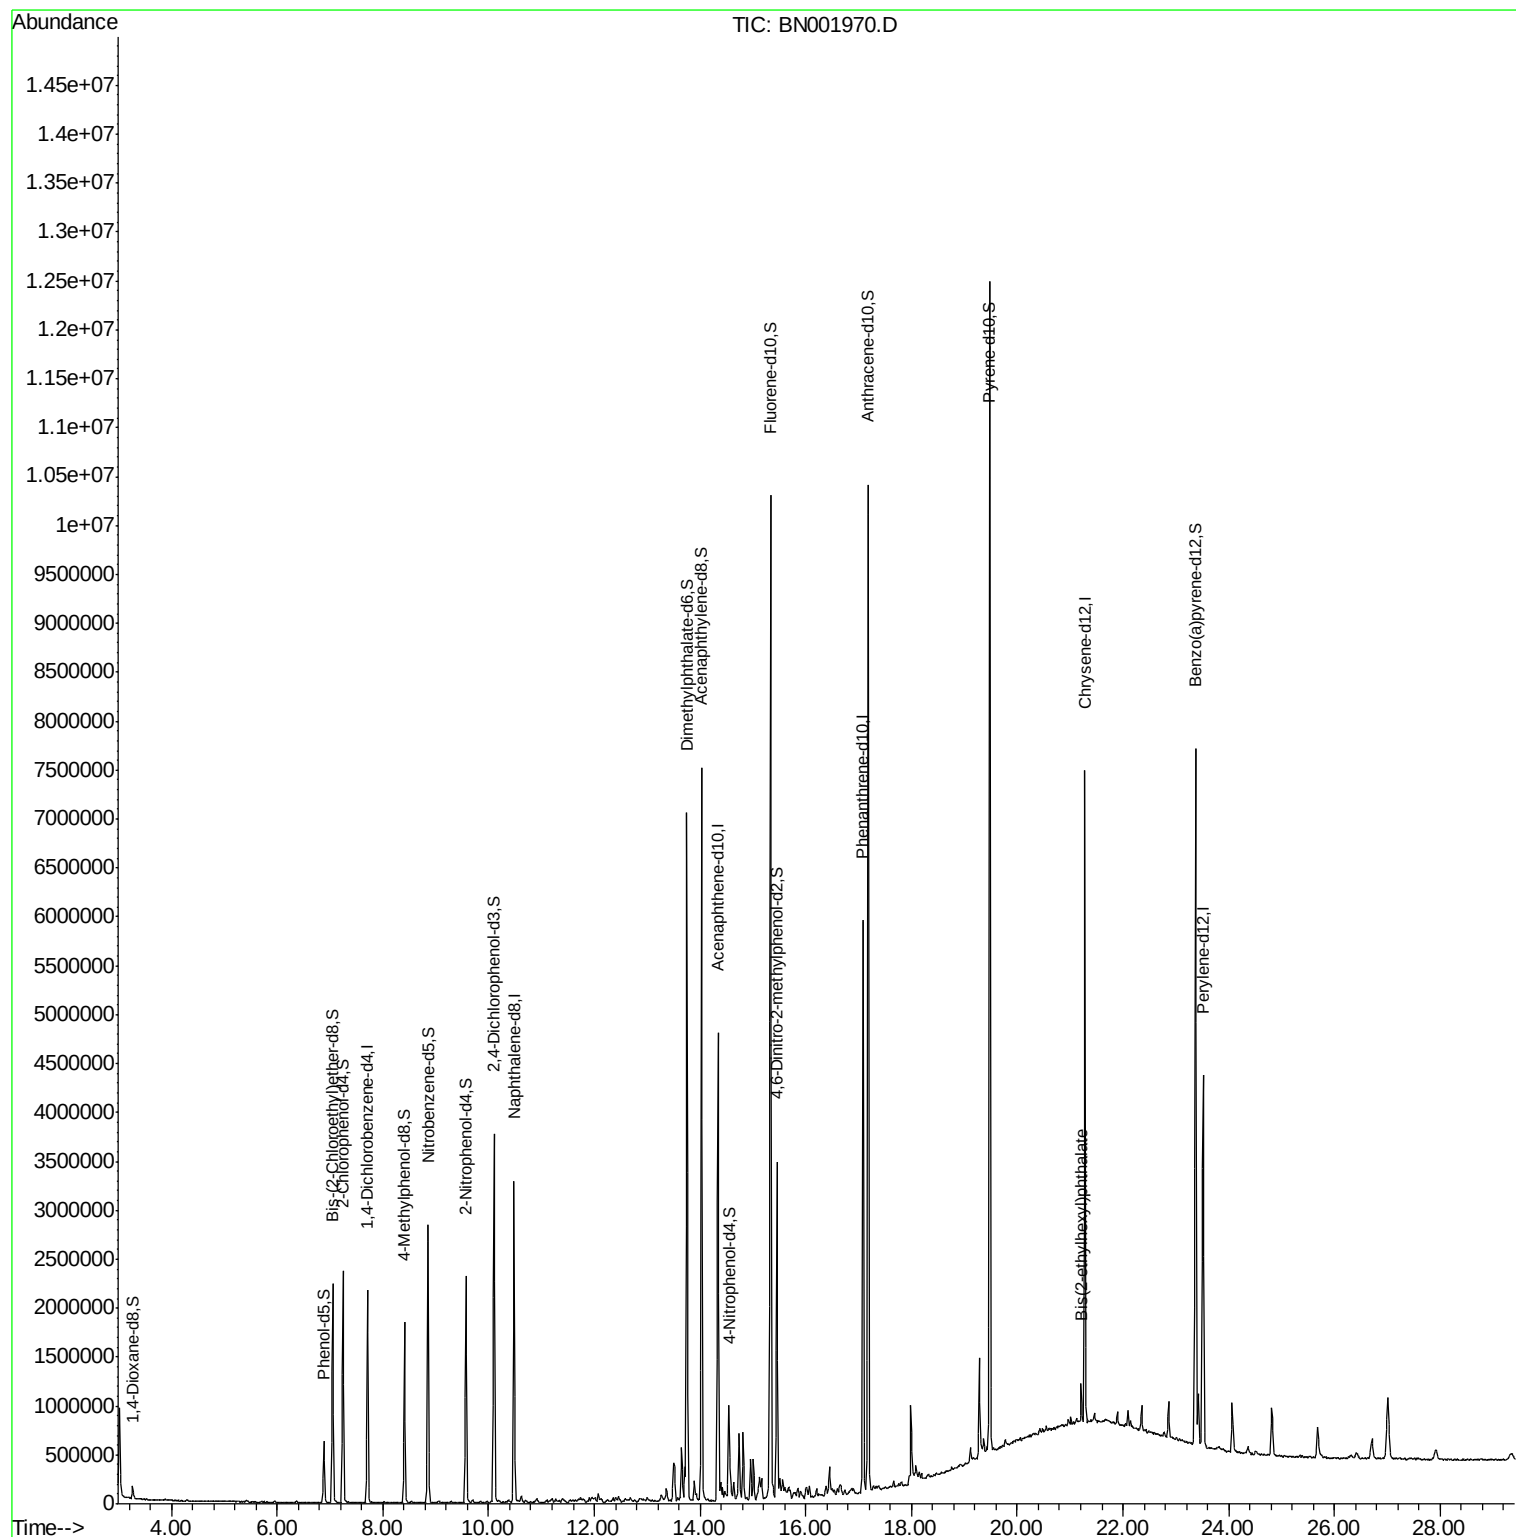

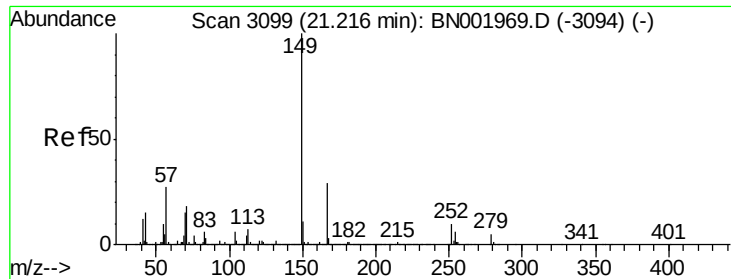

#81
 Bis(2-ethylhexyl)phthalate
 Concen: 1.176 ng/ul
 RT: 21.21 min Scan# 3098
 Delta R.T. -0.01 min
 Lab File: BN001970.D
 Acq: 05 Jul 2018 16:44

Instrument :
 BNA_N
 ClientSampleId :
 DAZR1

Tgt Ion	Ratio	Resp Lower	Resp Upper
149	100		
167	26.8	23.0	34.6
279	4.0	4.3	6.5

Manual Integrations
 APPROVED

Sohil
 7/6/2018 5:19:34 PM

