
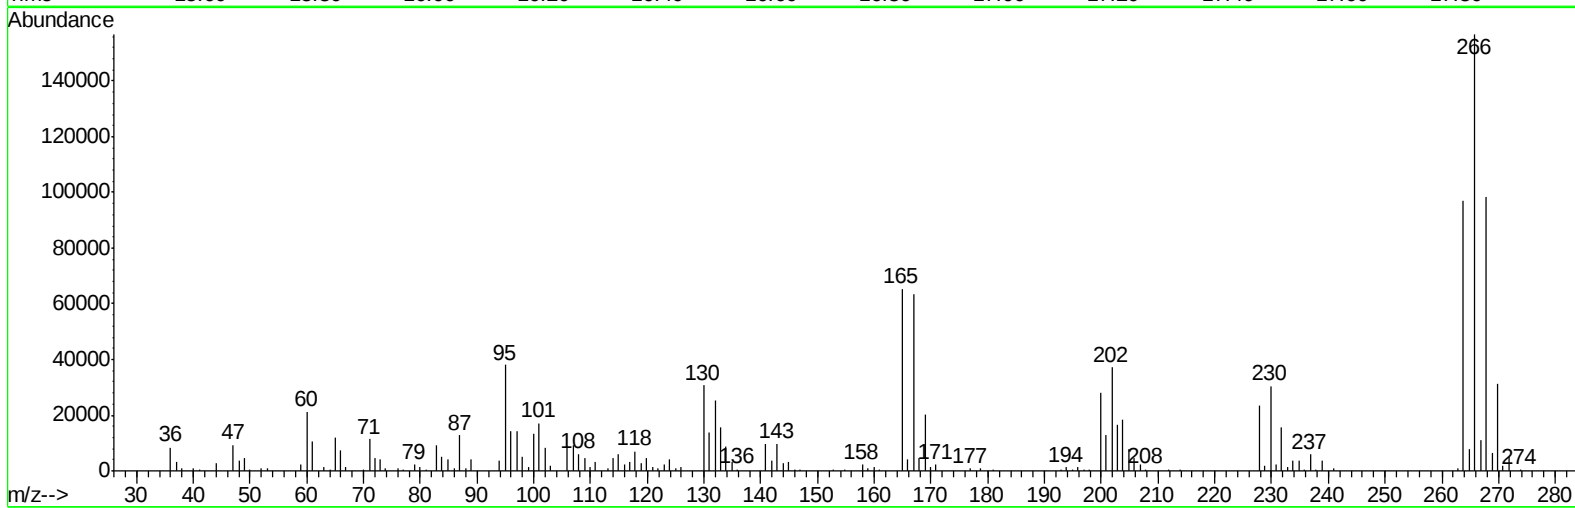


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN070519\
Data File : BN006730.D
Acq On : 06 Jul 2019 00:03
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 01:07:14 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 27 05:27:09 2019
Response via : Initial Calibration

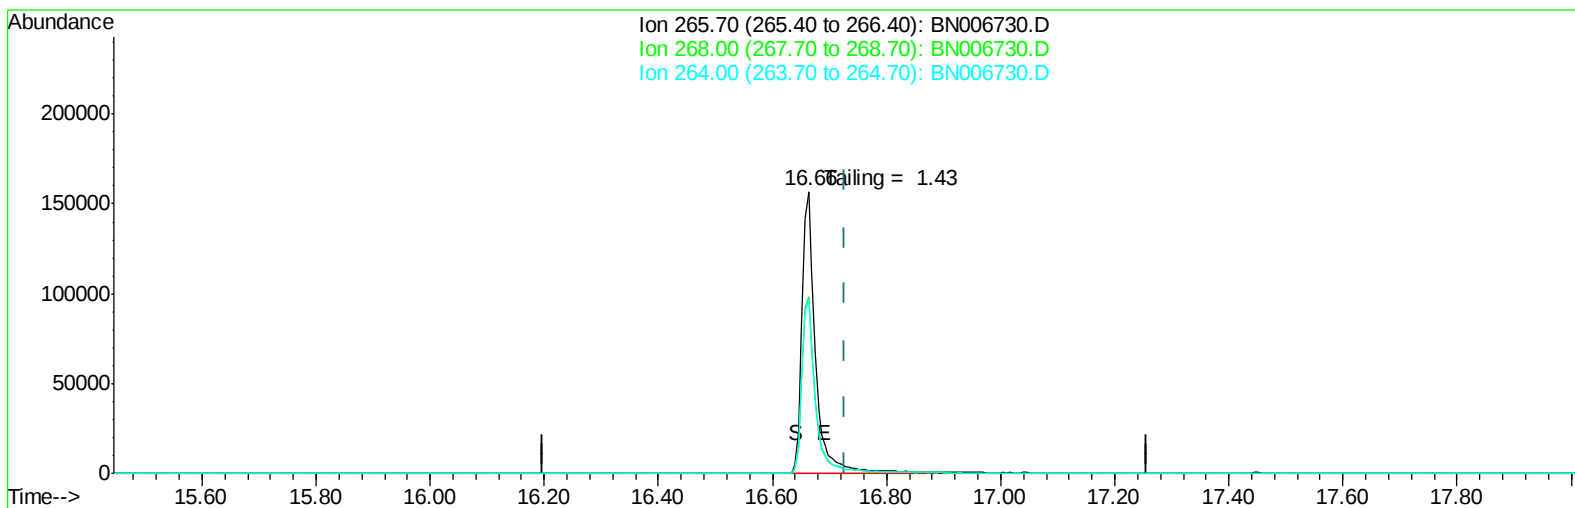

TIC: BN006730.D

(70) Pentachlorophenol (C)



16.663min (-0.064) 28566.72ng

response 256480

Ion	Exp%	Act%
265.70	100	100
268.00	63.50	62.81
264.00	62.50	61.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN070519\
 Data File : BN006730.D
 Acq On : 06 Jul 2019 00:03
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 01:07:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-BN032619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 27 05:27:09 2019
 Response via : Initial Calibration

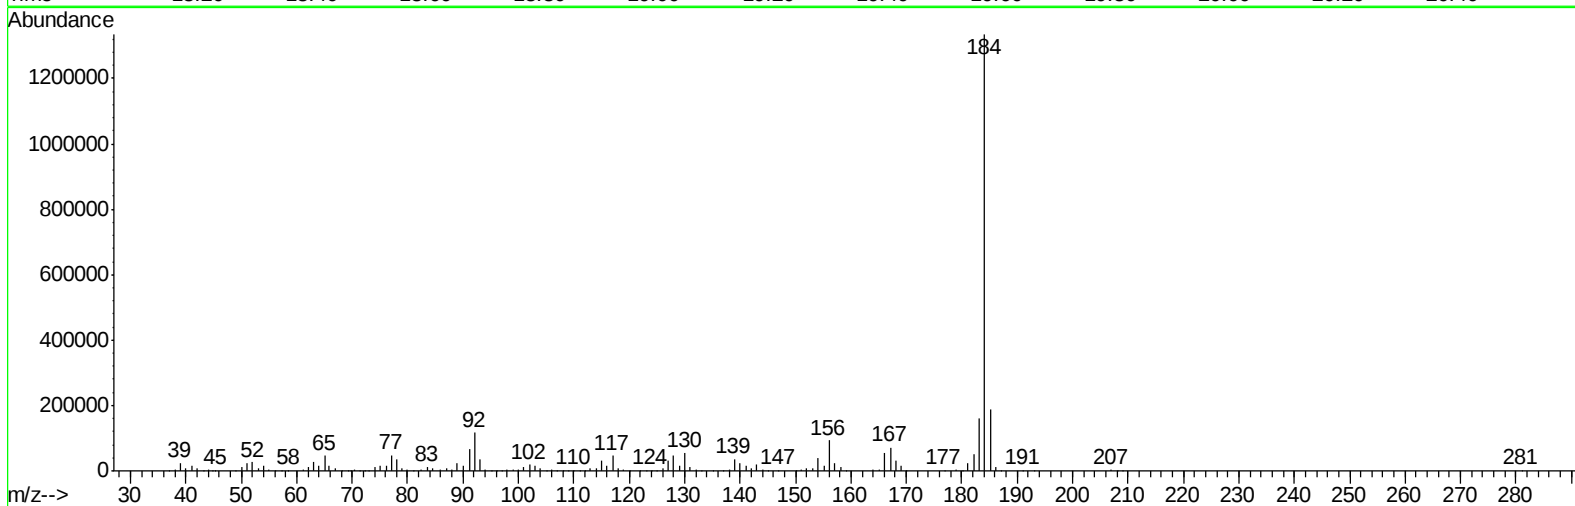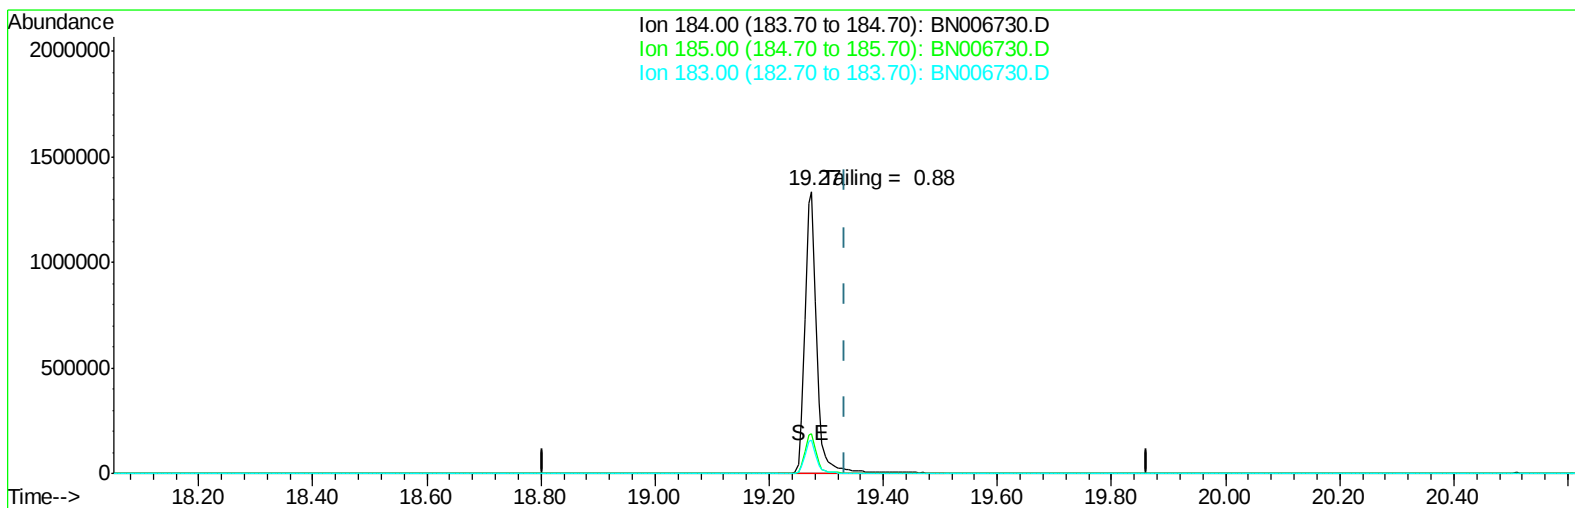

TIC: BN006730.D

(77) Benzidine

19.275min (-0.058) 0.00ng

response 1903159

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.02
183.00	12.40	11.90
0.00	0.00	0.00