


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN070519\  
Data File : BN006704.D  
Acq On : 05 Jul 2019 08:29  
Operator : HP/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\8270-SIM-BN070219.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Jul 05 05:30:28 2019

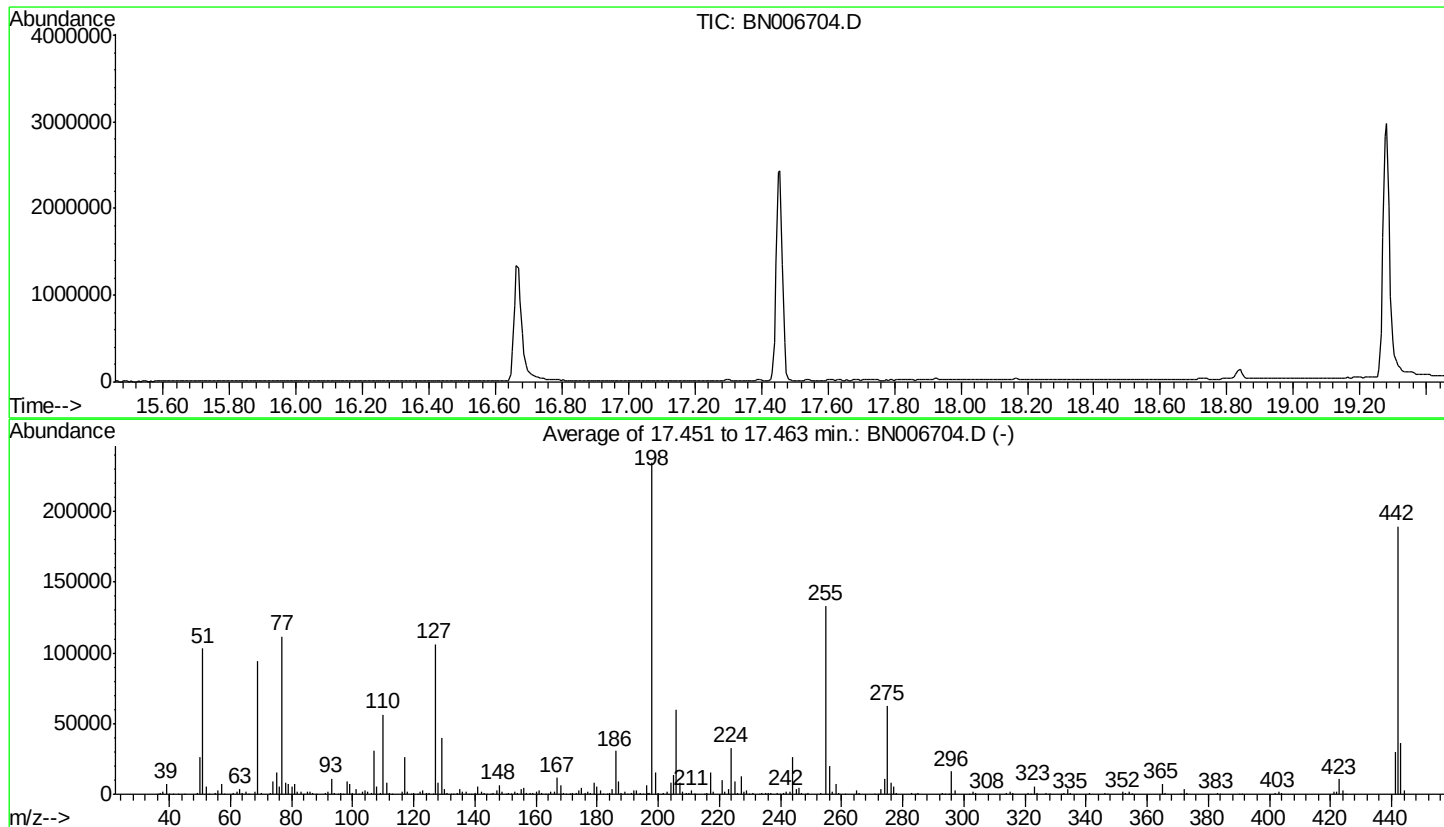

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 44.0      | 103069  | PASS             |
| 68          | 69           | 0.00         | 2            | 2.0       | 1832    | PASS             |
| 69          | 198          | 0.00         | 100          | 40.0      | 93797   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.7       | 666     | PASS             |
| 127         | 198          | 10           | 80           | 45.3      | 106202  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 1051    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 234474  | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 15370   | PASS             |
| 275         | 198          | 10           | 60           | 26.8      | 62920   | PASS             |
| 365         | 198          | 1            | 100          | 3.1       | 7301    | PASS             |
| 441         | 198          | 0.01         | 100          | 12.7      | 29818   | PASS             |
| 442         | 198          | 50           | 100          | 80.8      | 189525  | PASS             |
| 443         | 442          | 15           | 24           | 19.1      | 36133   | PASS             |