


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN070519\
 Data File : BN006711.D
 Acq On : 05 Jul 2019 12:31
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN070219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 05 05:30:28 2019

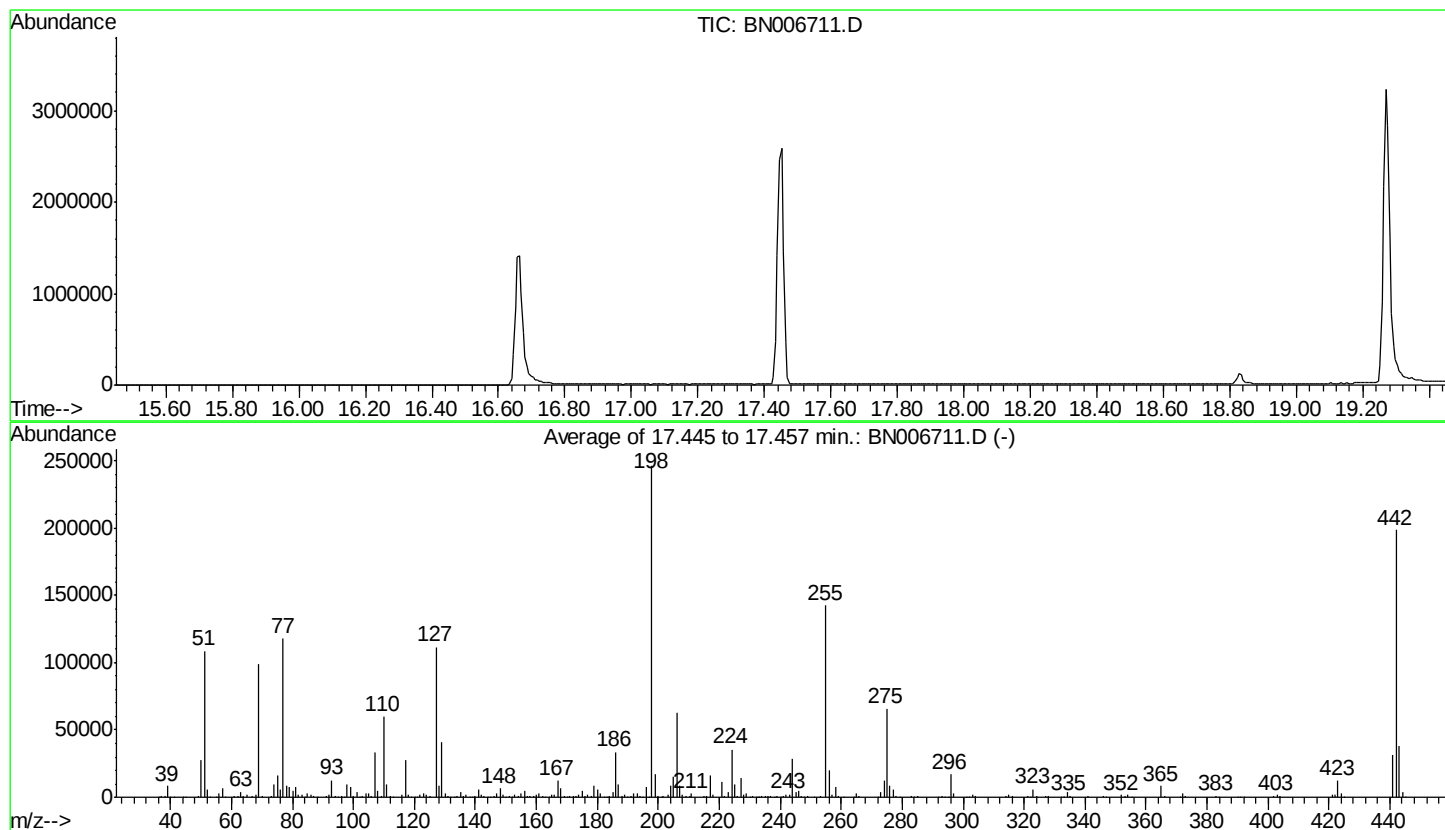

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	108938	PASS
68	69	0.00	2	1.9	1834	PASS
69	198	0.00	100	40.1	98874	PASS
70	69	0.00	2	0.6	622	PASS
127	198	10	80	45.2	111472	PASS
197	198	0.00	2	0.1	361	PASS
198	198	100	100	100.0	246528	PASS
199	198	5	9	6.9	16937	PASS
275	198	10	60	26.7	65898	PASS
365	198	1	100	3.4	8443	PASS
441	198	0.01	100	12.8	31573	PASS
442	198	50	100	80.6	198805	PASS
443	442	15	24	19.4	38544	PASS