


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN070519\
 Data File : BN006730.D
 Acq On : 06 Jul 2019 00:03
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN070219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 05 05:30:28 2019

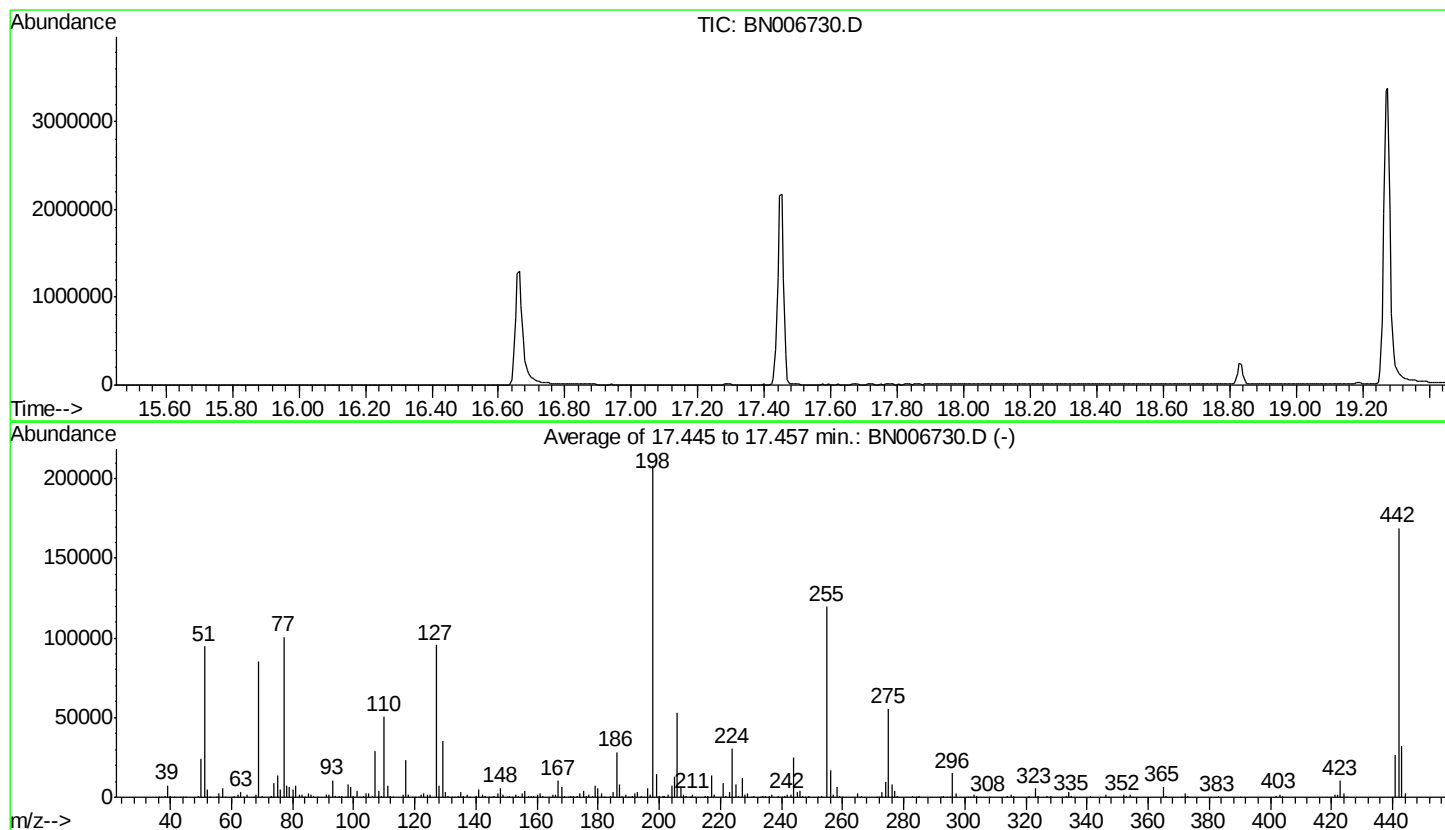

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	94509	PASS
68	69	0.00	2	2.0	1723	PASS
69	198	0.00	100	40.8	84858	PASS
70	69	0.00	2	0.6	513	PASS
127	198	10	80	45.8	95277	PASS
197	198	0.00	2	0.6	1253	PASS
198	198	100	100	100.0	208192	PASS
199	198	5	9	6.8	14211	PASS
275	198	10	60	26.7	55536	PASS
365	198	1	100	3.1	6531	PASS
441	198	0.01	100	12.7	26421	PASS
442	198	50	100	81.1	168789	PASS
443	442	15	24	19.1	32309	PASS