

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
 Data File : BN026332.D
 Acq On : 06 Jul 2023 16:18
 Operator : MA/JU
 Sample : PB153584BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK584

Quant Time: Jul 07 00:57:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 06 17:50:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.938	152	6730	0.400	ng/ul	0.00
4) Naphthalene-d8	10.748	136	22508	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	13050	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.330	188	24941	0.400	ng/ul	0.00
17) Chrysene-d12	21.541	240	13123	0.400	ng/ul	0.01
23) Perylene-d12	23.996	264	16942	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	36027	4.753	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.343	152	9283	0.268	ng/ul	0.00
18) Fluoranthene-d10	19.363	212	15405	0.308	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.726	202	2642	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.835	252	4996	0.080	ng/ul#	22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
Data File : BN026332.D
Acq On : 06 Jul 2023 16:18
Operator : MA/JU
Sample : PB153584BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK584

Quant Time: Jul 07 00:57:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 06 17:50:03 2023
Response via : Initial Calibration




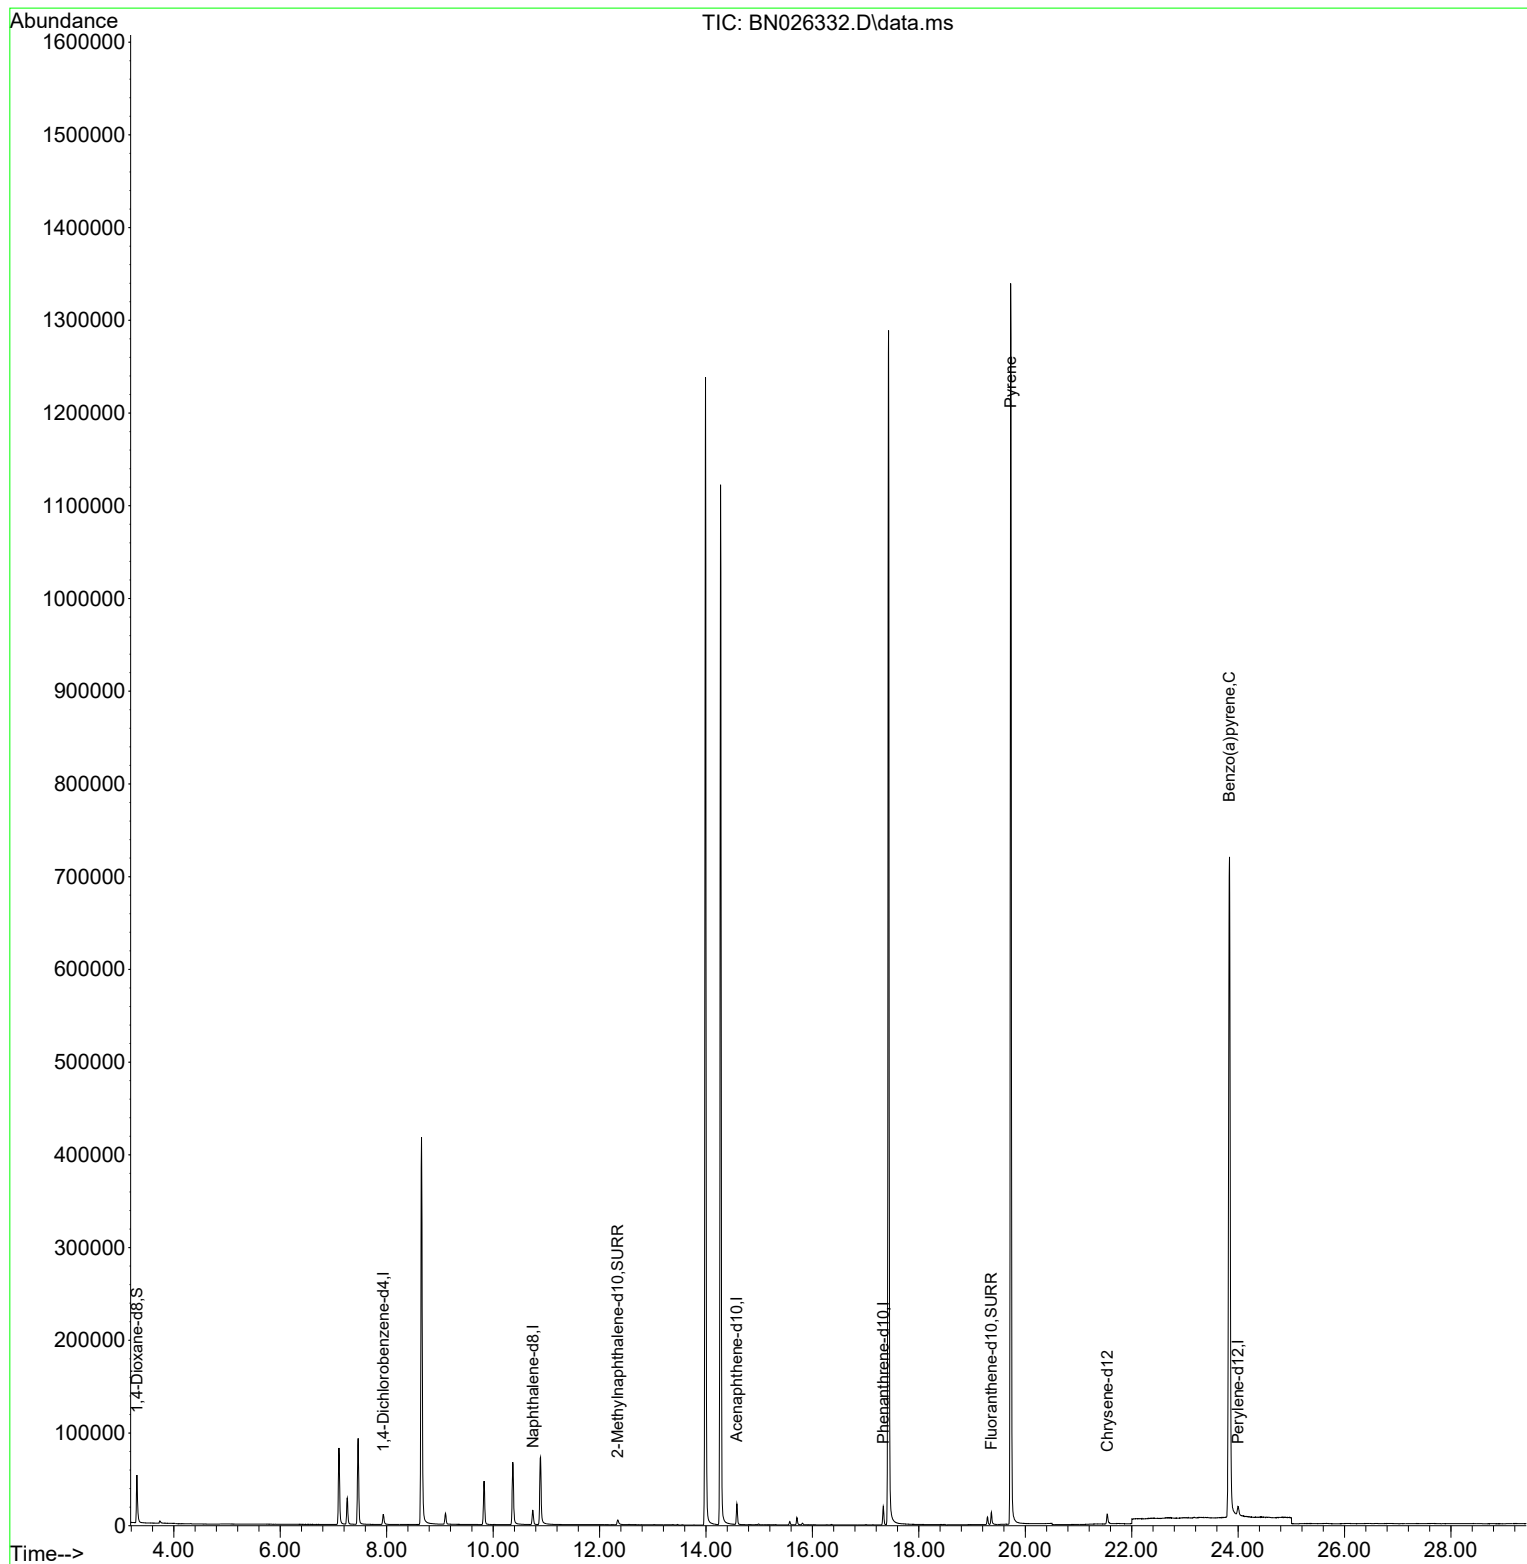


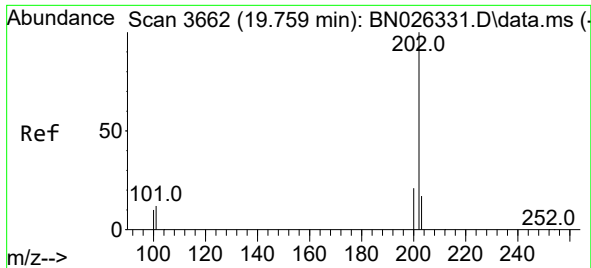

#20
Pyrene
Concen: 0.036 ng/ul
RT: 19.726 min Scan# 3655
Delta R.T. -0.033 min
Lab File: BN026332.D
Acq: 06 Jul 2023 16:18

Instrument :
BNA_N
ClientSampleId :
SBLK584

Tgt Ion:202 Resp: 2642
Ion Ratio Lower Upper
202 100
101 182.9 11.4 17.0#
100 1404.9 9.1 13.7#

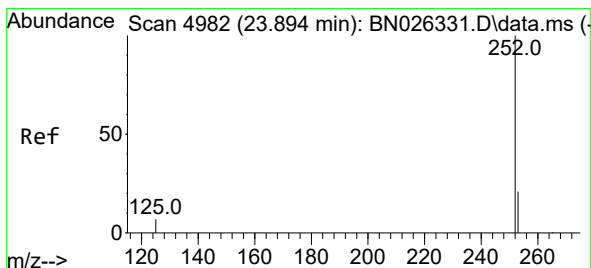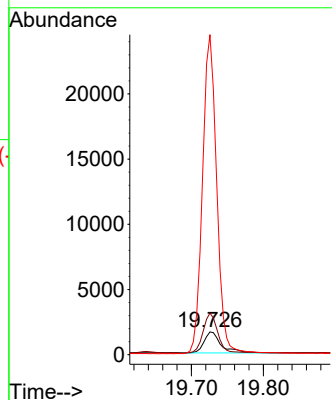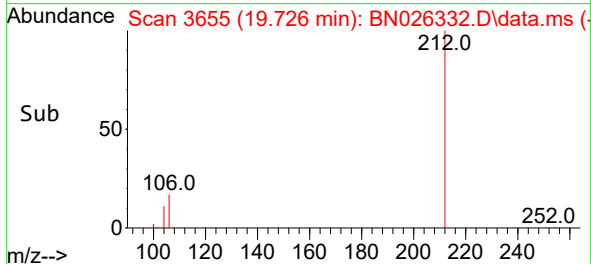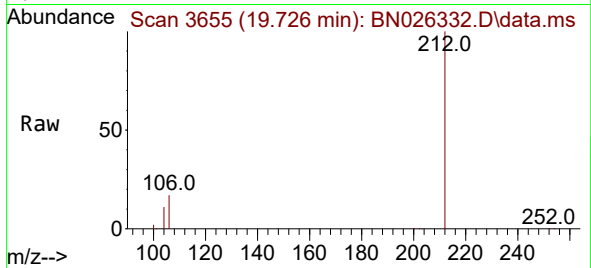

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.835 min Scan# 4962
Delta R.T. -0.050 min
Lab File: BN026332.D
Acq: 06 Jul 2023 16:18

Tgt Ion:252 Resp: 4996
Ion Ratio Lower Upper
252 100
253 67.6 26.0 39.0#
125 69.2 17.3 25.9#

