

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
 Data File : BN026333.D
 Acq On : 06 Jul 2023 16:56
 Operator : MA/JU
 Sample : PB153811BL
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK811

Quant Time: Jul 07 00:57:41 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 06 17:50:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	6763	0.400	ng/ul	0.00
4) Naphthalene-d8	10.748	136	22759	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	13204	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.330	188	21386	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.541	240	13380	0.400	ng/ul	0.01
23) Perylene-d12	23.999	264	17694	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.306	96	35308	4.636	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.343	152	9265	0.265	ng/ul	0.00
18) Fluoranthene-d10	19.363	212	15312	0.301	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.574	166	2703	0.047	ng/ul#	14
20) Pyrene	19.726	202	2628	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.841	252	4620	0.070	ng/ul#	26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
Data File : BN026333.D
Acq On : 06 Jul 2023 16:56
Operator : MA/JU
Sample : PB153811BL
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK811

Quant Time: Jul 07 00:57:41 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 06 17:50:03 2023
Response via : Initial Calibration




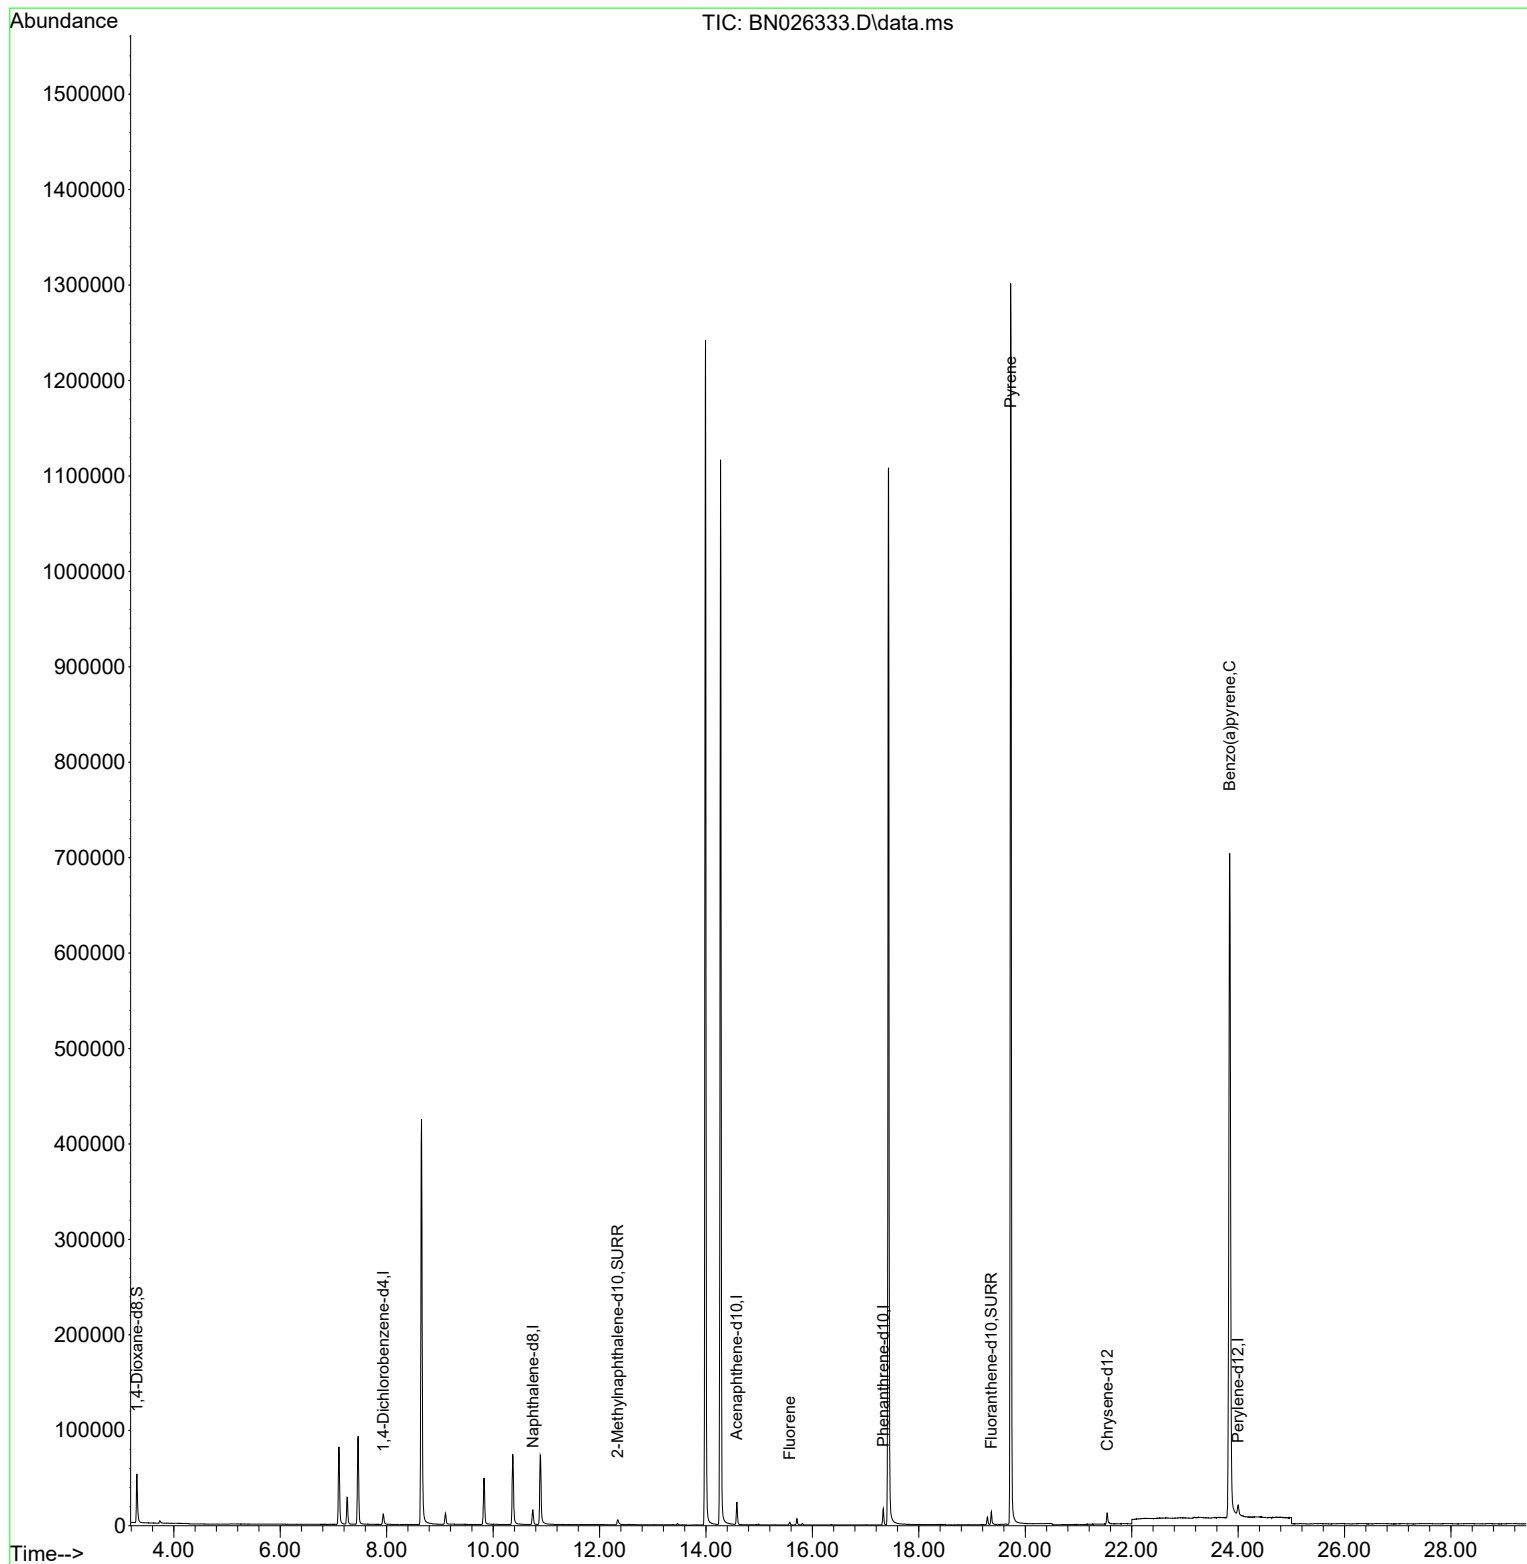


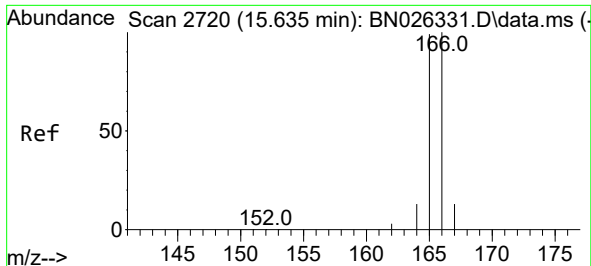

#12
Fluorene
Concen: 0.047 ng/ul
RT: 15.574 min Scan# 21
Delta R.T. -0.060 min
Lab File: BN026333.D
Acq: 06 Jul 2023 16:56




Instrument :
BNA_N
ClientSampleId :
SBLK811


Tgt Ion:166 Resp: 2703
Ion Ratio Lower Upper
166 100
165 9.4 79.9 119.9#
167 33.9 10.8 16.2#

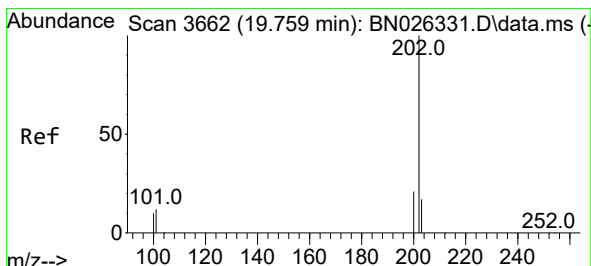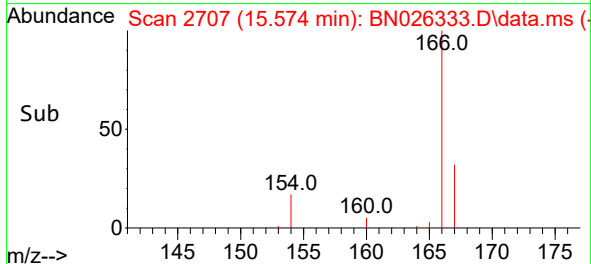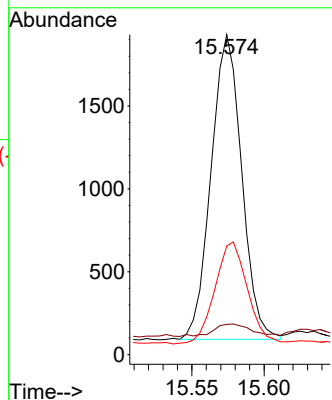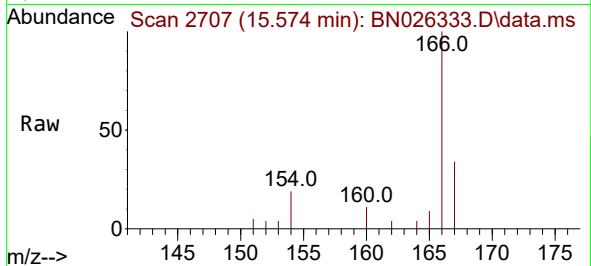

#20
Pyrene
Concen: 0.035 ng/ul
RT: 19.726 min Scan# 3655
Delta R.T. -0.033 min
Lab File: BN026333.D
Acq: 06 Jul 2023 16:56

Tgt Ion:202 Resp: 2628
Ion Ratio Lower Upper
202 100
101 182.8 11.4 17.0#
100 1422.9 9.1 13.7#

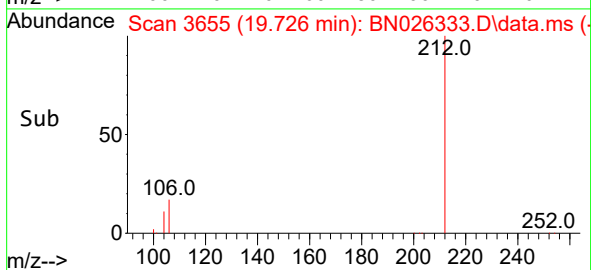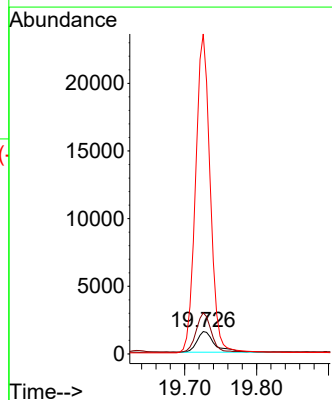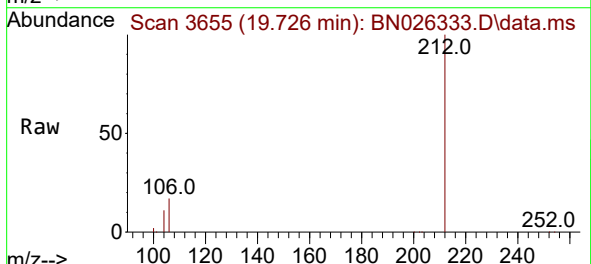

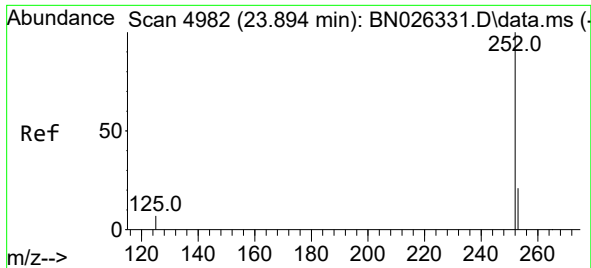

#26

Benzo(a)pyrene

Concen: 0.070 ng/ul

RT: 23.841 min Scan# 49

Delta R.T. -0.044 min

Lab File: BN026333.D


Acq: 06 Jul 2023 16:56

Instrument :

BNA_N

ClientSampleId :

SBLK811

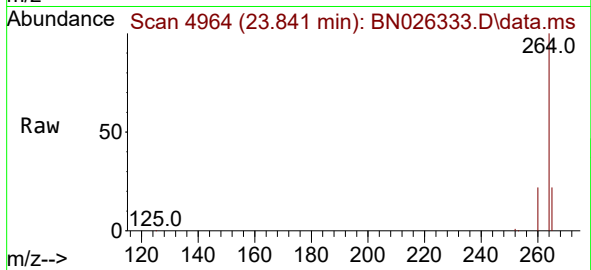

Tgt Ion:252 Resp: 4620

Ion Ratio Lower Upper

252 100

253 67.4 26.0 39.0#

125 64.7 17.3 25.9#

