

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
 Data File : BN026337.D
 Acq On : 06 Jul 2023 19:26
 Operator : MA/JU
 Sample : 03257-11
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYY1

Quant Time: Jul 07 00:58:06 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 06 17:50:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.938	152	6563	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136	22311	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	12982	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.330	188	24640	0.400	ng/ul	0.00
17) Chrysene-d12	21.532	240	13461	0.400	ng/ul	0.00
23) Perylene-d12	23.978	264	18246	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.306	96	22722	3.074	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.343	152	9125	0.266	ng/ul	0.00
18) Fluoranthene-d10	19.363	212	16759	0.327	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.726	202	3164	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.821	252	5613	0.083	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
Data File : BN026337.D
Acq On : 06 Jul 2023 19:26
Operator : MA/JU
Sample : 03257-11
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYY1

Quant Time: Jul 07 00:58:06 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 06 17:50:03 2023
Response via : Initial Calibration

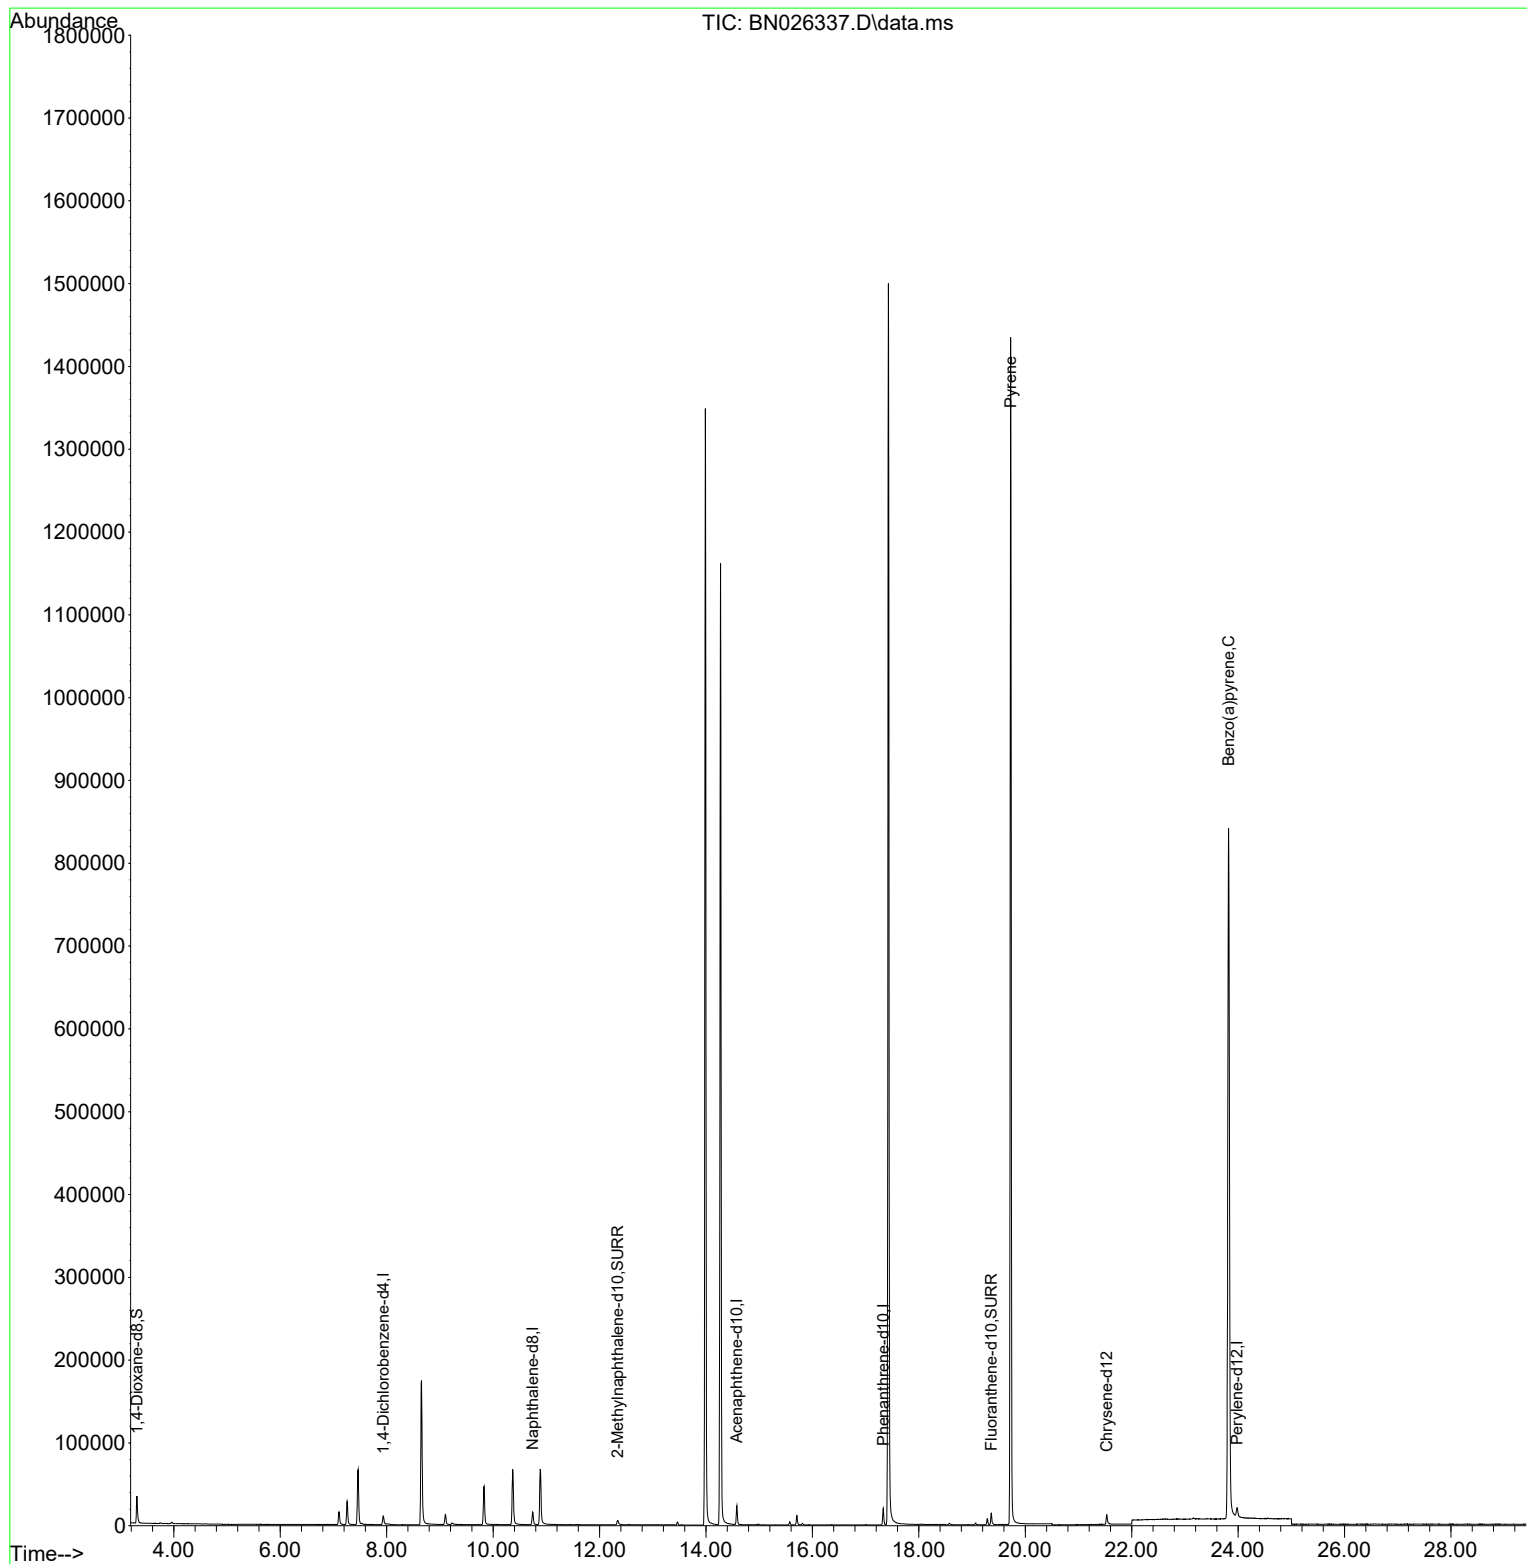

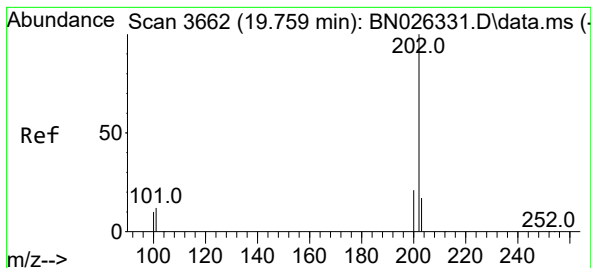

#20

Pyrene

Concen: 0.042 ng/ul

RT: 19.726 min Scan# 3

Delta R.T. -0.033 min

Lab File: BN026337.D

Acq: 06 Jul 2023 19:26

Instrument :

BNA_N

ClientSampleId :

EXYY1





Tgt Ion:202 Resp: 3164

Ion Ratio Lower Upper

202 100

101 181.8 11.4 17.0#

100 1413.6 9.1 13.7#

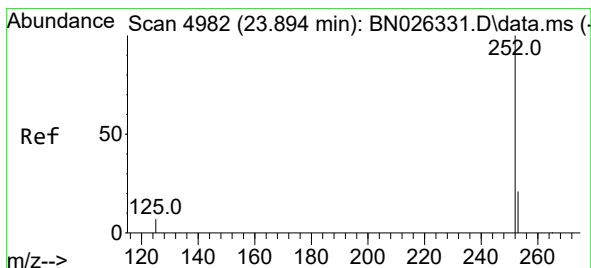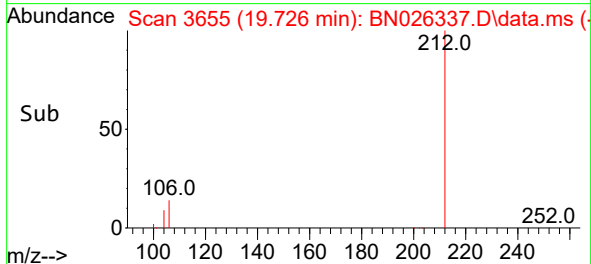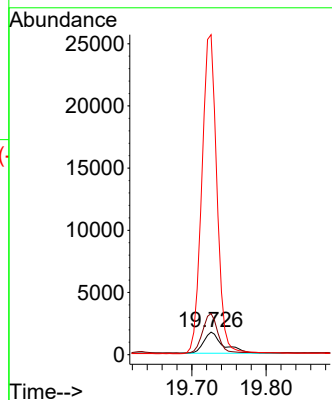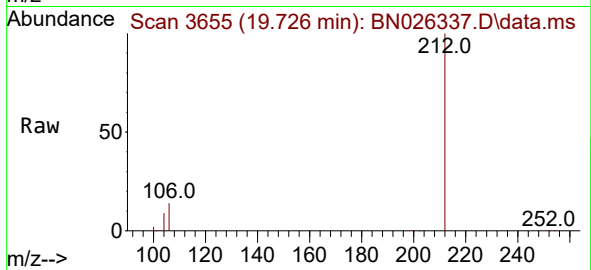

#26

Benzo(a)pyrene

Concen: 0.083 ng/ul

RT: 23.821 min Scan# 4957

Delta R.T. -0.064 min

Lab File: BN026337.D

Acq: 06 Jul 2023 19:26

Tgt Ion:252 Resp: 5613

Ion Ratio Lower Upper

252 100

253 63.7 26.0 39.0#

125 61.3 17.3 25.9#

