

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
 Data File : BN026340.D
 Acq On : 06 Jul 2023 21:19
 Operator : MA/JU
 Sample : 03258-06
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCGW5

Quant Time: Jul 07 00:58:25 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 06 17:50:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	7515	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136	25141	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	14890	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.330	188	28223	0.400	ng/ul	0.00
17) Chrysene-d12	21.529	240	14497	0.400	ng/ul	0.00
23) Perylene-d12	23.981	264	19703	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	33661	3.977	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.337	152	10166	0.263	ng/ul	0.00
18) Fluoranthene-d10	19.359	212	23872	0.433	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.726	202	4142	0.051	ng/ul#	1
26) Benzo(a)pyrene	23.832	252	6822	0.093	ng/ul#	49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
Data File : BN026340.D
Acq On : 06 Jul 2023 21:19
Operator : MA/JU
Sample : 03258-06
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCGW5

Quant Time: Jul 07 00:58:25 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 06 17:50:03 2023
Response via : Initial Calibration




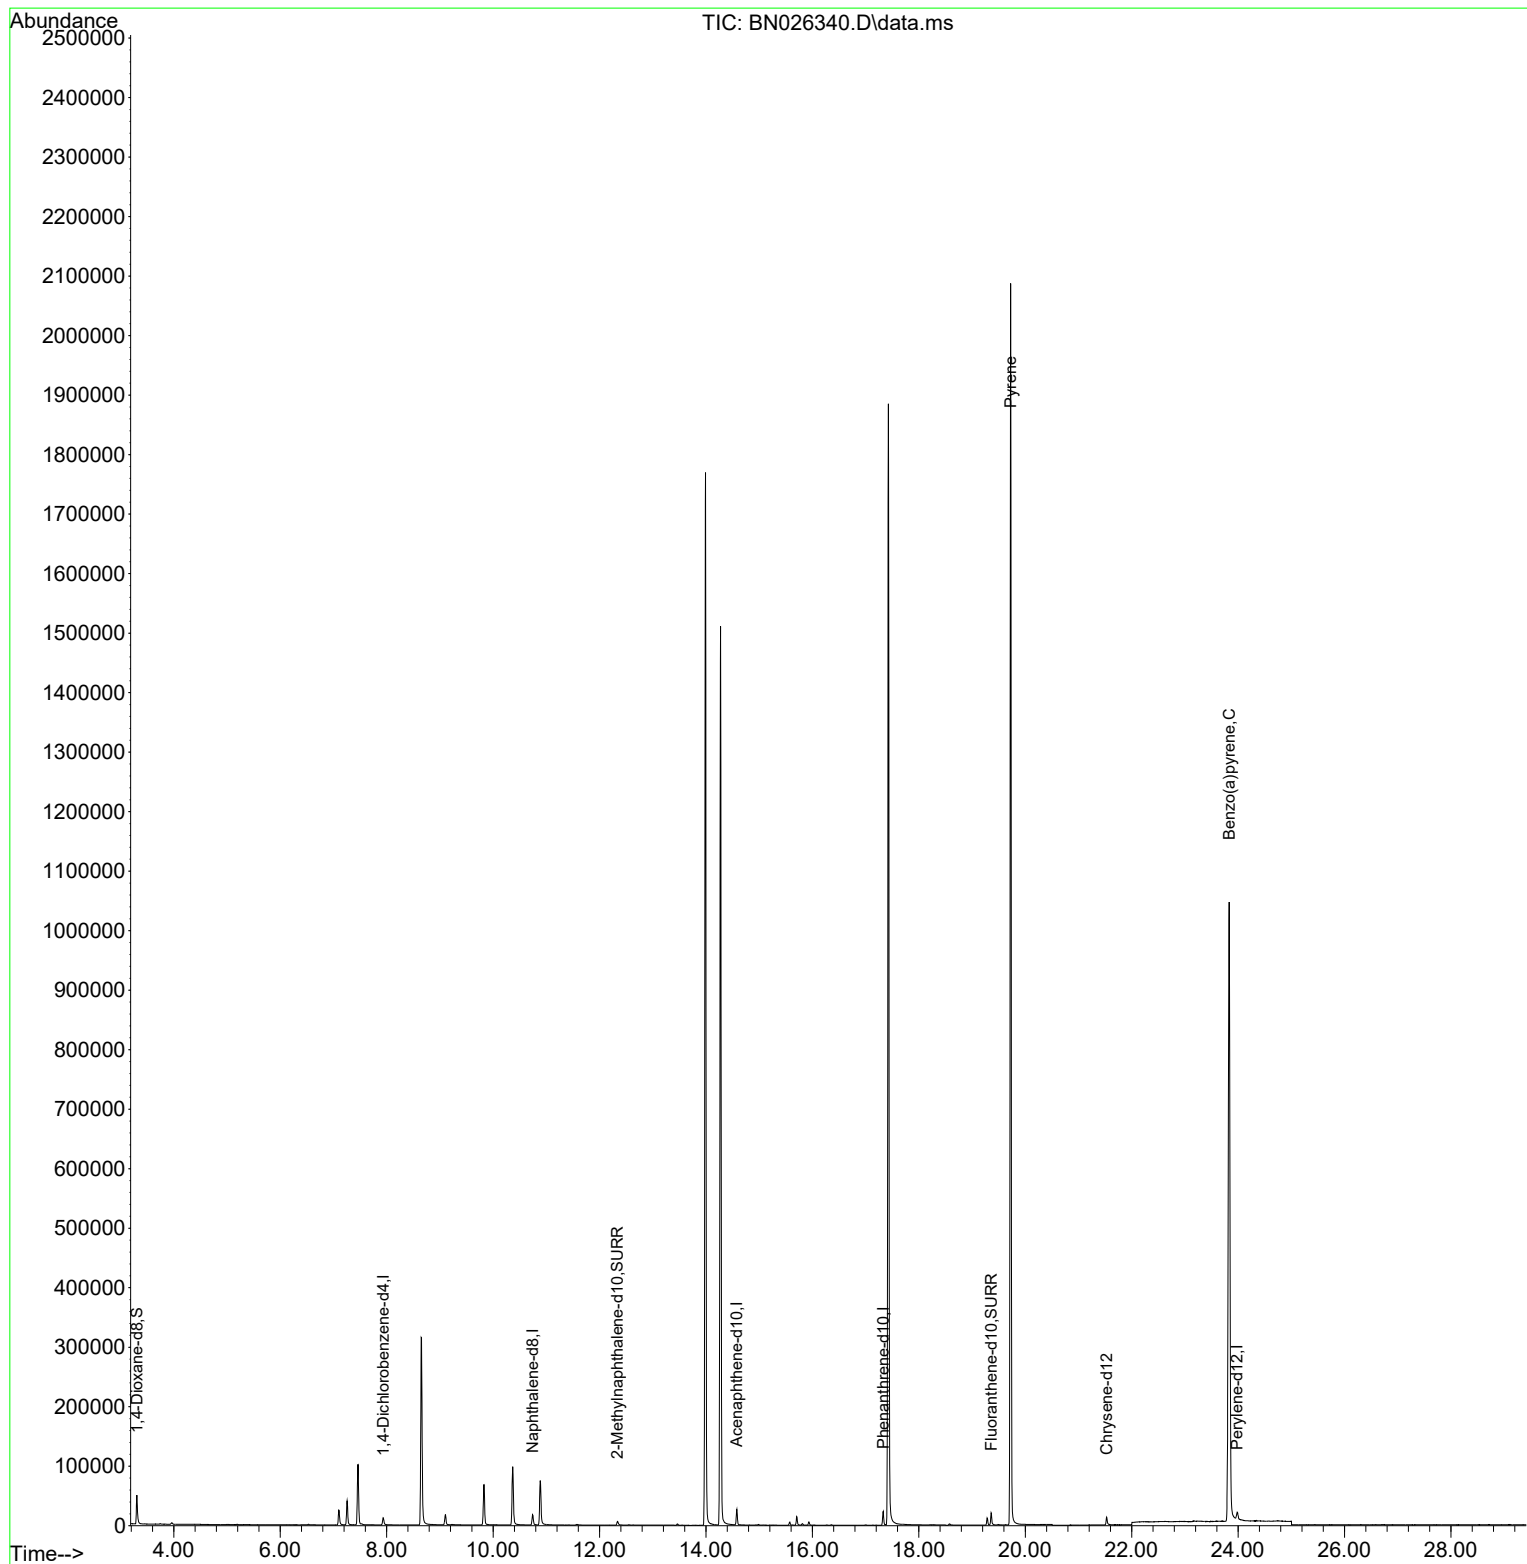


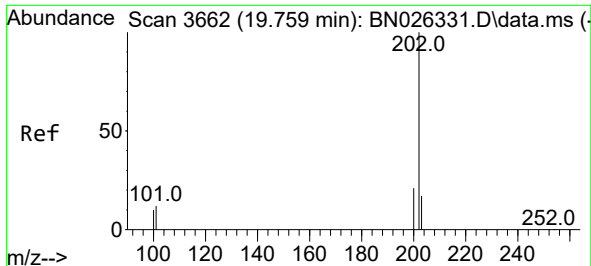

#20
Pyrene
Concen: 0.051 ng/ul
RT: 19.726 min Scan# 3655
Delta R.T. -0.033 min
Lab File: BN026340.D
Acq: 06 Jul 2023 21:19

Instrument :
BNA_N
ClientSampleId :
DCGW5

Tgt Ion:202 Resp: 4142
Ion Ratio Lower Upper
202 100
101 182.0 11.4 17.0#
100 1413.5 9.1 13.7#

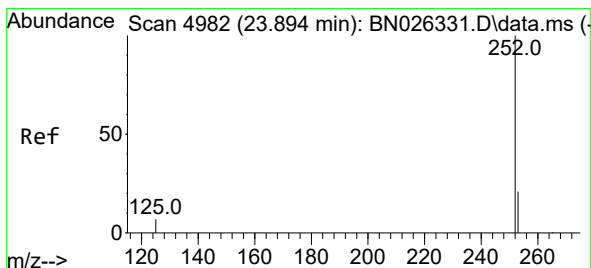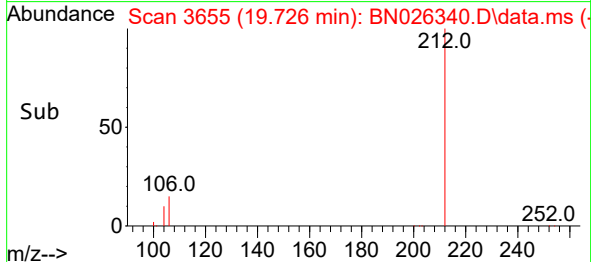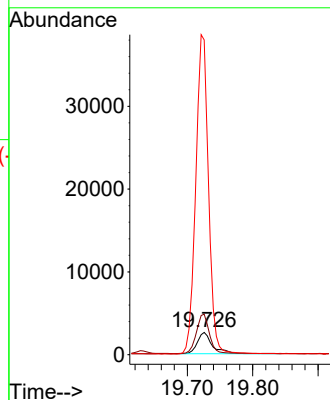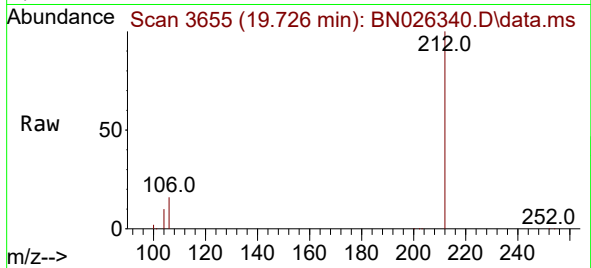

#26
Benzo(a)pyrene
Concen: 0.093 ng/ul
RT: 23.832 min Scan# 4961
Delta R.T. -0.053 min
Lab File: BN026340.D
Acq: 06 Jul 2023 21:19

Tgt Ion:252 Resp: 6822
Ion Ratio Lower Upper
252 100
253 54.1 26.0 39.0#
125 54.5 17.3 25.9#

