

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
 Data File : BN026302.D
 Acq On : 05 Jul 2023 21:09
 Operator : MA/JU
 Sample : 03293-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZF3

Quant Time: Jul 06 00:43:13 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 05 00:03:30 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.942	152	6845	0.400	ng/ul	0.00
4) Naphthalene-d8	10.752	136	20255	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.584	164	13483	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.334	188	25170	0.400	ng/ul	0.00
17) Chrysene-d12	21.534	240	13676	0.400	ng/ul	0.00
23) Perylene-d12	23.975	264	17977	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.310	96	27278	3.539	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.347	152	9325	0.299	ng/ul	0.00
18) Fluoranthene-d10	19.367	212	16498	0.317	ng/ul	0.00
Target Compounds						
						Qvalue
15) Phenanthrene	17.376	178	1677	0.020	ng/ul#	78
16) Anthracene	17.465	178	1775	0.024	ng/ul#	73
19) Fluoranthene	19.395	202	1664	0.023	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
 Data File : BN026302.D
 Acq On : 05 Jul 2023 21:09
 Operator : MA/JU
 Sample : 03293-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BFZF3

Quant Time: Jul 06 00:43:13 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 05 00:03:30 2023
 Response via : Initial Calibration




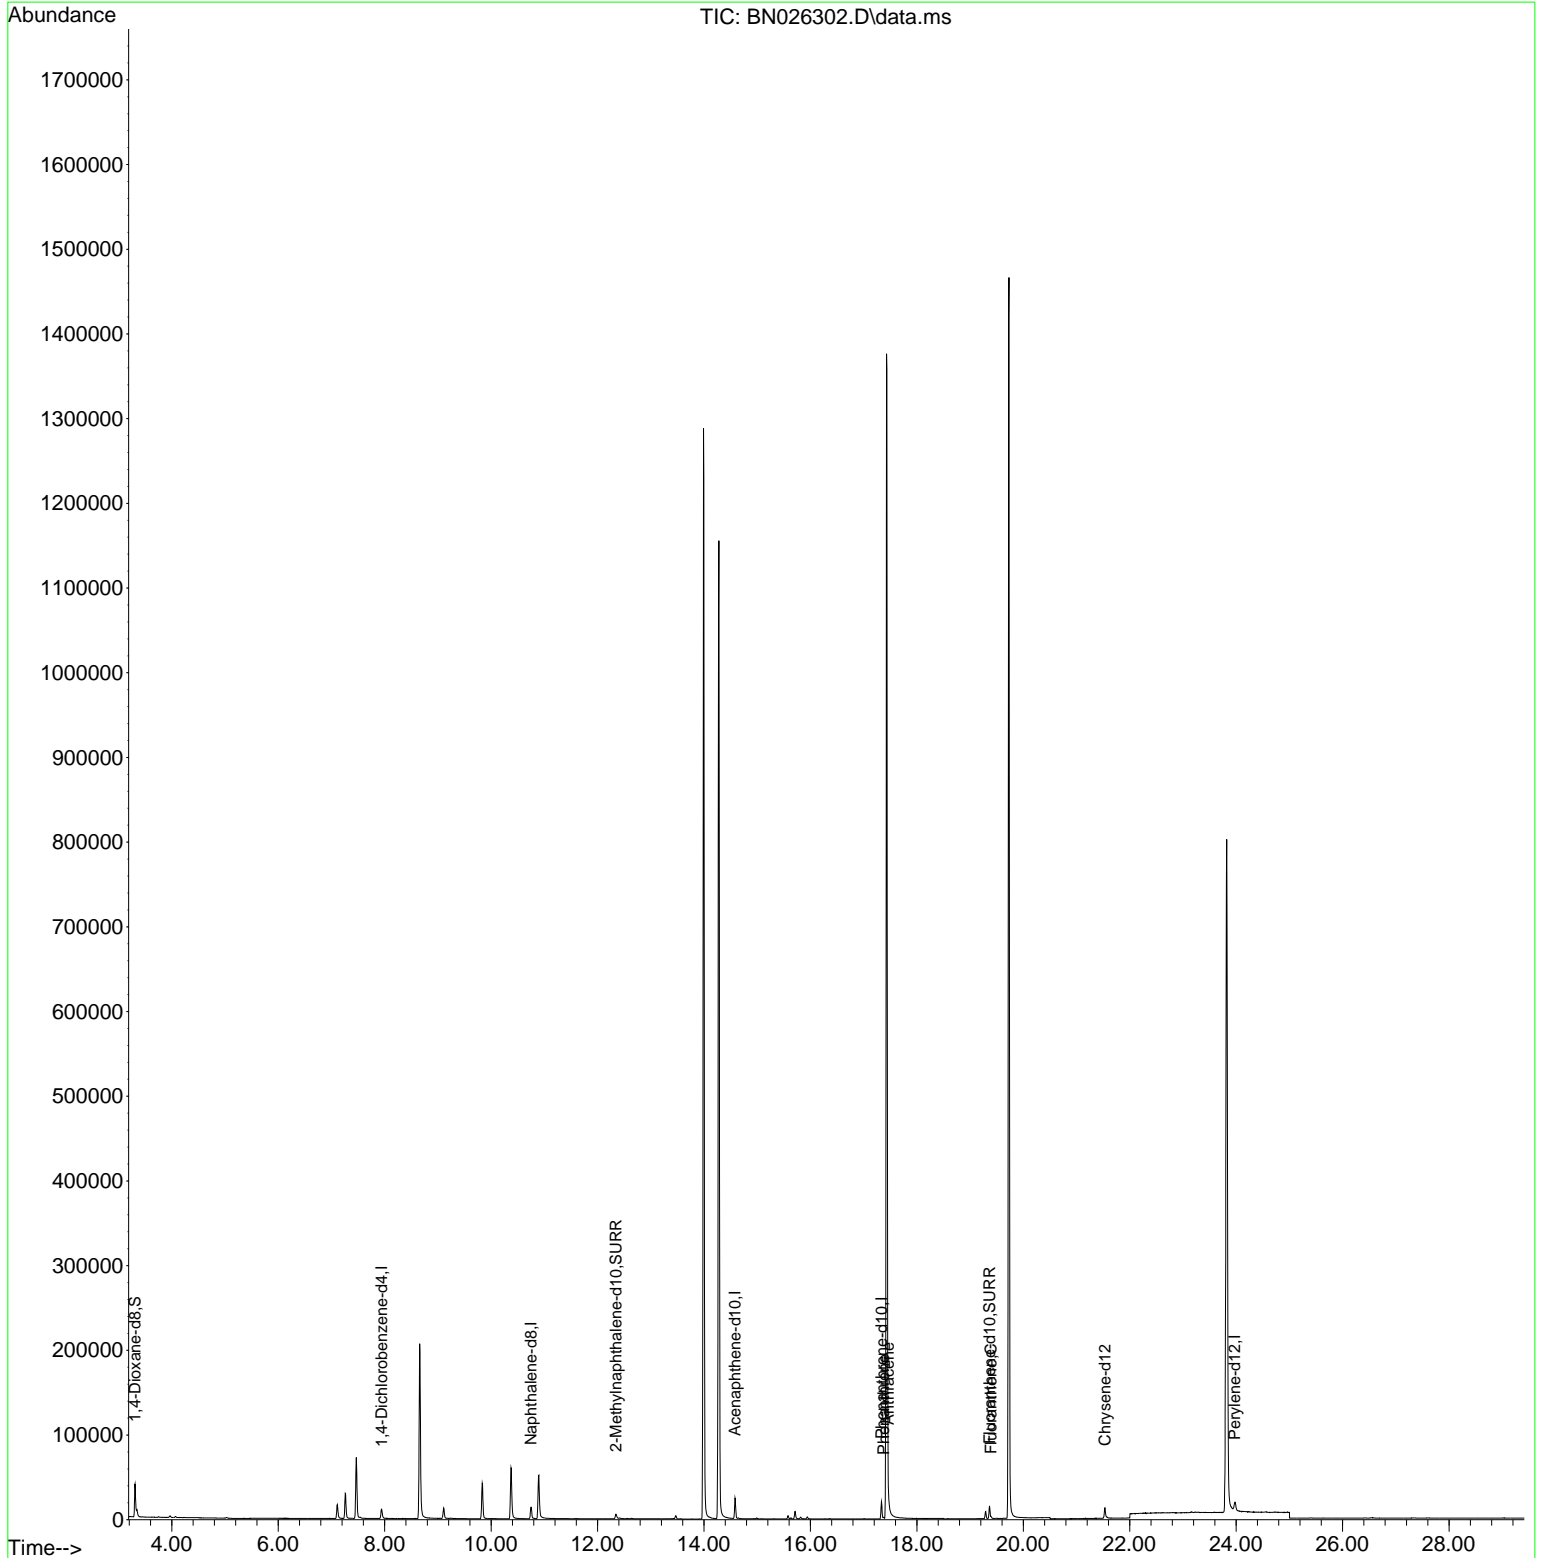


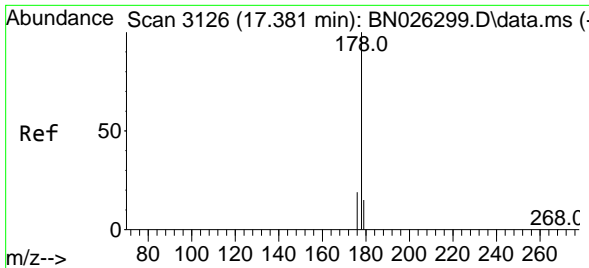

#15
 Phenanthrene
 Concen: 0.020 ng/u1
 RT: 17.376 min Scan# 3126
 Delta R.T. -0.010 min
 Lab File: BN026302.D
 Acq: 05 Jul 2023 21:09




Instrument :
 BNA_N
 ClientSampleId :
 BFZF3


Tgt Ion	Resp	Lower	Upper
178	1677		
179	27.6	12.6	19.0#
176	27.7	15.8	23.6#

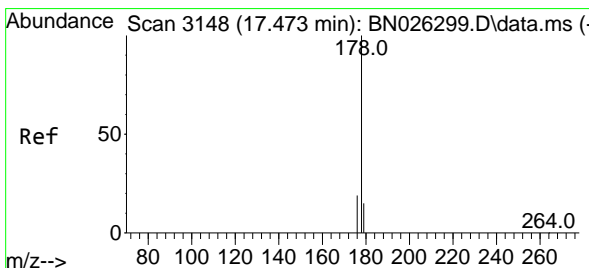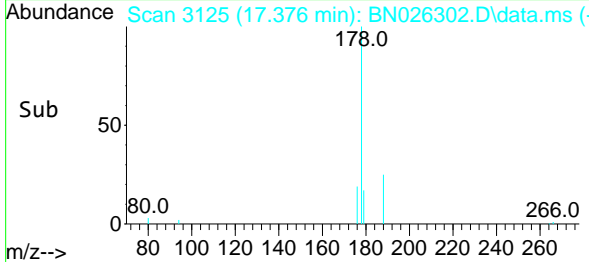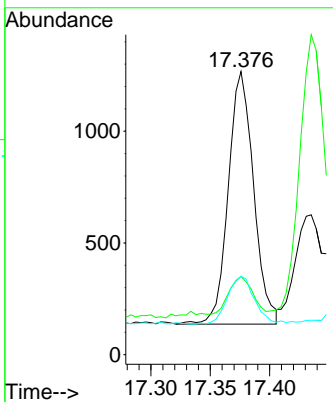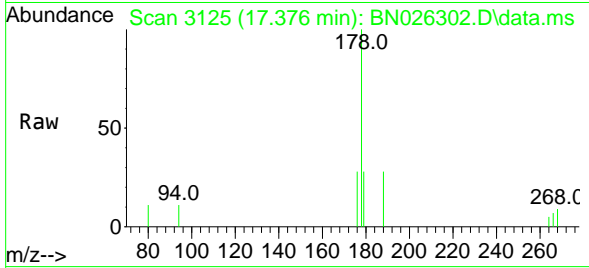

#16
 Anthracene
 Concen: 0.024 ng/u1
 RT: 17.465 min Scan# 3146
 Delta R.T. -0.014 min
 Lab File: BN026302.D
 Acq: 05 Jul 2023 21:09


Tgt Ion	Resp	Lower	Upper
178	1775		
179	30.8	12.6	18.8#
176	27.7	15.1	22.7#

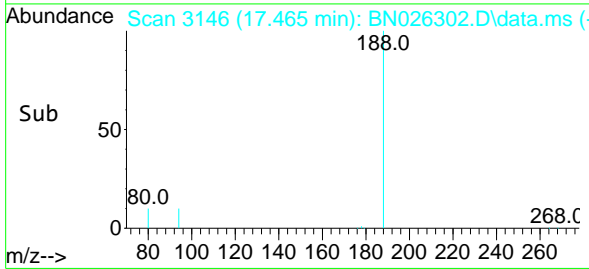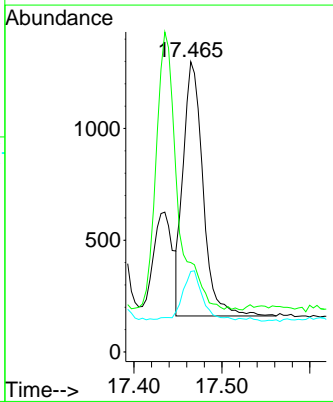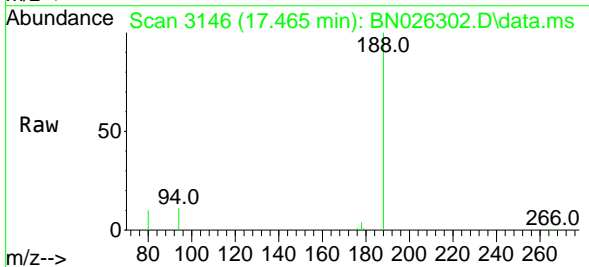

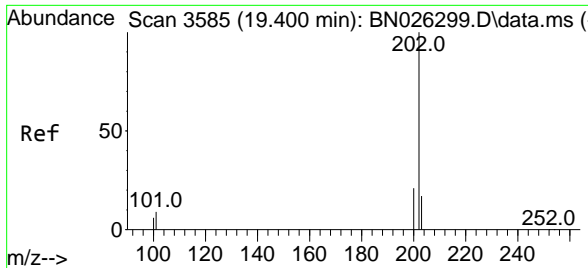

#19
 Fluoranthene
 Concen: 0.023 ng/ul
 RT: 19.395 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BN026302.D
 Acq: 05 Jul 2023 21:09

Instrument :
 BNA_N
 ClientSampleId :
 BFZF3

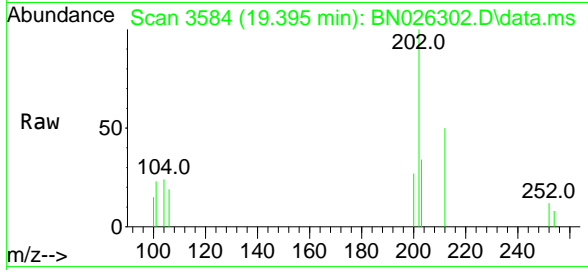

Tgt Ion:202 Resp: 1664

Ion	Ratio	Lower	Upper
202	100		
101	23.3	9.5	14.3#
100	15.4	7.3	10.9#

