

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
 Data File : BN026325.D
 Acq On : 06 Jul 2023 11:56
 Operator : MA/JU
 Sample : 03258-13DL 10X
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCGY5DL

Quant Time: Jul 06 18:00:57 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 06 17:50:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.938	152	5716	0.400	ng/ul	0.00
4) Naphthalene-d8	10.748	136	19456	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	11458	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.330	188	21930	0.400	ng/ul	0.00
17) Chrysene-d12	21.531	240	12263	0.400	ng/ul	0.00
23) Perylene-d12	23.998	264	13397	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.310	96	420	0.065	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.337	152	1072	0.036	ng/ul	0.00
18) Fluoranthene-d10	19.363	212	1827	0.039	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.343	88	8007	1.171	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
Data File : BN026325.D
Acq On : 06 Jul 2023 11:56
Operator : MA/JU
Sample : 03258-13DL 10X
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCGY5DL

Quant Time: Jul 06 18:00:57 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 06 17:50:03 2023
Response via : Initial Calibration

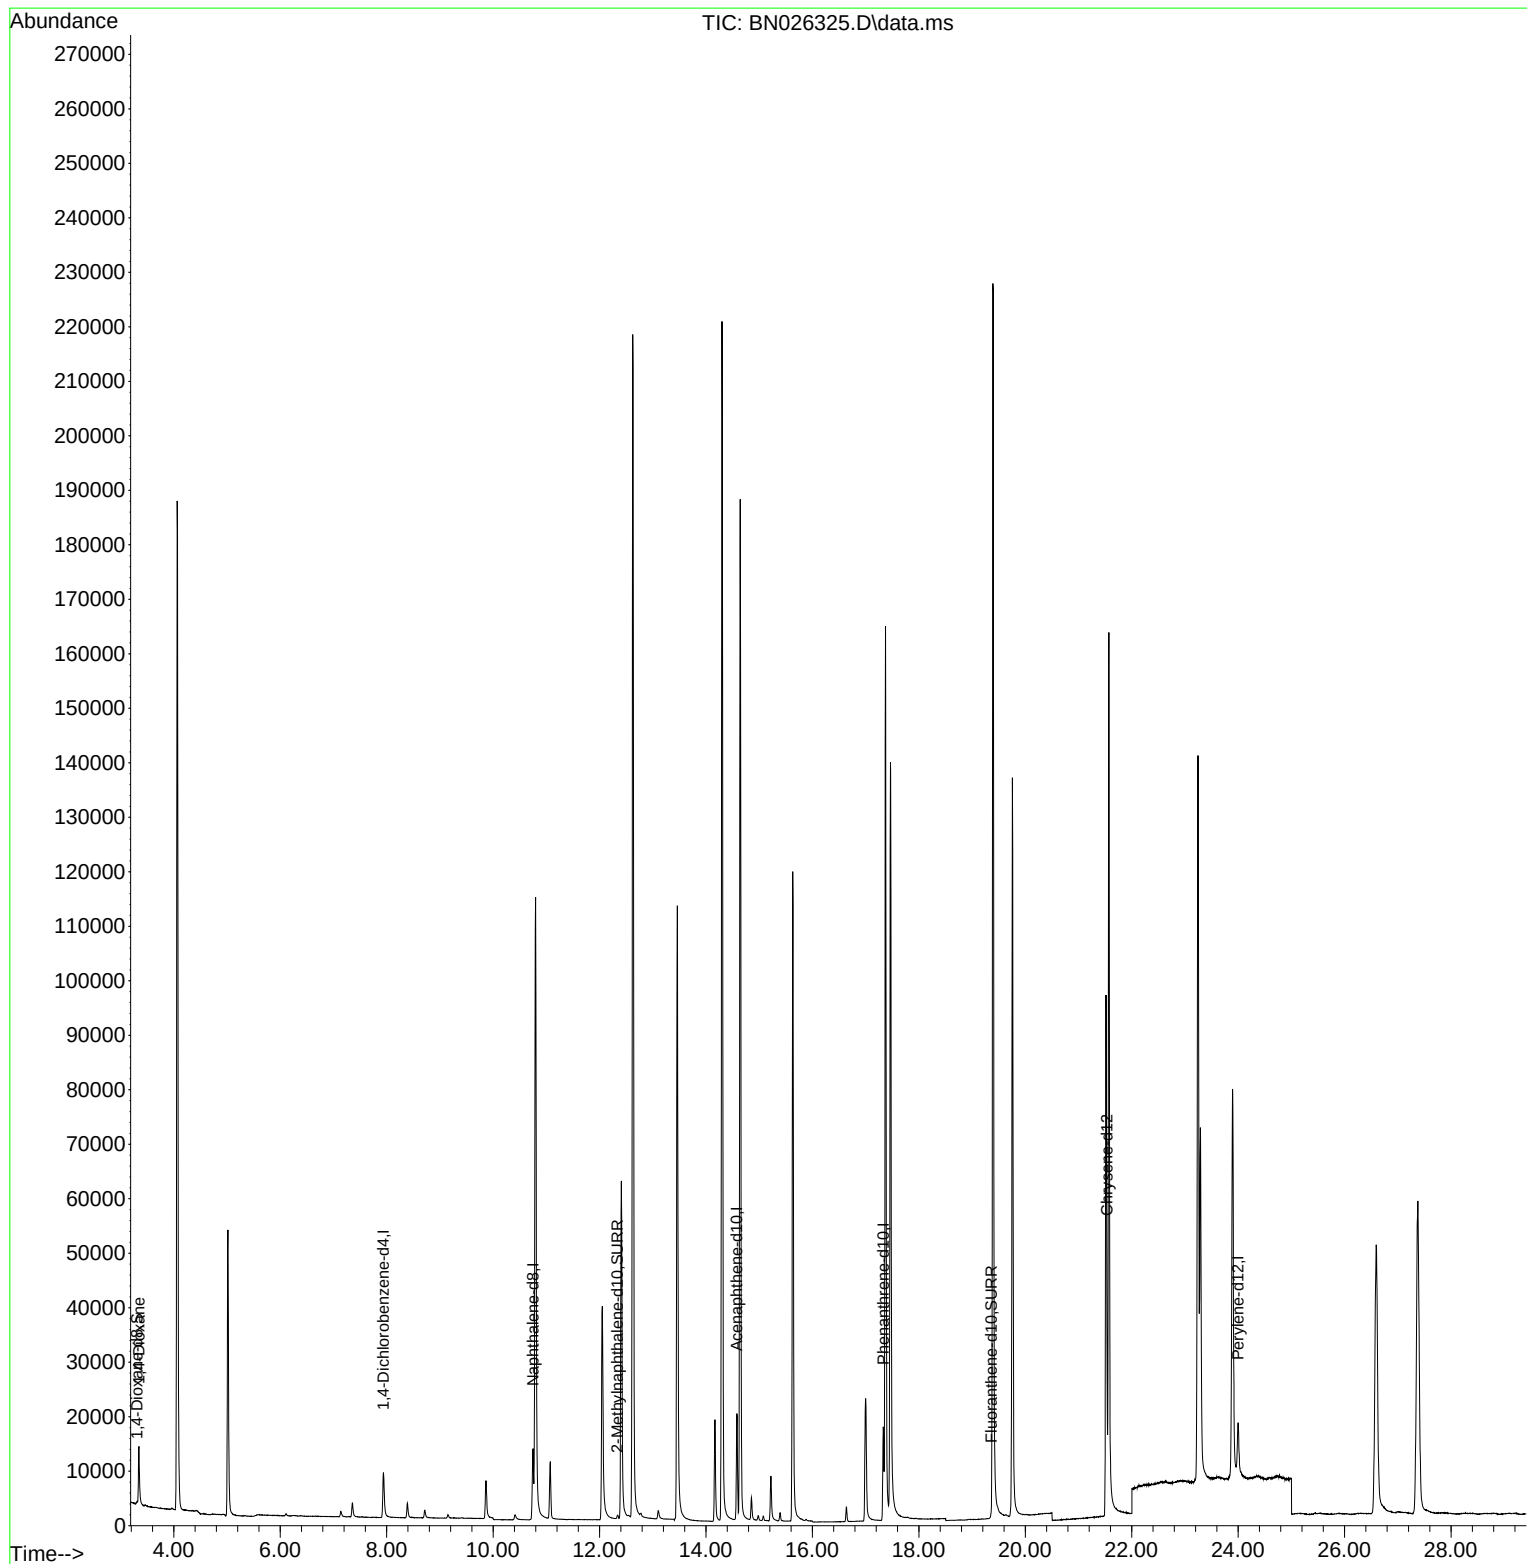

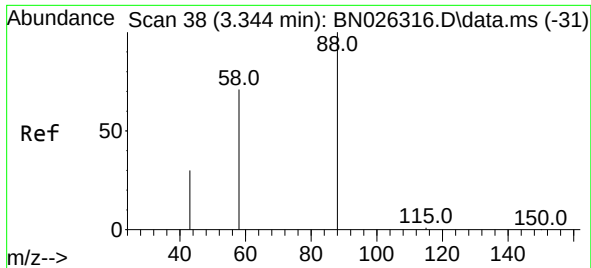

#2
 1,4-Dioxane
 Concen: 1.171 ng/ul
 RT: 3.343 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN026325.D
 Acq: 06 Jul 2023 11:56

Instrument :
 BNA_N
 ClientSampleId :
 DCGY5DL

Tgt Ion:	88	Resp:	8007
Ion	Ratio	Lower	Upper
88	100		
43	46.7	29.5	44.3#
58	61.8	37.4	56.2#

