

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
 Data File : BN026326.D
 Acq On : 06 Jul 2023 12:33
 Operator : MA/JU
 Sample : 03284-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCHB6

Quant Time: Jul 06 14:11:12 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 05 00:03:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.942	152	5343	0.400	ng/ul	0.00
4) Naphthalene-d8	10.754	136	18514	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.589	164	9735	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.343	188	14738	0.400	ng/ul	0.00
17) Chrysene-d12	21.535	240	10140	0.400	ng/ul	# 0.00
23) Perylene-d12	23.990	264	11958	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.310	96	3325	0.553	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.354	152	6513	0.229	ng/ul	0.00
18) Fluoranthene-d10	19.368	212	12145	0.315	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.343	88	19581	3.065	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
Data File : BN026326.D
Acq On : 06 Jul 2023 12:33
Operator : MA/JU
Sample : 03284-01
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCHB6

Quant Time: Jul 06 14:11:12 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 05 00:03:30 2023
Response via : Initial Calibration

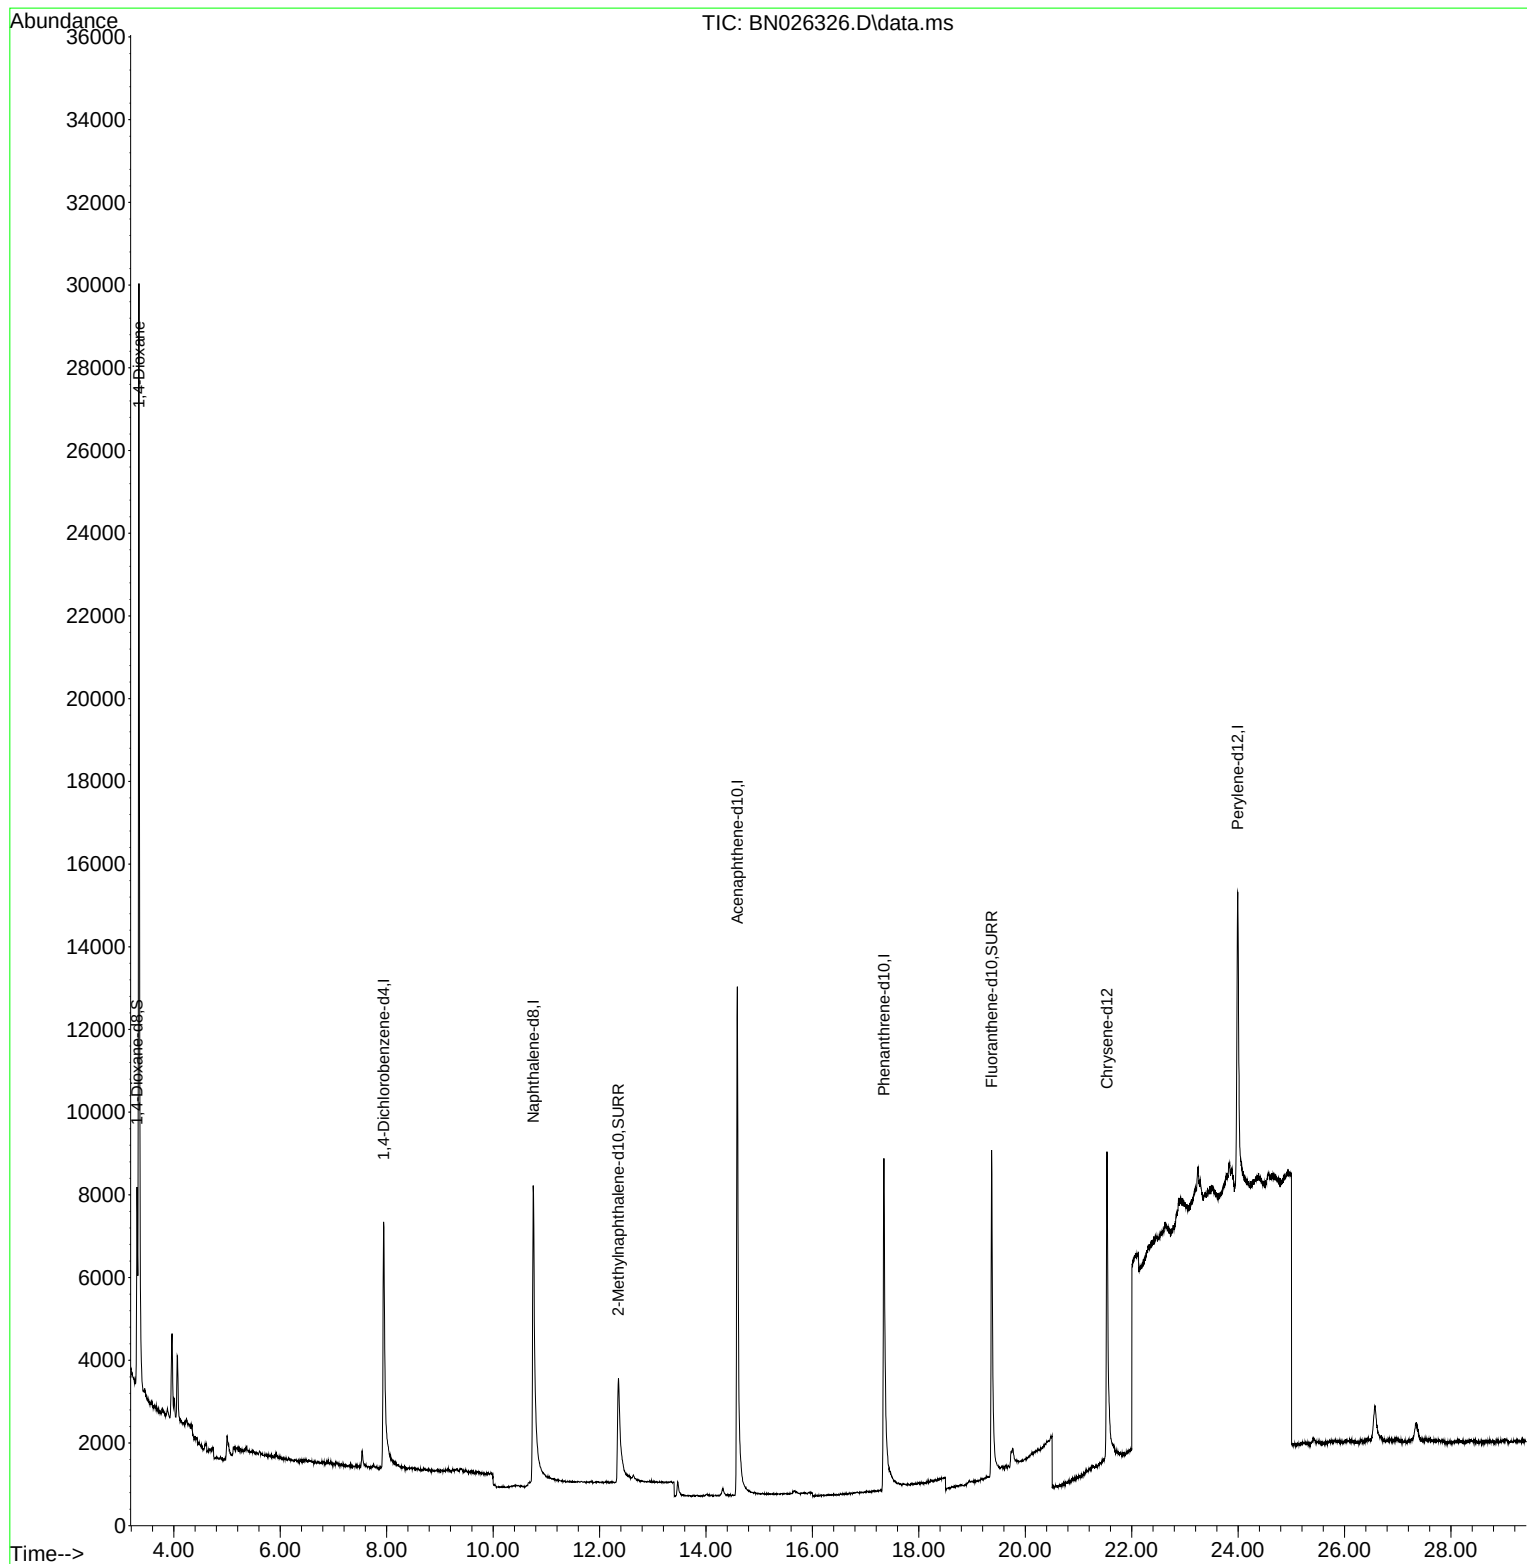

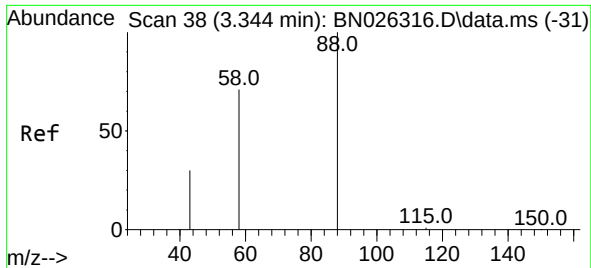

#2
 1,4-Dioxane
 Concen: 3.065 ng/ul
 RT: 3.343 min Scan# 31
 Delta R.T. -0.008 min
 Lab File: BN026326.D
 Acq: 06 Jul 2023 12:33

Instrument :
 BNA_N
 ClientSampleId :
 DCHB6

Tgt Ion: 88 Resp: 19581
 Ion Ratio Lower Upper
 88 100
 43 33.9 29.5 44.3
 58 64.0 37.4 56.2#

