

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
 Data File : BN026338.D
 Acq On : 06 Jul 2023 20:04
 Operator : MA/JU
 Sample : 03257-19
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW6

Quant Time: Jul 07 00:58:12 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 06 17:50:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	7107	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136	26849	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	15999	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.330	188	31229	0.400	ng/ul	0.00
17) Chrysene-d12	21.526	240	16585	0.400	ng/ul	0.00
23) Perylene-d12	23.981	264	20317	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.306	96	28812	3.600	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.337	152	10475	0.254	ng/ul	0.00
18) Fluoranthene-d10	19.359	212	22936	0.363	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.343	88	6085	0.716	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
Data File : BN026338.D
Acq On : 06 Jul 2023 20:04
Operator : MA/JU
Sample : 03257-19
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW6


Quant Time: Jul 07 00:58:12 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 06 17:50:03 2023
Response via : Initial Calibration

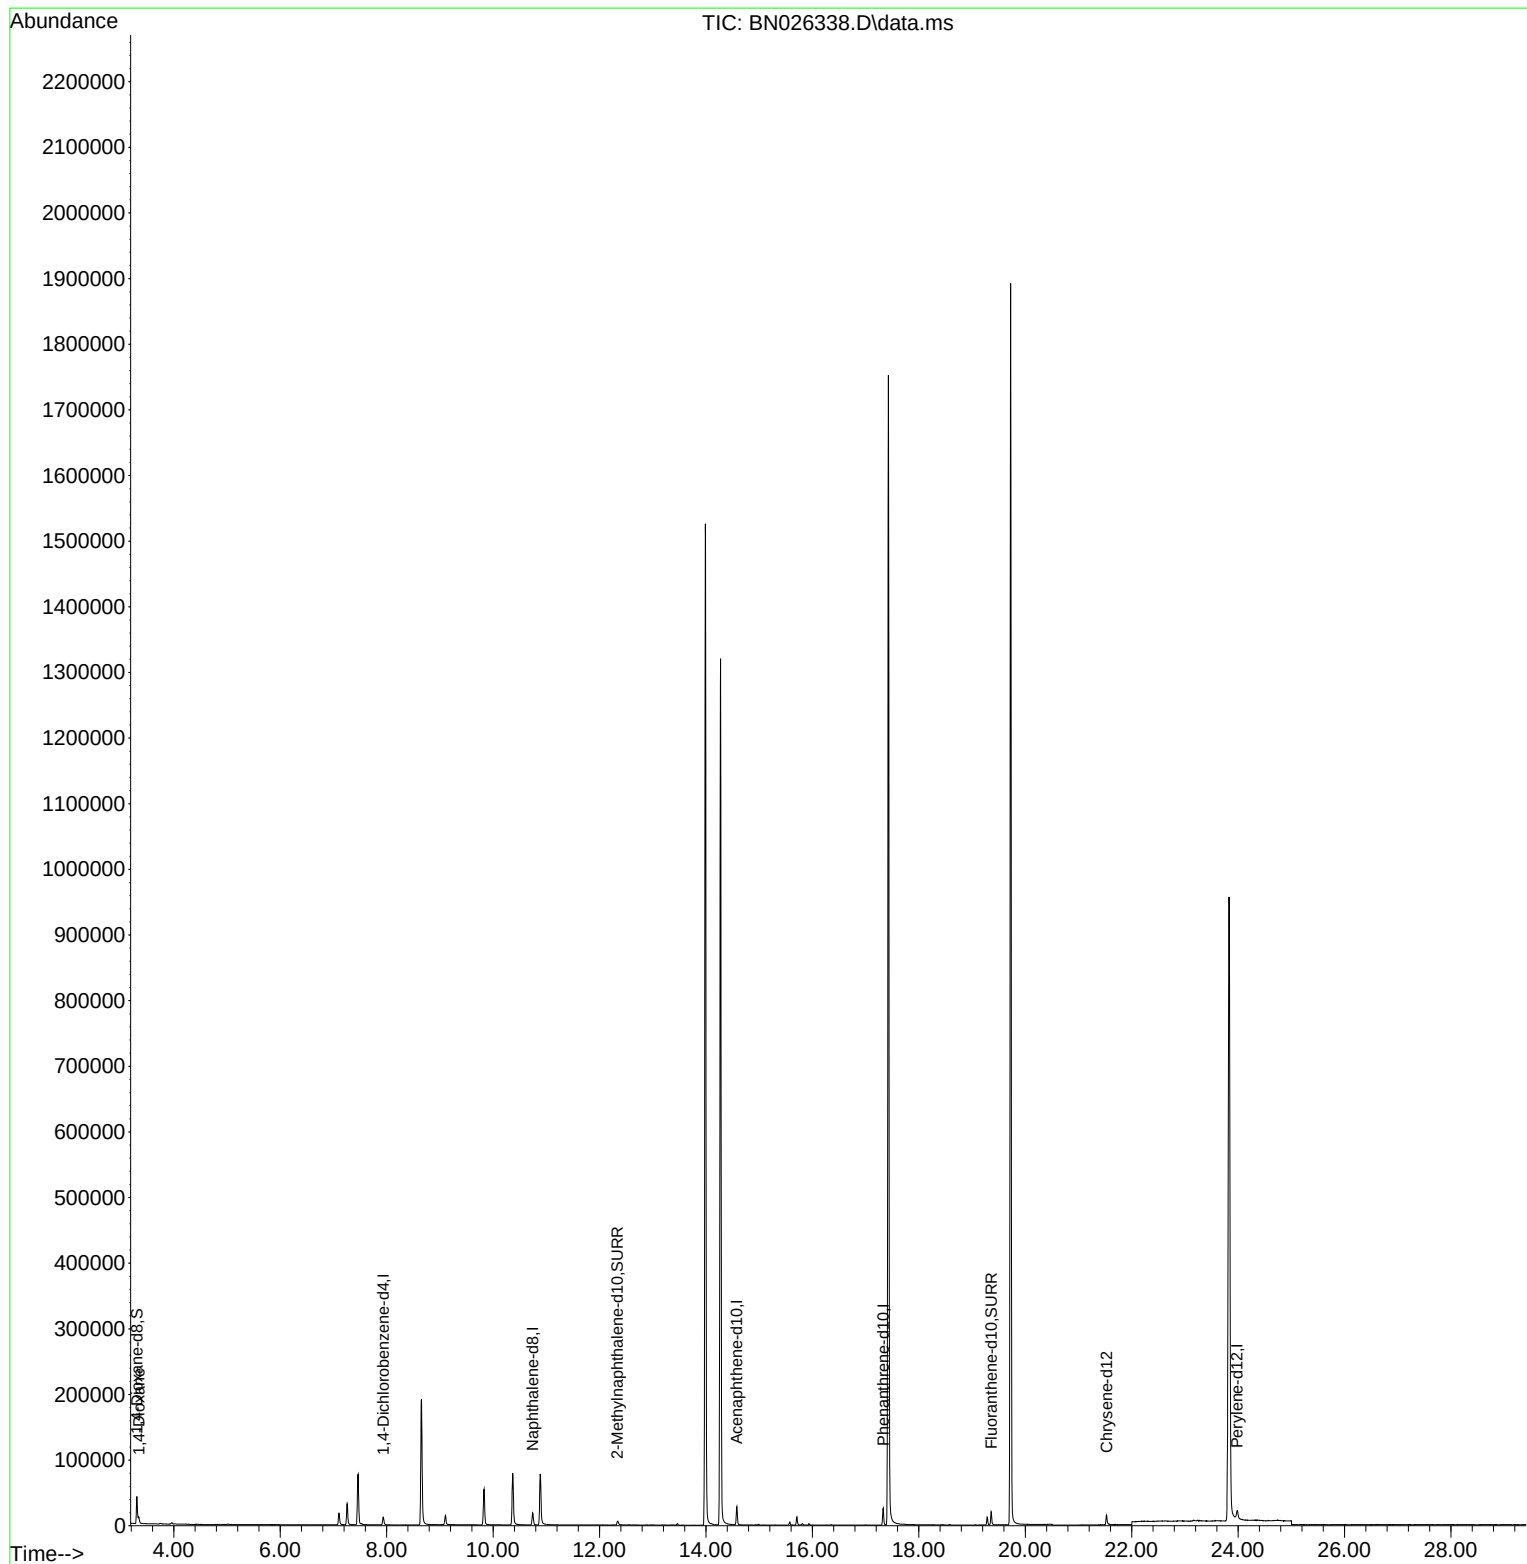

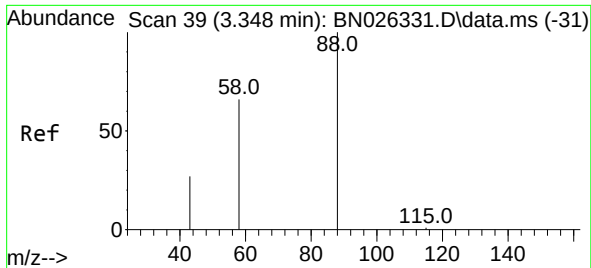

#2
 1,4-Dioxane
 Concen: 0.716 ng/ul
 RT: 3.343 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN026338.D
 Acq: 06 Jul 2023 20:04

Instrument :
 BNA_N
 ClientSampleId :
 EXYW6

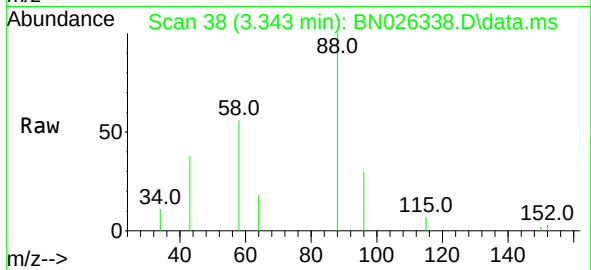

Tgt Ion: 88 Resp: 6085

Ion	Ratio	Lower	Upper
88	100		
43	38.0	29.5	44.3
58	55.8	37.4	56.2

