

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
 Data File : BN026339.D
 Acq On : 06 Jul 2023 20:42
 Operator : MA/JU
 Sample : 03257-20
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYW7

Quant Time: Jul 07 00:58:18 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 06 17:50:03 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	7244	0.400	ng/ul	0.00
4) Naphthalene-d8	10.743	136	28575	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.579	164	16681	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.330	188	31294	0.400	ng/ul	0.00
17) Chrysene-d12	21.529	240	15150	0.400	ng/ul	# 0.00
23) Perylene-d12	23.973	264	20439	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.306	96	26672	3.269	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.338	152	9287	0.211	ng/ul	0.00
18) Fluoranthene-d10	19.359	212	17984	0.312	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.344	88	1165	0.134	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070523\
Data File : BN026339.D
Acq On : 06 Jul 2023 20:42
Operator : MA/JU
Sample : 03257-20
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXYW7


Quant Time: Jul 07 00:58:18 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 06 17:50:03 2023
Response via : Initial Calibration

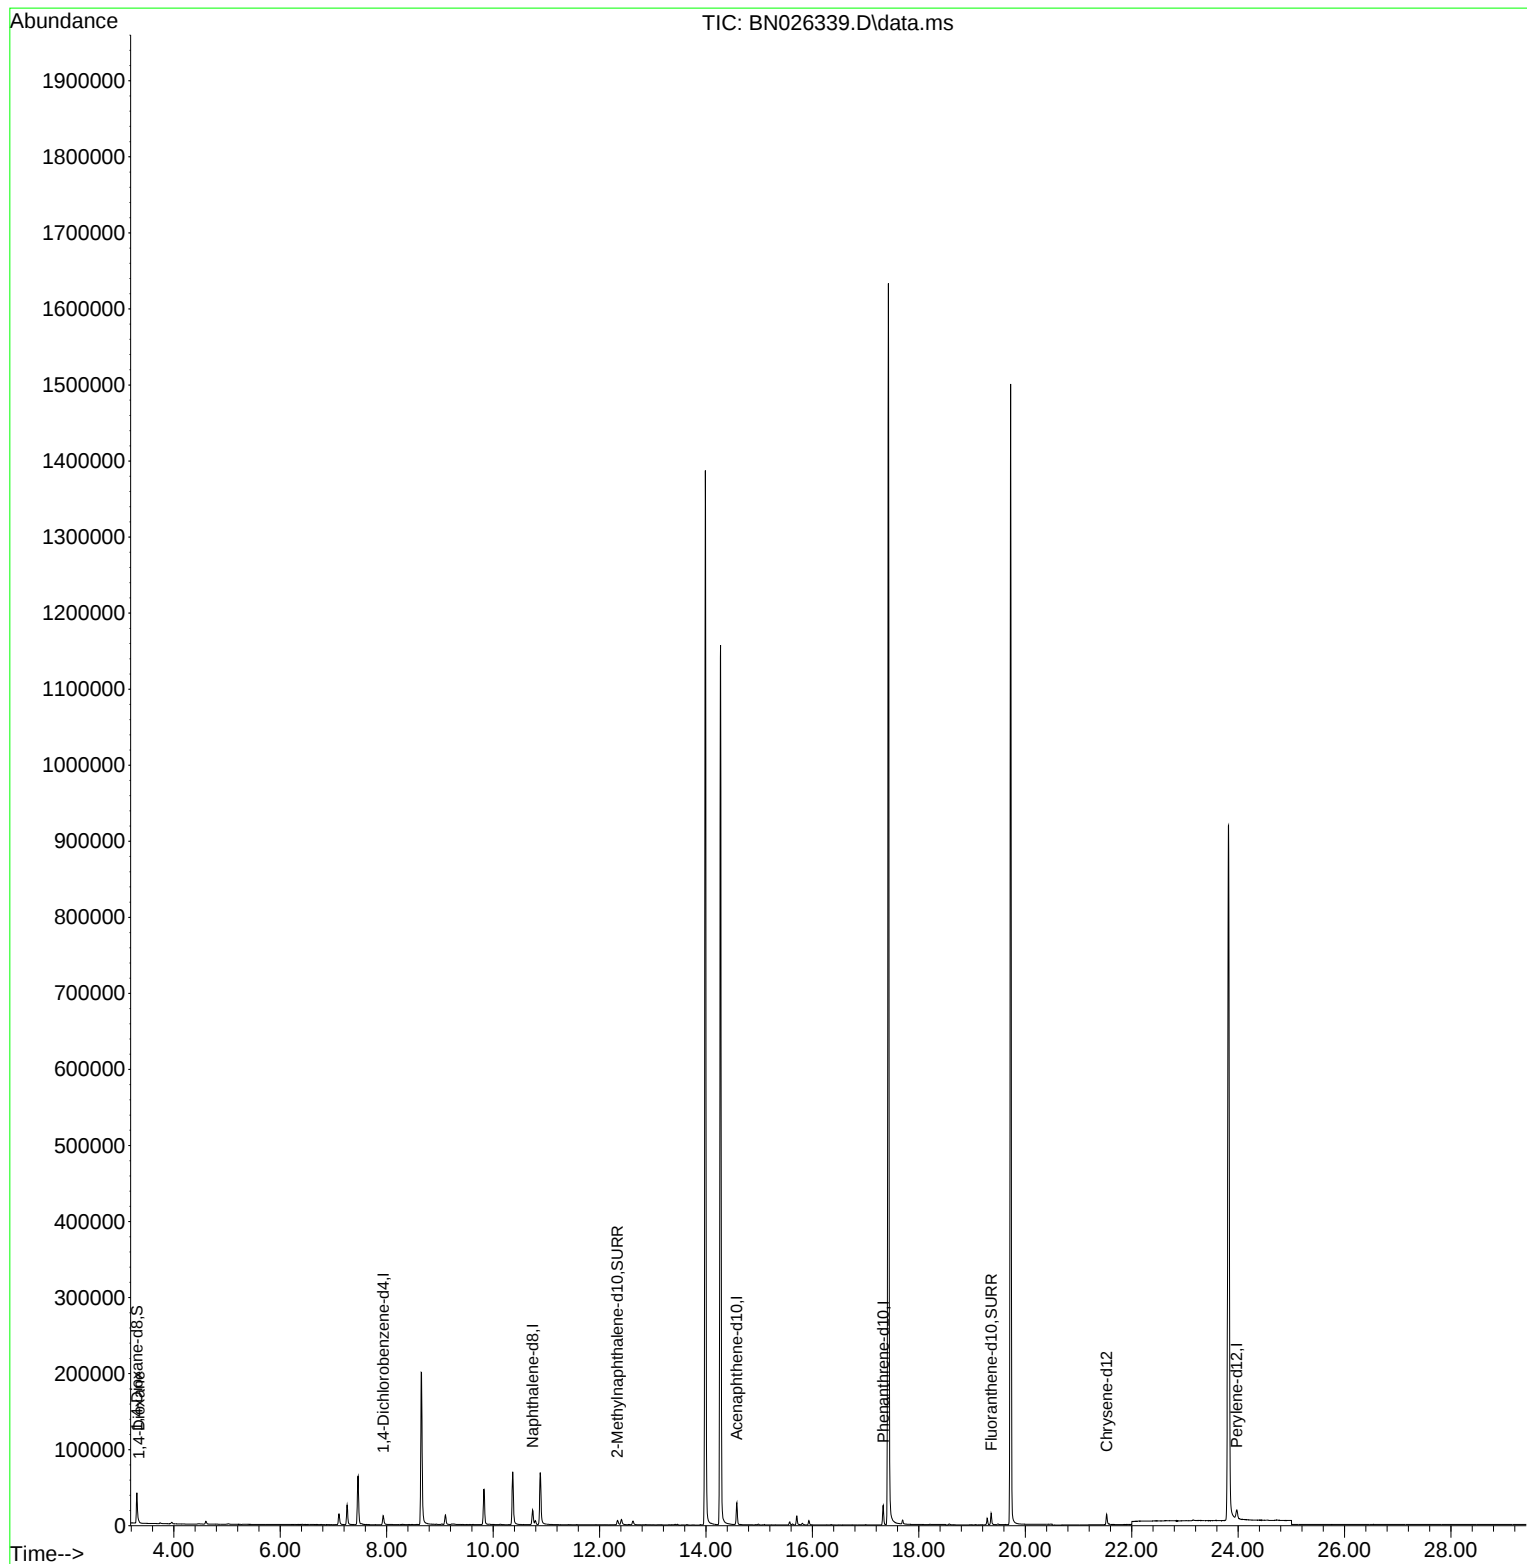

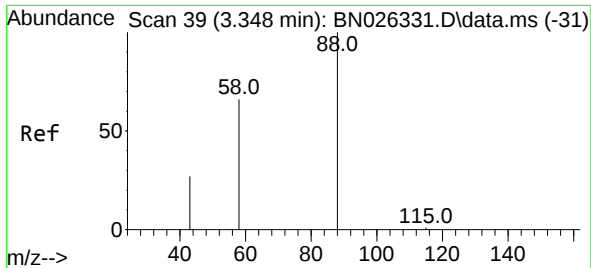

#2
 1,4-Dioxane
 Concen: 0.134 ng/ul
 RT: 3.344 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN026339.D
 Acq: 06 Jul 2023 20:42

Instrument :
 BNA_N
 ClientSampleId :
 EXYW7

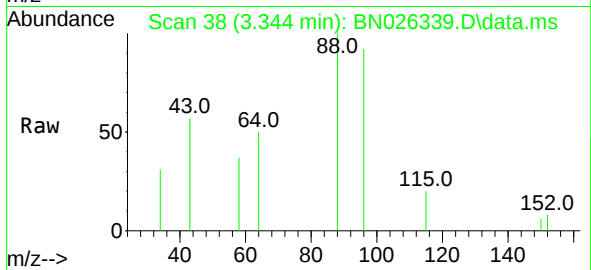

Tgt Ion: 88 Resp: 1165

Ion	Ratio	Lower	Upper
88	100		
43	57.5	29.5	44.3#
58	37.4	37.4	56.2#

