

Quantitation Report (QT Reviewed)


Instrument :
BNA_N
ClientSampled :
SBLK93

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN070618\
Data File : BN001982.D
Acq On : 06 Jul 2018 10:30
Operator : JU/SJ
Sample : PB110793BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Manual Integrations
APPROVED

Sohil
7/9/2018 2:09:07 PM

Quant Time: Jul 06 23:24:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 04 00:59:54 2018
Response via : Initial Calibration

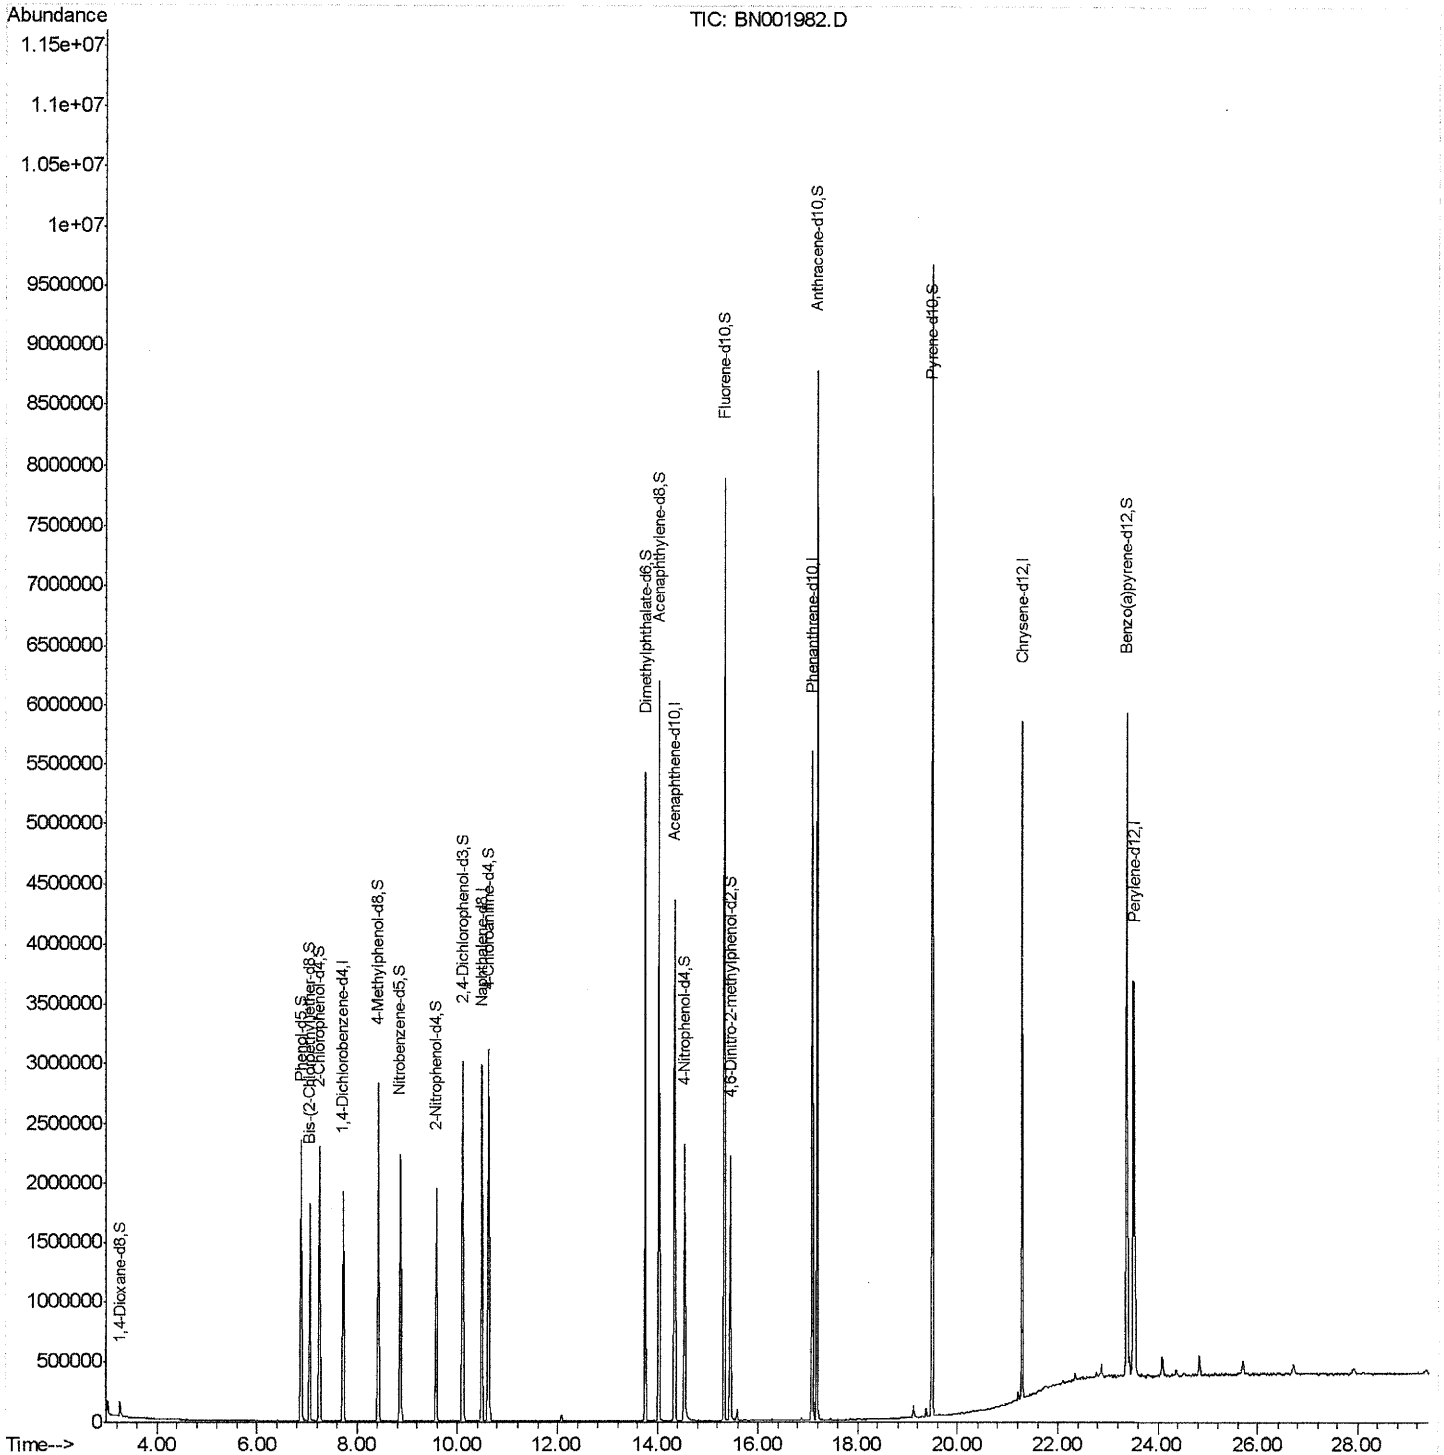

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN070618\
 Data File : BN001982.D
 Acq On : 06 Jul 2018 10:30
 Operator : JU/SJ
 Sample : PB110793BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 SBLK93

Manual Integrations
 APPROVED

Sohil
 7/9/2018 2:09:07 PM

Quant Time: Jul 06 23:07:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 04 00:59:54 2018
 Response via : Initial Calibration

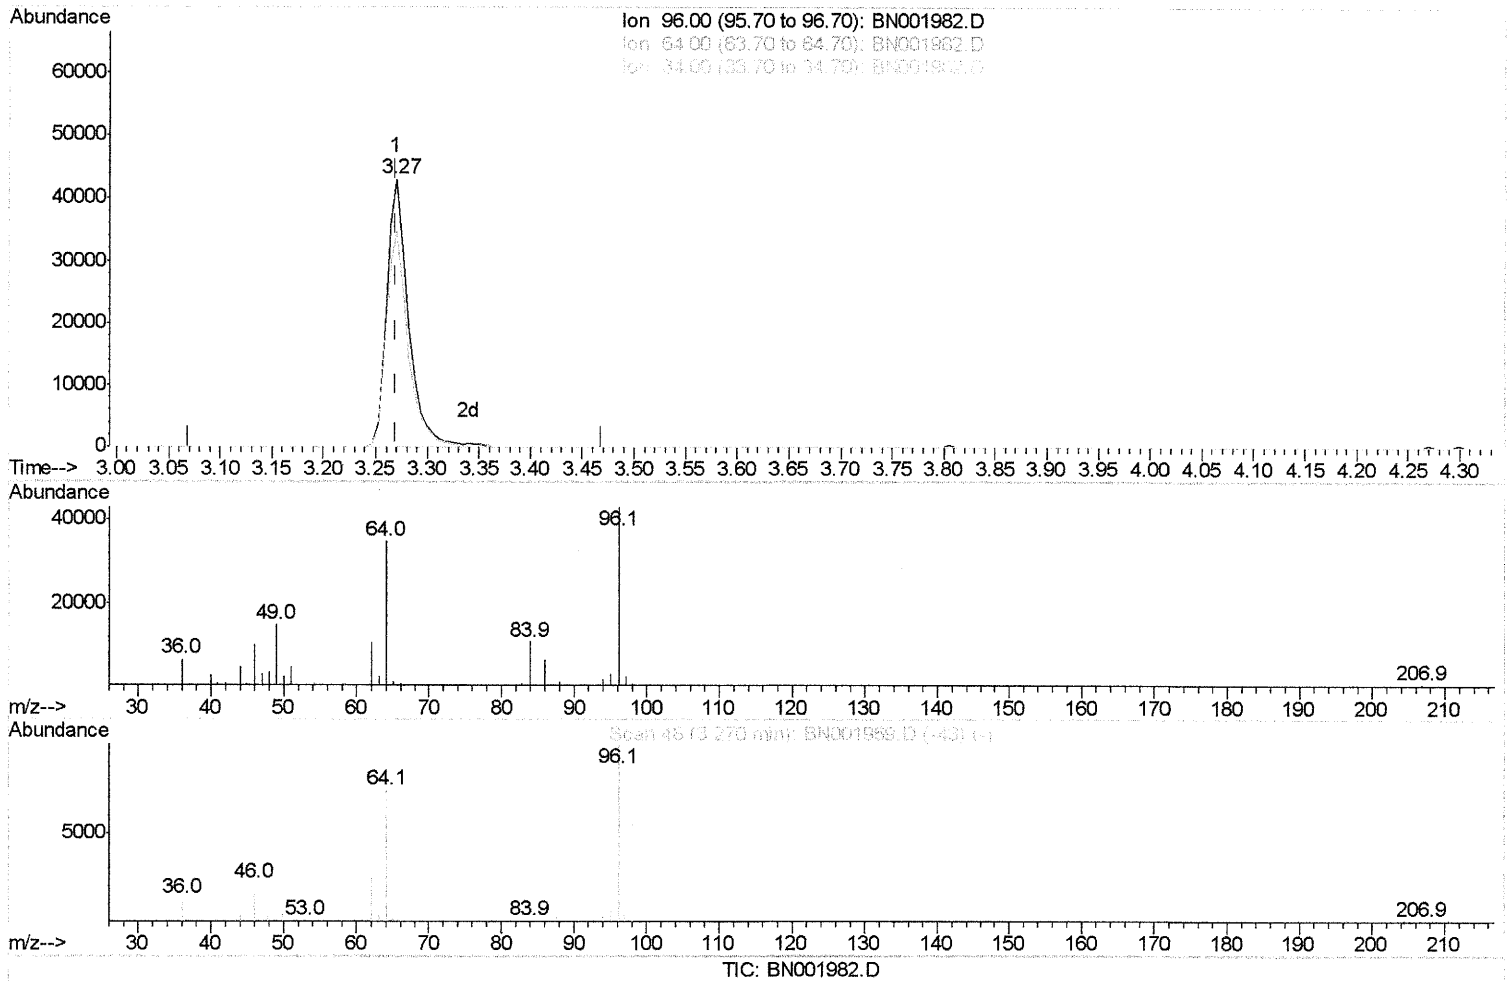

(3) 1,4-Dioxane-d8 (S)
 3.269min (+0.000) 5.14ng/uL
 response 62415

Ion	Exp%	Act%
96.00	100	100
64.00	74.00	80.80
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN070618\
 Data File : BN001982.D
 Acq On : 06 Jul 2018 10:30
 Operator : JU/SJ
 Sample : PB110793BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 SBLK93

Manual Integrations
 APPROVED

Sohil
 7/9/2018 2:09:07 PM

Quant Time: Jul 06 23:07:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 04 00:59:54 2018
 Response via : Initial Calibration

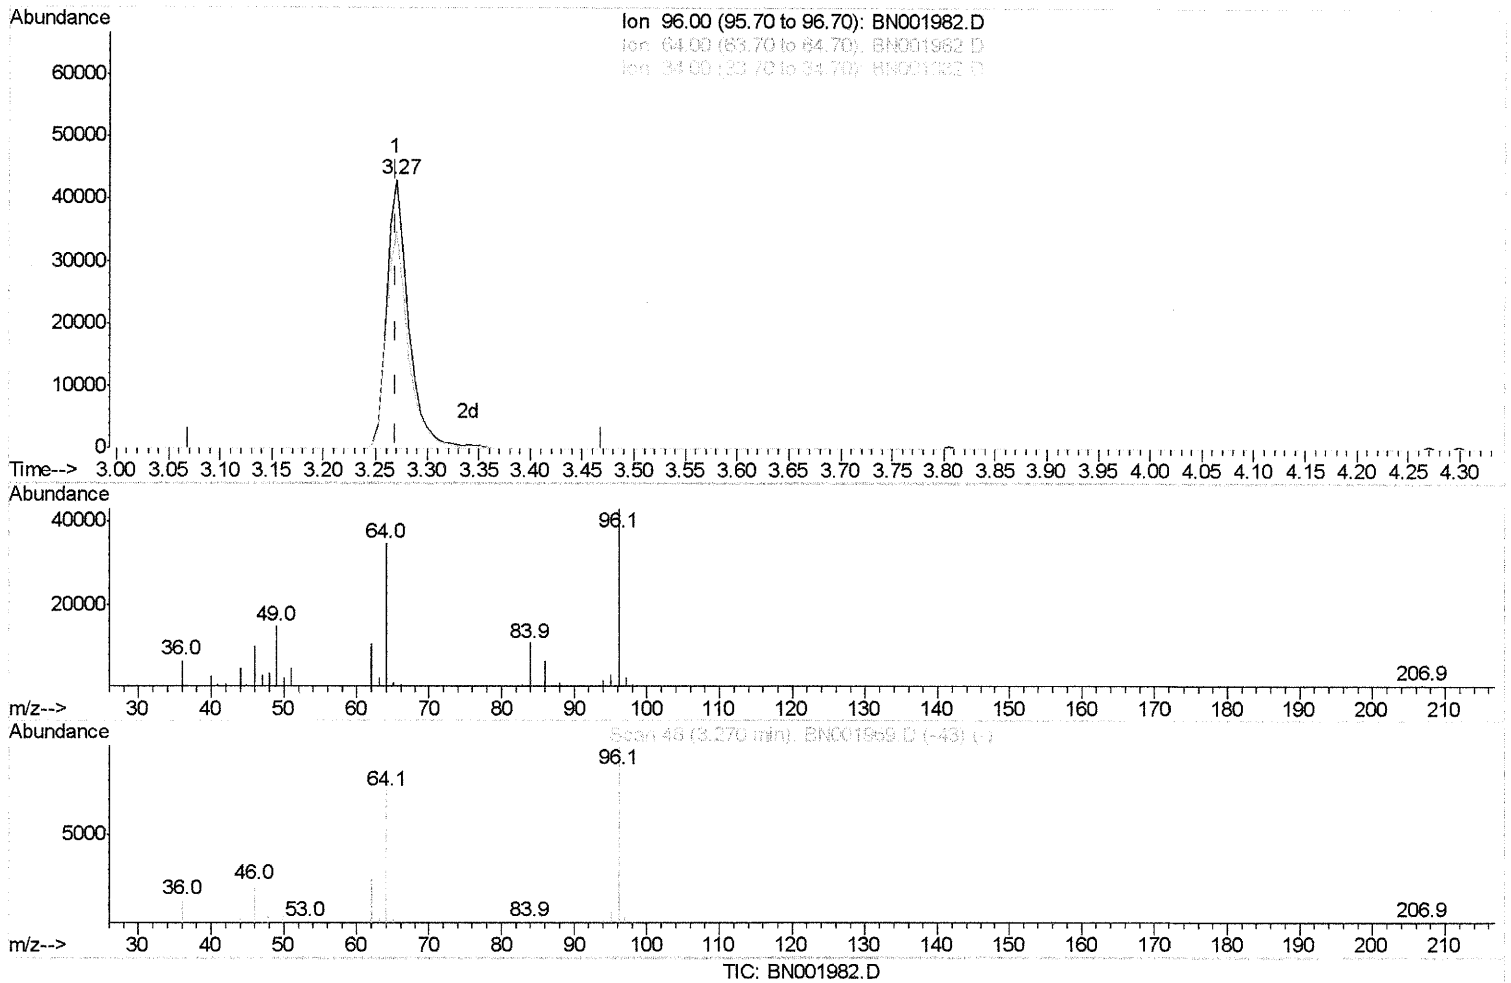

(3) 1,4-Dioxane-d8 (S)

3.269min (+0.000) 5.19ng/uL m

SJ 7/9/18

response 62965

Ion	Exp%	Act%
96.00	100	100
64.00	74.00	80.80
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN070618\
 Data File : BN001982.D
 Acq On : 06 Jul 2018 10:30
 Operator : JU/SJ
 Sample : PB110793BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK93

Manual Integrations
 APPROVED

Sohil
 7/9/2018 2:09:07 PM

Quant Time: Jul 06 23:24:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN061918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 04 00:59:54 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	526880	20.00	ng/ul	0.00
18) Naphthalene-d8	10.48	136	2448601	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.33	164	1458695	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.08	188	3182698	20.00	ng/ul	0.00
75) Chrysene-d12	21.28	240	2599948	20.00	ng/ul	0.00
83) Perylene-d12	23.51	264	2291288	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.27	96	62965m	5.19	ng/uL	0.00
5) Phenol-d5	6.88	99	1329340	27.88	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.05	67	847869	28.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.25	132	1054083	27.88	ng/ul	0.00
13) 4-Methylphenol-d8	8.41	113	1086339	28.44	ng/ul	0.00
19) Nitrobenzene-d5	8.85	128	557148	30.64	ng/ul	0.00
22) 2-Nitrophenol-d4	9.57	143	624282	33.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.10	165	1099107	27.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.62	131	1644363	39.53	ng/ul	0.00
43) Dimethylphthalate-d6	13.75	166	3578490	29.05	ng/ul	0.00
46) Acenaphthylene-d8	14.03	160	4426829	29.11	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	584961	25.78	ng/ul	0.00
57) Fluorene-d10	15.33	176	3116121	28.86	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.45	200	448506	25.87	ng/ul	0.00
70) Anthracene-d10	17.18	188	4769034	31.01	ng/ul	0.00
76) Pyrene-d10	19.48	212	4732782	36.11	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.37	264	3946384	31.67	ng/ul	0.00

5/7/9/18

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed