

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
 Data File : BN026369.D
 Acq On : 07 Jul 2023 21:56
 Operator : MA/JU
 Sample : 03237-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW77

Quant Time: Jul 08 04:47:06 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 14:46:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	5850	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.736	136	20272	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.574	164	12845	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.321	188	23009	0.400	ng/ul	-0.01
17) Chrysene-d12	21.522	240	13373	0.400	ng/ul	0.00
23) Perylene-d12	23.963	264	17599	0.400	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	22812	3.463	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.336	152	7506	0.241	ng/ul	0.00
18) Fluoranthene-d10	19.353	212	16804	0.330	ng/ul	-0.01
Target Compounds						
					Qvalue	
20) Pyrene	19.720	202	3137	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.802	252	5216	0.080	ng/ul#	30


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
Data File : BN026369.D
Acq On : 07 Jul 2023 21:56
Operator : MA/JU
Sample : 03237-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YBW77

Quant Time: Jul 08 04:47:06 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 14:46:07 2023
Response via : Initial Calibration




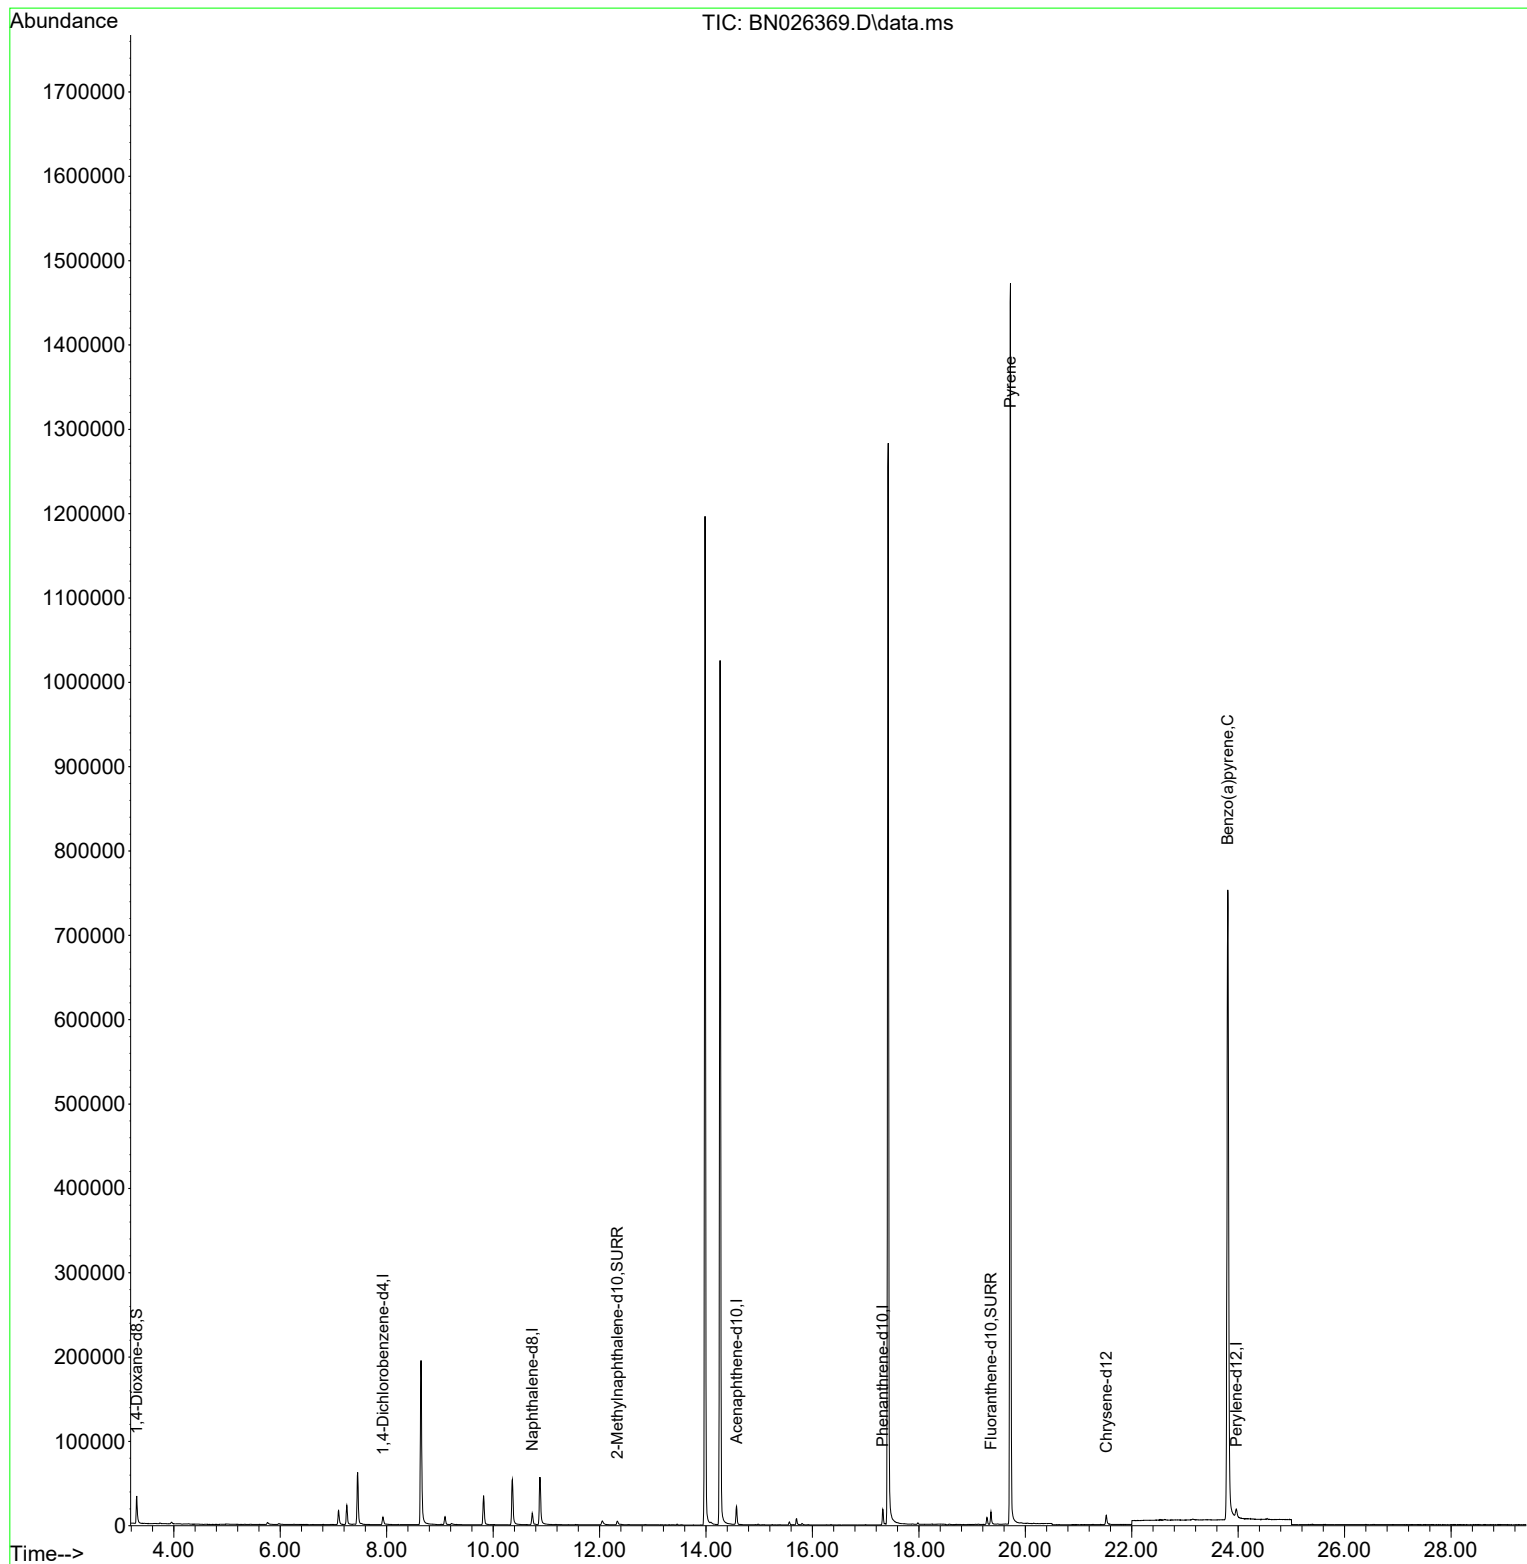


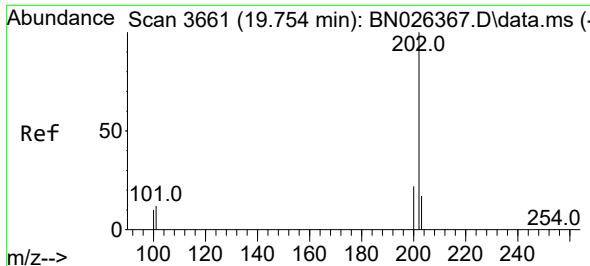

#20
Pyrene
Concen: 0.042 ng/ul
RT: 19.720 min Scan# 3137
Delta R.T. -0.038 min
Lab File: BN026369.D
Acq: 07 Jul 2023 21:56

Instrument :
BNA_N
ClientSampleId :
YBW77

Tgt Ion:202 Resp: 3137
Ion Ratio Lower Upper
202 100
101 170.3 11.4 17.0#
100 1261.5 9.1 13.7#

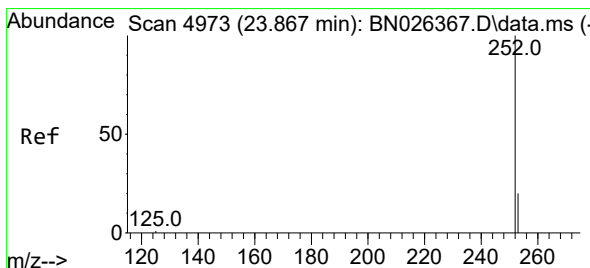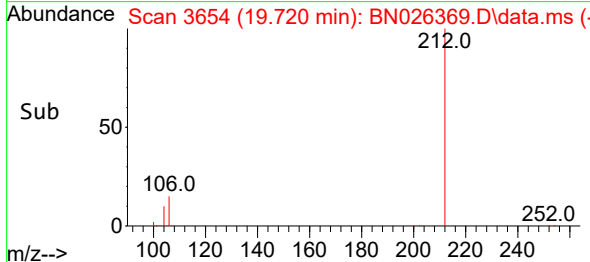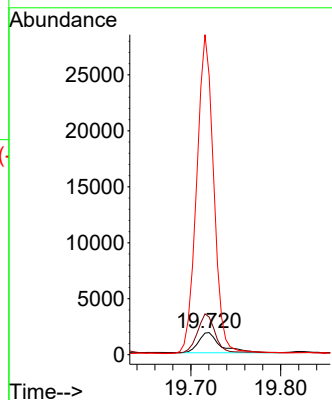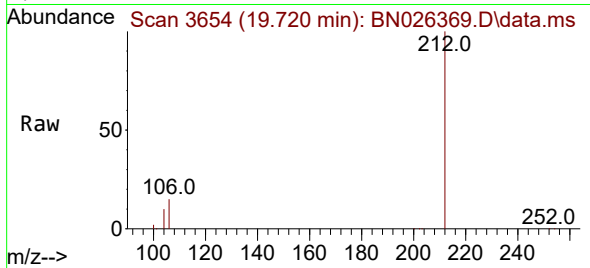

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.802 min Scan# 4951
Delta R.T. -0.083 min
Lab File: BN026369.D
Acq: 07 Jul 2023 21:56

Tgt Ion:252 Resp: 5216
Ion Ratio Lower Upper
252 100
253 61.2 26.0 39.0#
125 67.8 17.3 25.9#

