

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
 Data File : BN026372.D
 Acq On : 07 Jul 2023 23:49
 Operator : MA/JU
 Sample : 03237-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW78

Quant Time: Jul 08 04:47:34 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 14:46:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.933	152	5419	0.400	ng/ul	0.00
4) Naphthalene-d8	10.737	136	17850	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.574	164	11029	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.325	188	18400	0.400	ng/ul	0.00
17) Chrysene-d12	21.525	240	10579	0.400	ng/ul	0.00
23) Perylene-d12	23.972	264	15298	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	22687	3.718	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	6863	0.250	ng/ul	-0.01
18) Fluoranthene-d10	19.358	212	10583	0.263	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.720	202	2052	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.817	252	4032	0.071	ng/ul#	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
Data File : BN026372.D
Acq On : 07 Jul 2023 23:49
Operator : MA/JU
Sample : 03237-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YBW78

Quant Time: Jul 08 04:47:34 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 14:46:07 2023
Response via : Initial Calibration

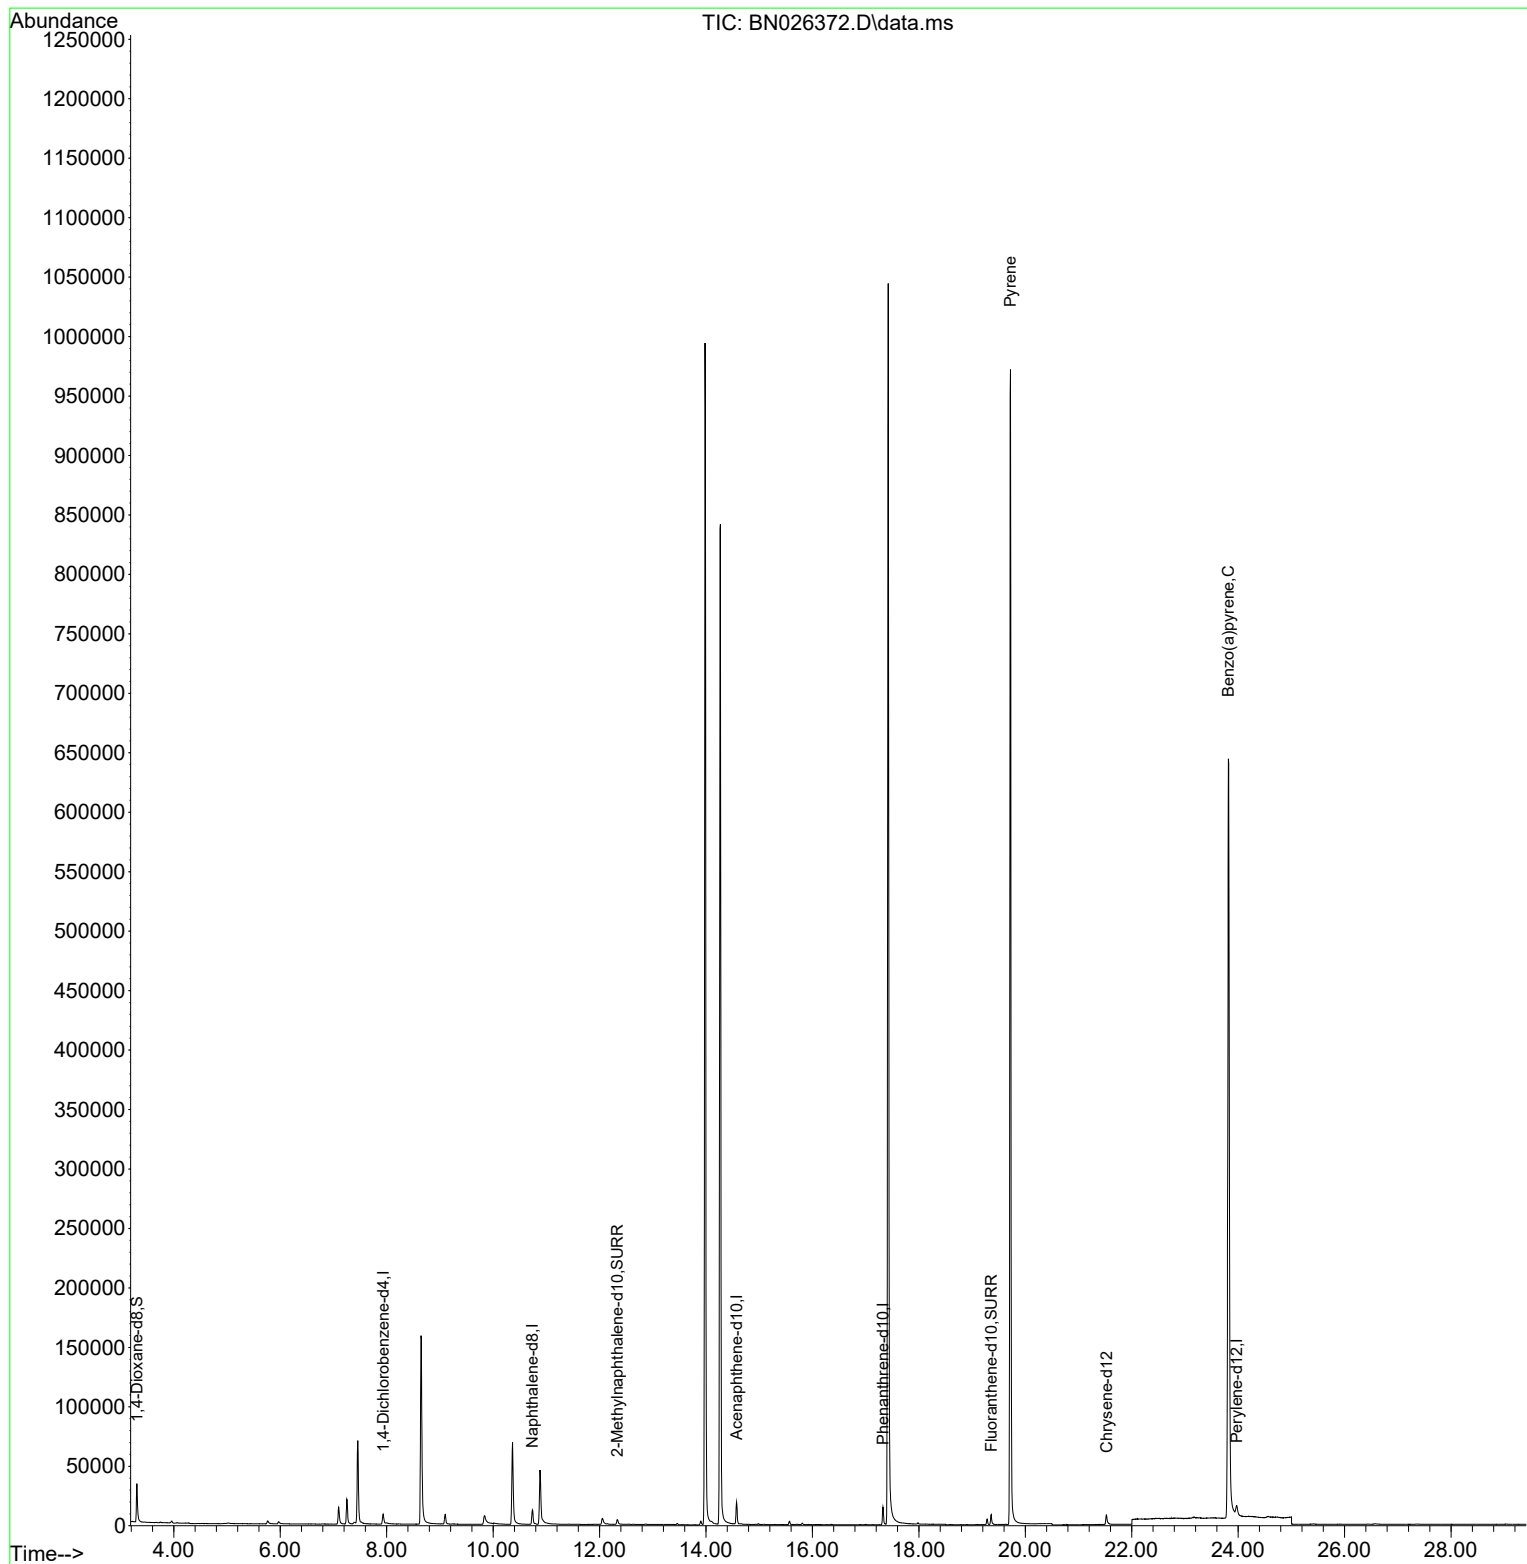

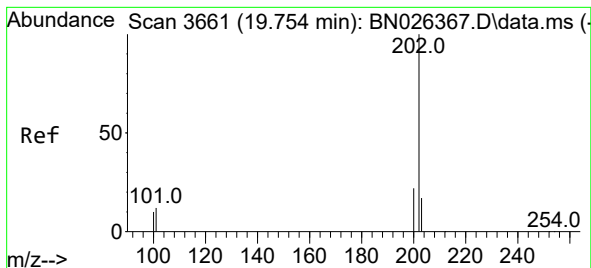

#20

Pyrene

Concen: 0.035 ng/ul

RT: 19.720 min Scan# 3

Delta R.T. -0.038 min

Lab File: BN026372.D

Acq: 07 Jul 2023 23:49

Instrument :

BNA_N

ClientSampleId :

YBW78





Tgt Ion:202 Resp: 2052

Ion Ratio Lower Upper

202 100

101 186.8 11.4 17.0#

100 1423.6 9.1 13.7#

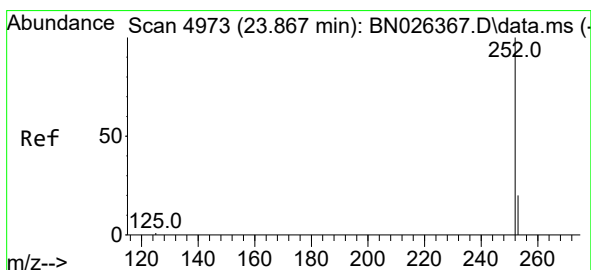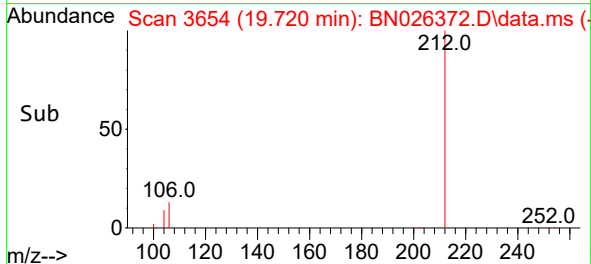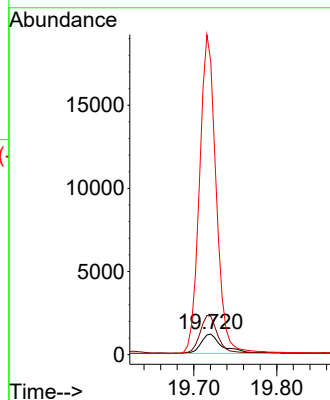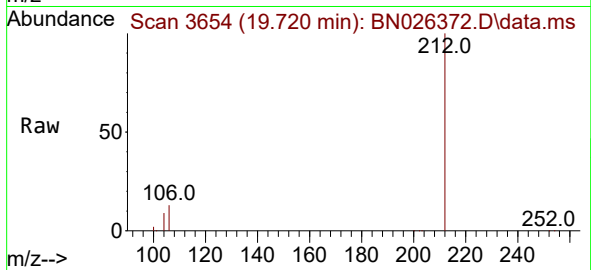

#26

Benzo(a)pyrene

Concen: 0.071 ng/ul

RT: 23.817 min Scan# 4956

Delta R.T. -0.068 min

Lab File: BN026372.D

Acq: 07 Jul 2023 23:49

Tgt Ion:252 Resp: 4032

Ion Ratio Lower Upper

252 100

253 62.3 26.0 39.0#

125 70.1 17.3 25.9#

