

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
 Data File : BN026373.D
 Acq On : 08 Jul 2023 00:27
 Operator : MA/JU
 Sample : 03237-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW79

Quant Time: Jul 08 04:47:40 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 14:46:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	3834	0.400	ng/ul	0.00
4) Naphthalene-d8	10.736	136	16941	0.400	ng/ul	#-0.01
9) Acenaphthene-d10	14.574	164	10732	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.325	188	18837	0.400	ng/ul	0.00
17) Chrysene-d12	21.519	240	10272	0.400	ng/ul	0.00
23) Perylene-d12	23.972	264	14009	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	18095	4.191	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.336	152	6942	0.266	ng/ul	0.00
18) Fluoranthene-d10	19.353	212	13858	0.354	ng/ul	-0.01
Target Compounds						
					Qvalue	
11) Acenaphthene	14.648	153	2845	0.069	ng/ul#	25
20) Pyrene	19.720	202	2553	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.808	252	4154	0.080	ng/ul#	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
Data File : BN026373.D
Acq On : 08 Jul 2023 00:27
Operator : MA/JU
Sample : 03237-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YBW79

Quant Time: Jul 08 04:47:40 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 14:46:07 2023
Response via : Initial Calibration




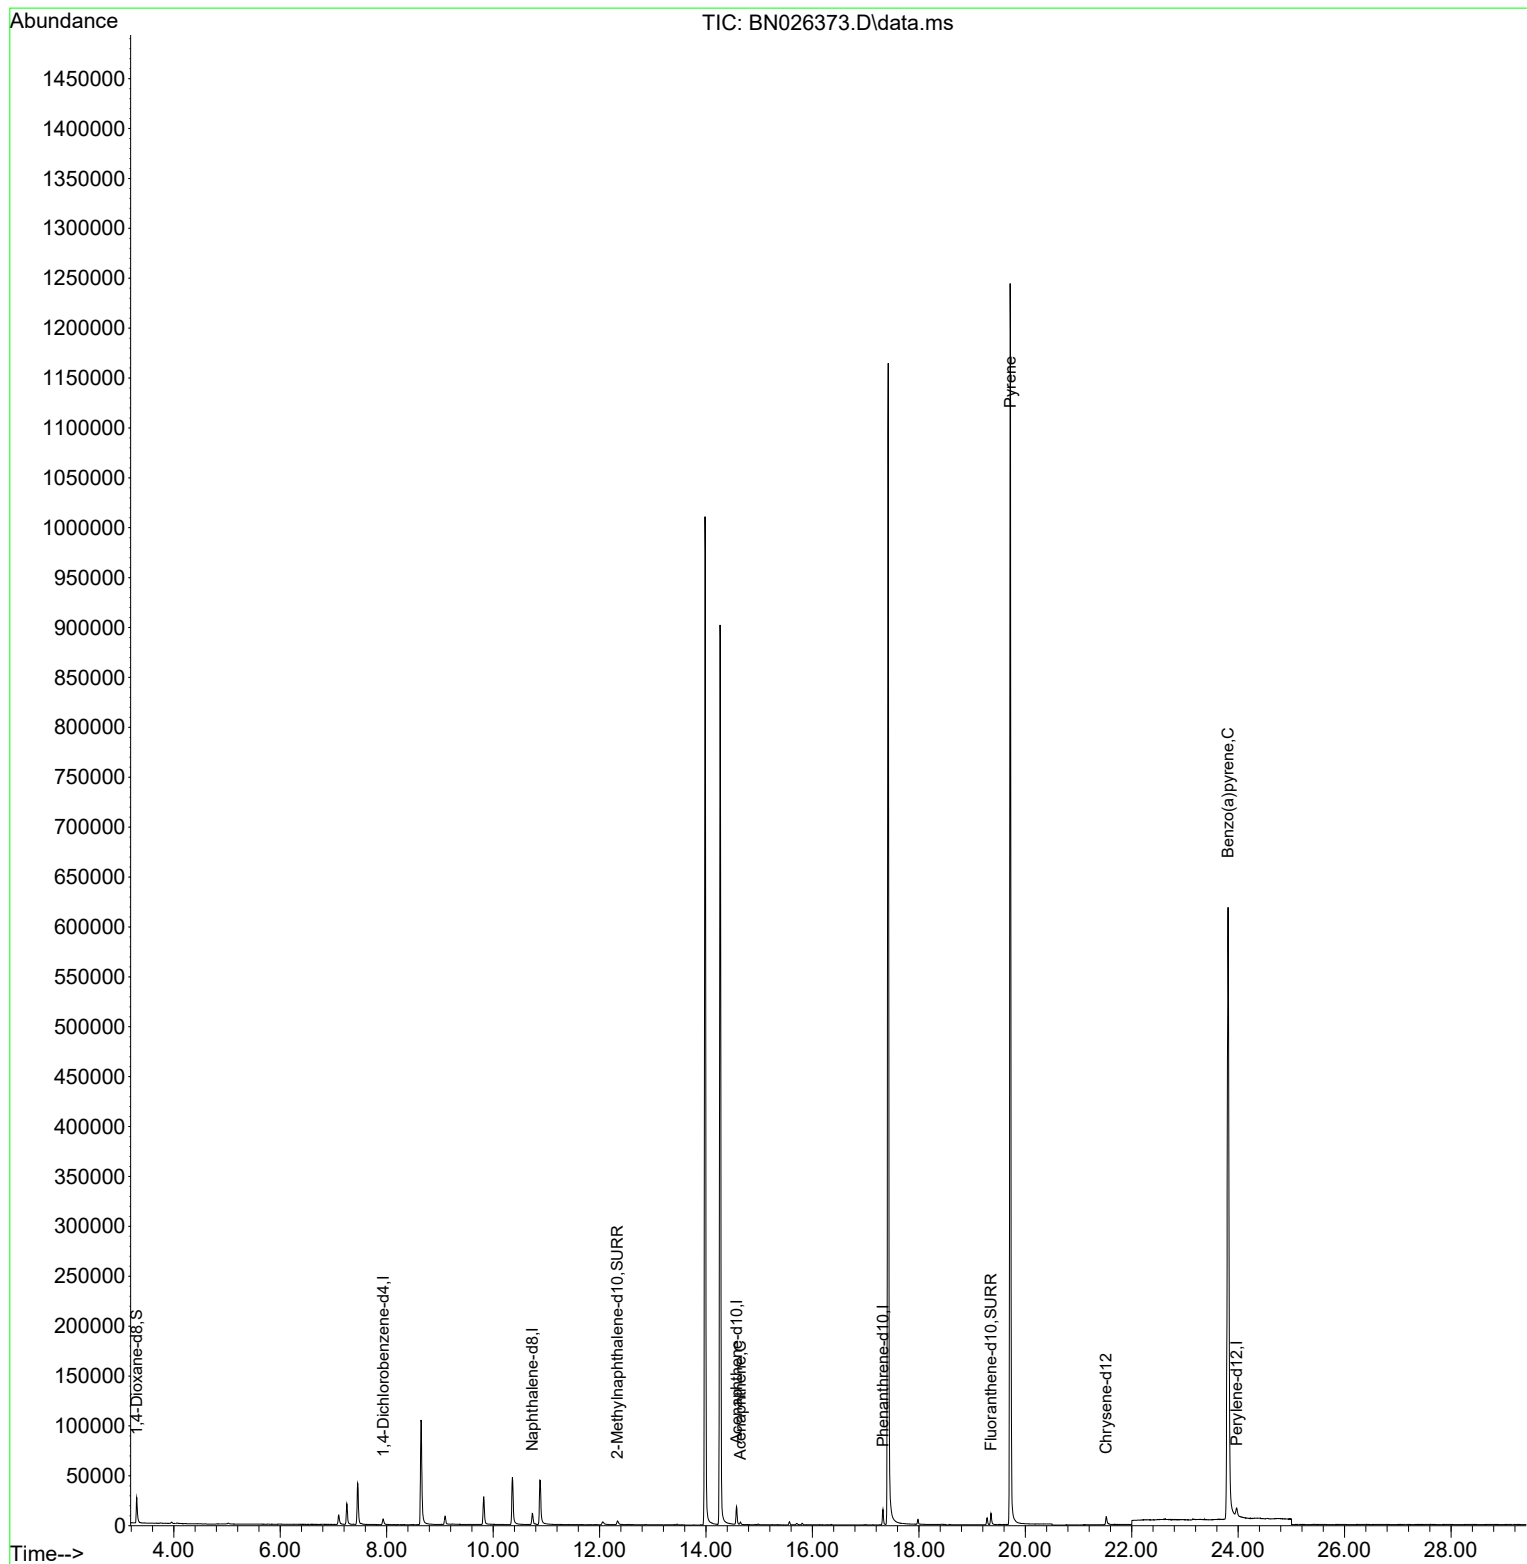


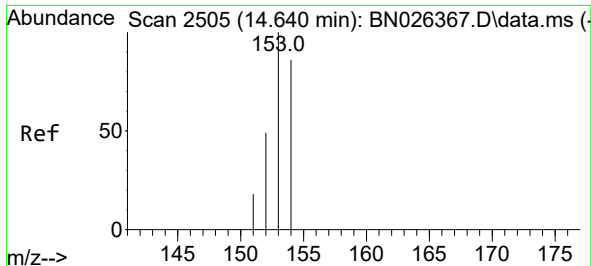

#11
Acenaphthene
Concen: 0.069 ng/ul
RT: 14.648 min Scan# 21
Delta R.T. 0.004 min
Lab File: BN026373.D
Acq: 08 Jul 2023 00:27




Instrument :
BNA_N
ClientSampleId :
YBW79


Tgt Ion:153 Resp: 2845
Ion Ratio Lower Upper
153 100
152 4.5 39.4 59.0#
154 12.5 68.9 103.3#

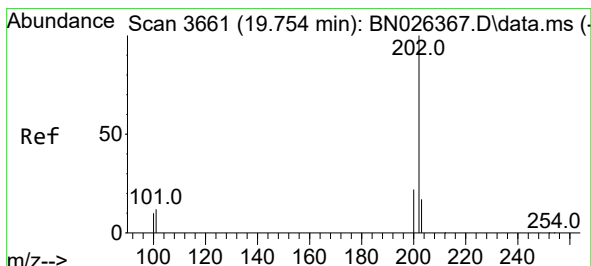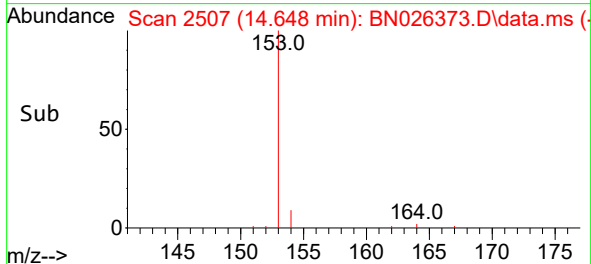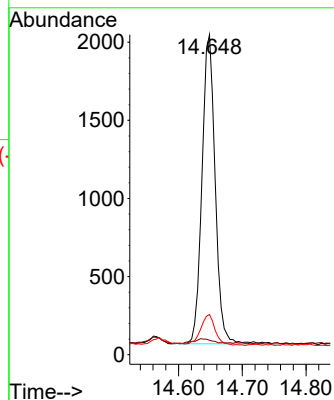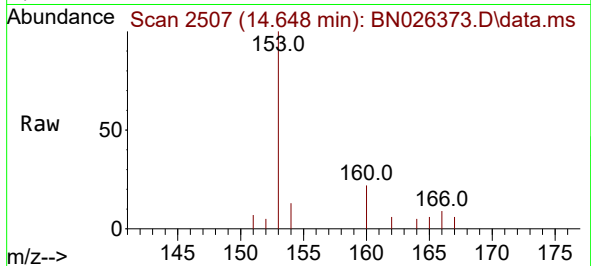

#20
Pyrene
Concen: 0.045 ng/ul
RT: 19.720 min Scan# 3654
Delta R.T. -0.038 min
Lab File: BN026373.D
Acq: 08 Jul 2023 00:27


Tgt Ion:202 Resp: 2553
Ion Ratio Lower Upper
202 100
101 176.1 11.4 17.0#
100 1300.9 9.1 13.7#

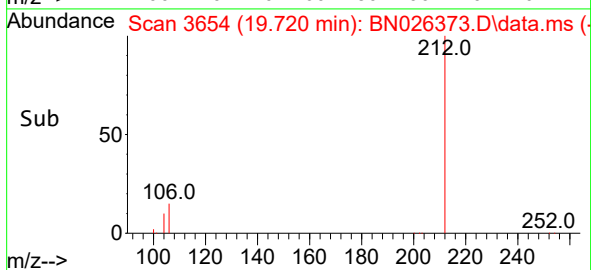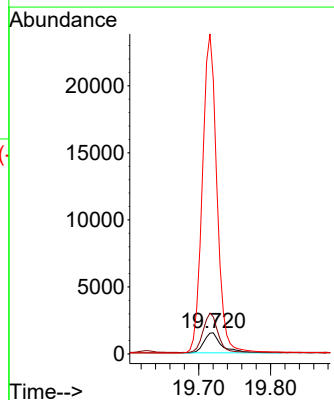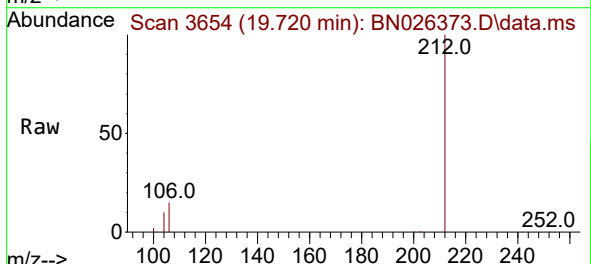

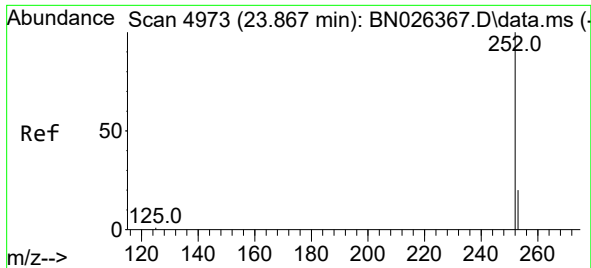

#26
Benzo(a)pyrene
Concen: 0.080 ng/ul
RT: 23.808 min Scan# 4953
Delta R.T. -0.077 min
Lab File: BN026373.D
Acq: 08 Jul 2023 00:27

Instrument :
BNA_N
ClientSampleId :
YBW79

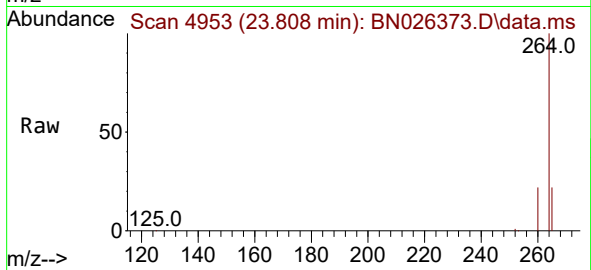

Tgt Ion:252 Resp: 4154
Ion Ratio Lower Upper
252 100
253 64.2 26.0 39.0#
125 68.4 17.3 25.9#

