

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
 Data File : BN026360.D
 Acq On : 07 Jul 2023 15:45
 Operator : MA/JU
 Sample : 03283-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXYX3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/07/2023
 Supervised By :Sohil Jodhani 07/07/2023

Quant Time: Jul 07 16:38:02 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 14:46:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.929	152	5267	0.400	ng/ul	# 0.00
4) Naphthalene-d8	10.741	136	15873	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.602	164	27459	0.400	ng/ul	# 0.03
13) Phenanthrene-d10	17.325	188	25040m	0.400	ng/ul	0.00
17) Chrysene-d12	21.528	240	13686	0.400	ng/ul	0.00
23) Perylene-d12	23.983	264	16306	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	20855	3.516	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.331	152	7852	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.358	212	16811	0.323	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.335	88	172768	27.432	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
Data File : BN026360.D
Acq On : 07 Jul 2023 15:45
Operator : MA/JU
Sample : 03283-07
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
EXYX3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/07/2023
Supervised By :Sohil Jodhani 07/07/2023


Quant Time: Jul 07 16:38:02 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 14:46:07 2023
Response via : Initial Calibration

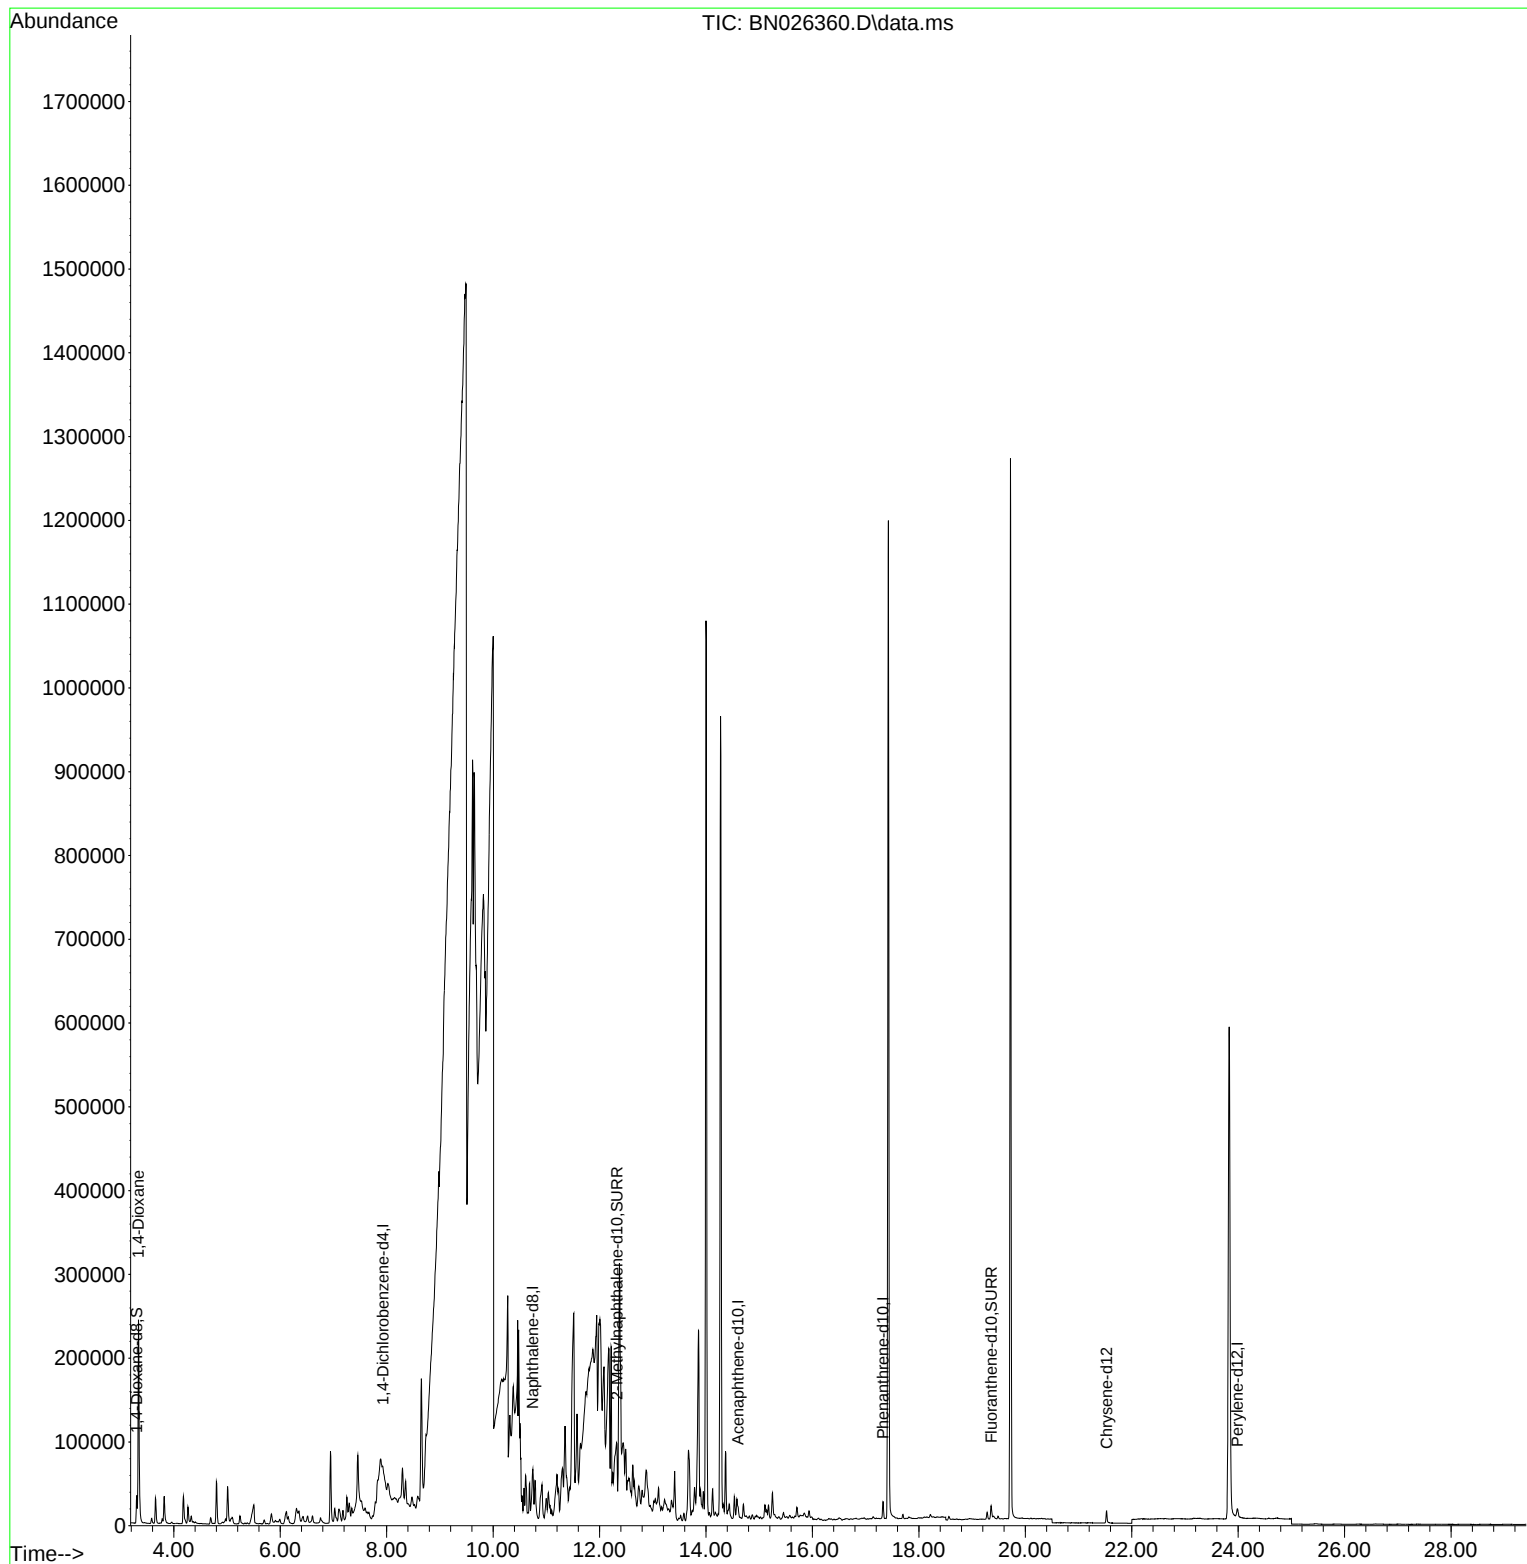

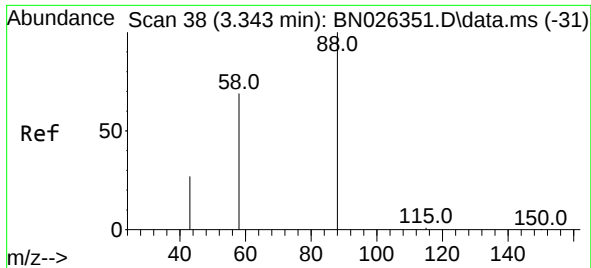

#2
 1,4-Dioxane
 Concen: 27.432 ng/ul
 RT: 3.335 min Scan# 30
 Delta R.T. -0.009 min
 Lab File: BN026360.D
 Acq: 07 Jul 2023 15:45

Instrument :
 BNA_N
 ClientSampleId :
 EXYX3

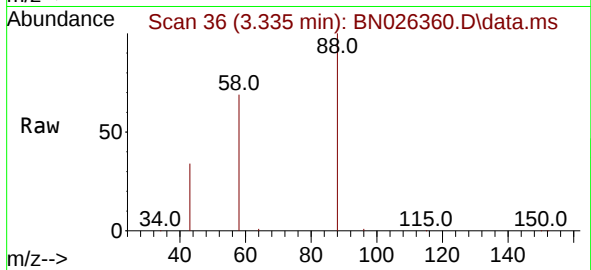

Tgt Ion: 88 Resp: 172768
 Ion Ratio Lower Upper
 88 100
 43 34.2 29.5 44.3
 58 69.0 37.4 56.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/07/2023
 Supervised By :Sohil Jodhani 07/07/2023

