

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
 Data File : BN026361.D
 Acq On : 07 Jul 2023 16:22
 Operator : MA/JU
 Sample : 03284-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCGZ3

Quant Time: Jul 07 17:24:19 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 14:46:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	5674	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.737	136	19353	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.575	164	11648	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.326	188	21881	0.400	ng/ul	0.00
17) Chrysene-d12	21.529	240	12293	0.400	ng/ul	0.00
23) Perylene-d12	23.973	264	15841	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.306	96	23493	3.677	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	7621	0.256	ng/ul	-0.01
18) Fluoranthene-d10	19.359	212	18326	0.392	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.339	88	382	0.056	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
Data File : BN026361.D
Acq On : 07 Jul 2023 16:22
Operator : MA/JU
Sample : 03284-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCGZ3

Quant Time: Jul 07 17:24:19 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 14:46:07 2023
Response via : Initial Calibration

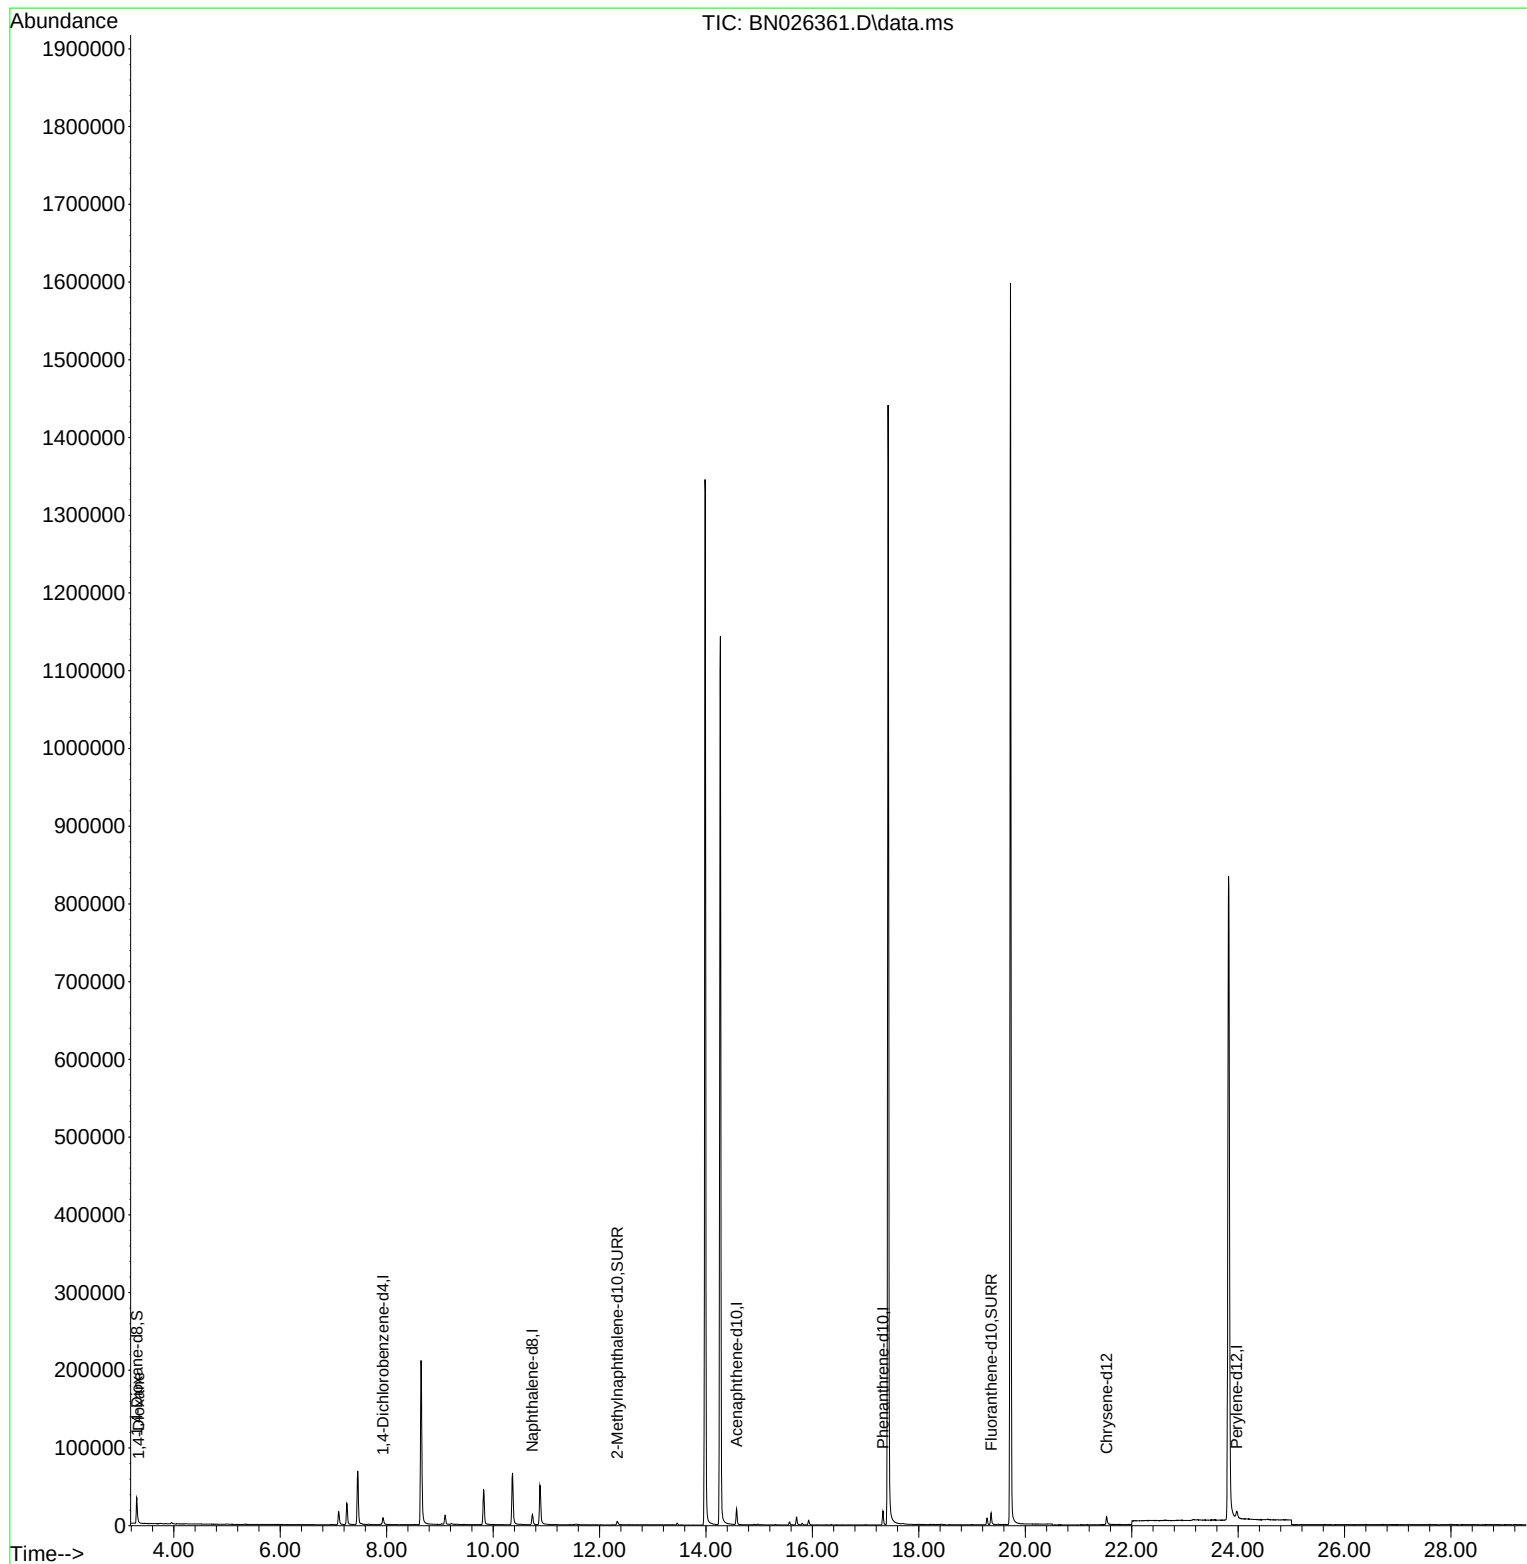

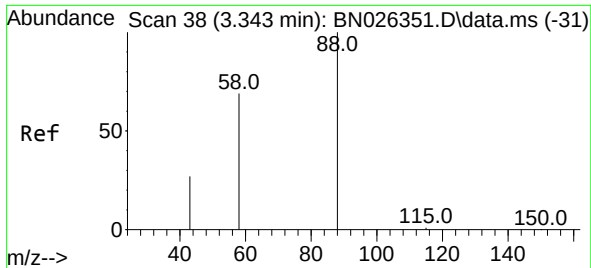

#2
 1,4-Dioxane
 Concen: 0.056 ng/ul
 RT: 3.339 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN026361.D
 Acq: 07 Jul 2023 16:22

Instrument :
 BNA_N
 ClientSampleId :
 DCGZ3

Tgt Ion: 88 Resp: 382
 Ion Ratio Lower Upper
 88 100
 43 65.1 29.5 44.3#
 58 18.7 37.4 56.2#

