

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
 Data File : BN026362.D
 Acq On : 07 Jul 2023 17:00
 Operator : MA/JU
 Sample : 03284-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCGZ4

Quant Time: Jul 07 20:53:53 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 14:46:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.934	152	5173	0.400	ng/ul	0.00
4) Naphthalene-d8	10.736	136	17692	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.574	164	10637	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.325	188	20219	0.400	ng/ul	0.00
17) Chrysene-d12	21.522	240	11212	0.400	ng/ul	0.00
23) Perylene-d12	23.978	264	15331	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	20976	3.601	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.336	152	7632	0.280	ng/ul	0.00
18) Fluoranthene-d10	19.358	212	16720	0.392	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.335	88	254	0.041	ng/ul#	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
Data File : BN026362.D
Acq On : 07 Jul 2023 17:00
Operator : MA/JU
Sample : 03284-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCGZ4

Quant Time: Jul 07 20:53:53 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 14:46:07 2023
Response via : Initial Calibration

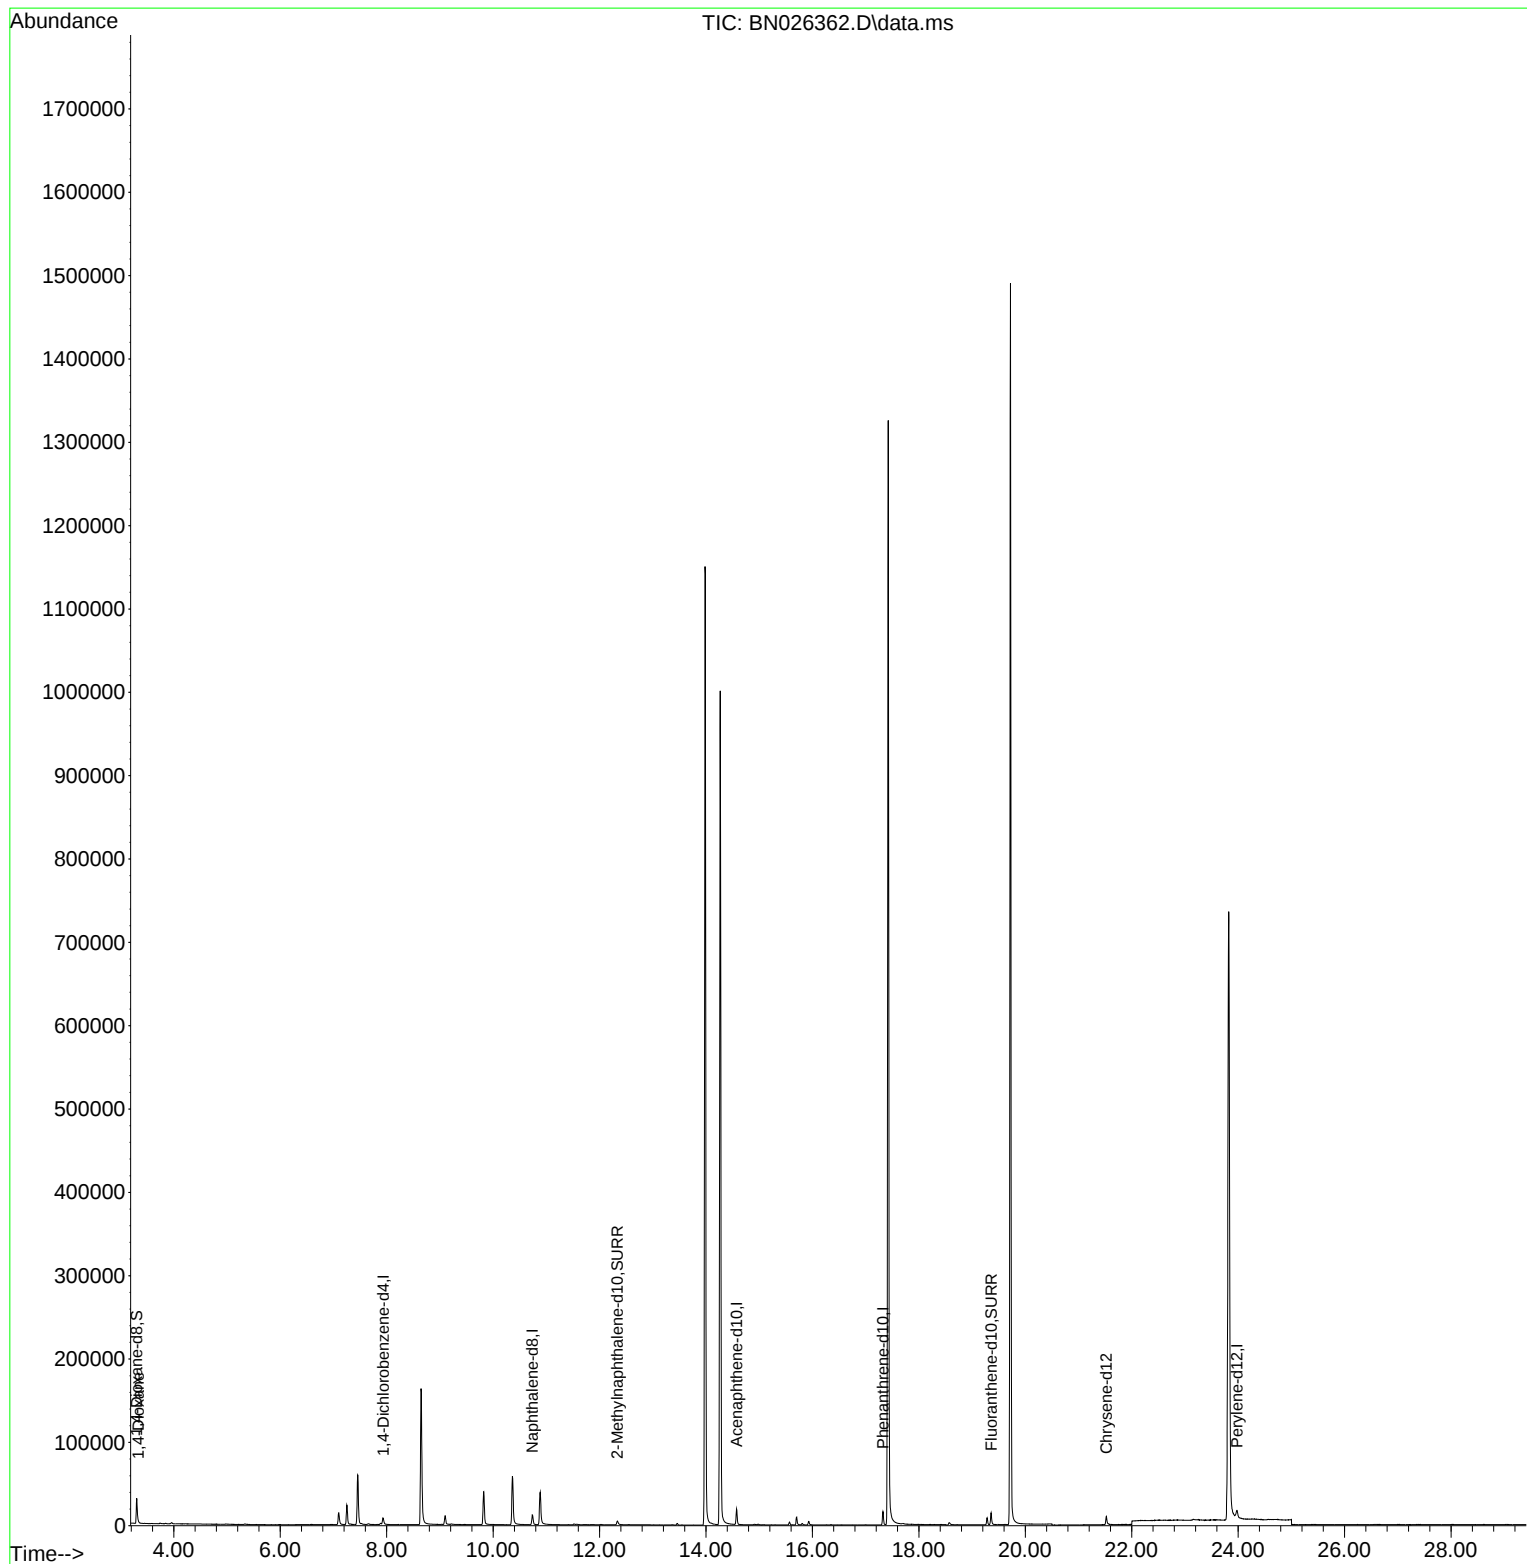

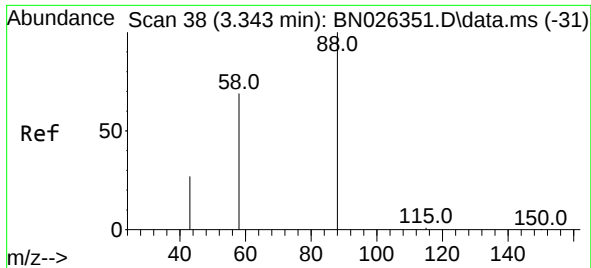

#2
 1,4-Dioxane
 Concen: 0.041 ng/ul
 RT: 3.335 min Scan# 30
 Delta R.T. -0.009 min
 Lab File: BN026362.D
 Acq: 07 Jul 2023 17:00

Instrument :
 BNA_N
 ClientSampleId :
 DCGZ4

Tgt Ion: 88 Resp: 254
 Ion Ratio Lower Upper
 88 100
 43 65.4 29.5 44.3#
 58 17.0 37.4 56.2#

