

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
 Data File : BN026364.D
 Acq On : 07 Jul 2023 18:14
 Operator : MA/JU
 Sample : 03284-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DCGZ9

Quant Time: Jul 07 19:17:17 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 07 14:46:07 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.930	152	5748	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.737	136	19738	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.575	164	12092	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.326	188	23637	0.400	ng/ul	0.00
17) Chrysene-d12	21.526	240	12438	0.400	ng/ul	0.00
23) Perylene-d12	23.970	264	17057	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	23966	3.702	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	9449	0.311	ng/ul	-0.01
18) Fluoranthene-d10	19.354	212	18988	0.401	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.339	88	1793	0.261	ng/ul#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070723\
Data File : BN026364.D
Acq On : 07 Jul 2023 18:14
Operator : MA/JU
Sample : 03284-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DCGZ9

Quant Time: Jul 07 19:17:17 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 07 14:46:07 2023
Response via : Initial Calibration

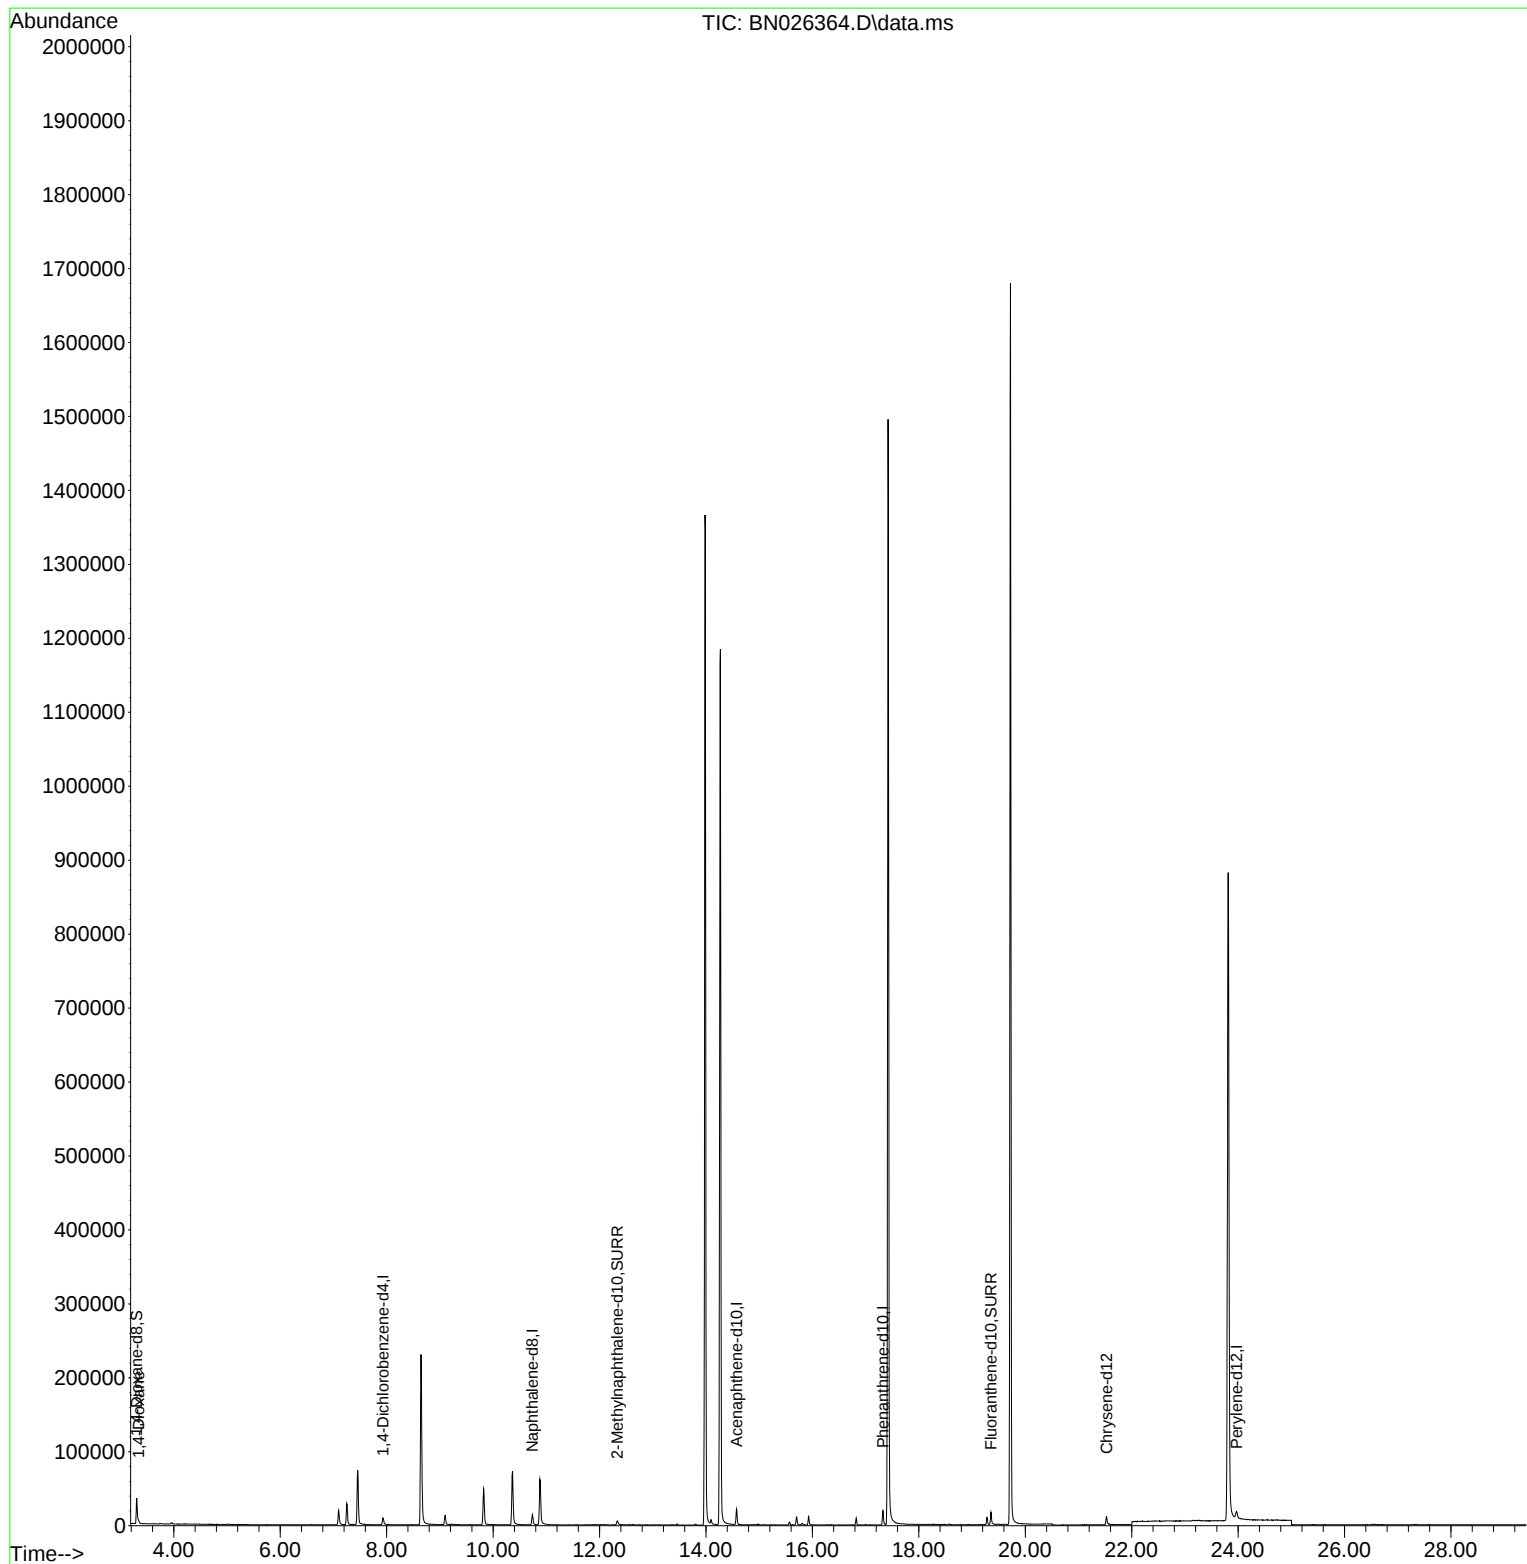

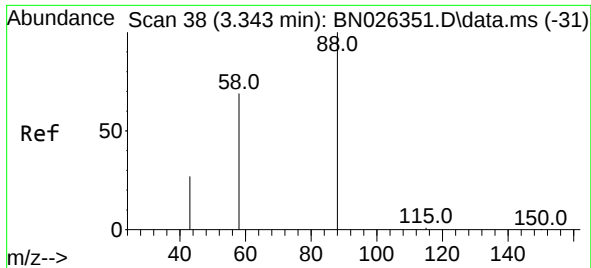

#2
 1,4-Dioxane
 Concen: 0.261 ng/ul
 RT: 3.339 min Scan# 31
 Delta R.T. -0.004 min
 Lab File: BN026364.D
 Acq: 07 Jul 2023 18:14

Instrument :
 BNA_N
 ClientSampleId :
 DCGZ9

Tgt Ion: 88 Resp: 1793

Ion	Ratio	Lower	Upper
88	100		
43	46.6	29.5	44.3#
58	43.8	37.4	56.2

