


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN070821\
Data File : BN015427.D
Acq On : 09 Jul 2021 03:04
Operator : CG/JU
Sample : PB137381BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK381

Quant Time: Jul 09 04:15:36 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 11:17:31 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
7/9/2021 3:04:19 PM

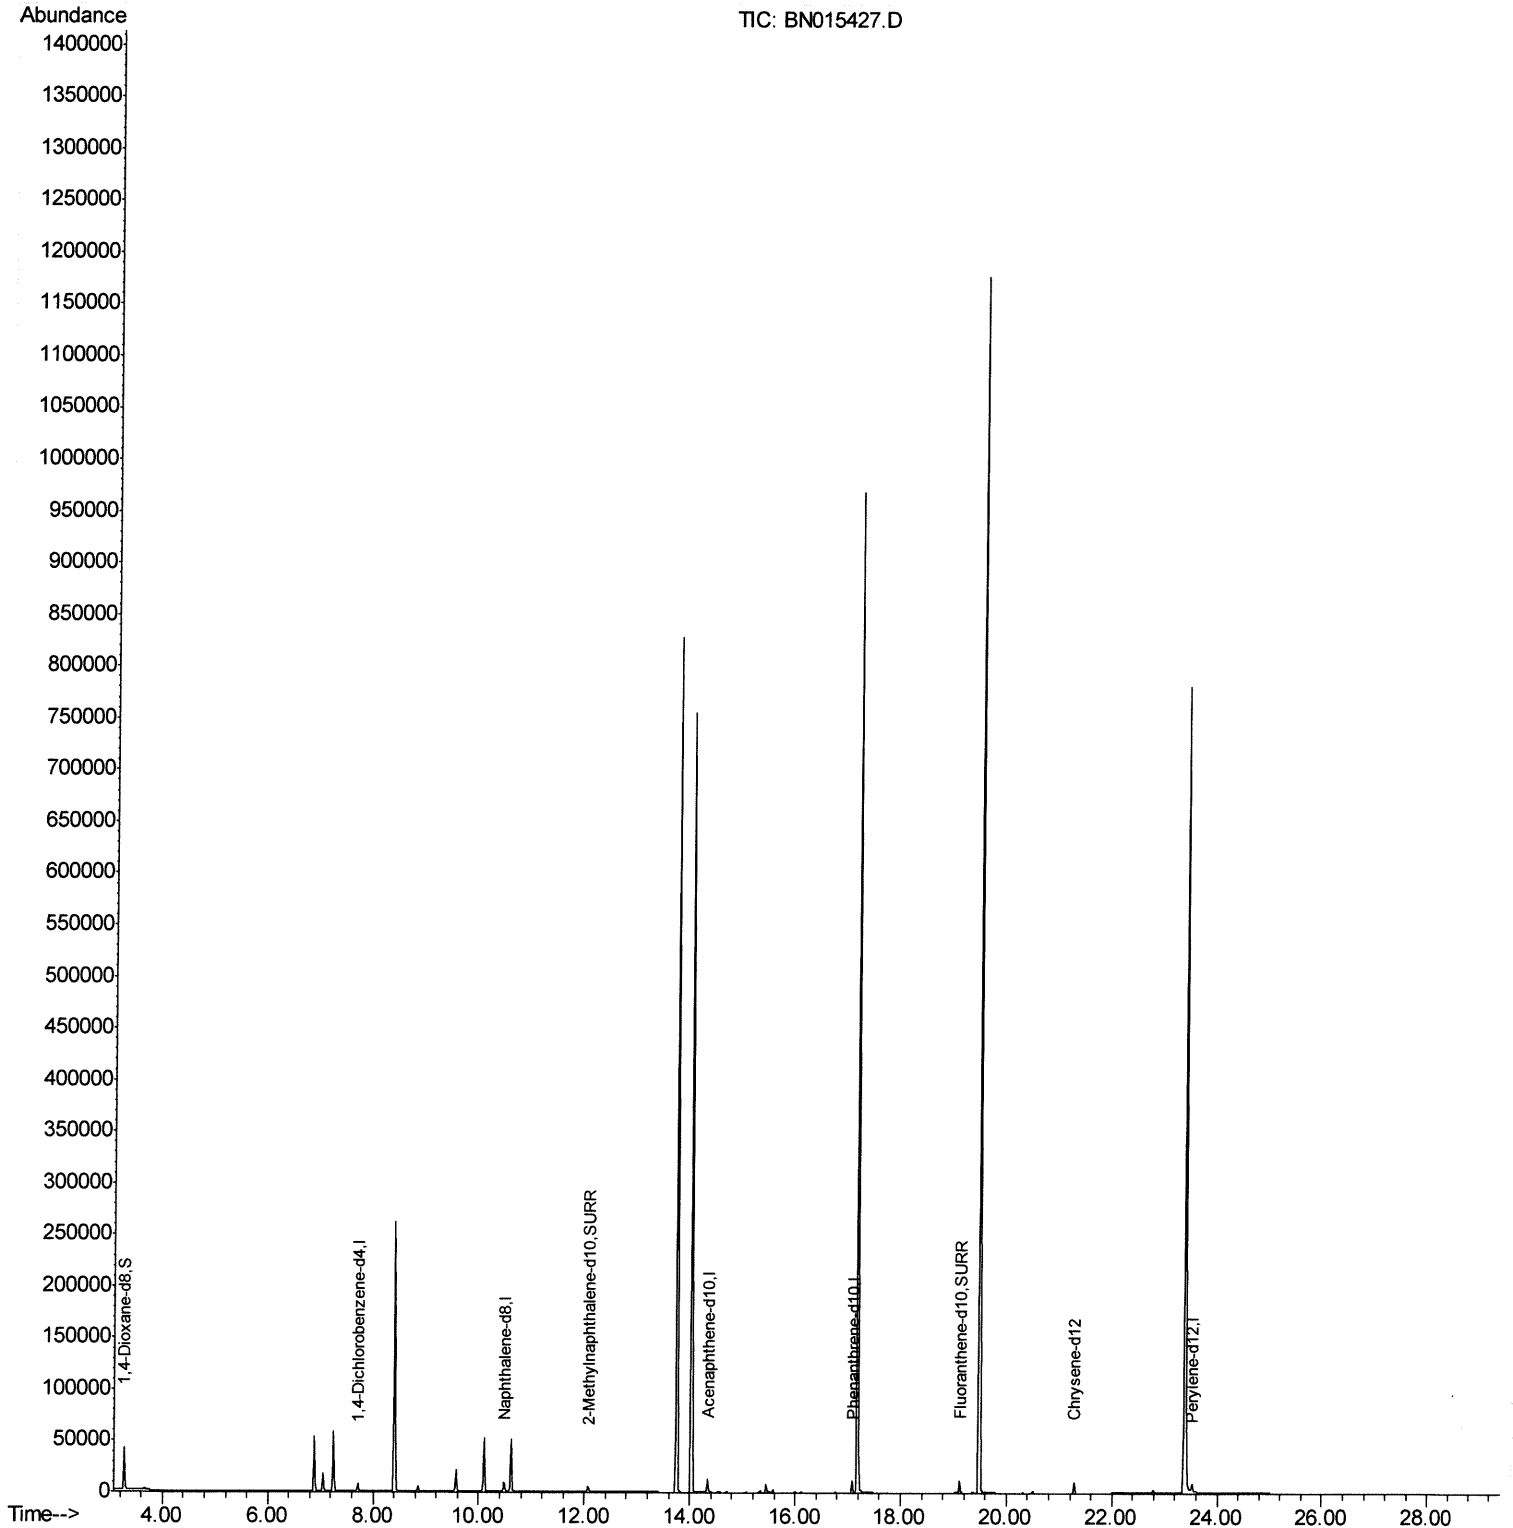




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN070821\
 Data File : BN015427.D
 Acq On : 09 Jul 2021 03:04
 Operator : CG/JU
 Sample : PB137381BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK381

Manual Integrations
 APPROVED

mohammad
 7/9/2021 3:04:19 PM

Quant Time: Jul 09 04:09:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 08 11:17:31 2021
 Response via : Initial Calibration

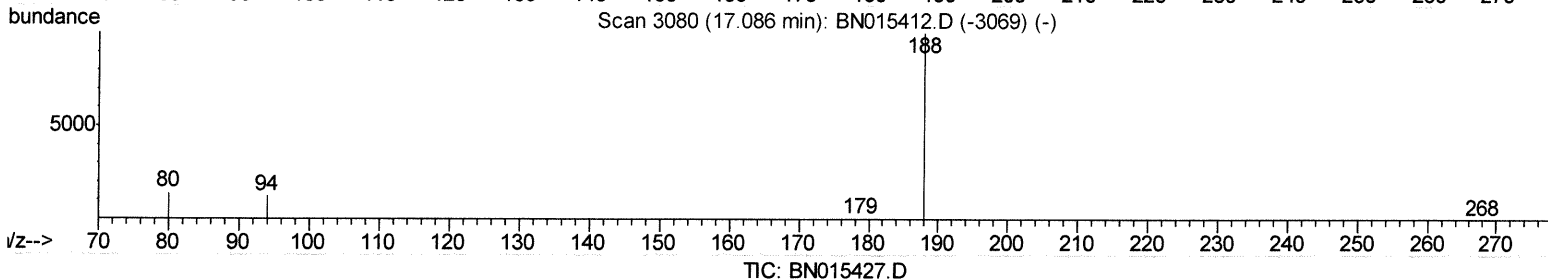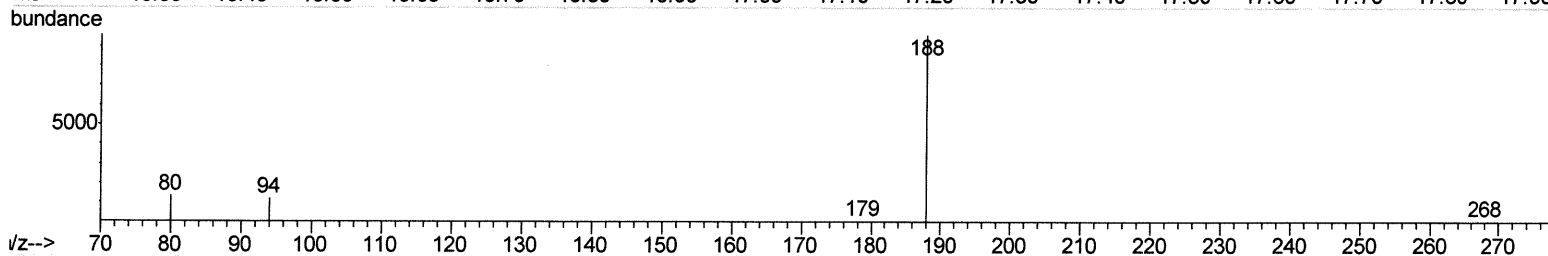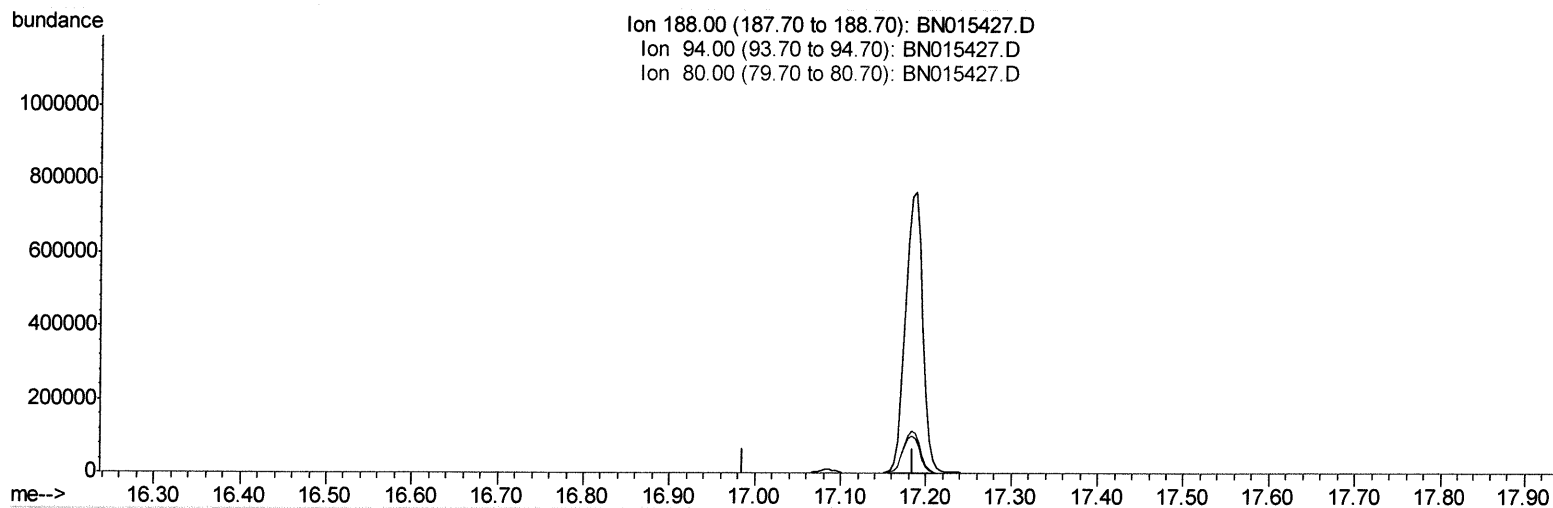

(13) Phenanthrene-d10 (I)

17.086min (-17.086) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	14.10	0.00#
80.00	14.40	0.00#
0.00	0.00	0.00



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN070821\
 Data File : BN015427.D
 Acq On : 09 Jul 2021 03:04
 Operator : CG/JU
 Sample : PB137381BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK381


Manual Integrations
 APPROVED

mohammad
 7/9/2021 3:04:19 PM

Quant Time: Jul 09 04:09:18 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 08 11:17:31 2021
 Response via : Initial Calibration

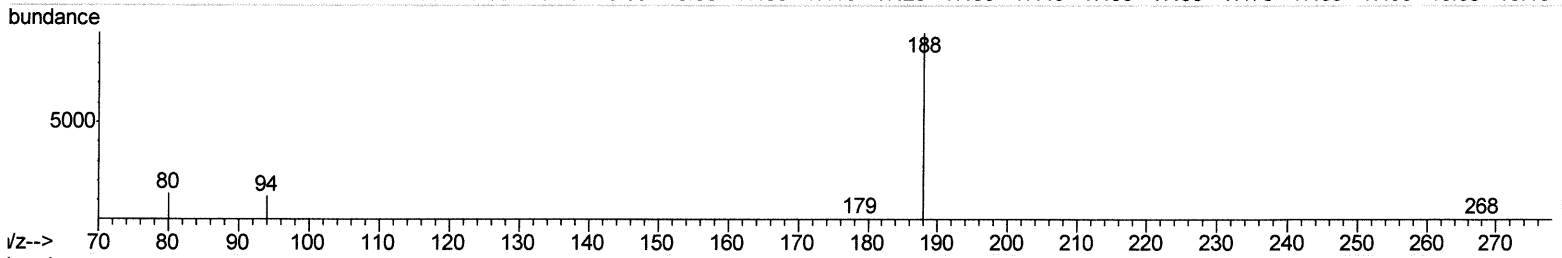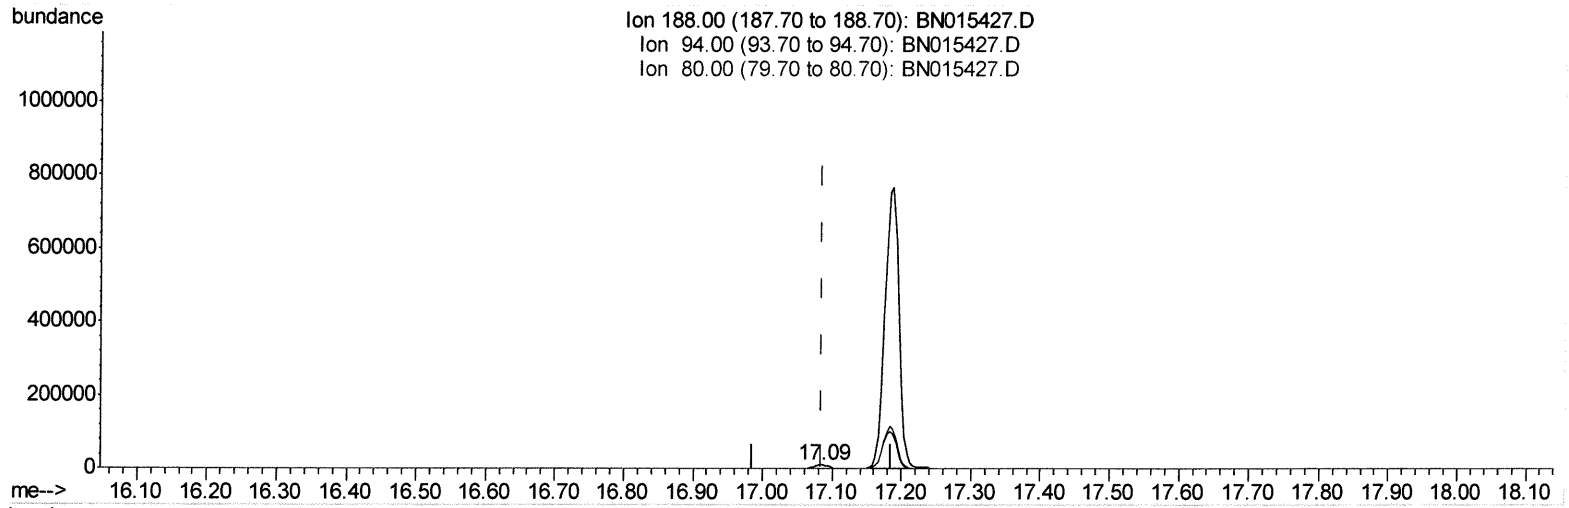

Scan 3080 (17.086 min): BN015412.D (-3069) (-)

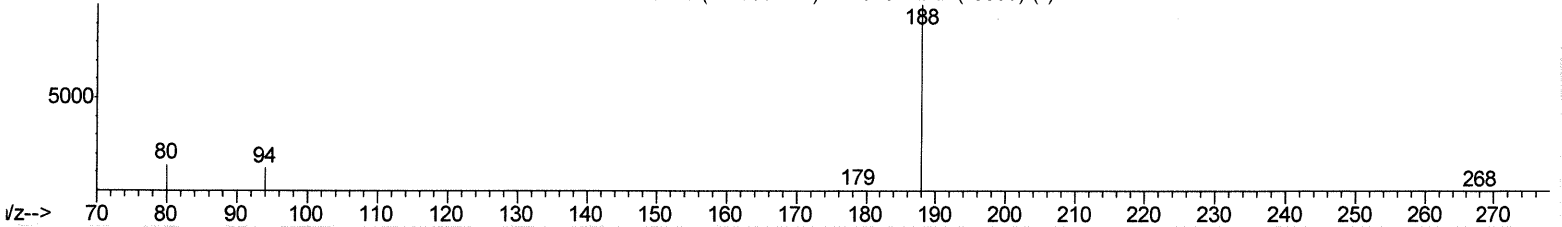

TIC: BN015427.D

(13) Phenanthrene-d10 (I)

17.086min (+0.000) 0.40ng/ul m 07/12/21 JU

response 13357

Ion	Exp%	Act%
188.00	100	100
94.00	14.10	12.69
80.00	14.40	13.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN070821\
 Data File : BN015427.D
 Acq On : 09 Jul 2021 03:04
 Operator : CG/JU
 Sample : PB137381BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK381

Manual Integrations
 APPROVED

mohammad
 7/9/2021 3:04:19 PM

Quant Time: Jul 09 04:15:36 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 08 11:17:31 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.71	152	3611	0.40	ng/ul	0.00
4) Naphthalene-d8	10.48	136	12370	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.34	164	6930	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.09	188	13357m>	0.40	ng/ul>	0.00
17) Chrysene-d12	21.28	240	9946	0.40	ng/ul	0.00
23) Perylene-d12	23.52	264	10417	0.40	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.28	96	27131	6.67	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.07	152	6577	0.34	ng/ul	0.00
18) Fluoranthene-d10	19.12	212	12673	0.39	ng/ul	0.00

Target Compounds	Ovalue
-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed