

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070821\
 Data File : BN015425.D
 Acq On : 09 Jul 2021 01:16
 Operator : CG/JU
 Sample : M2905-14
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBK37

Manual Integrations
 APPROVED

mohammad
 7/9/2021 3:04:16 PM

Quant Time: Jul 09 02:47:58 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 08 11:17:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.716	152	2656	0.400	ng/ul	0.00
4) Naphthalene-d8	10.479	136	9267	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.340	164	5189	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.086	188	10561m	0.400	ng/ul	0.00
17) Chrysene-d12	21.284	240	8400	0.400	ng/ul	0.00
23) Perylene-d12	23.520	264	8399	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.277	96	15811	5.281	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.074	152	3420	0.235	ng/ul	0.00
18) Fluoranthene-d10	19.117	212	8580	0.311	ng/ul	0.00
Target Compounds						
2) 1,4-Dioxane	3.315	88	2722	0.841	ng/ul	Qvalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070821\
Data File : BN015425.D
Acq On : 09 Jul 2021 01:16
Operator : CG/JU
Sample : M2905-14
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
DBK37

Manual Integrations
APPROVED


mohammad
7/9/2021 3:04:16 PM

Quant Time: Jul 09 02:47:58 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 08 11:17:31 2021
Response via : Initial Calibration

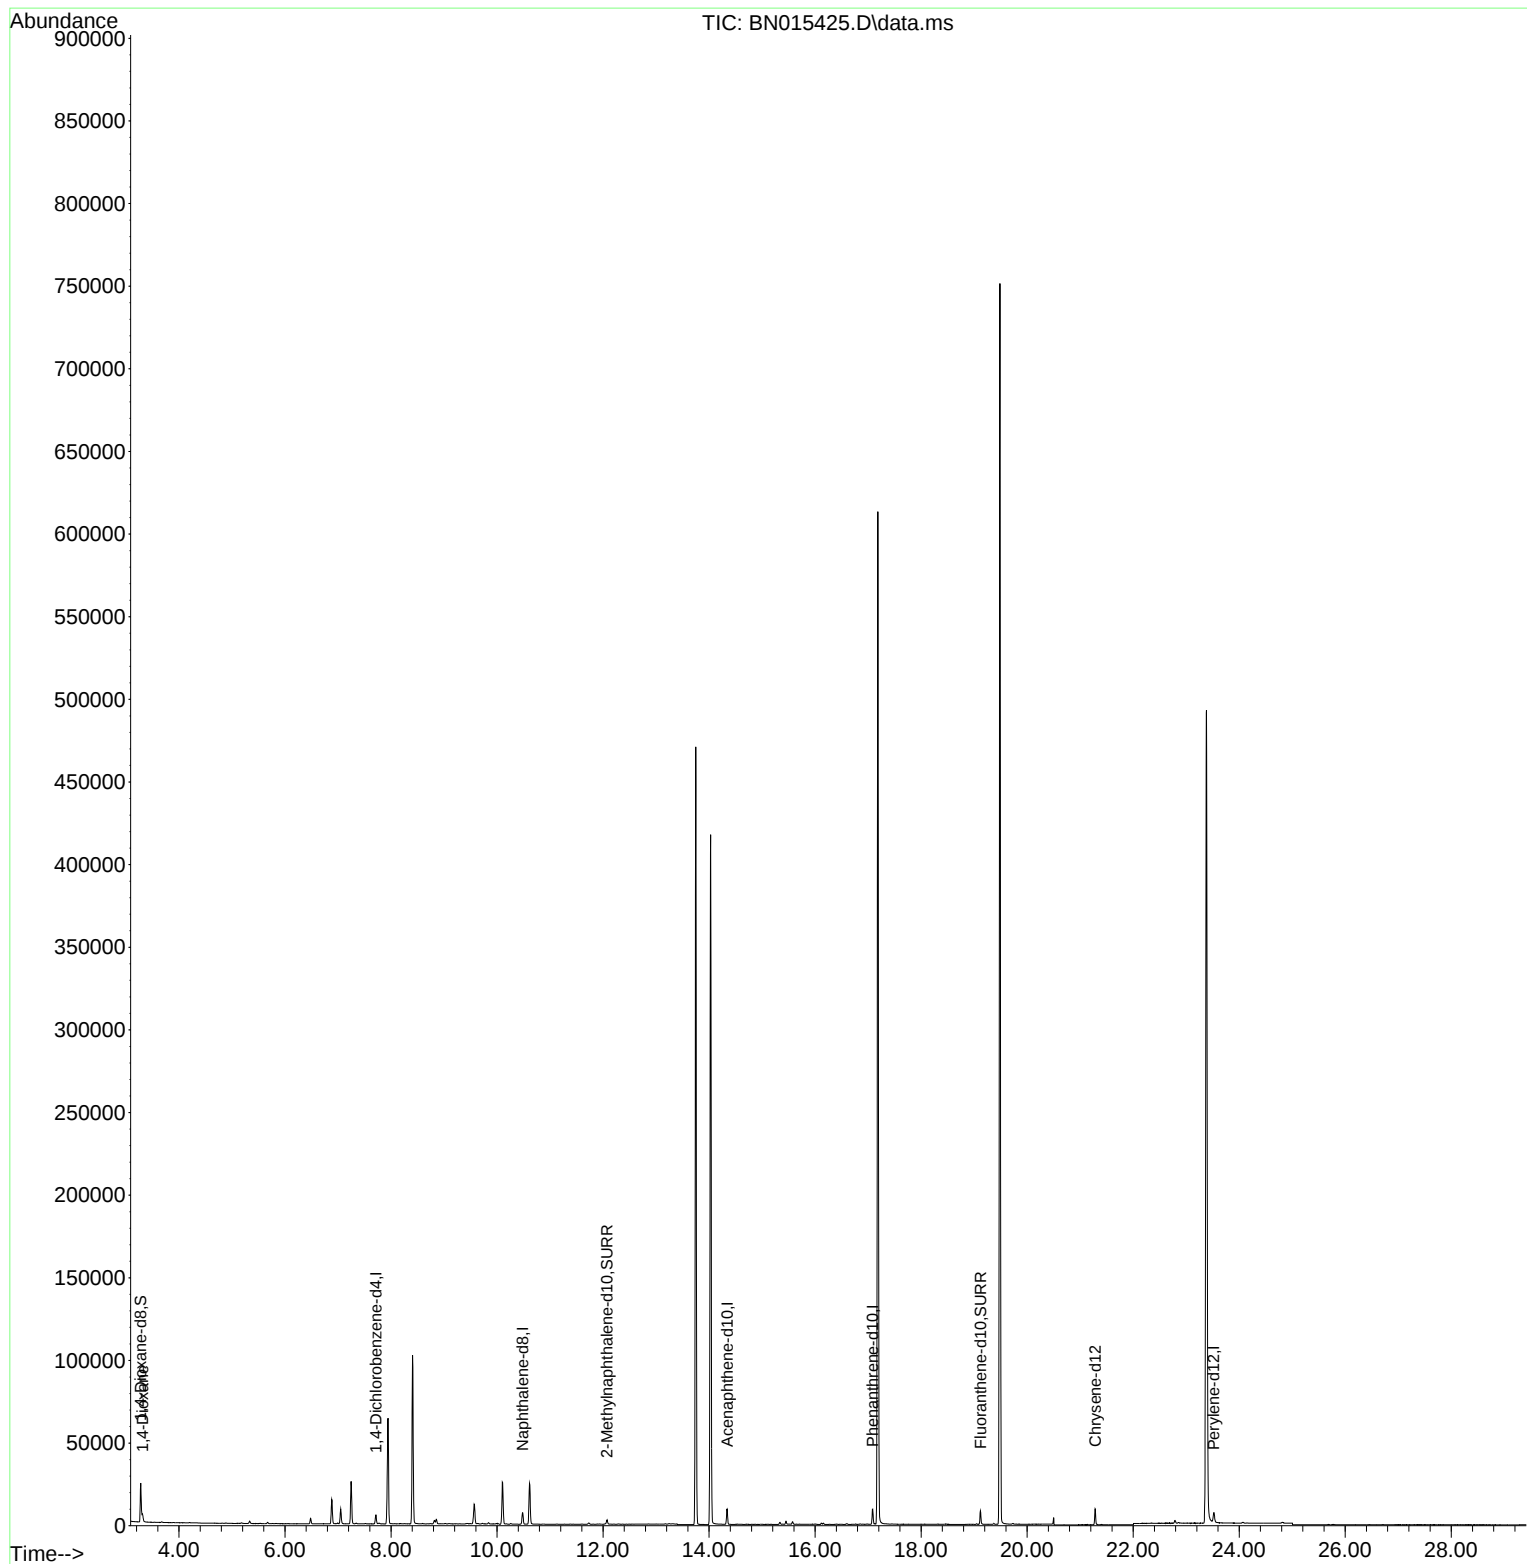


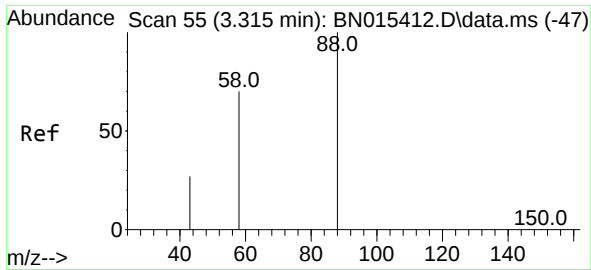


#2
 1,4-Dioxane
 Concen: 0.841 ng/ul
 RT: 3.315 min Scan# 55
 Delta R.T. 0.000 min
 Lab File: BN015425.D
 Acq: 09 Jul 2021 01:16

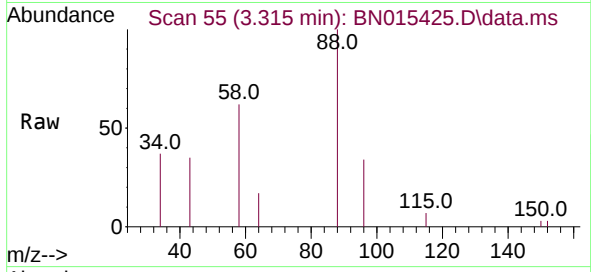

Tgt Ion: 88 Resp: 2722

Ion	Ratio	Lower	Upper
88	100		
43	34.9	24.9	37.3
58	61.9	43.4	65.0

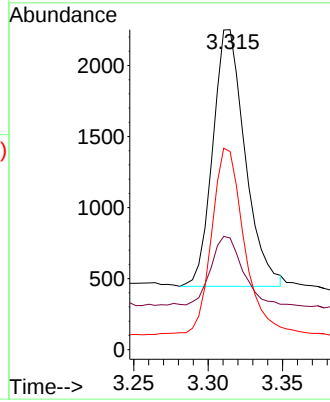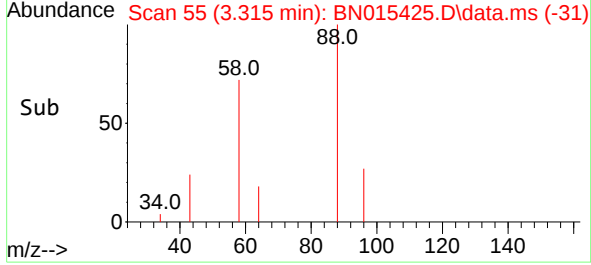

Instrument :
 BNA_N
 ClientSampleId :
 DBK37

Manual Integrations
 APPROVED

mohammad
 7/9/2021 3:04:16 PM