

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070823\
 Data File : BN026393.D
 Acq On : 08 Jul 2023 19:49
 Operator : MA/JU
 Sample : PB153851BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK851

Quant Time: Jul 08 23:53:36 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 09:20:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	4111	0.400	ng/ul	0.00
4) Naphthalene-d8	10.732	136	14468	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.570	164	8280	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.322	188	19202	0.400	ng/ul	0.00
17) Chrysene-d12	21.526	240	10826	0.400	ng/ul	0.00
23) Perylene-d12	23.958	264	14289	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	13520	2.920	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	6352	0.285	ng/ul	0.00
18) Fluoranthene-d10	19.349	212	21537	0.523	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.717	202	3850	0.064	ng/ul#	1
26) Benzo(a)pyrene	23.806	252	6562	0.124	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070823\
Data File : BN026393.D
Acq On : 08 Jul 2023 19:49
Operator : MA/JU
Sample : PB153851BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK851

Quant Time: Jul 08 23:53:36 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 09:20:18 2023
Response via : Initial Calibration




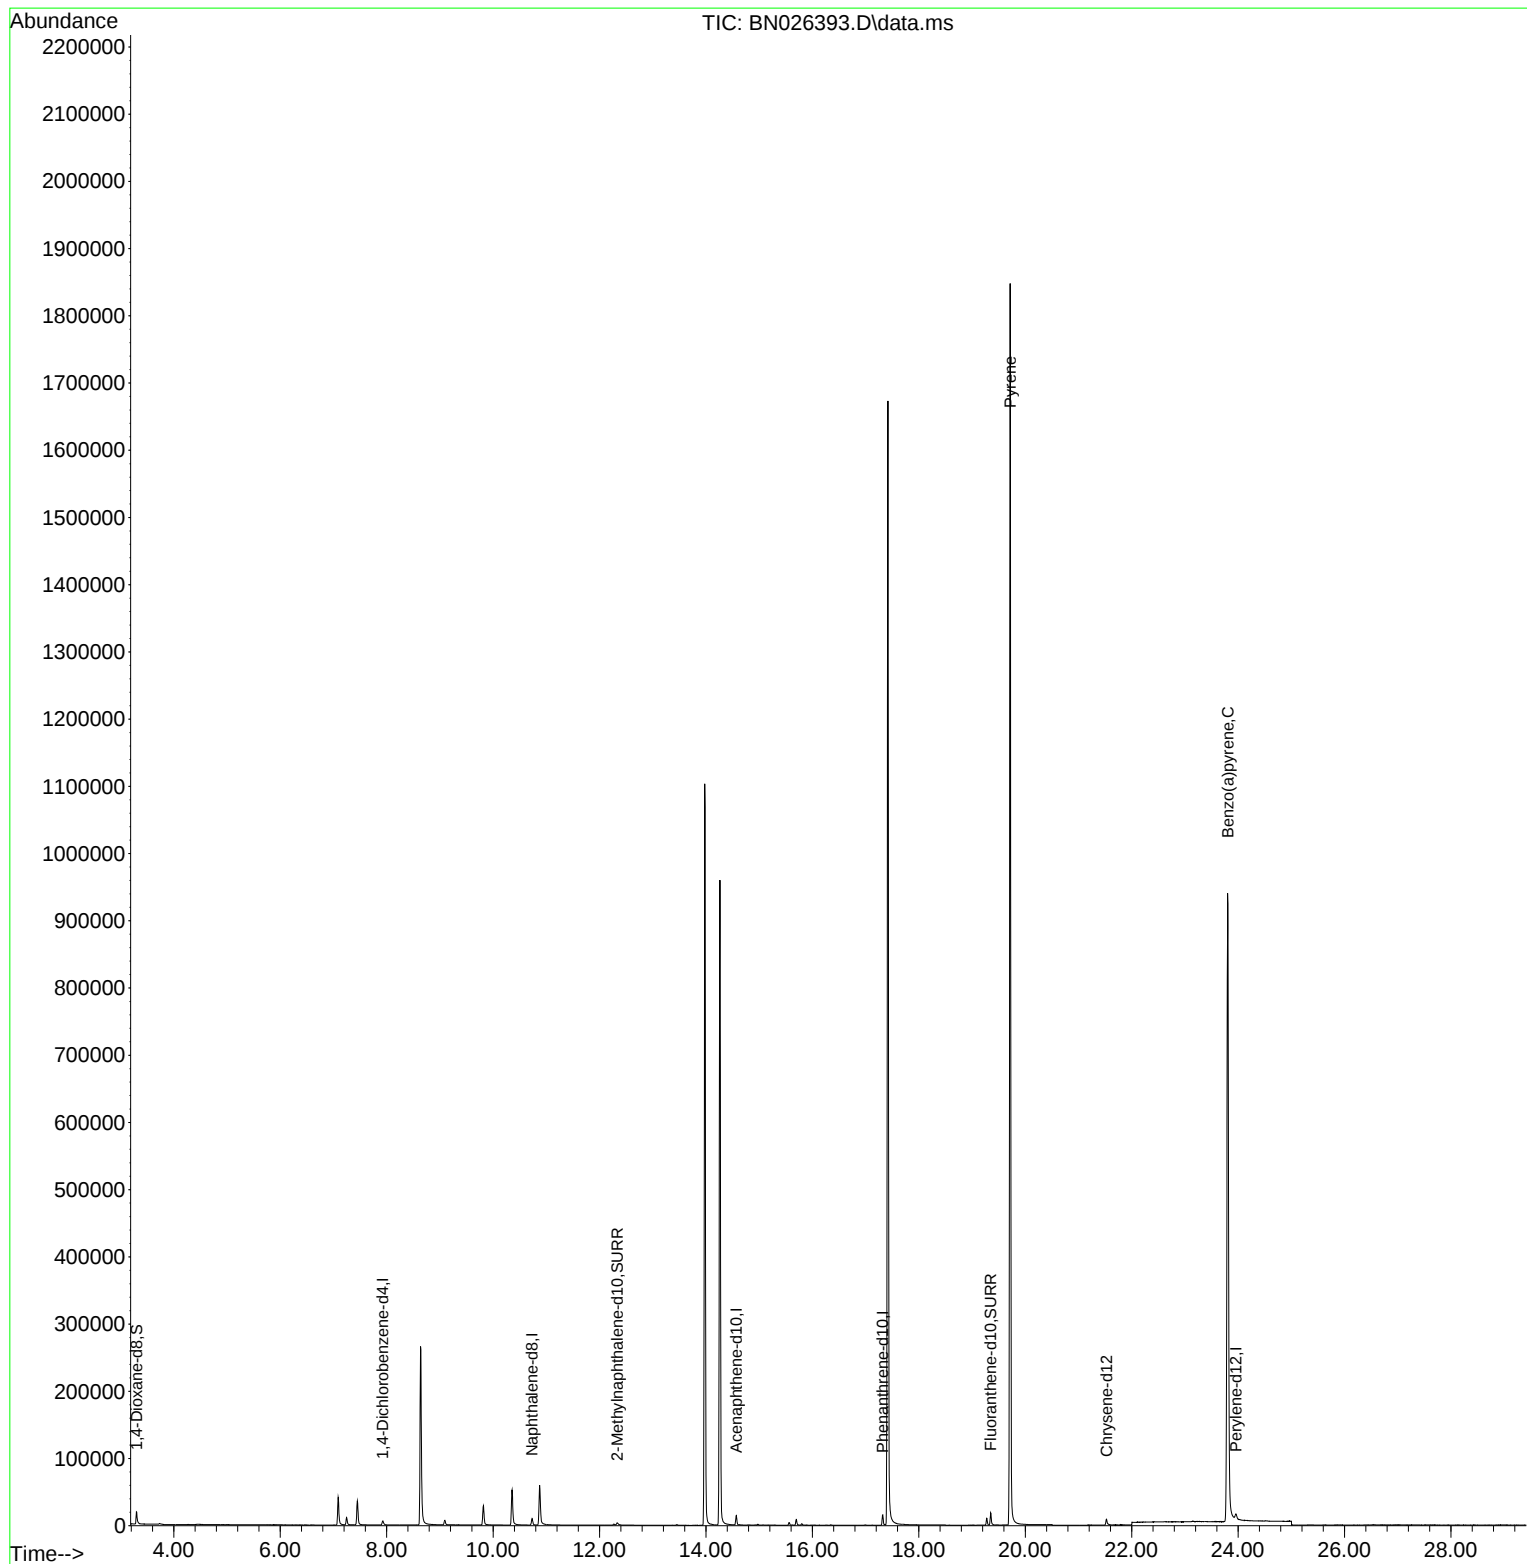


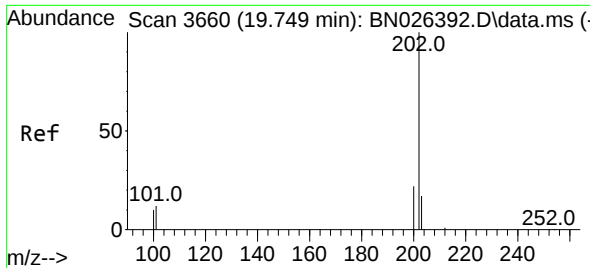

#20
Pyrene
Concen: 0.064 ng/ul
RT: 19.717 min Scan# 3653
Delta R.T. -0.036 min
Lab File: BN026393.D
Acq: 08 Jul 2023 19:49

Instrument :
BNA_N
ClientSampleId :
SBLK851

Tgt Ion:202 Resp: 3850
Ion Ratio Lower Upper
202 100
101 187.4 11.4 17.0#
100 1473.2 9.1 13.7#

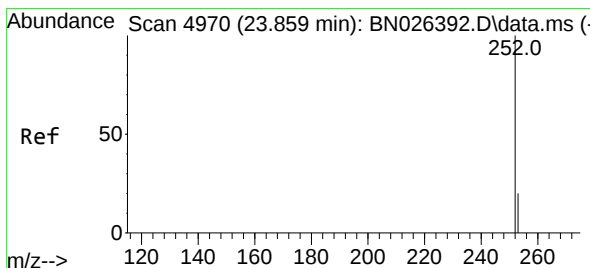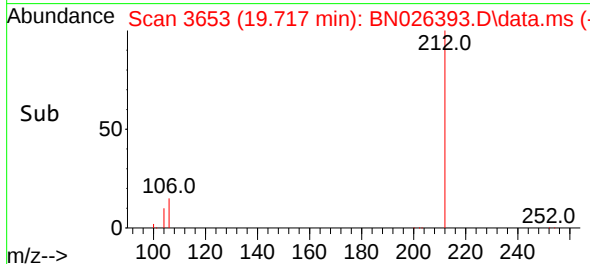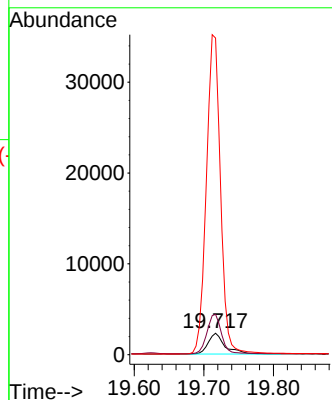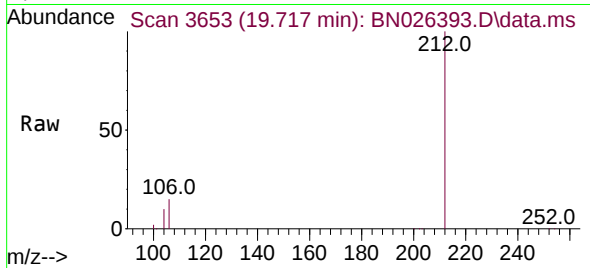

#26
Benzo(a)pyrene
Concen: 0.124 ng/ul
RT: 23.806 min Scan# 4952
Delta R.T. -0.060 min
Lab File: BN026393.D
Acq: 08 Jul 2023 19:49

Tgt Ion:252 Resp: 6562
Ion Ratio Lower Upper
252 100
253 53.4 26.0 39.0#
125 57.2 17.3 25.9#

