

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070823\
 Data File : BN026395.D
 Acq On : 08 Jul 2023 21:03
 Operator : MA/JU
 Sample : 03350-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW27

Quant Time: Jul 08 23:54:02 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 09:20:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	4784	0.400	ng/ul	0.00
4) Naphthalene-d8	10.732	136	13296	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.566	164	9868	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.317	188	18561	0.400	ng/ul	-0.01
17) Chrysene-d12	21.517	240	10479	0.400	ng/ul	-0.01
23) Perylene-d12	23.964	264	13012	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	31152	5.782	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.327	152	8434	0.412	ng/ul	0.00
18) Fluoranthene-d10	19.349	212	15055	0.377	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.335	88	392	0.069	ng/ul#	68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070823\
Data File : BN026395.D
Acq On : 08 Jul 2023 21:03
Operator : MA/JU
Sample : 03350-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YBW27

Quant Time: Jul 08 23:54:02 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 08 09:20:18 2023
Response via : Initial Calibration

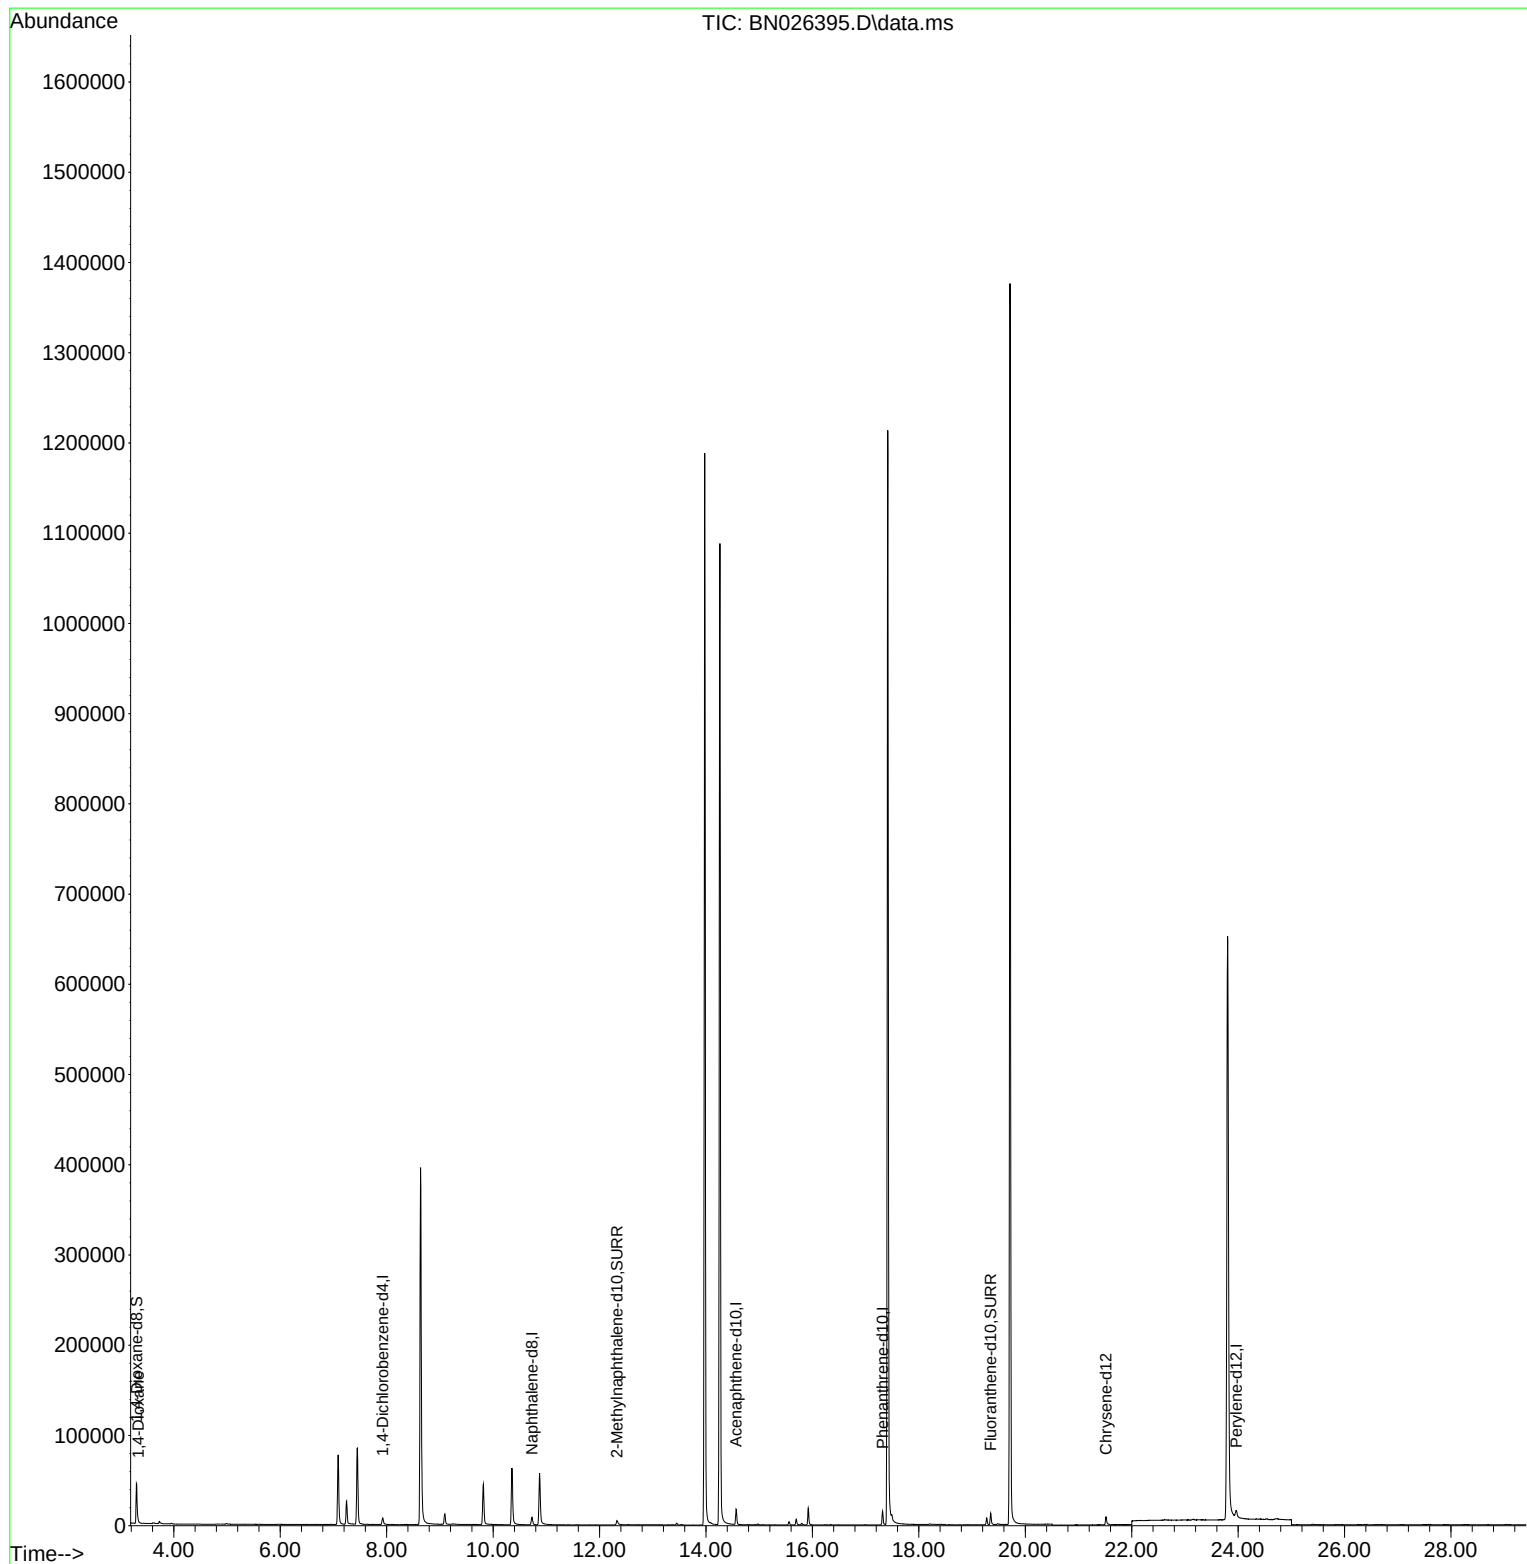

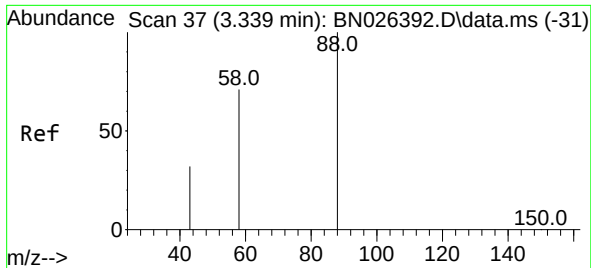

#2

1,4-Dioxane

Concen: 0.069 ng/ul

RT: 3.335 min Scan# 30

Delta R.T. -0.008 min

Lab File: BN026395.D


Acq: 08 Jul 2023 21:03

Instrument :

BNA_N

ClientSampleId :

YBW27

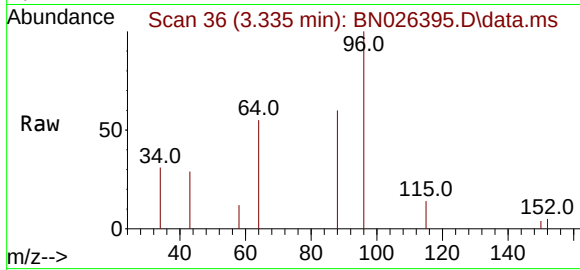

Tgt Ion: 88 Resp: 392

Ion Ratio Lower Upper

88 100

43 49.1 29.5 44.3#

58 19.8 37.4 56.2#

