

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070823\
 Data File : BN026398.D
 Acq On : 08 Jul 2023 22:54
 Operator : MA/JU
 Sample : 03350-06
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW29


Quant Time: Jul 08 23:54:48 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 08 09:20:18 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	5146	0.400	ng/ul	0.00
4) Naphthalene-d8	10.732	136	17899	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.570	164	10507	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.321	188	20027	0.400	ng/ul	0.00
17) Chrysene-d12	21.517	240	11384	0.400	ng/ul	-0.01
23) Perylene-d12	23.961	264	13162	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.301	96	21828	3.767	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.332	152	5744	0.209	ng/ul	0.00
18) Fluoranthene-d10	19.354	212	10012	0.231	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.335	88	578	0.094	ng/ul#	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Quant Time: Jul 08 23:54:48 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Sat Jul 08 09:20:18 2023
Response via : Initial Calibration

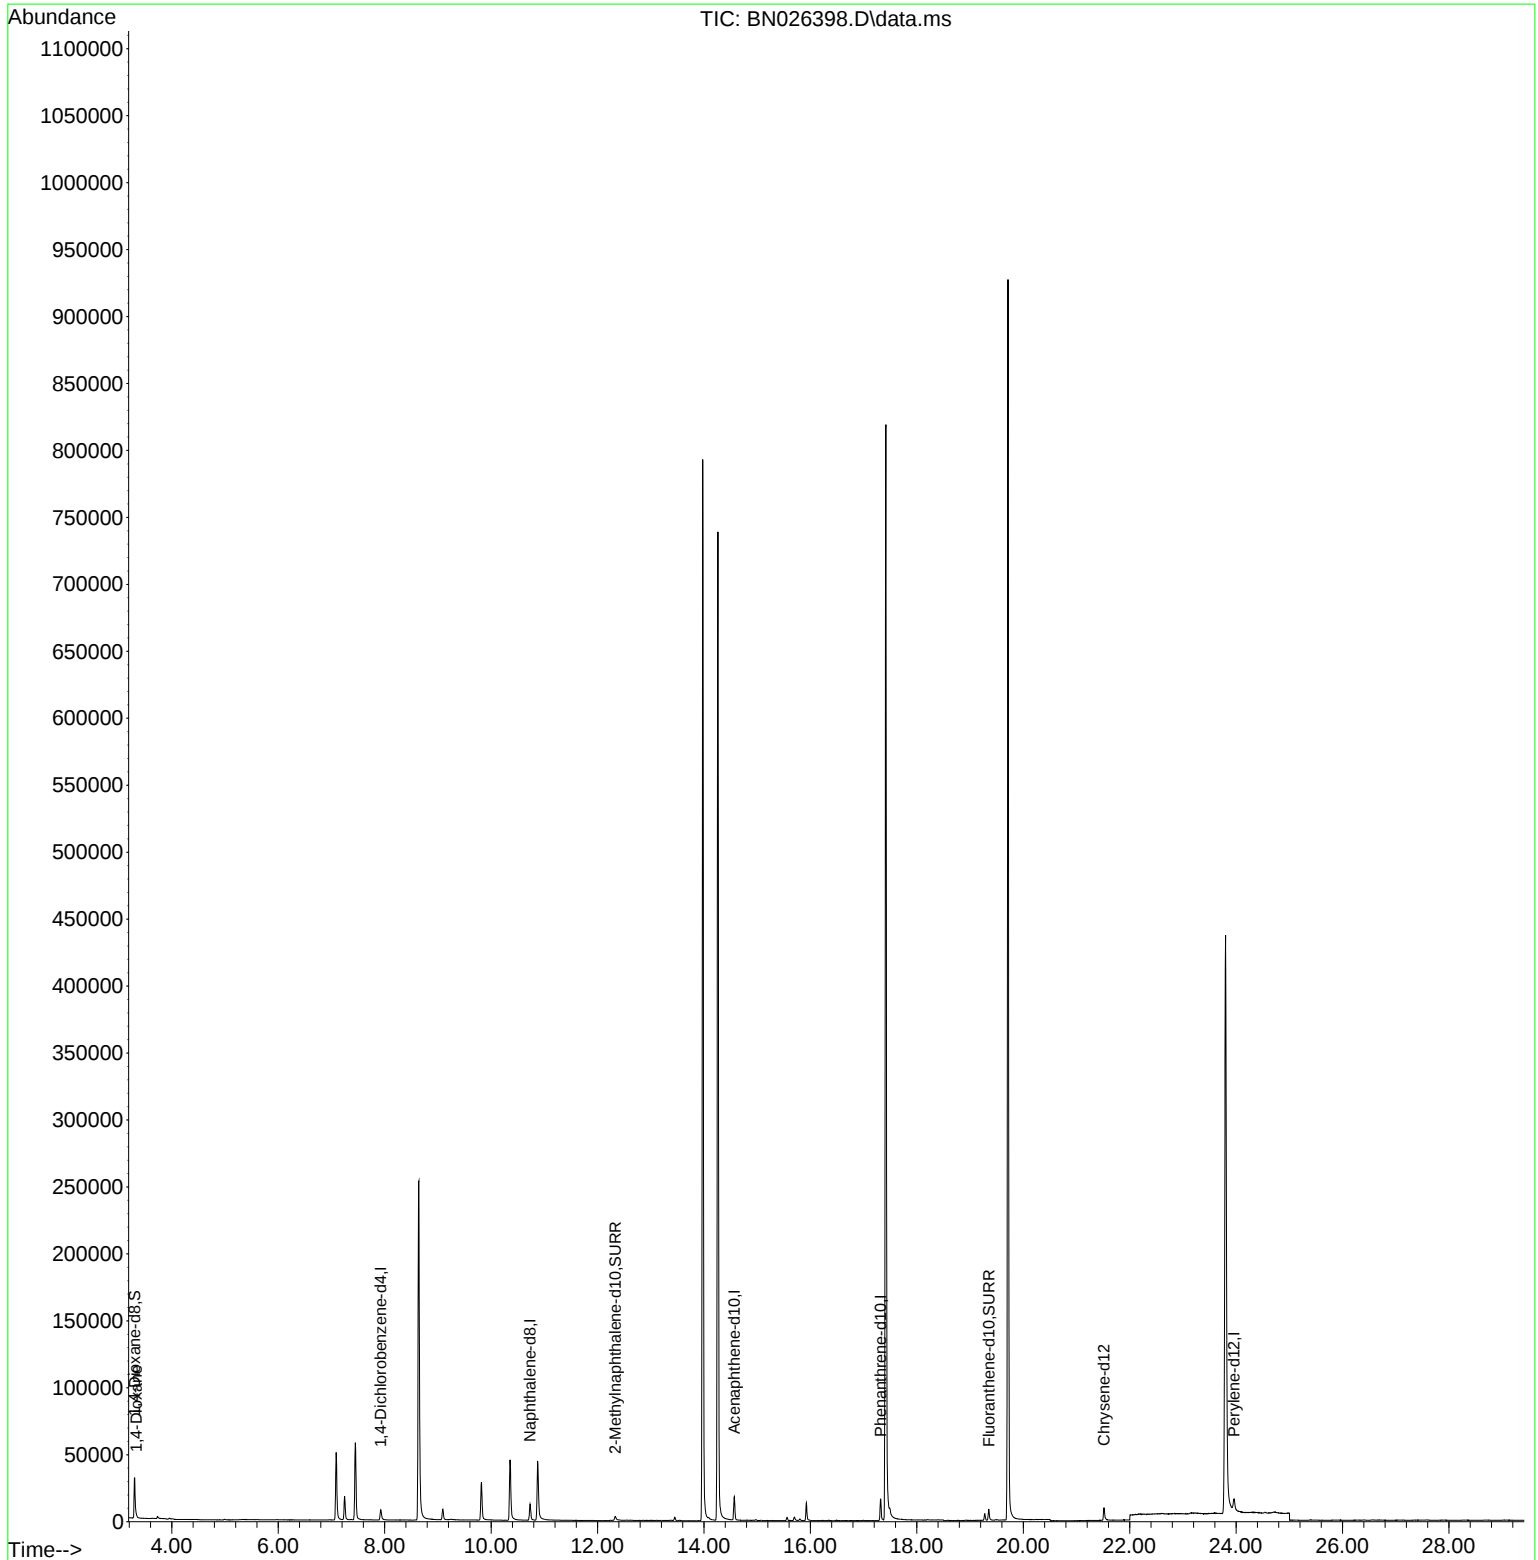

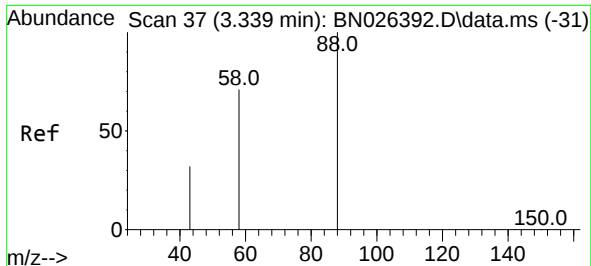

#2
 1,4-Dioxane
 Concen: 0.094 ng/ul
 RT: 3.335 min Scan# 30
 Delta R.T. -0.008 min
 Lab File: BN026398.D
 Acq: 08 Jul 2023 22:54

Instrument :
 BNA_N
 ClientSampleId :
 YBW29

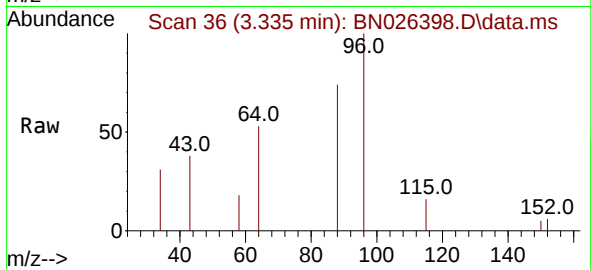

Tgt Ion: 88 Resp: 578

Ion	Ratio	Lower	Upper
88	100		
43	52.1	29.5	44.3#
58	24.9	37.4	56.2#

