

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070823\
 Data File : BN026414.D
 Acq On : 09 Jul 2023 09:20
 Operator : MA/JU
 Sample : 03349-10
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW03

Quant Time: Jul 09 15:56:47 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 15:51:14 2023
 Response via : Initial Calibration




Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.921	152	5376	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.726	136	18869	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.565	164	10792	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.313	188	19747	0.400	ng/ul	-0.01
17) Chrysene-d12	21.520	240	11166	0.400	ng/ul	0.00
23) Perylene-d12	23.967	264	14220	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	25039	4.136	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.326	152	7376	0.254	ng/ul	0.00
18) Fluoranthene-d10	19.349	212	11557	0.272	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.335	88	1059	0.165	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jul 09 15:56:47 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jul 09 15:51:14 2023
Response via : Initial Calibration



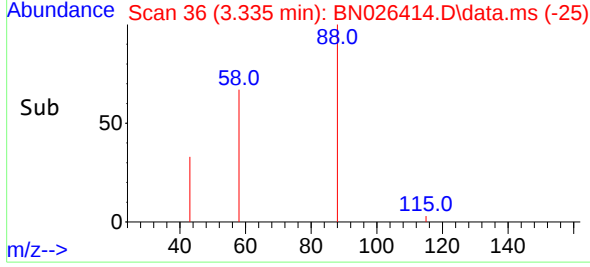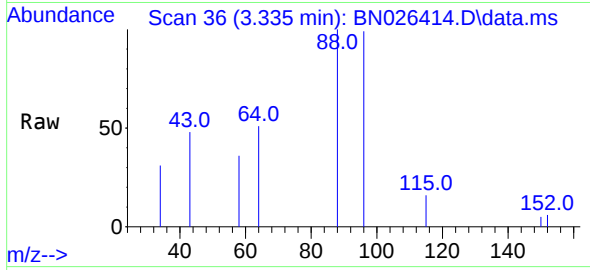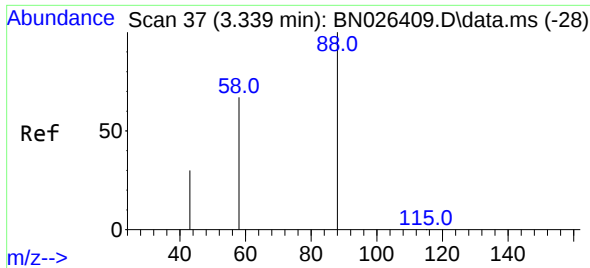

#2
1,4-Dioxane
Concen: 0.165 ng/ul
RT: 3.335 min Scan# 30
Delta R.T. -0.004 min
Lab File: BN026414.D
Acq: 09 Jul 2023 09:20

Instrument :
BNA_N
ClientSampleId :
YBW03

Tgt Ion: 88 Resp: 1059

Ion	Ratio	Lower	Upper
88	100		
43	48.2	29.5	44.3#
58	35.7	37.4	56.2#

