

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070823\
 Data File : BN026429.D
 Acq On : 09 Jul 2023 19:07
 Operator : MA/JU
 Sample : 03349-17
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 YBW11

Quant Time: Jul 10 01:21:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 15:51:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.921	152	5617	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.726	136	16659	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.561	164	10422	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.313	188	16108	0.400	ng/ul	-0.01
17) Chrysene-d12	21.517	240	11067	0.400	ng/ul	0.00
23) Perylene-d12	23.958	264	14799	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	41283	6.526	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.321	152	12167	0.475	ng/ul	-0.01
18) Fluoranthene-d10	19.344	212	21031	0.499	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.335	88	14840	2.209	ng/ul#	85




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN070823\
Data File : BN026429.D
Acq On : 09 Jul 2023 19:07
Operator : MA/JU
Sample : 03349-17
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
YBW11

Quant Time: Jul 10 01:21:55 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jul 09 15:51:14 2023
Response via : Initial Calibration

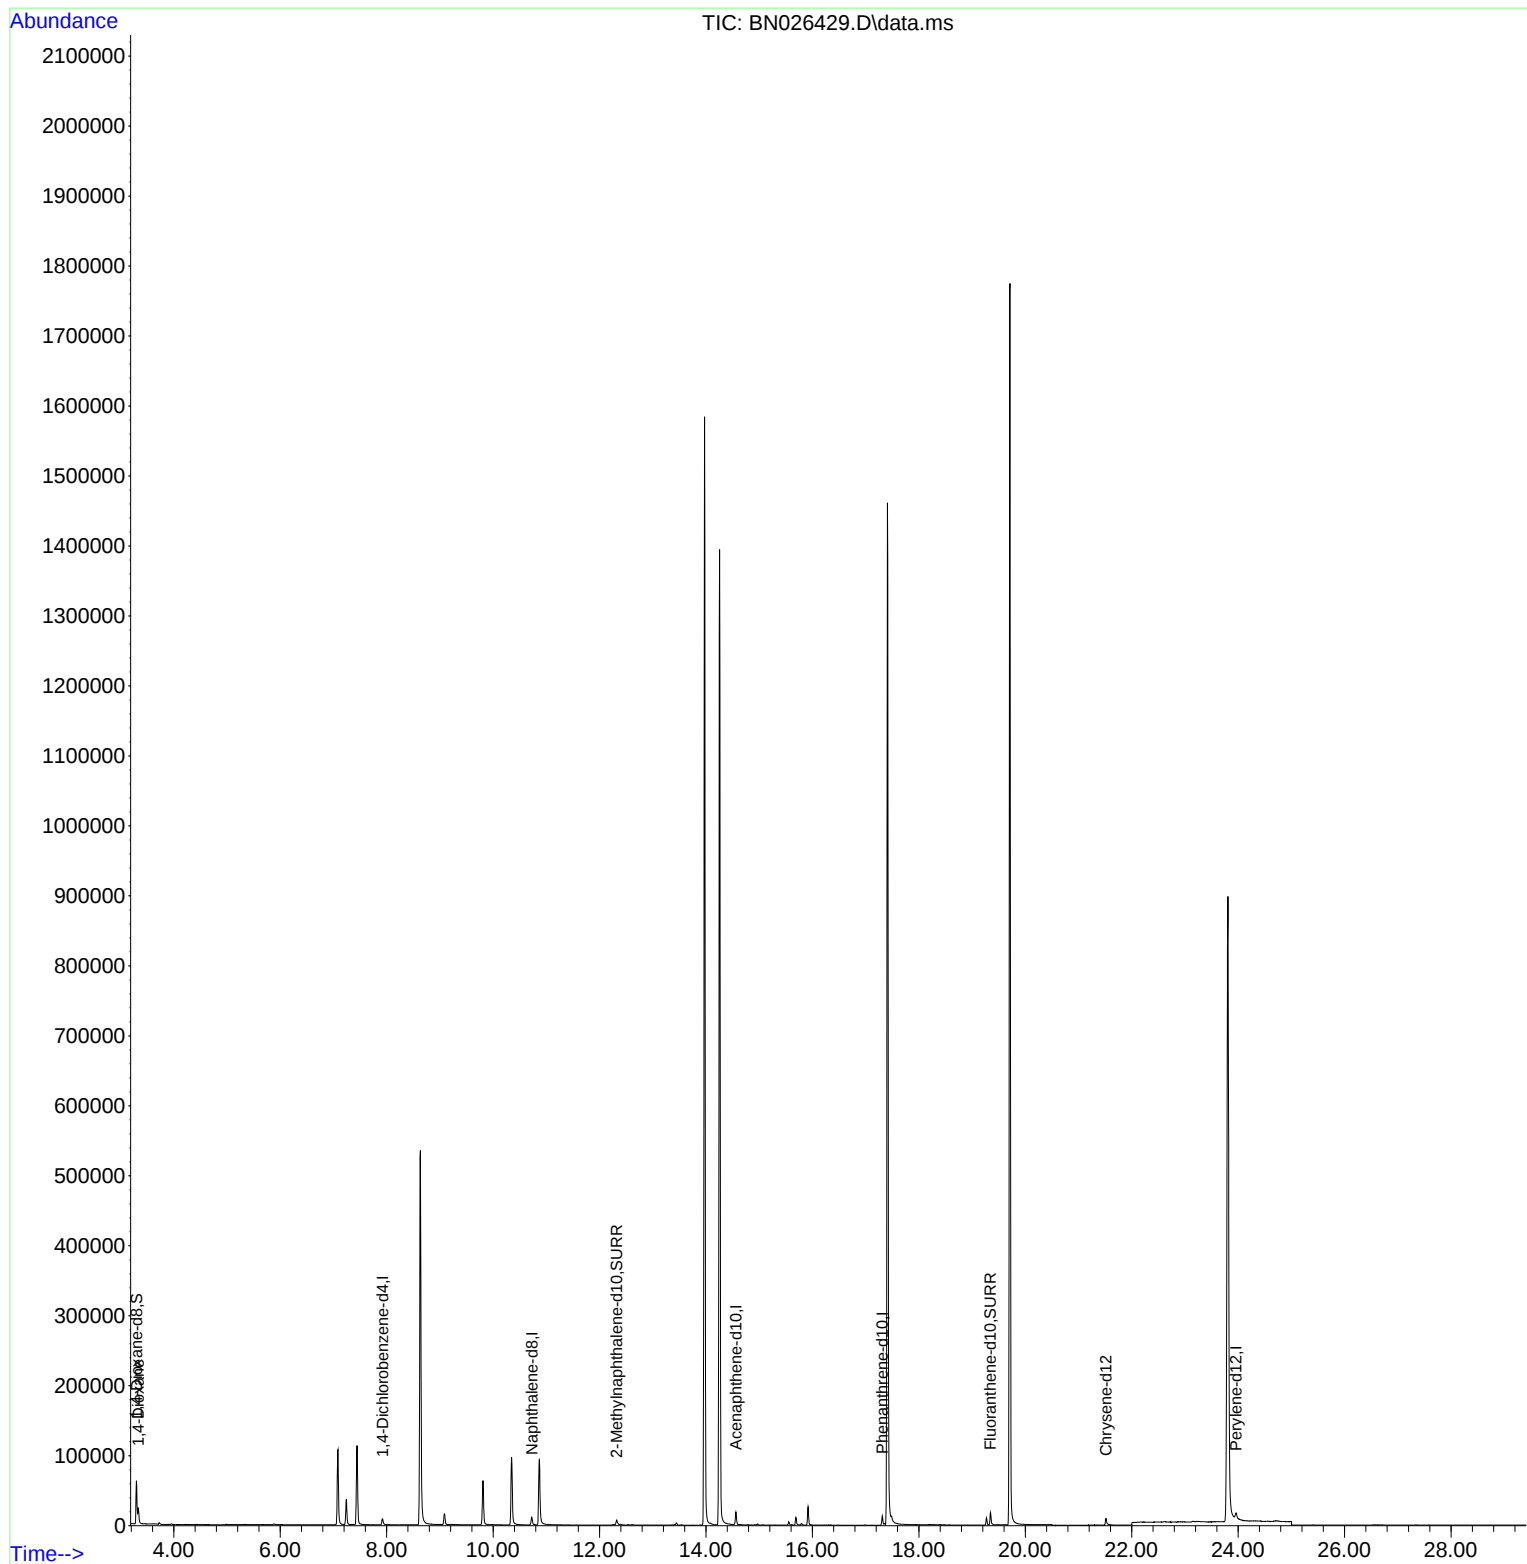

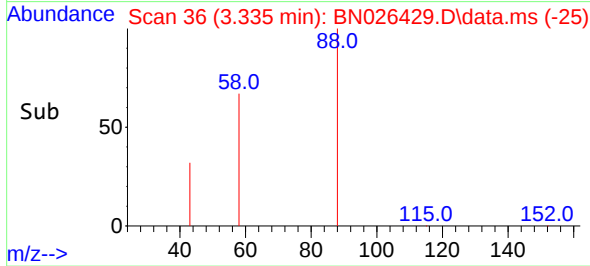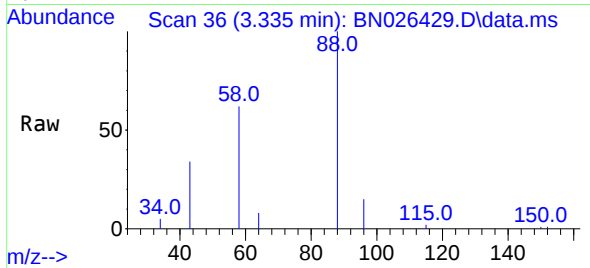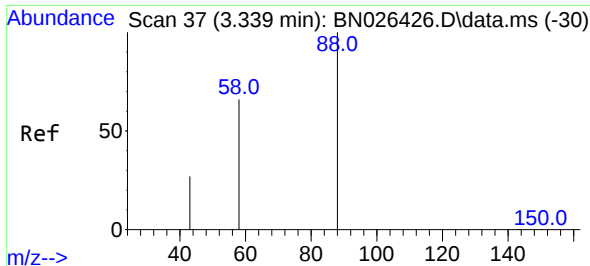

#2
1,4-Dioxane
Concen: 2.209 ng/ul
RT: 3.335 min Scan# 30
Delta R.T. -0.004 min
Lab File: BN026429.D
Acq: 09 Jul 2023 19:07

Instrument :
BNA_N
ClientSampleId :
YBW11

Tgt Ion: 88 Resp: 14840
Ion Ratio Lower Upper
88 100
43 34.2 29.5 44.3
58 62.3 37.4 56.2#

