
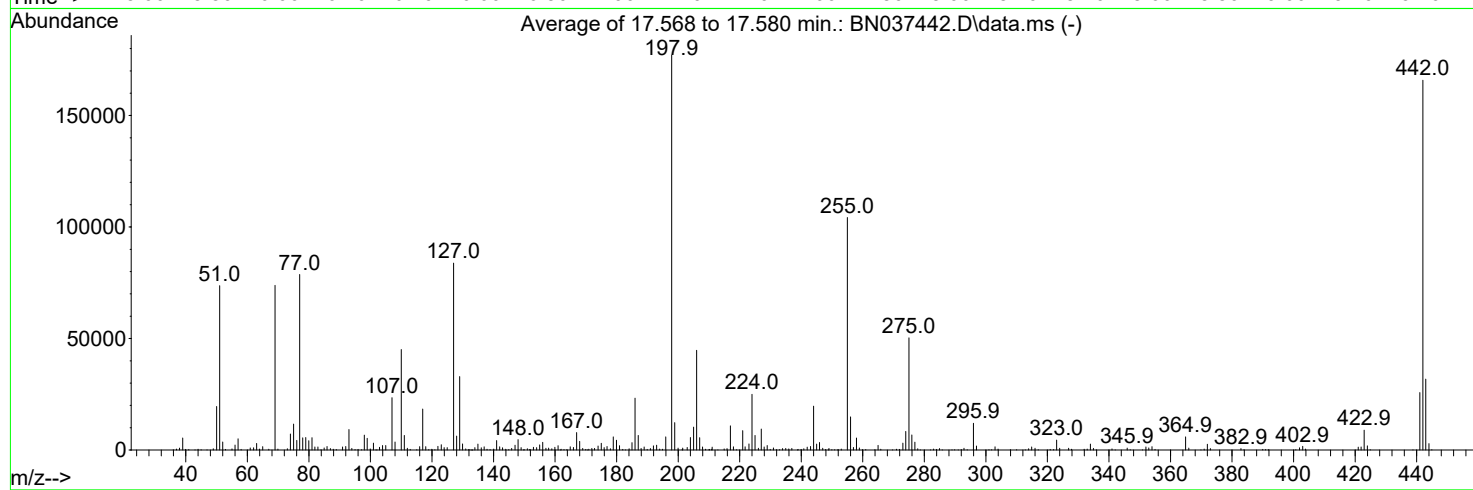


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN070925\  
Data File : BN037442.D  
Acq On : 09 Jul 2025 16:56  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270-SIM-BN070925.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Jul 10 00:48:38 2025

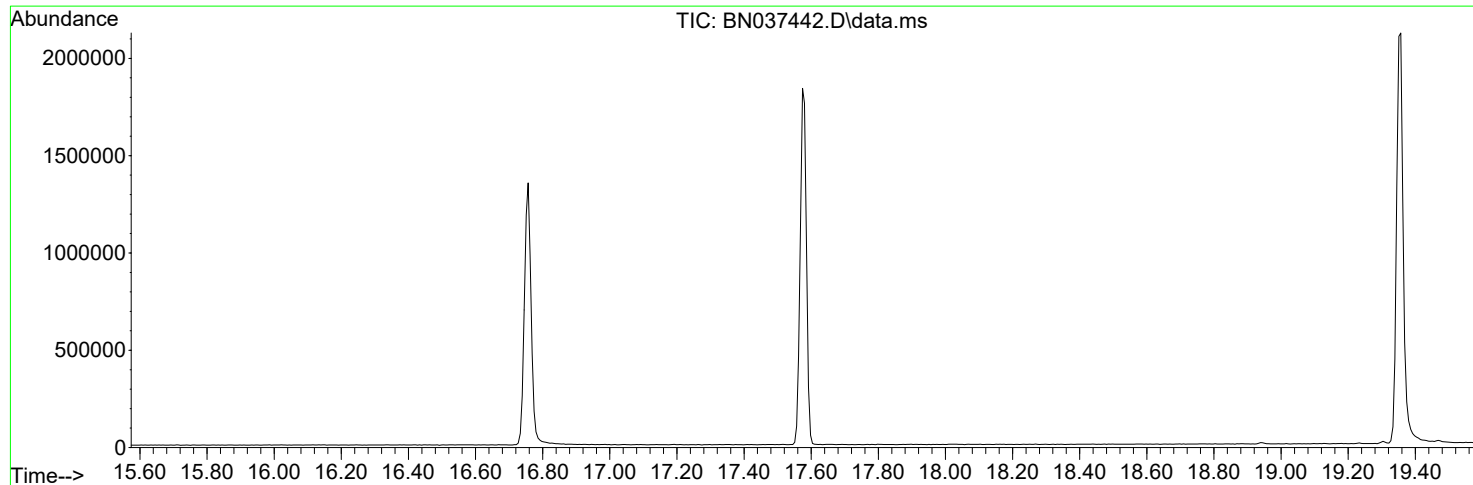

AutoFind: Scans 2462, 2463, 2464; Background Corrected with Scan 2456

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 69              | 100             | 100             | 100.0        | 73827      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 445        | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 177045     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 12252      | PASS                |
| 365            | 198             | 1               | 100             | 3.3          | 5927       | PASS                |
| 441            | 443             | 0.01            | 150             | 81.2         | 25792      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 165811     | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 31773      | PASS                |

### DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 7/9/2025      | BNA_N            | <u>BN037442.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 339451           | 20.604             |
| DDD           | 4419             | 20.157             |
| DDE           | 431              | 19.657             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 4850          | 344301           | 1.41               |
|               |                  |                    |

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN070925\  
Data File : BN037442.D  
Acq On : 09 Jul 2025 16:56  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Jul 10 02:21:08 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 10 02:20:59 2025  
Response via : Initial Calibration

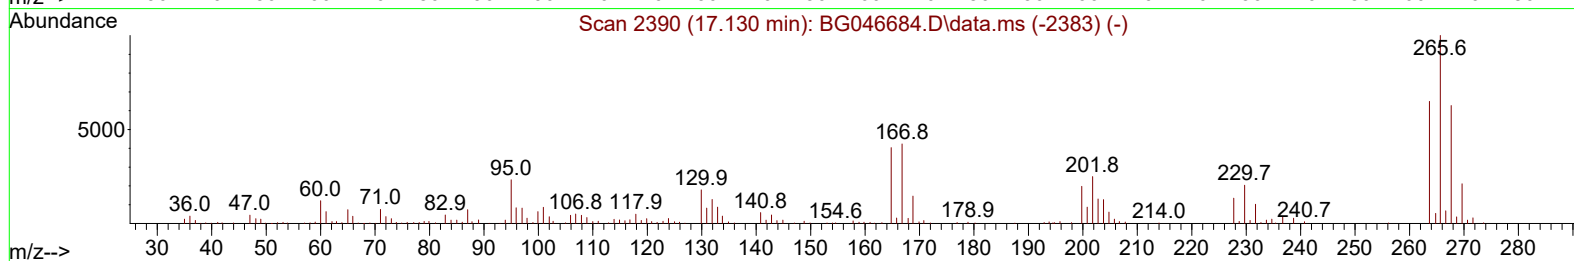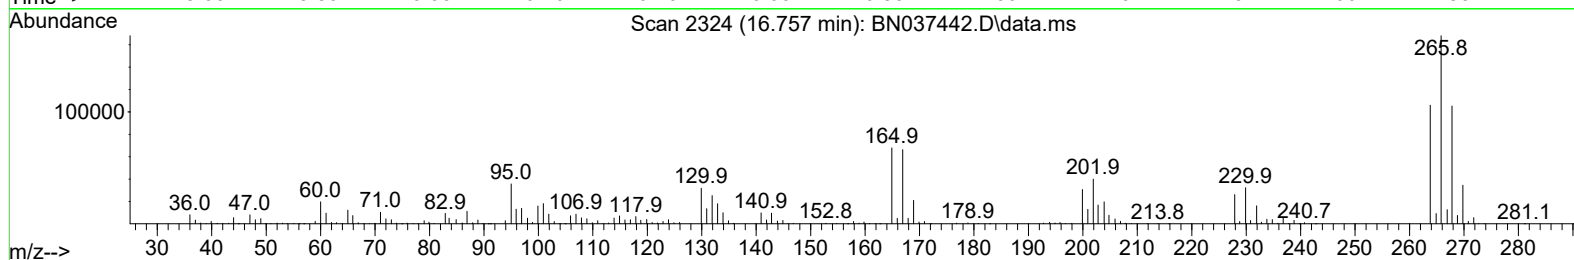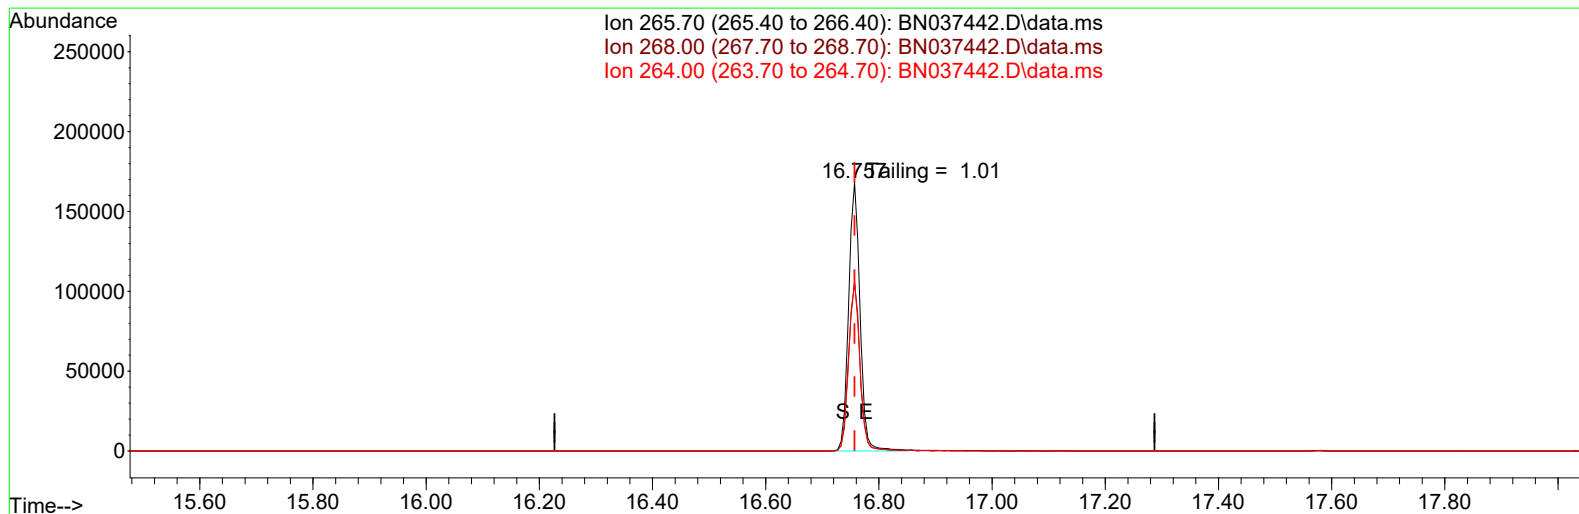

TIC: BN037442.D\data.ms

**(70) Pentachlorophenol (C)**

16.757min ( 0.000) 32738.29 ng




response 236625

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 62.68  |
| 264.00 | 61.60  | 63.09  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN070925\  
Data File : BN037442.D  
Acq On : 09 Jul 2025 16:56  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_N  
ClientSampleId :  
DFTPP

Quant Time: Jul 10 02:21:08 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 10 02:20:59 2025  
Response via : Initial Calibration

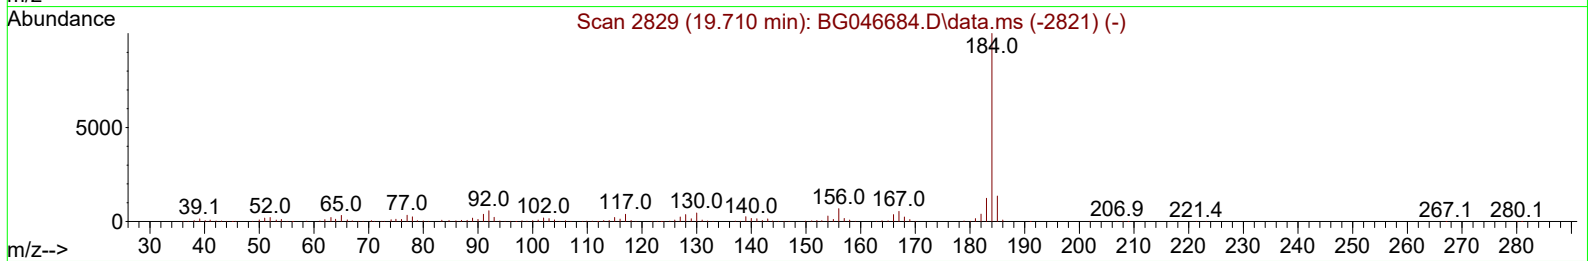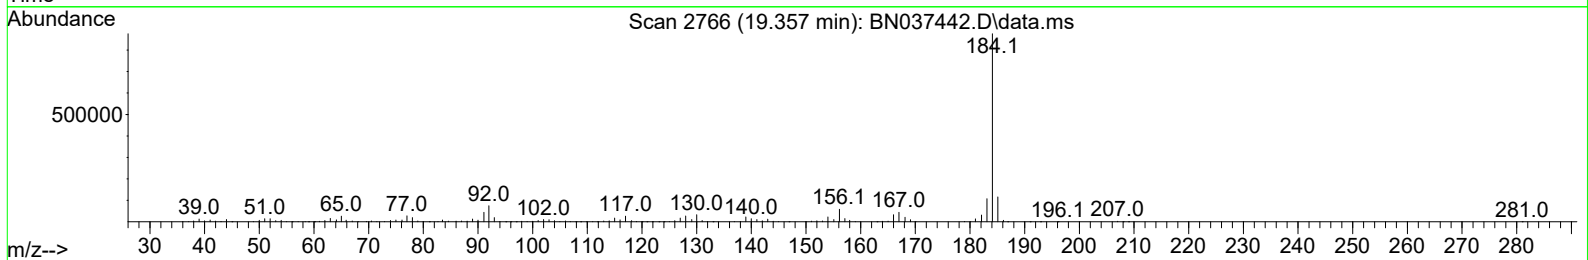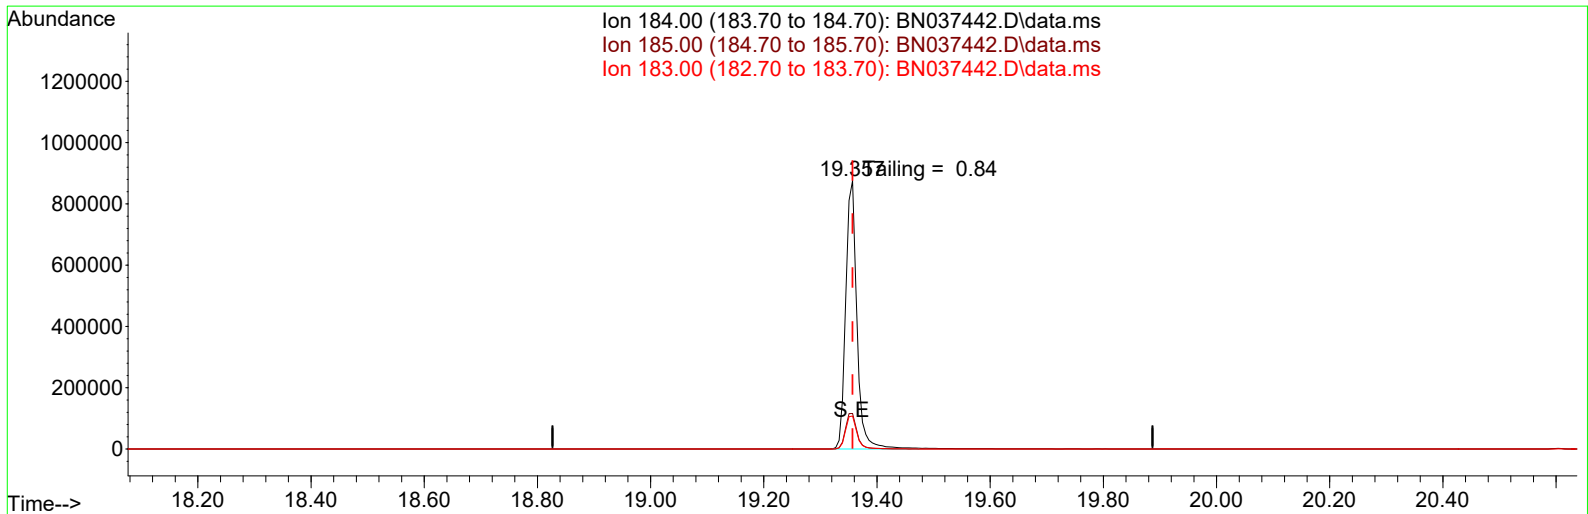

TIC: BN037442.D\data.ms

(77) Benzidine

19.357min ( 0.000) 0.00 ng

response 1214917

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.23  |
| 183.00 | 13.20  | 12.30  |
| 0.00   | 0.00   | 0.00   |