

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071023\
 Data File : BN026445.D
 Acq On : 10 Jul 2023 13:30
 Operator : MA/JU
 Sample : 03404-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 11 04:18:46 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 15:51:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	4826	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.721	136	18497	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.561	164	8056	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.313	188	17270	0.400	ng/ul	-0.01
17) Chrysene-d12	21.514	240	10322	0.400	ng/ul	0.00
23) Perylene-d12	23.961	264	12870	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	19054	3.506	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.326	152	4920	0.173	ng/ul	0.00
18) Fluoranthene-d10	19.345	212	8286	0.211	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.707	202	1627	0.028	ng/ul#	1
26) Benzo(a)pyrene	23.803	252	2391	0.050	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071023\
Data File : BN026445.D
Acq On : 10 Jul 2023 13:30
Operator : MA/JU
Sample : 03404-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 11 04:18:46 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jul 09 15:51:14 2023
Response via : Initial Calibration




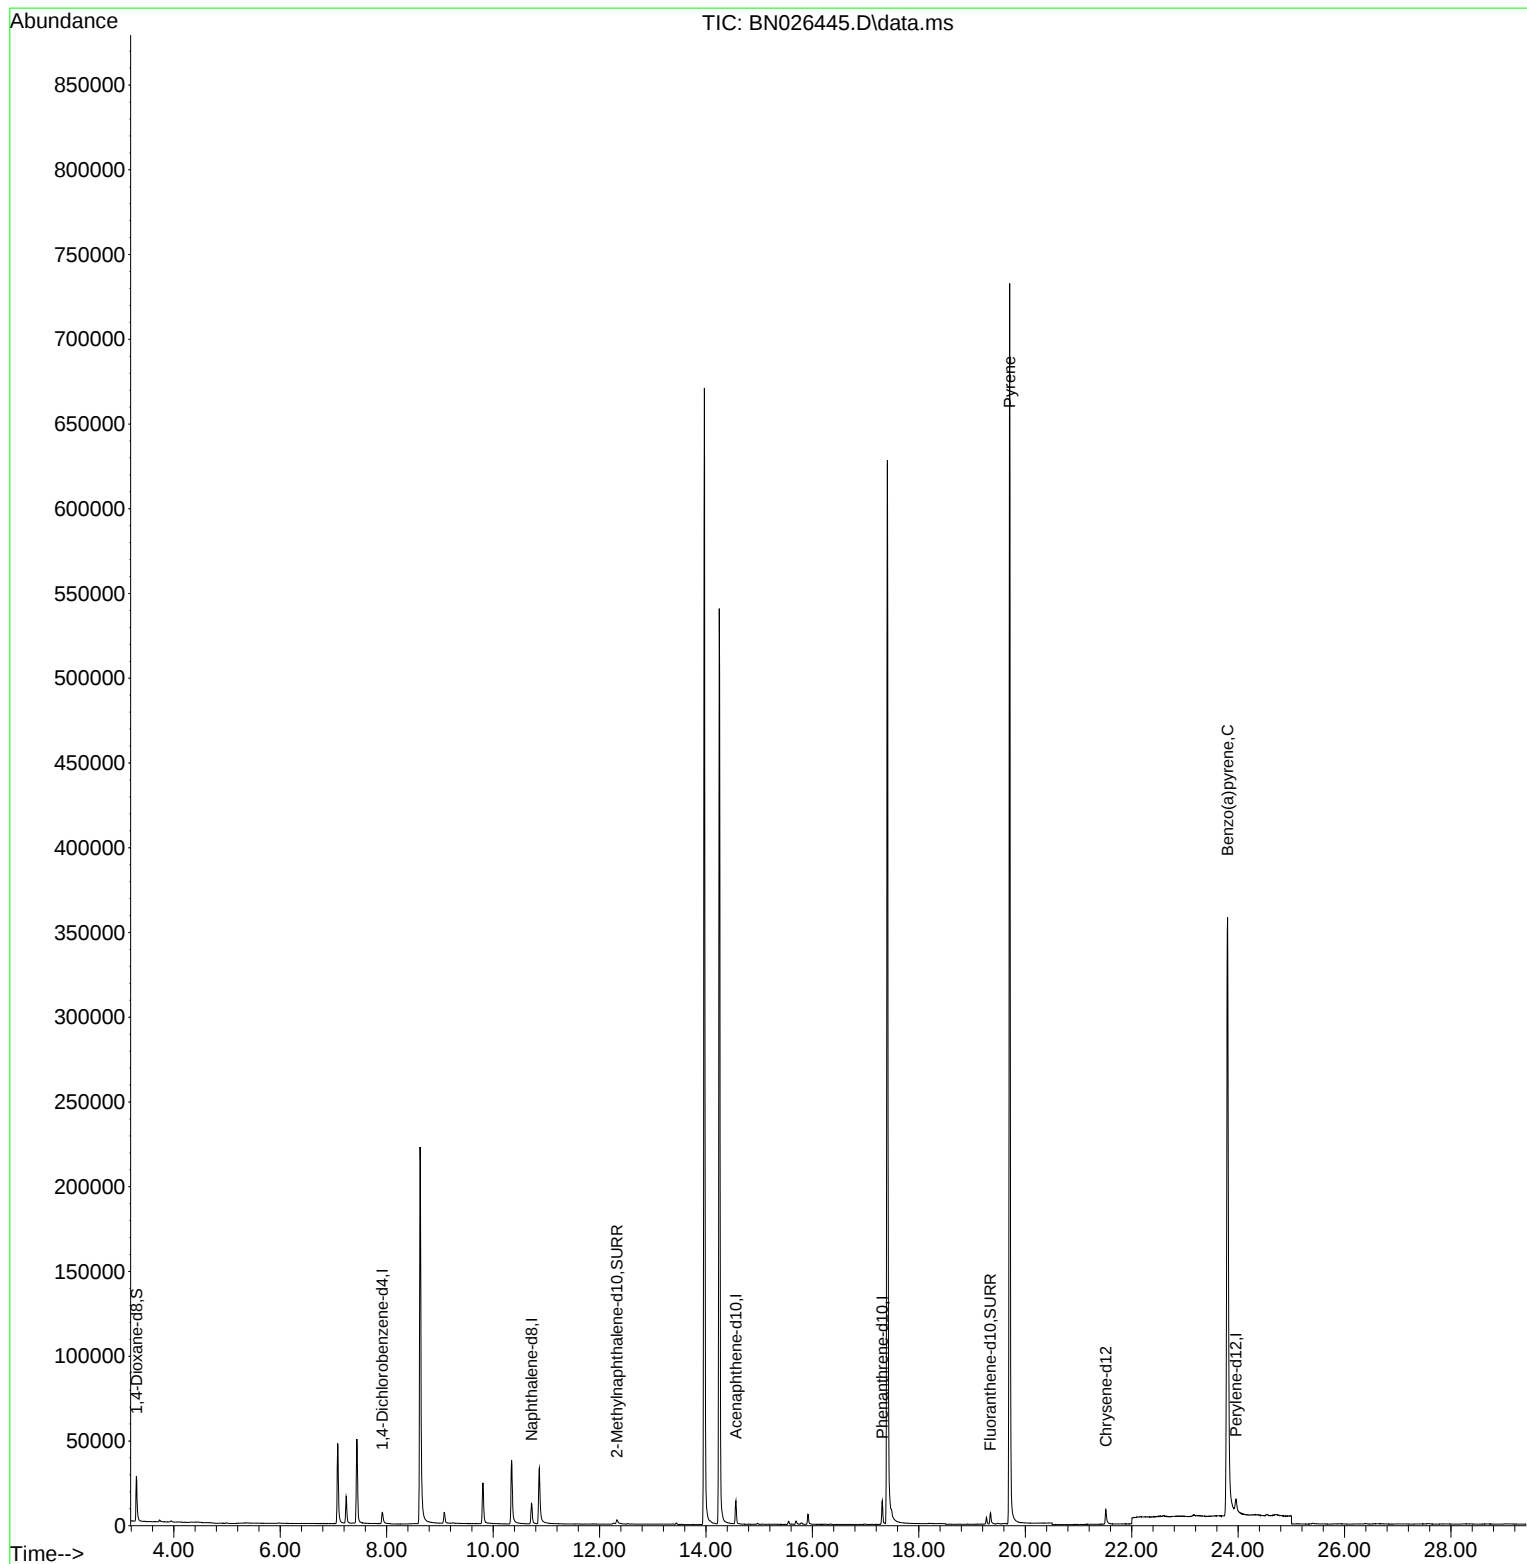


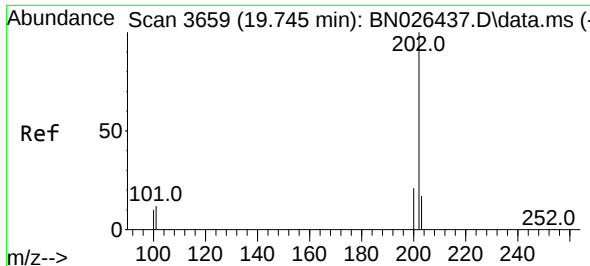

#20
Pyrene
Concen: 0.028 ng/ul
RT: 19.707 min Scan# 30
Delta R.T. -0.042 min
Lab File: BN026445.D
Acq: 10 Jul 2023 13:30

Instrument :
BNA_N
ClientSampleId :

Tgt Ion:202 Resp: 1627
Ion Ratio Lower Upper
202 100
101 183.9 11.4 17.0#
100 1358.8 9.1 13.7#

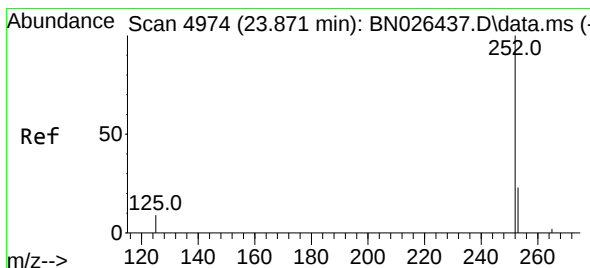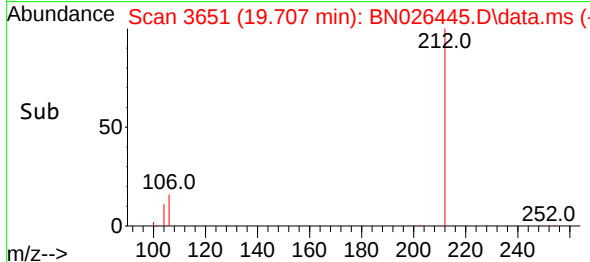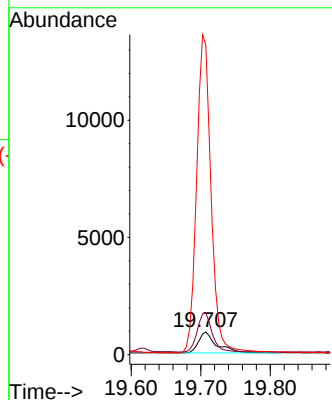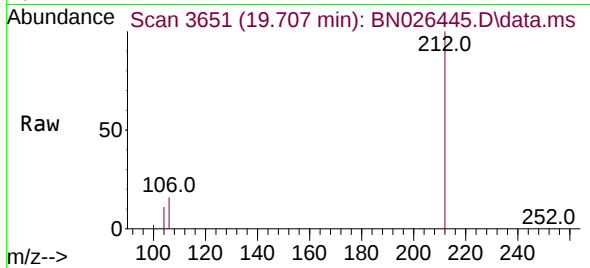

#26
Benzo(a)pyrene
Concen: 0.050 ng/ul
RT: 23.803 min Scan# 4951
Delta R.T. -0.067 min
Lab File: BN026445.D
Acq: 10 Jul 2023 13:30

Tgt Ion:252 Resp: 2391
Ion Ratio Lower Upper
252 100
253 76.2 26.0 39.0#
125 119.4 17.3 25.9#

