

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071023\
 Data File : BN026446.D
 Acq On : 10 Jul 2023 14:07
 Operator : MA/JU
 Sample : 03404-15
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 11 04:18:55 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 15:51:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.921	152	5502	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.726	136	19052	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.561	164	10311	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.313	188	14730	0.400	ng/ul	#-0.01
17) Chrysene-d12	21.517	240	10658	0.400	ng/ul	0.00
23) Perylene-d12	23.949	264	14360	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	23567	3.803	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.321	152	6757	0.231	ng/ul	-0.01
18) Fluoranthene-d10	19.345	212	11278	0.278	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.707	202	2120	0.036	ng/ul#	1
26) Benzo(a)pyrene	23.791	252	3534	0.066	ng/ul#	4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071023\
Data File : BN026446.D
Acq On : 10 Jul 2023 14:07
Operator : MA/JU
Sample : 03404-15
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 11 04:18:55 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jul 09 15:51:14 2023
Response via : Initial Calibration

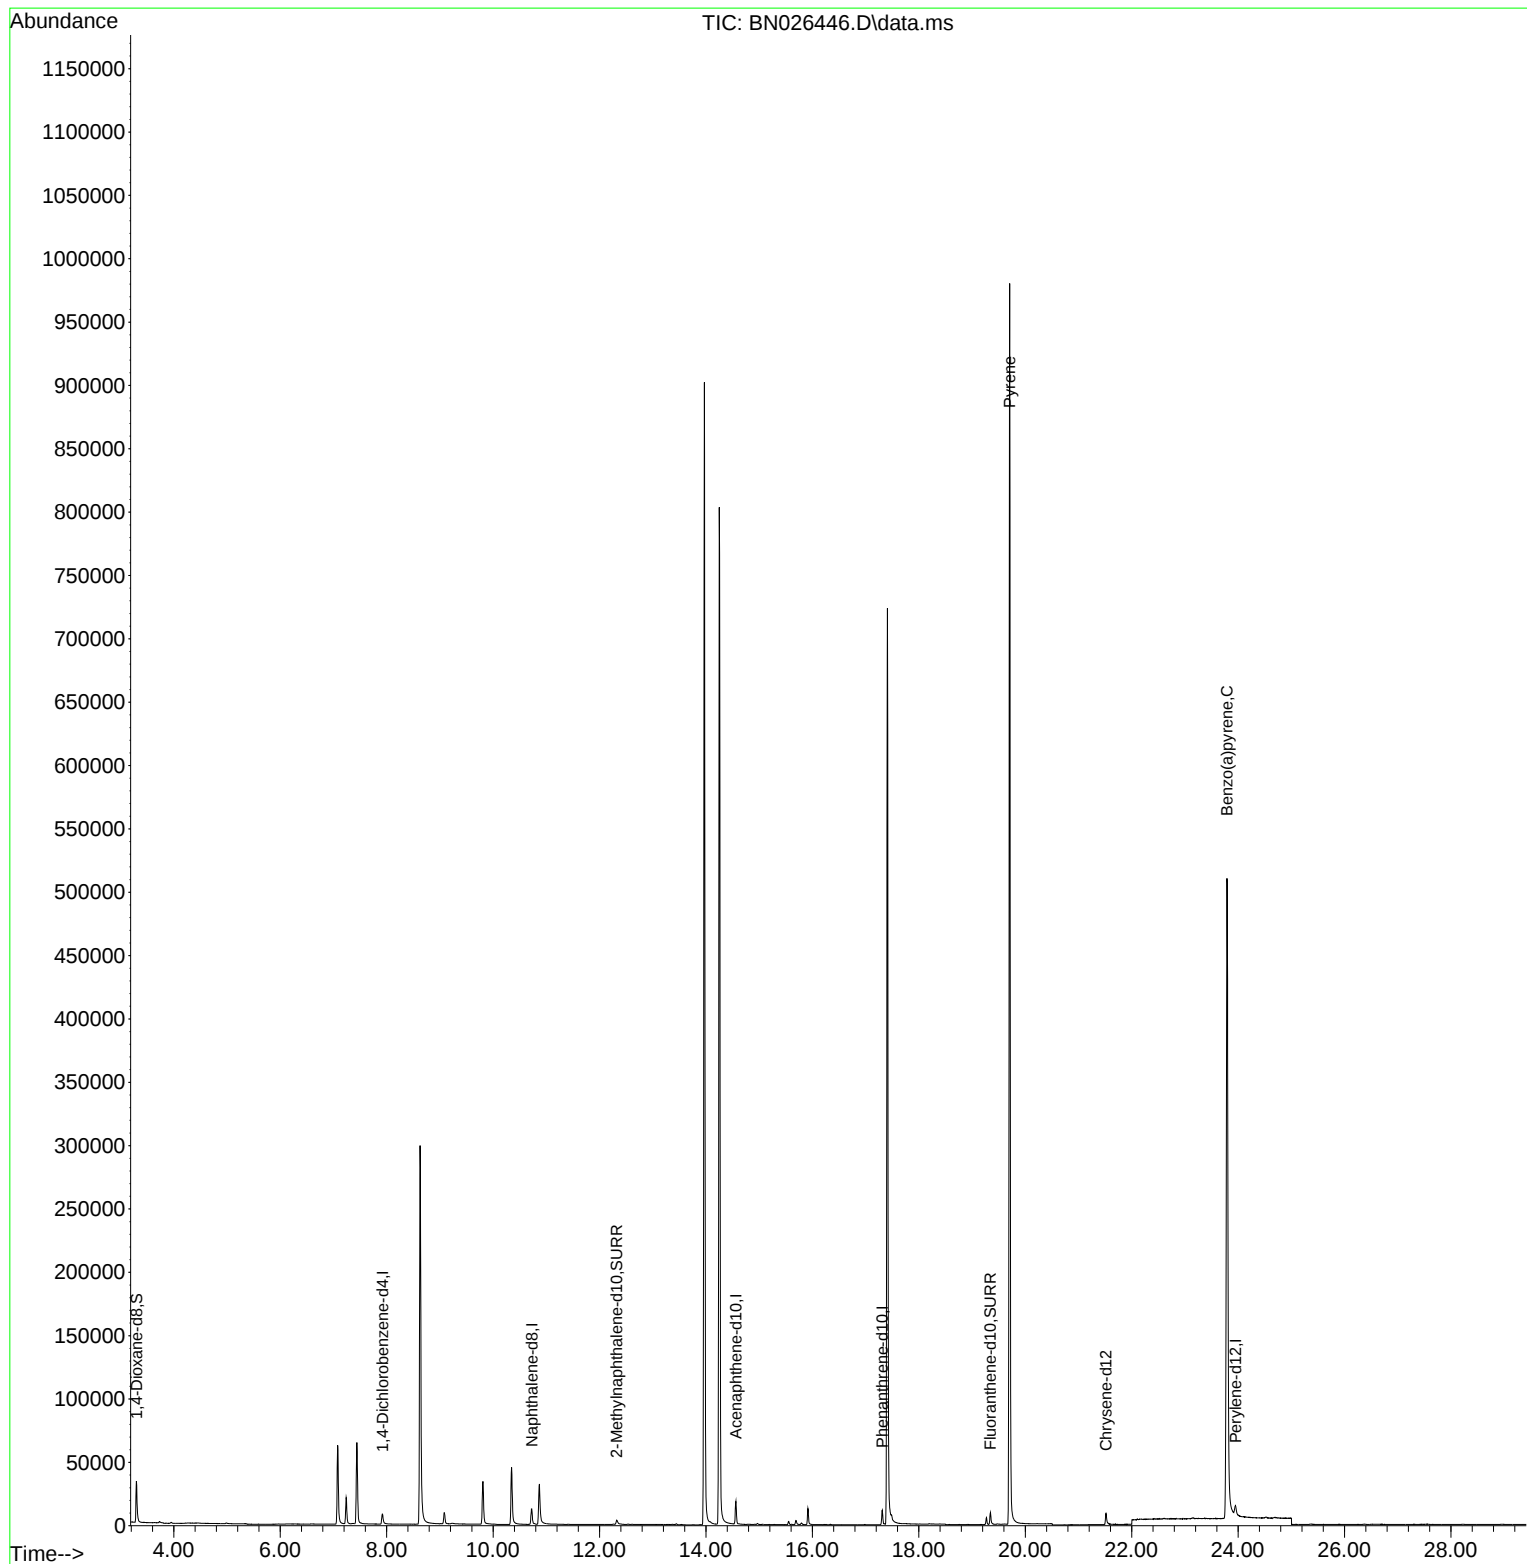

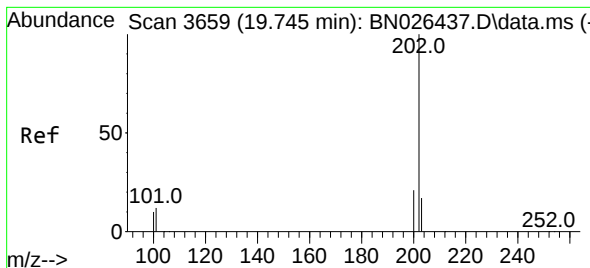

#20

Pyrene

Concen: 0.036 ng/ul

RT: 19.707 min Scan# 3651

Delta R.T. -0.042 min


Lab File: BN026446.D

Acq: 10 Jul 2023 14:07




Instrument :

BNA_N

ClientSampleId :

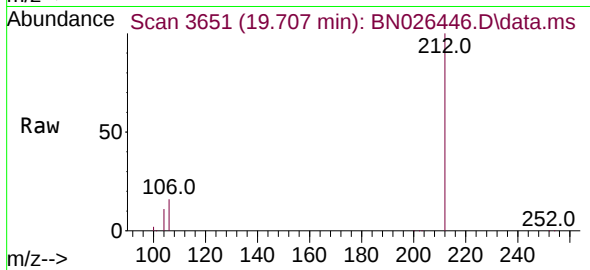

Tgt Ion:	202	Resp:	2120
Ion Ratio	Lower	Upper	
202	100		
101	189.3	11.4	17.0#
100	1419.7	9.1	13.7#

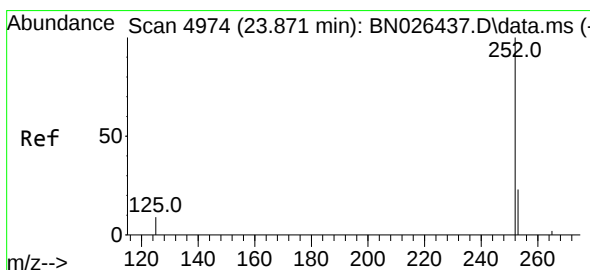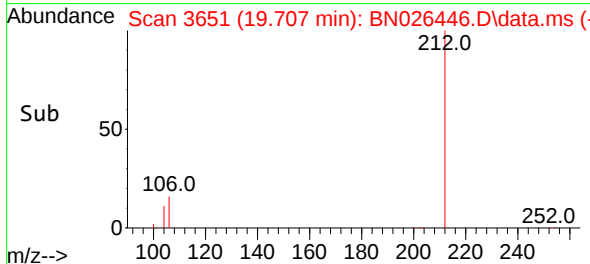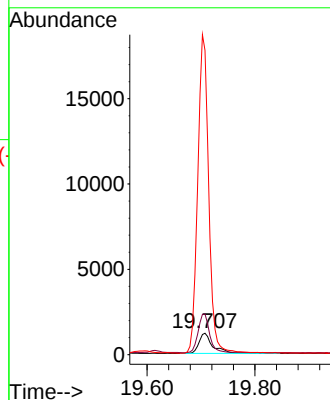

#26

Benzo(a)pyrene

Concen: 0.066 ng/ul

RT: 23.791 min Scan# 4947

Delta R.T. -0.079 min

Lab File: BN026446.D

Acq: 10 Jul 2023 14:07

Tgt Ion:	252	Resp:	3534
Ion Ratio	Lower	Upper	
252	100		
253	68.5	26.0	39.0#
125	90.0	17.3	25.9#

