

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071023\
 Data File : BN026447.D
 Acq On : 10 Jul 2023 14:43
 Operator : MA/JU
 Sample : 03404-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 11 04:19:04 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 15:51:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.921	152	4670	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.721	136	15809	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.561	164	8785	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.313	188	15370	0.400	ng/ul	-0.01
17) Chrysene-d12	21.520	240	8559	0.400	ng/ul	0.00
23) Perylene-d12	23.964	264	12369	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	25717	4.890	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.321	152	7482	0.308	ng/ul	-0.01
18) Fluoranthene-d10	19.345	212	12674	0.389	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.707	202	2313	0.049	ng/ul#	1
26) Benzo(a)pyrene	23.803	252	3794	0.083	ng/ul#	2


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071023\
Data File : BN026447.D
Acq On : 10 Jul 2023 14:43
Operator : MA/JU
Sample : 03404-16
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 11 04:19:04 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jul 09 15:51:14 2023
Response via : Initial Calibration

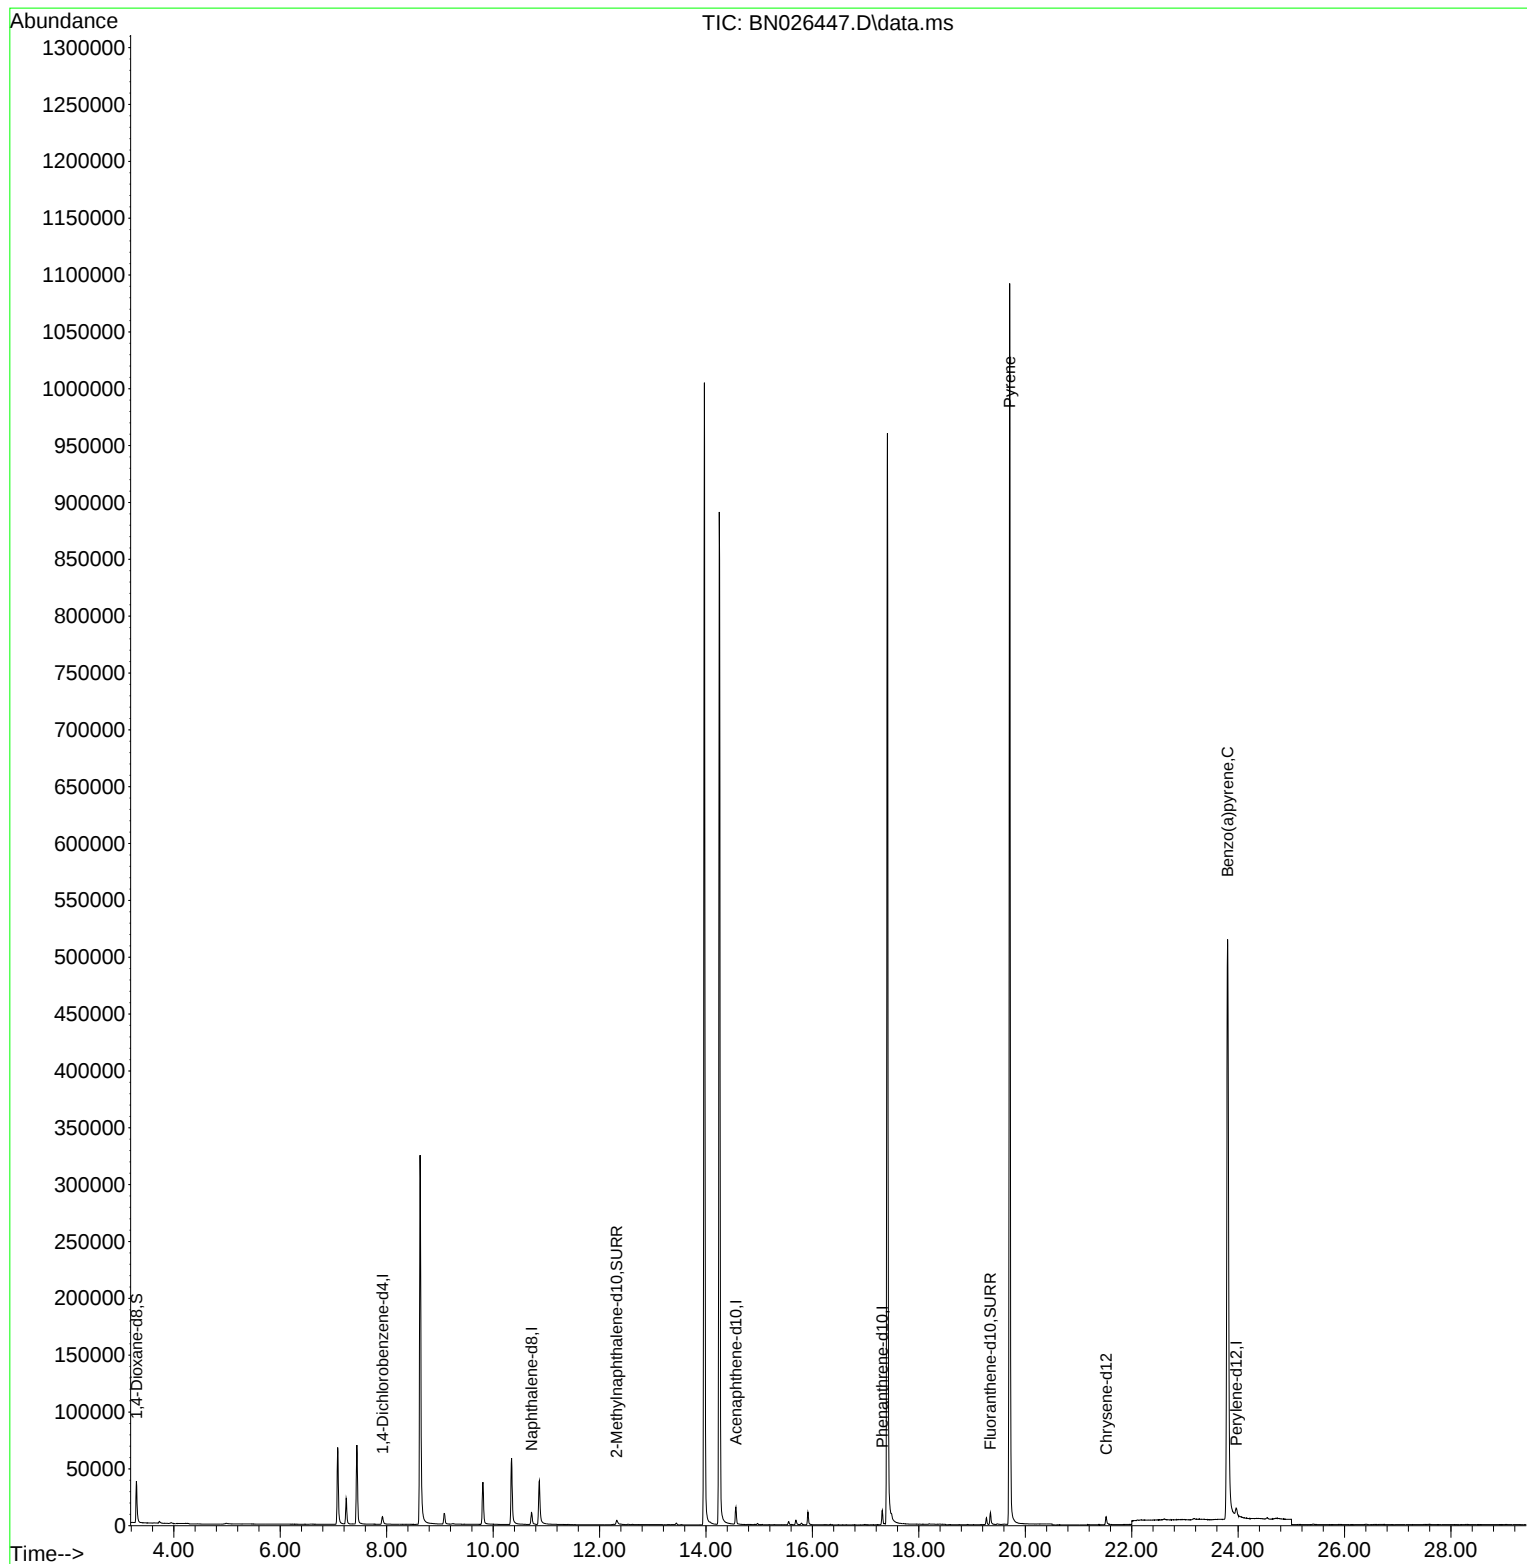

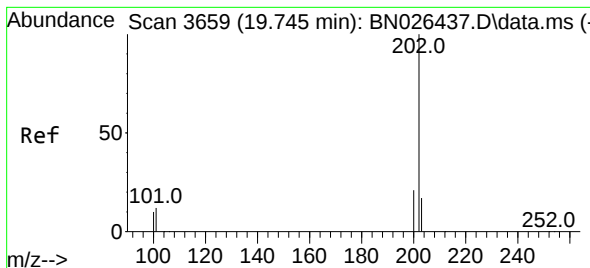

#20

Pyrene

Concen: 0.049 ng/ul

RT: 19.707 min Scan# 30

Delta R.T. -0.042 min


Lab File: BN026447.D

Acq: 10 Jul 2023 14:43




Instrument :

BNA_N

ClientSampleId :

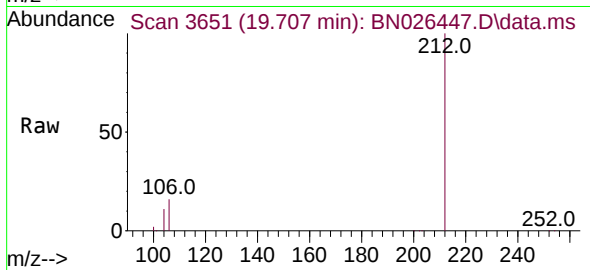

Tgt Ion:	202	Resp:	2313
Ion Ratio	Lower	Upper	
202	100		
101	193.2	11.4	17.0#
100	1494.0	9.1	13.7#

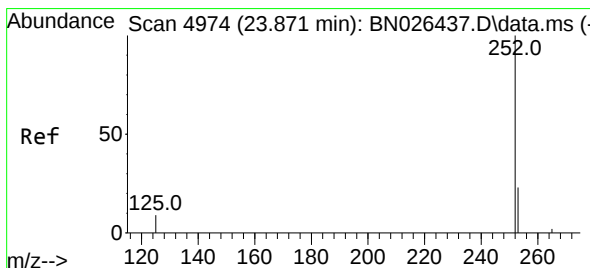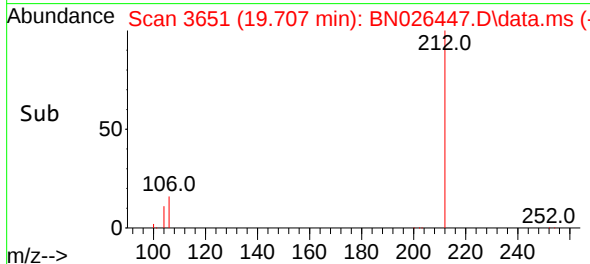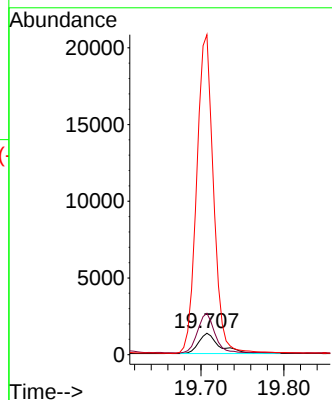

#26

Benzo(a)pyrene

Concen: 0.083 ng/ul

RT: 23.803 min Scan# 4951

Delta R.T. -0.067 min

Lab File: BN026447.D

Acq: 10 Jul 2023 14:43

Tgt Ion:	252	Resp:	3794
Ion Ratio	Lower	Upper	
252	100		
253	64.1	26.0	39.0#
125	97.3	17.3	25.9#

