

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071023\
 Data File : BN026448.D
 Acq On : 10 Jul 2023 15:20
 Operator : MA/JU
 Sample : 03404-17
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 11 04:19:14 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 15:51:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.921	152	5251	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.721	136	18032	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.562	164	9692	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.314	188	16677	0.400	ng/ul	-0.01
17) Chrysene-d12	21.516	240	9711	0.400	ng/ul	0.00
23) Perylene-d12	23.960	264	12580	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	20269	3.428	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.327	152	5479	0.198	ng/ul	0.00
18) Fluoranthene-d10	19.346	212	8421	0.228	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.708	202	1761	0.033	ng/ul#	1
26) Benzo(a)pyrene	23.805	252	2806	0.060	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071023\
Data File : BN026448.D
Acq On : 10 Jul 2023 15:20
Operator : MA/JU
Sample : 03404-17
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Jul 11 04:19:14 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jul 09 15:51:14 2023
Response via : Initial Calibration

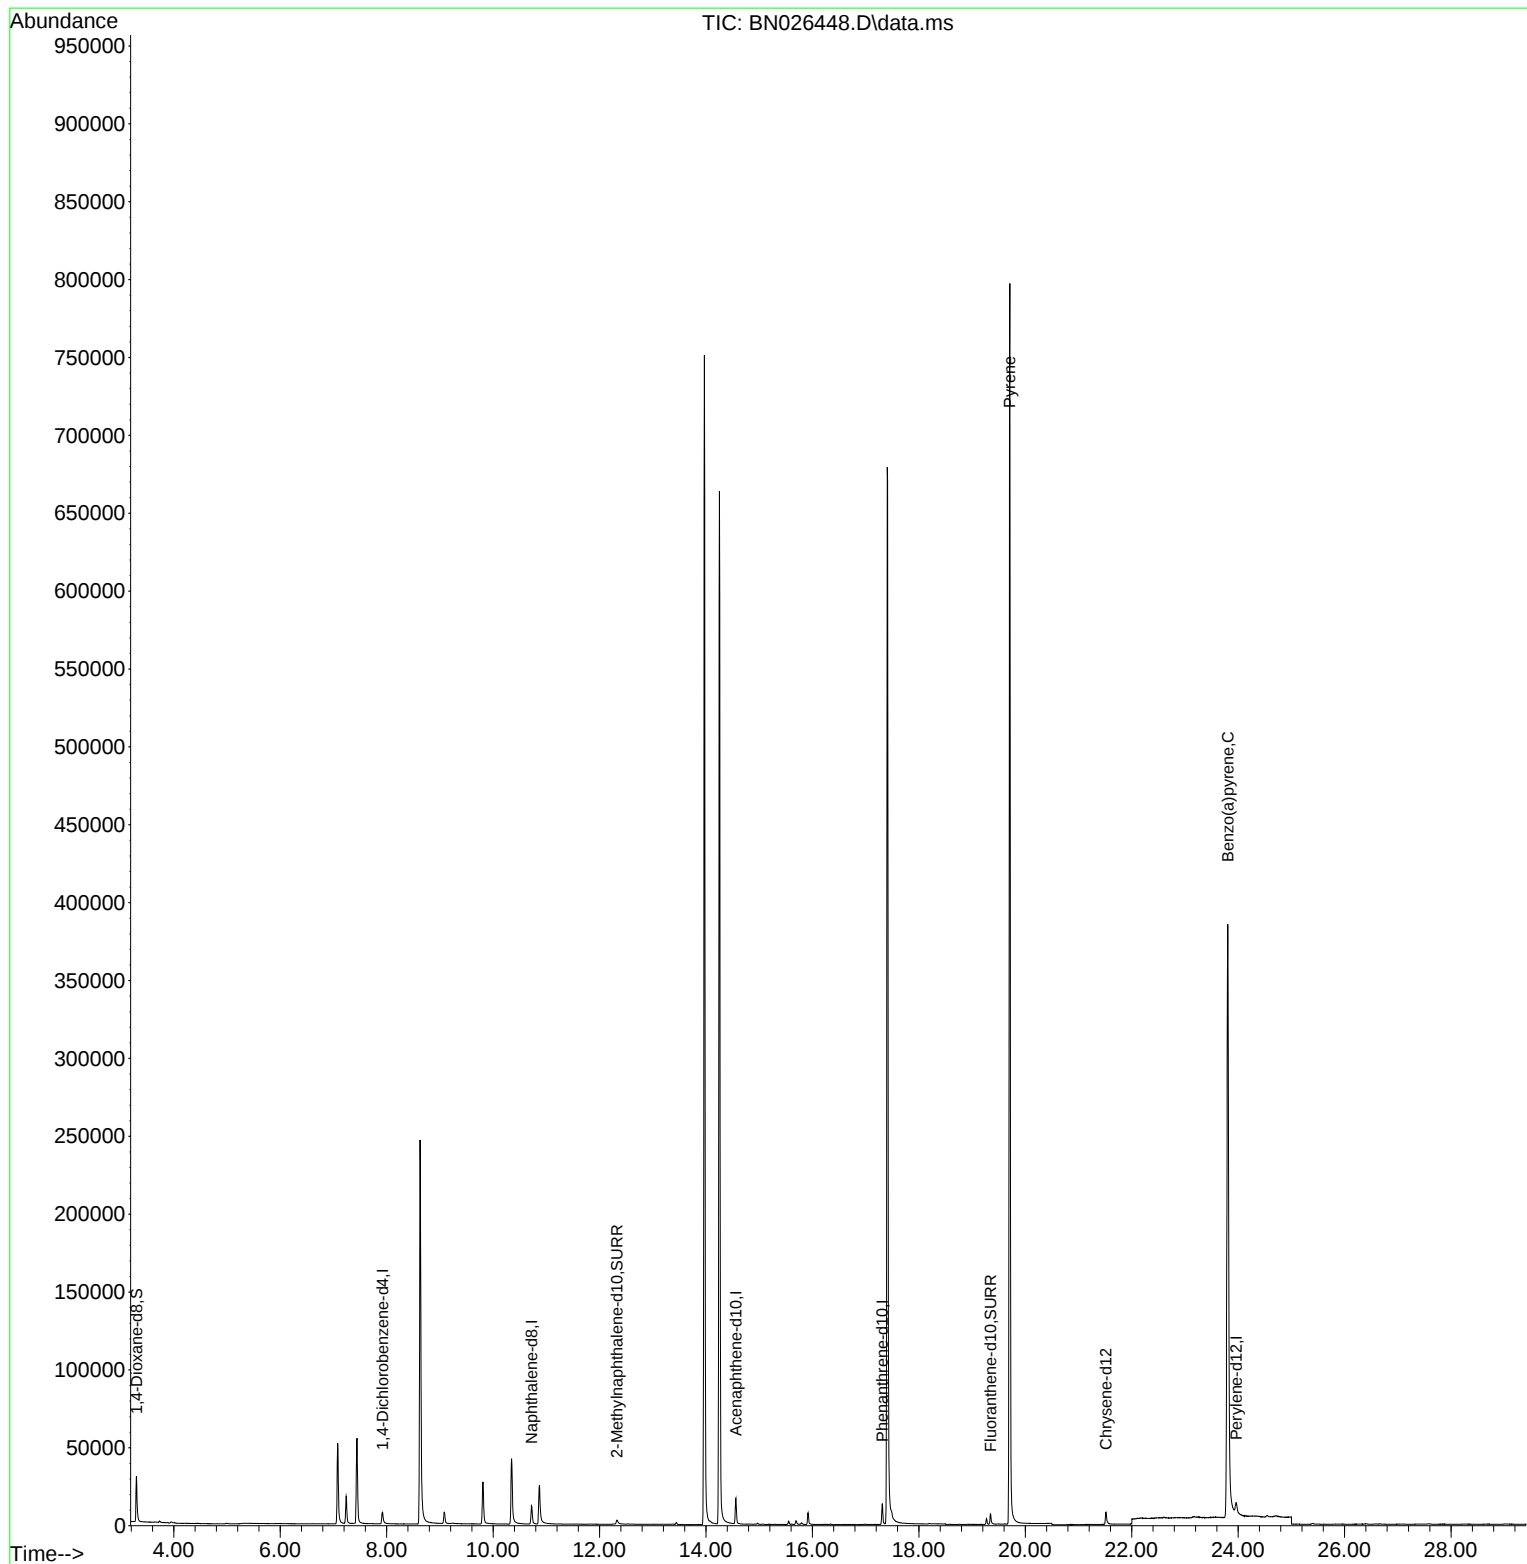



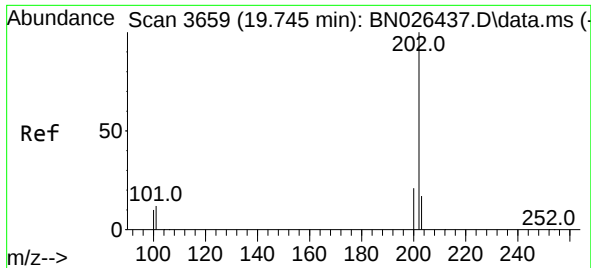


#20
Pyrene
Concen: 0.033 ng/ul
RT: 19.708 min Scan# 3651
Delta R.T. -0.041 min
Lab File: BN026448.D
Acq: 10 Jul 2023 15:20

Instrument :
BNA_N
ClientSampleId :

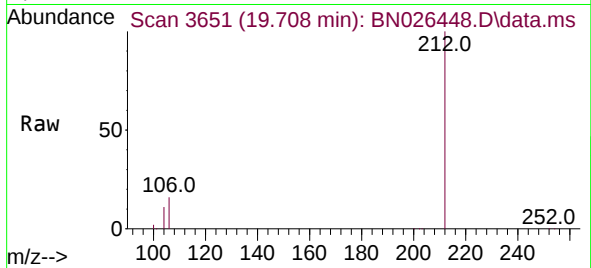

Tgt Ion:202 Resp: 1761
Ion Ratio Lower Upper
202 100
101 186.1 11.4 17.0#
100 1387.2 9.1 13.7#

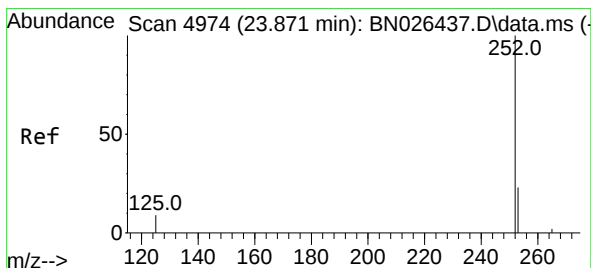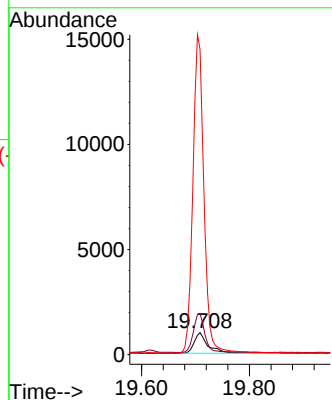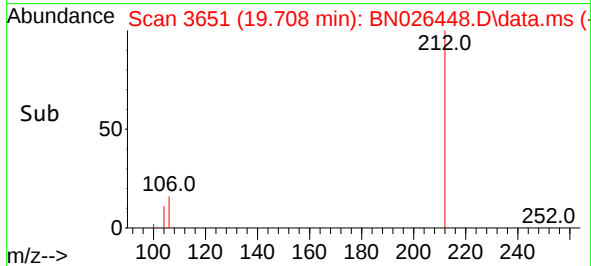

#26
Benzo(a)pyrene
Concen: 0.060 ng/ul
RT: 23.805 min Scan# 4952
Delta R.T. -0.065 min
Lab File: BN026448.D
Acq: 10 Jul 2023 15:20

Tgt Ion:252 Resp: 2806
Ion Ratio Lower Upper
252 100
253 74.6 26.0 39.0#
125 102.0 17.3 25.9#

