

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006790.D
 Acq On : 11 Jul 2019 10:40
 Operator : HP/JU
 Sample : PB121038BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 12 03:52:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 11 02:31:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	3496	0.40	ng/ul	-0.03
2) Naphthalene-d8	10.35	136	12625	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	6670	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	979493	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.31	264	970088	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	5718	0.29	ng/ul	-0.02
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.24	166	1773	0.061	ng/ul#	Ovalue 13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
Data File : BN006790.D
Acq On : 11 Jul 2019 10:40
Operator : HP/JU
Sample : PB121038BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 12 03:52:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 02:31:55 2019
Response via : Initial Calibration

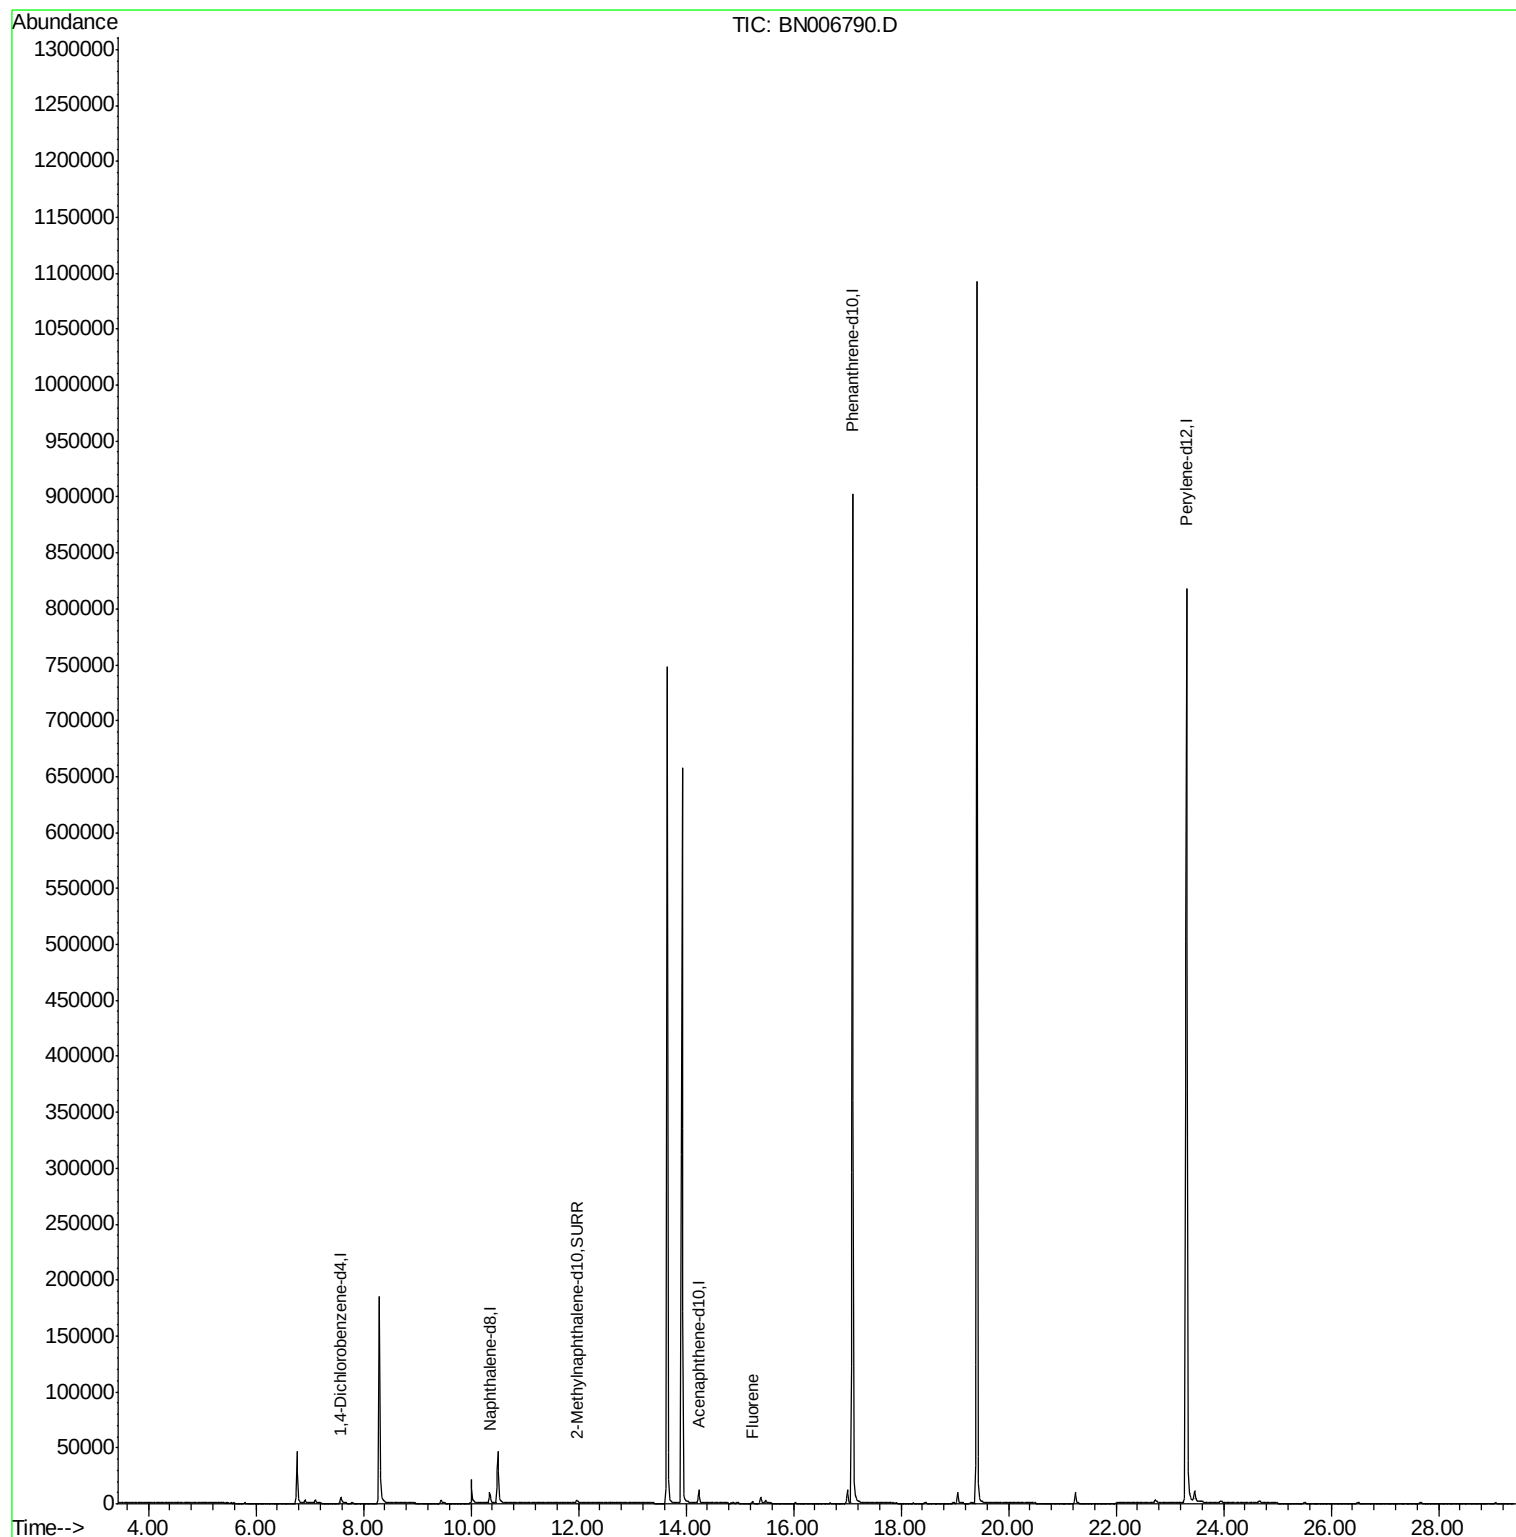

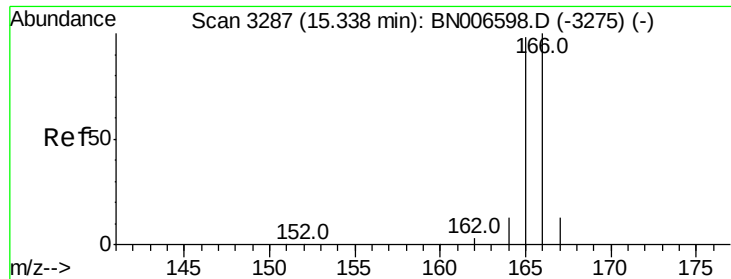

#9

Fluorene

Concen: 0.061 ng/ul

RT: 15.24 min Scan# 3266

Delta R.T. -0.07 min

Lab File: BN006790.D

Acq: 11 Jul 2019 10:40

Instrument :

BNA_N

ClientSampleId :



Tot Ion:166 Resp: 1773

Ion Ratio Lower Upper

166 100

165 8.1 78.2 117.4#

167 38.2 11.3 16.9#

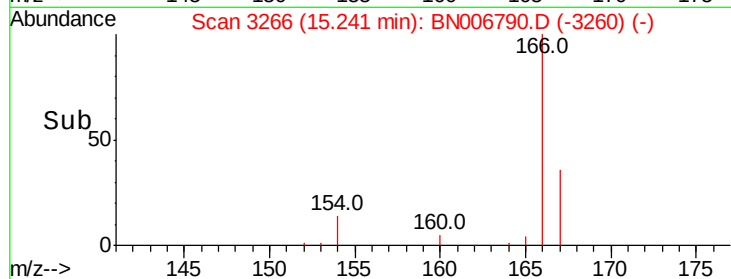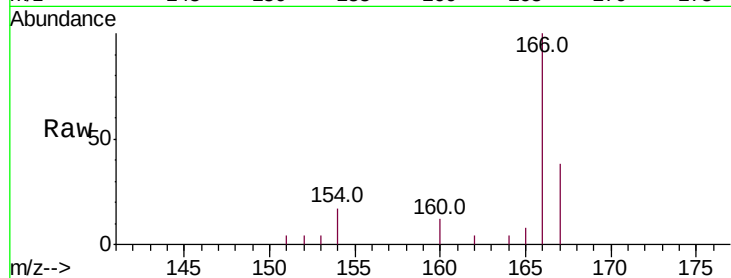

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

