

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006792.D
 Acq On : 11 Jul 2019 11:50
 Operator : HP/JU
 Sample : K3578-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 12 03:52:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 11 02:31:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	3454	0.40	ng/ul	-0.03
2) Naphthalene-d8	10.35	136	12646	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	6887	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	1272989	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.31	264	1212811	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	7179	0.37	ng/ul	-0.02
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.24	166	2297	0.076	ng/ul#	14




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
Data File : BN006792.D
Acq On : 11 Jul 2019 11:50
Operator : HP/JU
Sample : K3578-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 12 03:52:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 02:31:55 2019
Response via : Initial Calibration

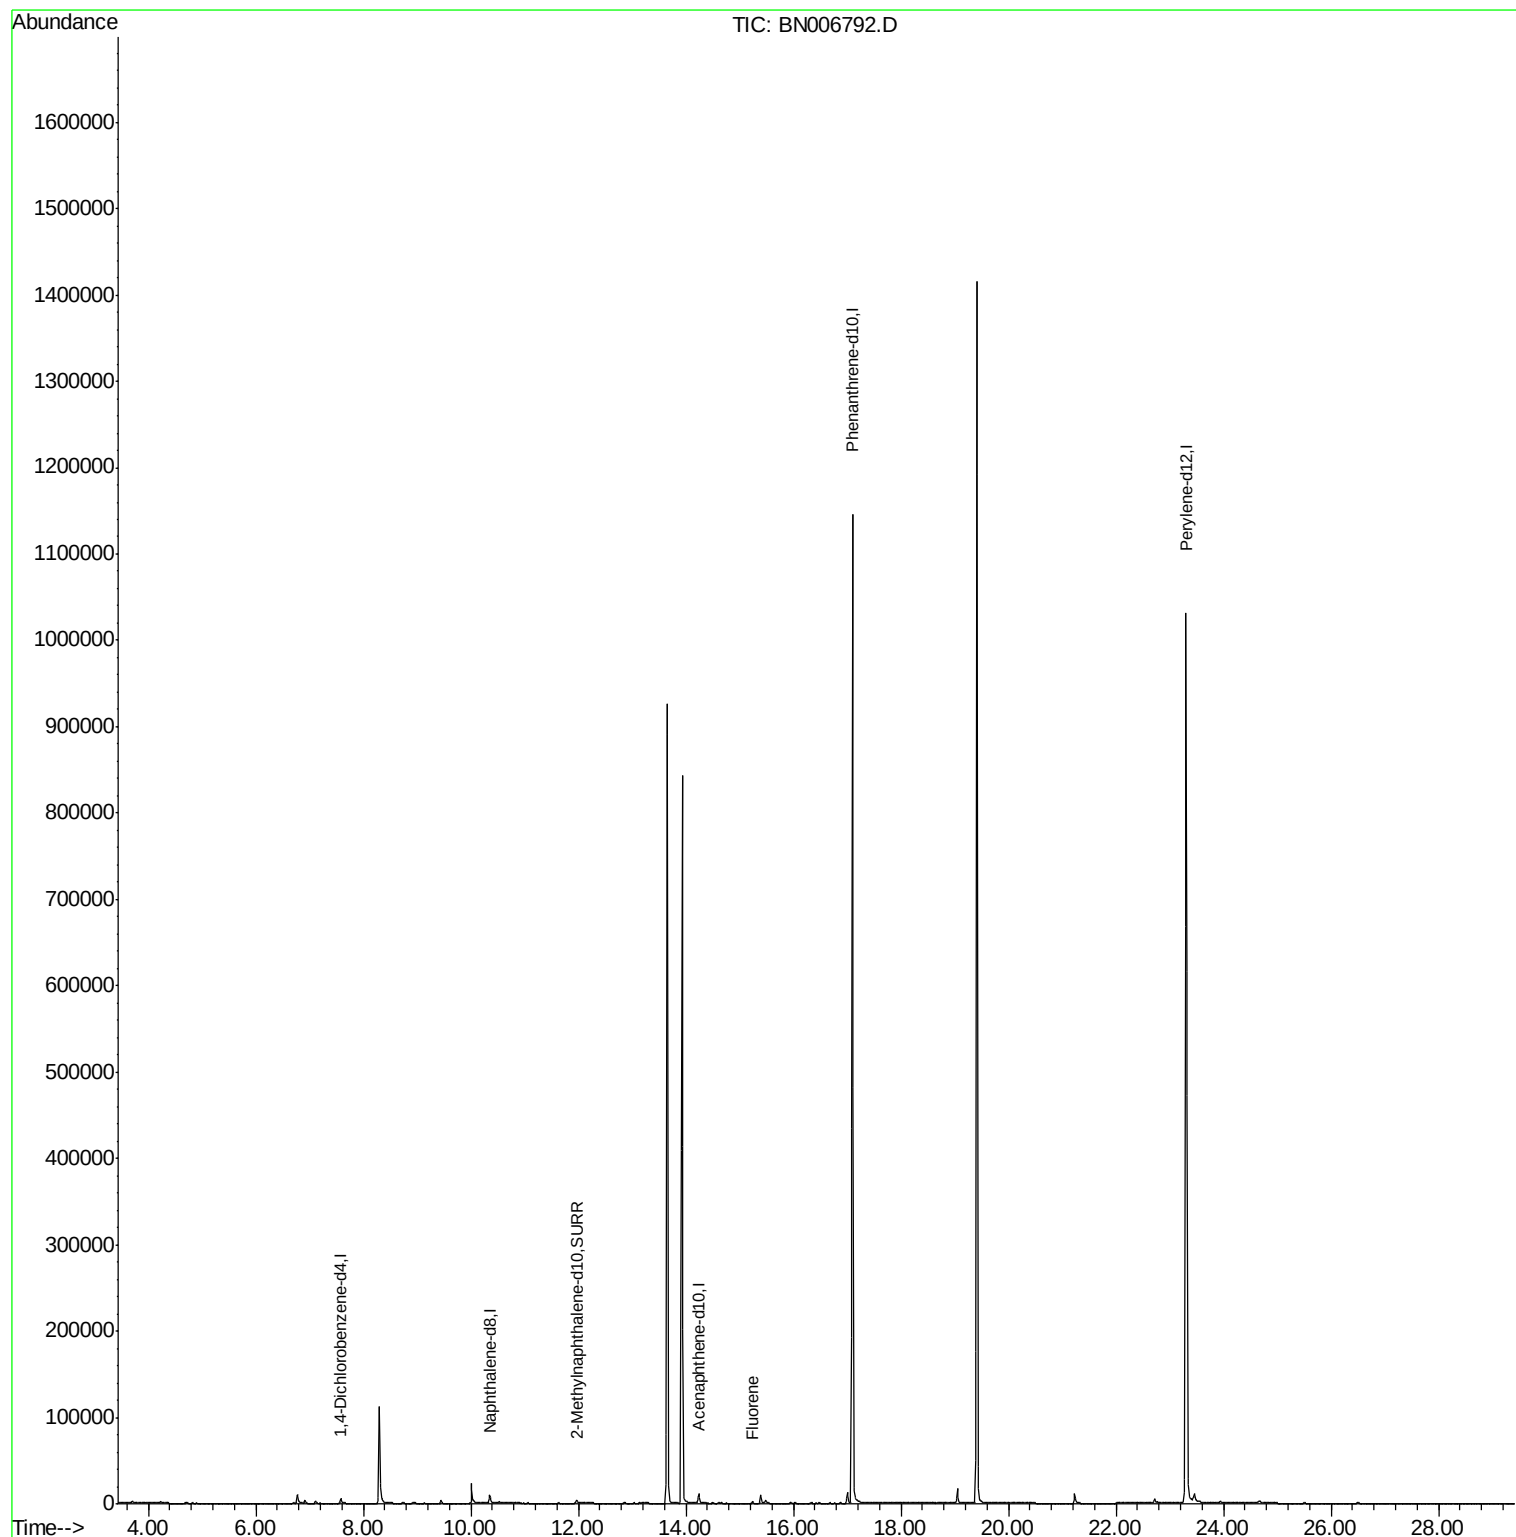

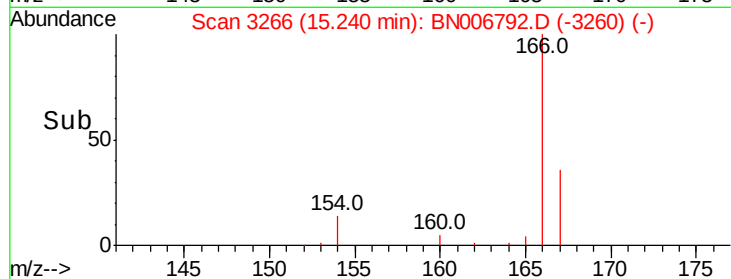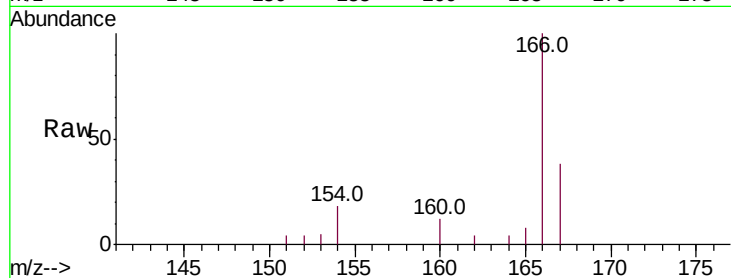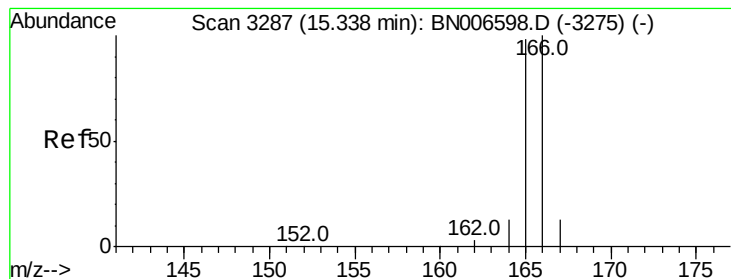

#9

Fluorene

Concen: 0.076 ng/ul

RT: 15.24 min Scan# 3266

Delta R.T. -0.07 min

Lab File: BN006792.D

Acq: 11 Jul 2019 11:50

Instrument :

BNA_N

ClientSampleId :

Tot Ion:166 Resp: 2297

Ion Ratio Lower Upper

166 100

165 8.4 78.2 117.4#

167 37.9 11.3 16.9#

