

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006793.D
 Acq On : 11 Jul 2019 12:25
 Operator : HP/JU
 Sample : K3578-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 12 03:52:22 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 11 02:31:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	3184	0.40	ng/ul	-0.03
2) Naphthalene-d8	10.35	136	11453	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	7651	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	1033071	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.31	264	975919	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.96	152	6680	0.38	ng/ul	-0.02
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
3) Naphthalene	10.40	128	4466	0.136	ng/ul#	1




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
Data File : BN006793.D
Acq On : 11 Jul 2019 12:25
Operator : HP/JU
Sample : K3578-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 12 03:52:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 02:31:55 2019
Response via : Initial Calibration

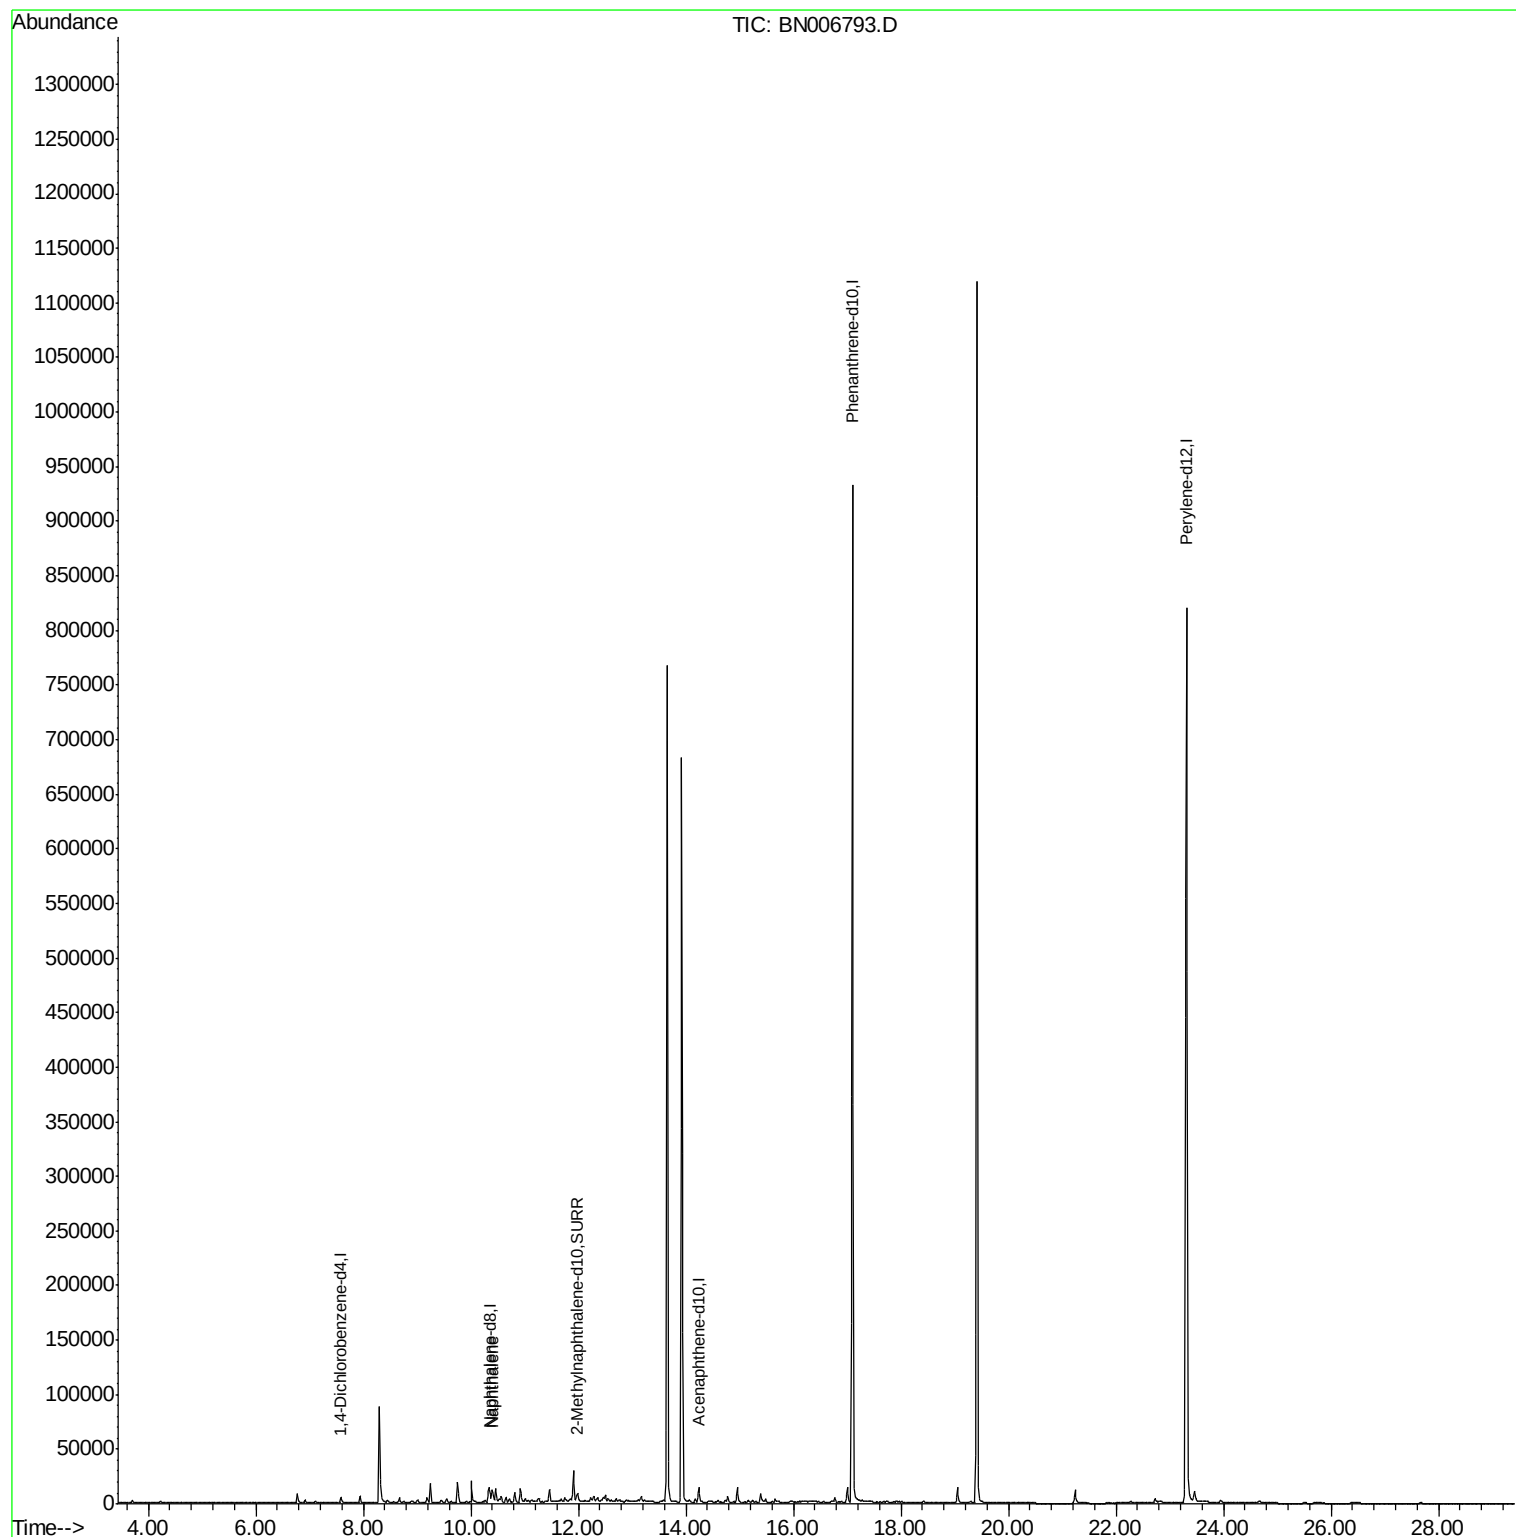

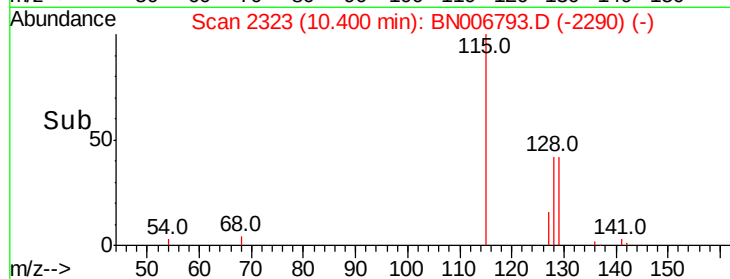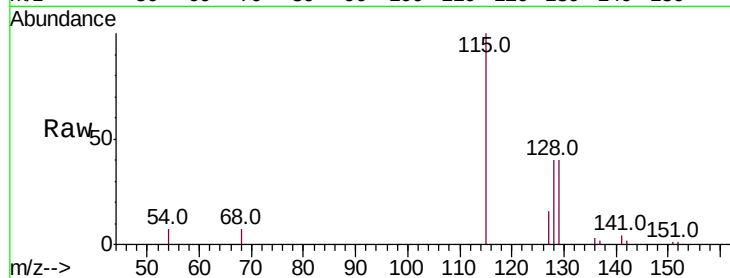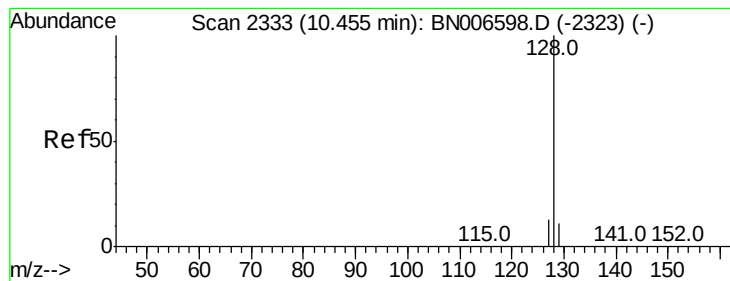

#3

Naphthalene

Concen: 0.136 ng/ul

RT: 10.40 min Scan# 2323

Delta R.T. -0.02 min

Lab File: BN006793.D

Acq: 11 Jul 2019 12:25

Instrument :

BNA_N

ClientSampleId :

Tot Ion:128 Resp: 4466

Ion Ratio Lower Upper

128 100

129 100.4 9.4 14.0#

127 39.6 10.6 16.0#

