

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006805.D
 Acq On : 11 Jul 2019 19:21
 Operator : HP/JU
 Sample : PB121054BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 12 03:53:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 11 02:31:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	2214	0.40	ng/ul	-0.03
2) Naphthalene-d8	10.36	136	7976	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	4170	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	763254	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.30	264	600244	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	3578	0.29	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.24	166	1332	0.073	ng/ul#	Ovalue 16


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
Data File : BN006805.D
Acq On : 11 Jul 2019 19:21
Operator : HP/JU
Sample : PB121054BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 12 03:53:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 02:31:55 2019
Response via : Initial Calibration

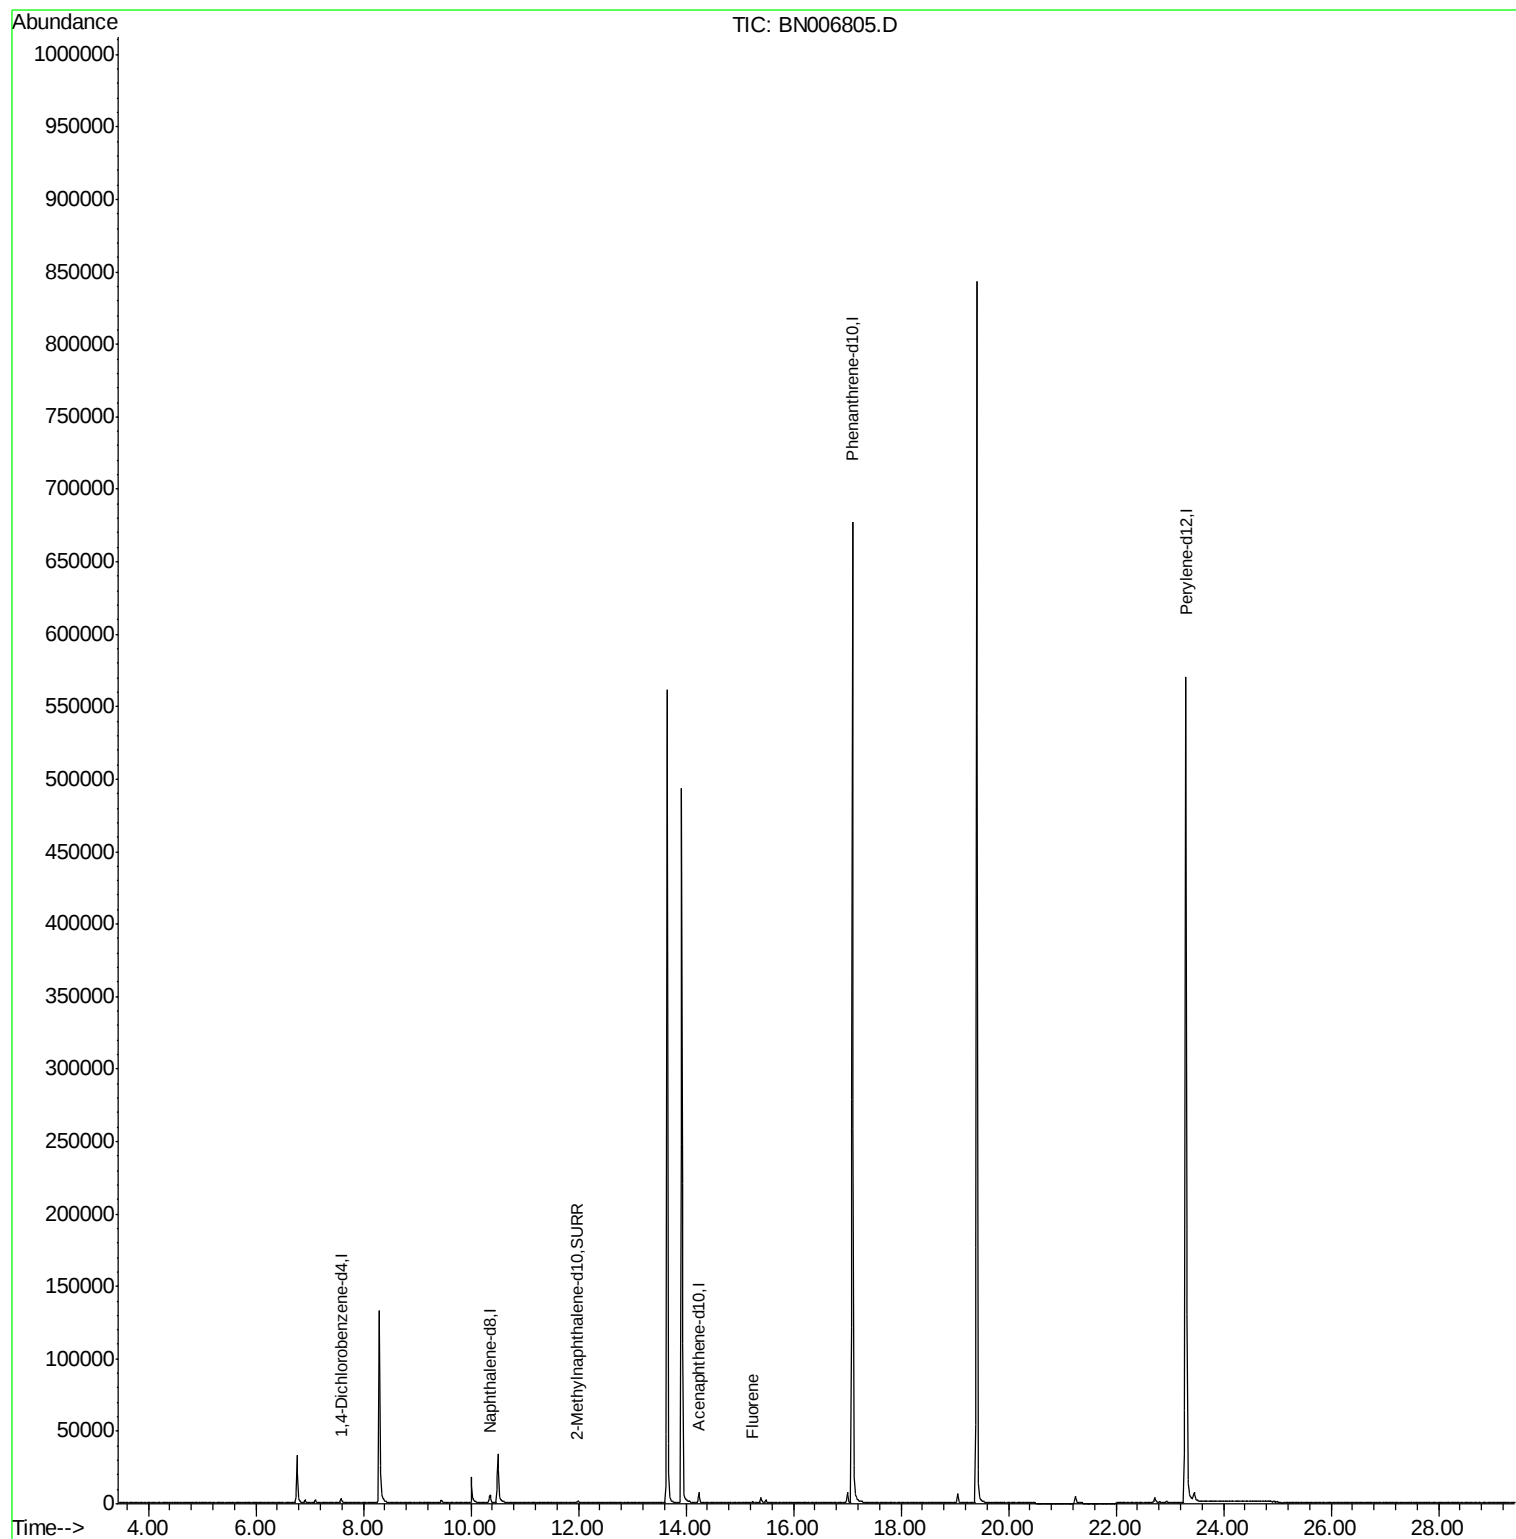

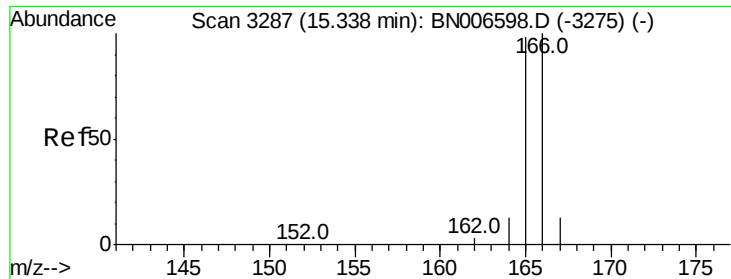

#9

Fluorene

Concen: 0.073 ng/ul

RT: 15.24 min Scan# 3265

Delta R.T. -0.08 min

Lab File: BN006805.D

Acq: 11 Jul 2019 19:21

Instrument :

BNA_N

ClientSampleId :


Tot Ion:166 Resp: 1332

Ion Ratio Lower Upper

166 100

165 9.3 78.2 117.4#

167 33.8 11.3 16.9#

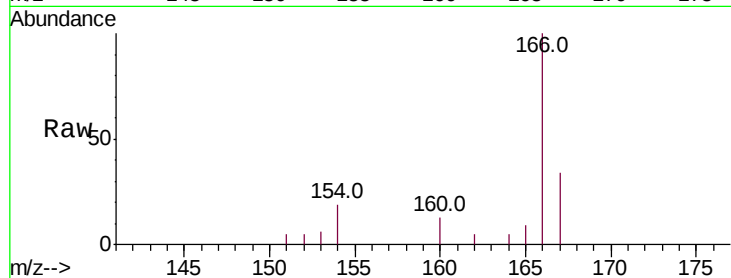

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

