

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006806.D
 Acq On : 11 Jul 2019 19:58
 Operator : HP/JU
 Sample : K3578-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 12 03:53:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 11 02:31:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	2258	0.40	ng/ul	-0.03
2) Naphthalene-d8	10.36	136	8012	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	4184	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.01	188	9086	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	7664	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	10844	0.40	ng/ul	-0.03
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	1320	0.11	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	3689	0.14	ng/ul	0.00
Target Compounds						
17) Pyrene	19.41	202	765	0.022	ng/ul#	1
23) Benzo(a)pyrene	23.30	252	1278	0.029	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
Data File : BN006806.D
Acq On : 11 Jul 2019 19:58
Operator : HP/JU
Sample : K3578-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 12 03:53:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 02:31:55 2019
Response via : Initial Calibration




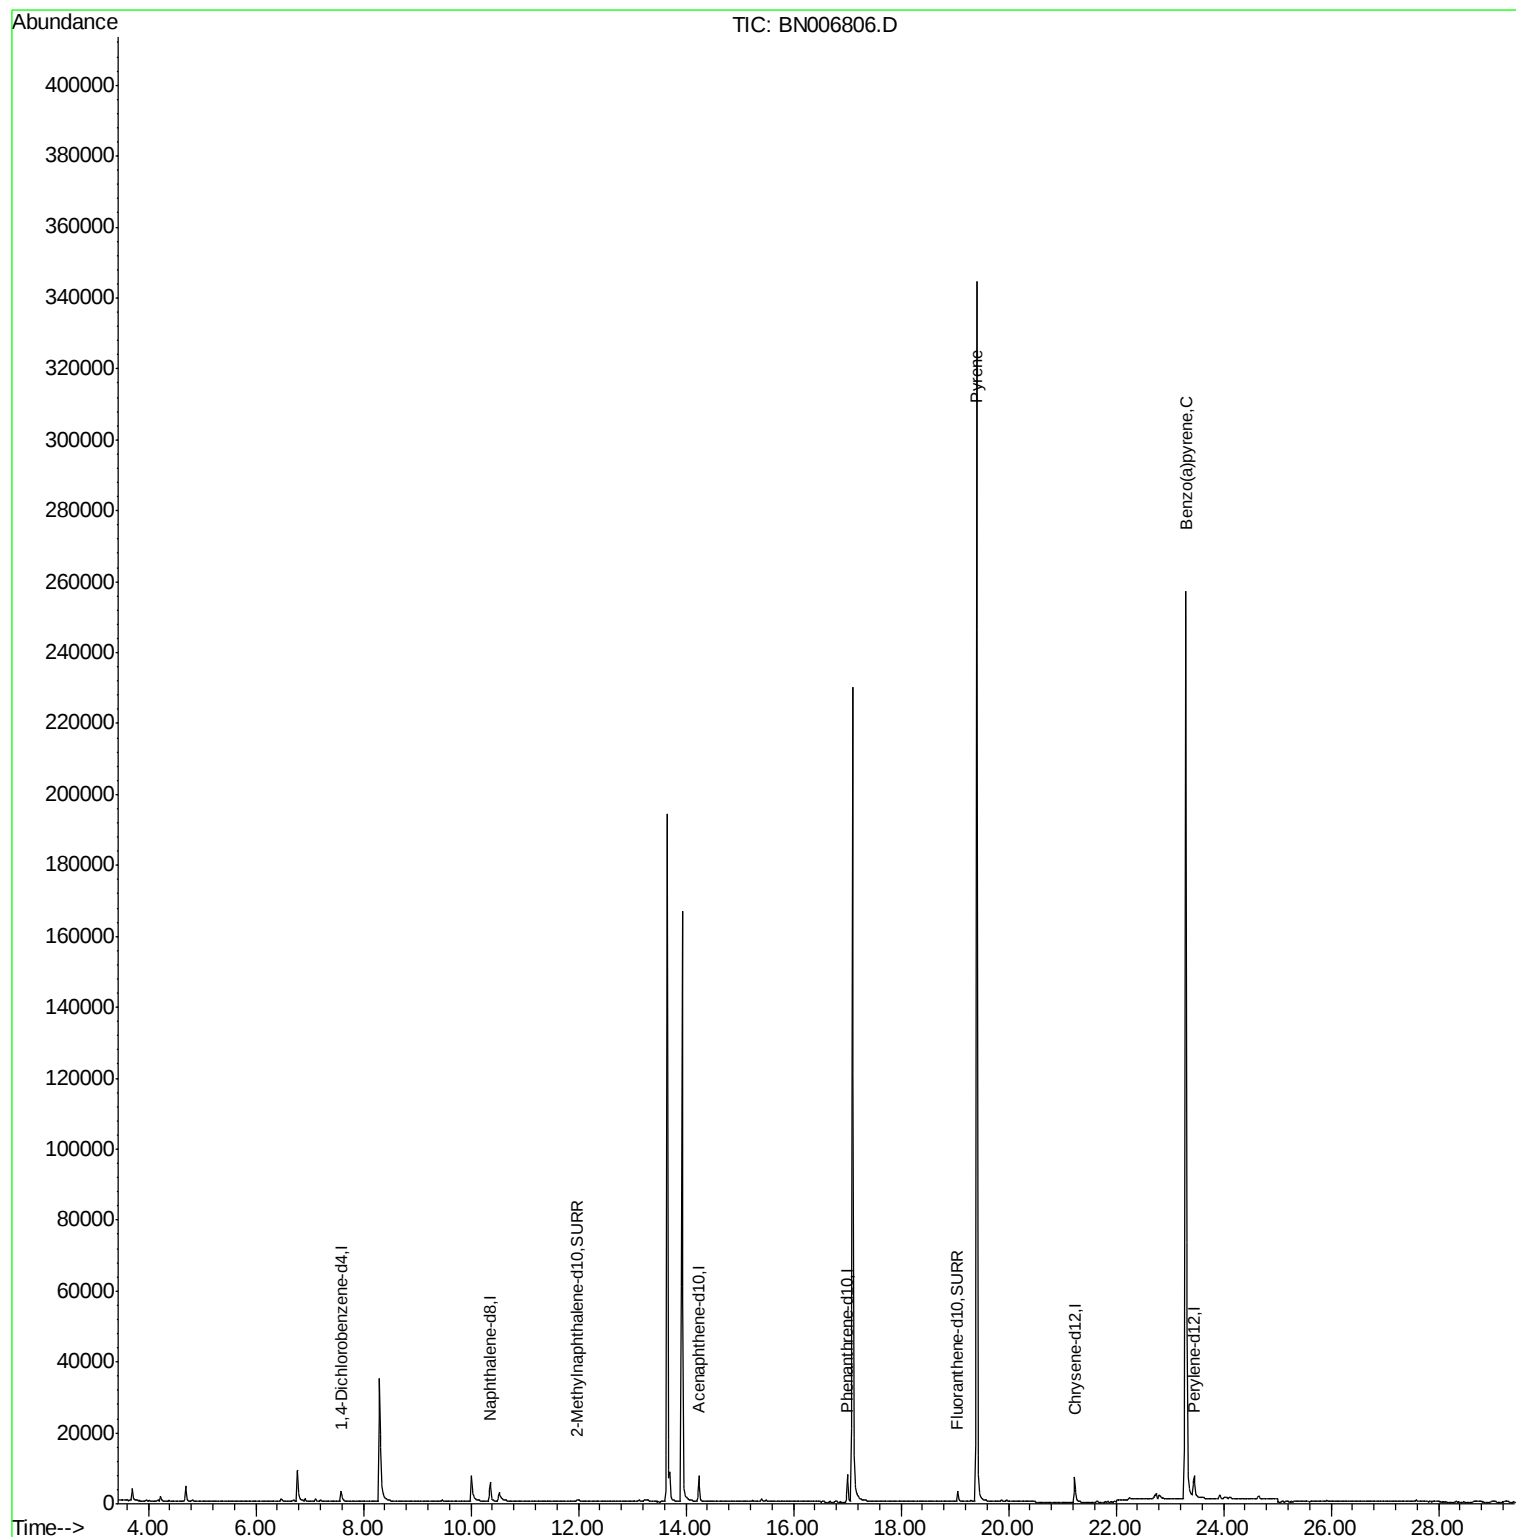


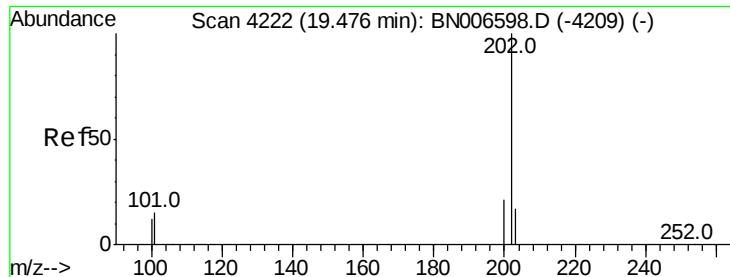

#17
Pvrene
Concen: 0.022 ng/ul
RT: 19.41 min Scan# 4207
Delta R.T. -0.05 min
Lab File: BN006806.D
Acq: 11 Jul 2019 19:58

Instrument :
BNA_N
ClientSampleId :

Tot Ion:202 Resp: 765
Ion Ratio Lower Upper
202 100
101 173.3 12.2 18.2#
100 1152.2 9.8 14.8#

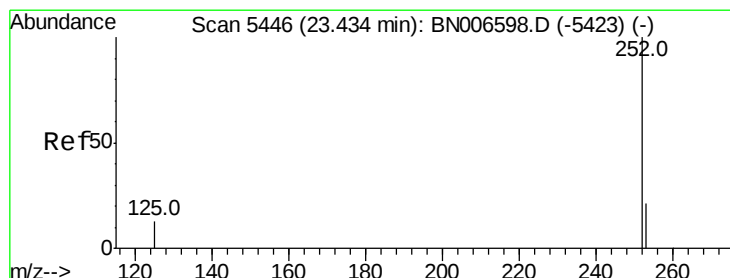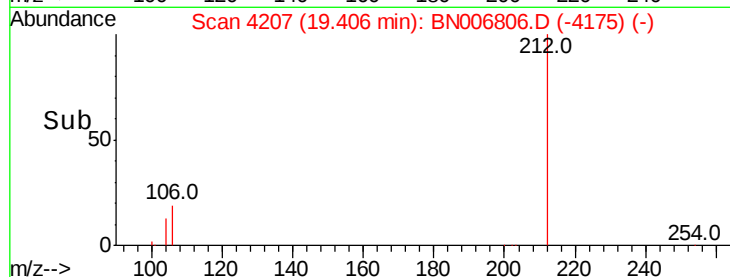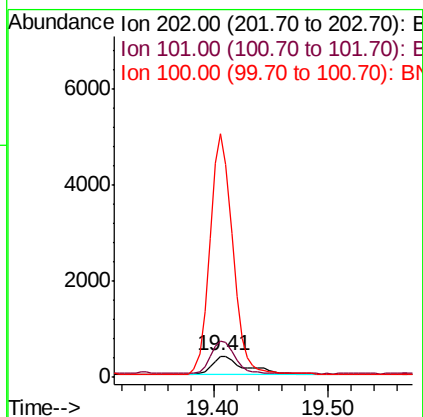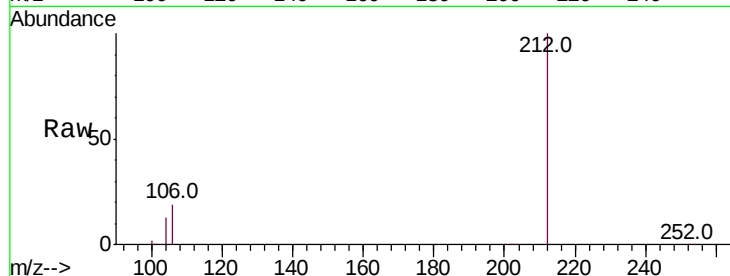

#23
Benzo(a)pyrene
Concen: 0.029 ng/ul
RT: 23.30 min Scan# 5399
Delta R.T. -0.09 min
Lab File: BN006806.D
Acq: 11 Jul 2019 19:58

Tgt Ion:252 Resp: 1278
Ion Ratio Lower Upper
252 100
253 62.0 19.4 29.2#
125 113.2 12.6 19.0#

