

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006808.D
 Acq On : 11 Jul 2019 21:08
 Operator : HP/JU
 Sample : K3578-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 12 03:53:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 11 02:31:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	2439	0.40	ng/ul	-0.03
2) Naphthalene-d8	10.36	136	8799	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.24	164	4564	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	580546	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.30	264	418405	0.40	ng/ul	-0.18
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	2899	0.21	ng/ul	-0.01
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
5) 2-Methylnaphthalene	12.05	142	1231	0.072	ng/ul	Ovalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
Data File : BN006808.D
Acq On : 11 Jul 2019 21:08
Operator : HP/JU
Sample : K3578-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 12 03:53:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 11 02:31:55 2019
Response via : Initial Calibration

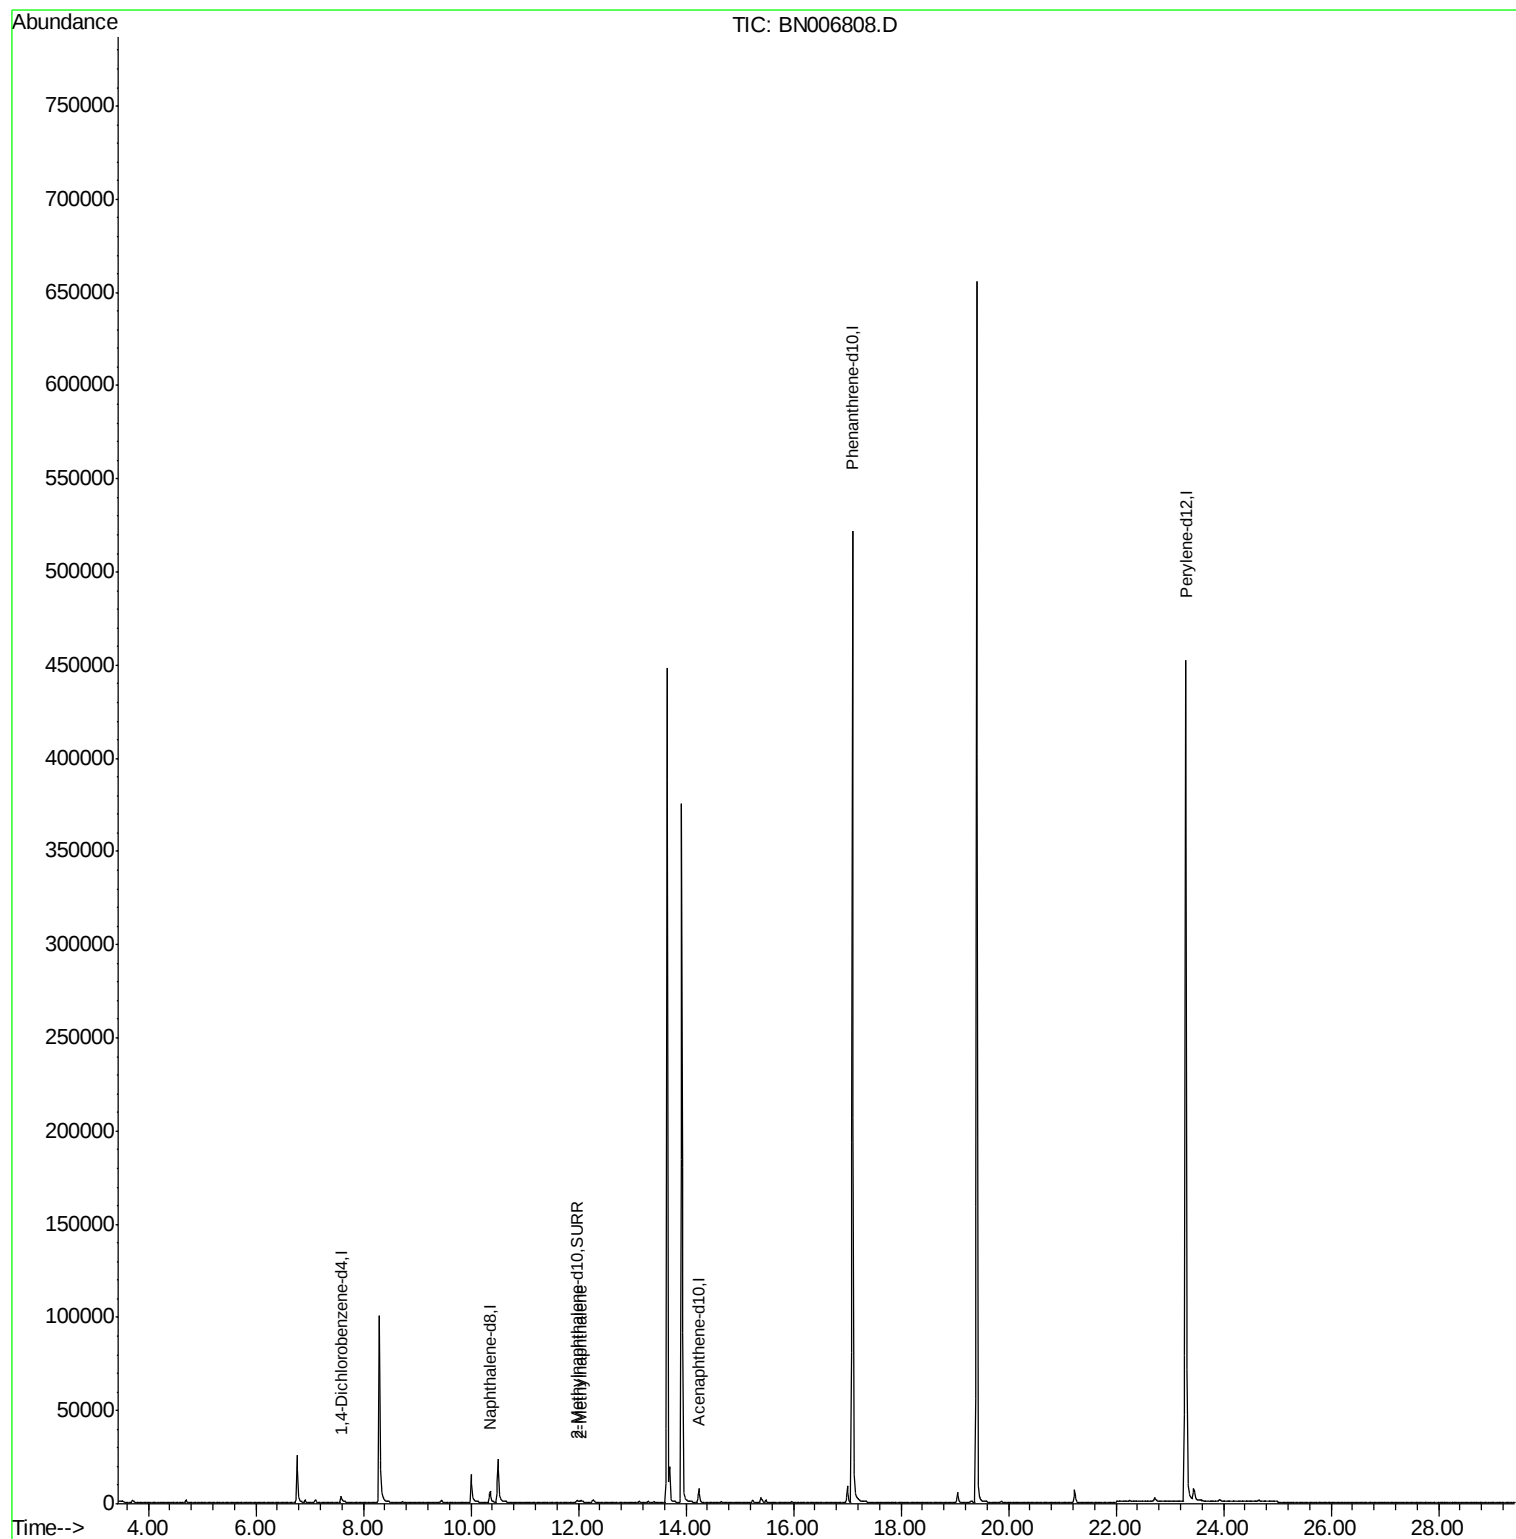

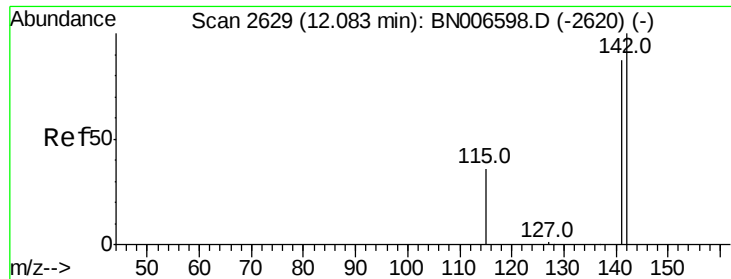

#5

2-Methylnaphthalene

Concen: 0.072 ng/ul

RT: 12.05 min Scan# 2623

Delta R.T. -0.01 min

Lab File: BN006808.D

Acq: 11 Jul 2019 21:08

Instrument :

BNA_N



ClientSampleId :

Tot Ion:142 Resp: 1231

Ion Ratio Lower Upper

142 100

141 87.2 71.8 107.6

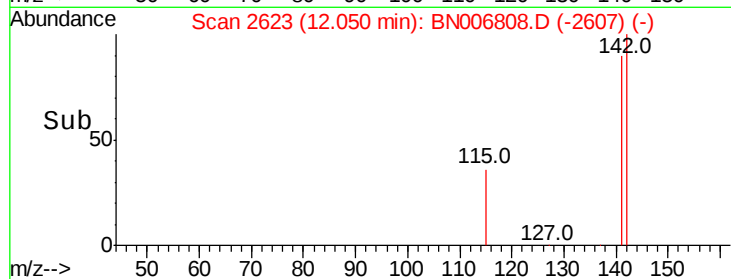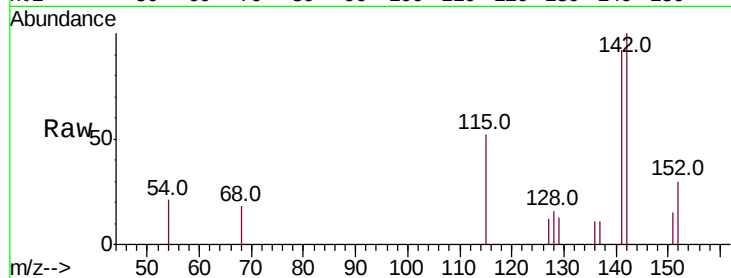

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

