

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006819.D
 Acq On : 12 Jul 2019 05:49
 Operator : HP/JU
 Sample : K3717-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 12 08:43:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	2820	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	10485	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	5391	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	888220	0.40	ng/ul	0.08
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.24
20) Perylene-d12	23.30	264	883608	0.40	ng/ul	-0.17
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.97	152	3539	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.15	212	456	0.00	ng/ul	0.09
Target Compounds						
8) Acenaphthene	14.32	153	2325	0.108	ng/ul#	Ovalue 25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
Data File : BN006819.D
Acq On : 12 Jul 2019 05:49
Operator : HP/JU
Sample : K3717-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 12 08:43:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

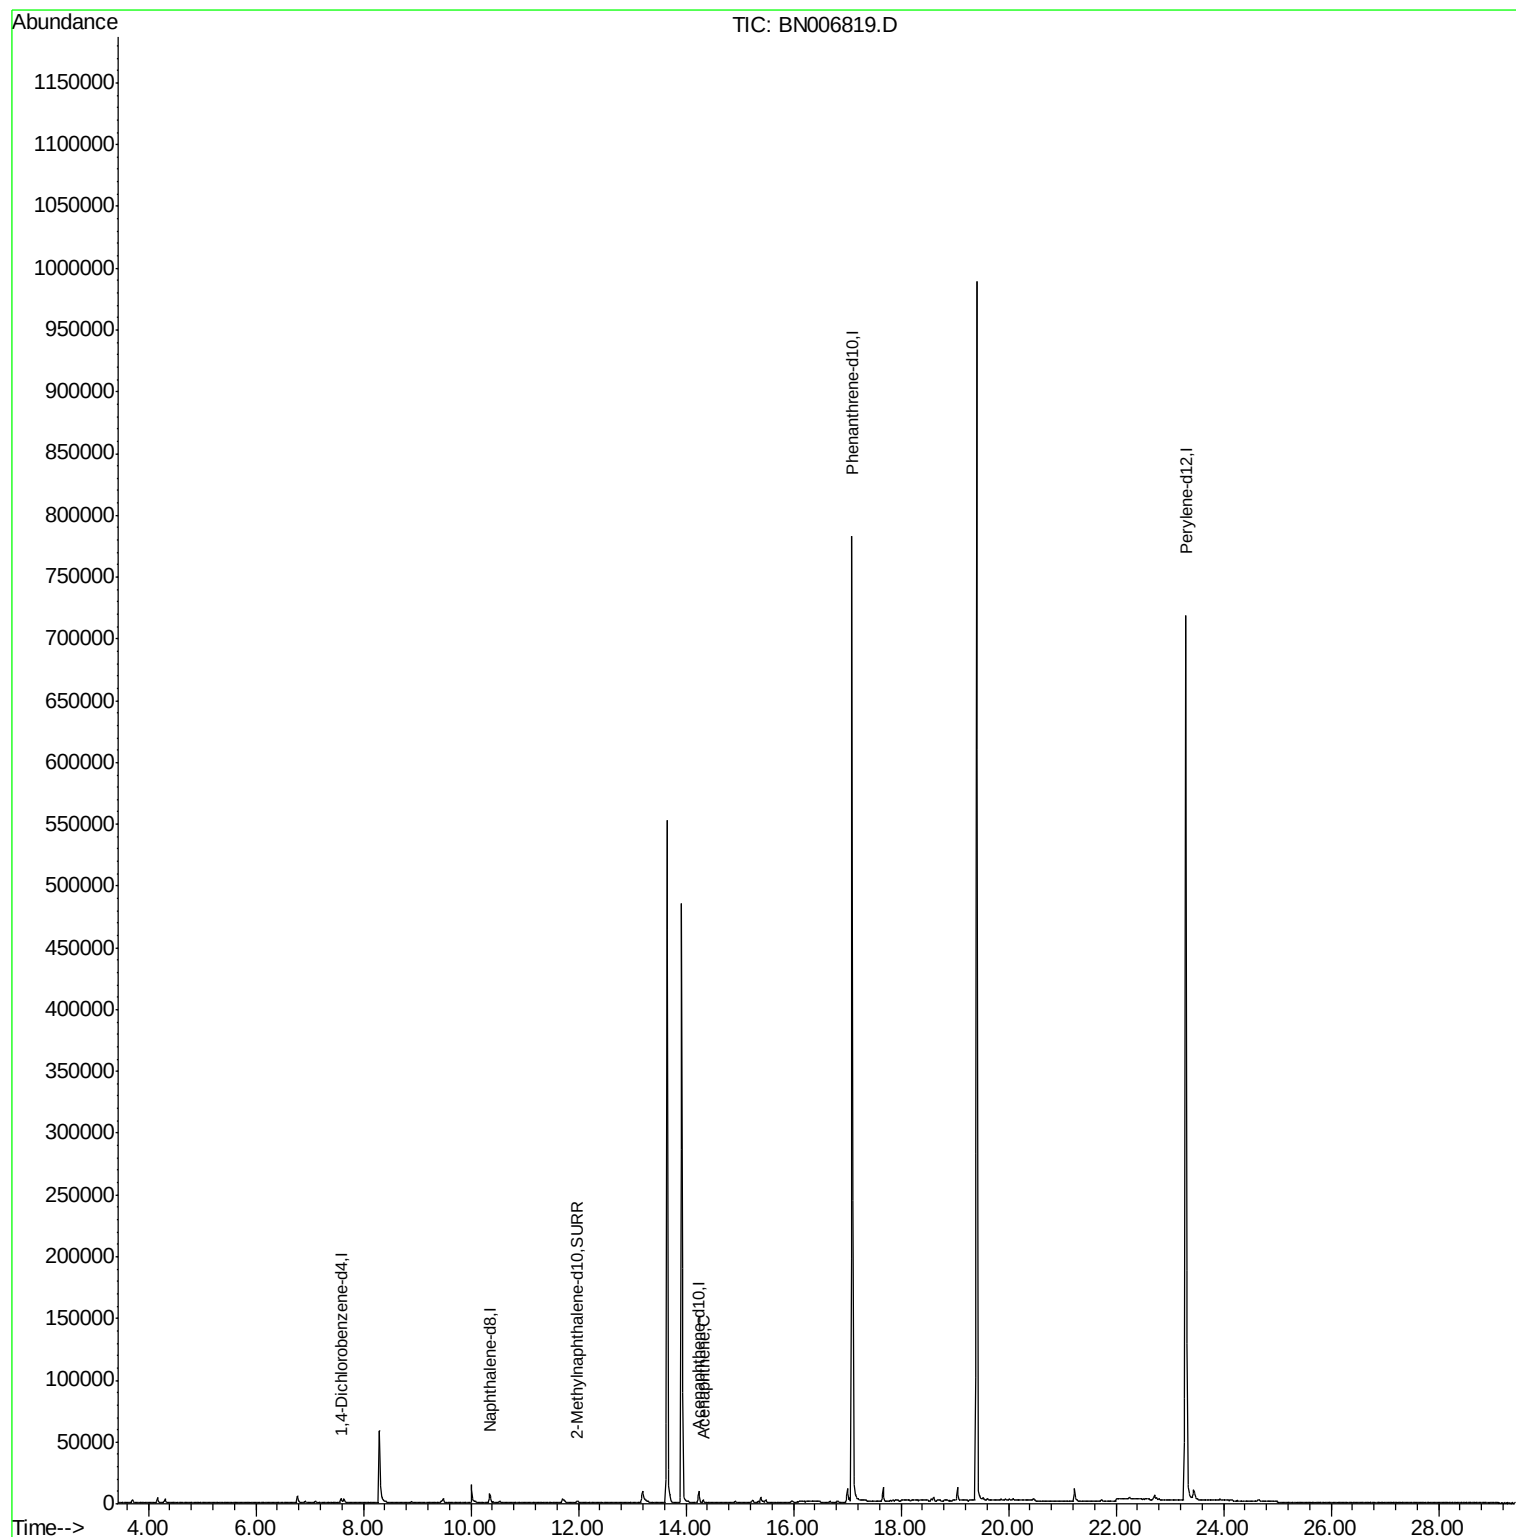

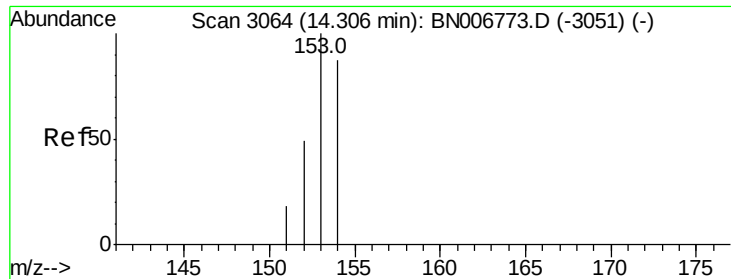

#8

Acenaphthene

Concen: 0.108 ng/ul

RT: 14.32 min Scan# 3067

Delta R.T. 0.01 min

Lab File: BN006819.D

Acq: 12 Jul 2019 05:49

Instrument :

BNA_N

ClientSampleId :


Tot Ion:153 Resp: 2325

Ion Ratio Lower Upper

153 100

152 6.1 39.3 58.9#

154 12.4 70.6 105.8#

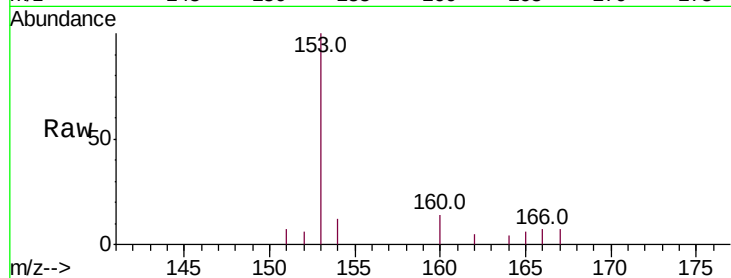

Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

