


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
Data File : BN006816.D
Acq On : 12 Jul 2019 04:05
Operator : HP/JU
Sample : K3717-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF4A8

Manual Integrations
APPROVED

mohammad
7/12/2019 10:27:46 PM

Quant Time: Jul 12 08:30:15 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

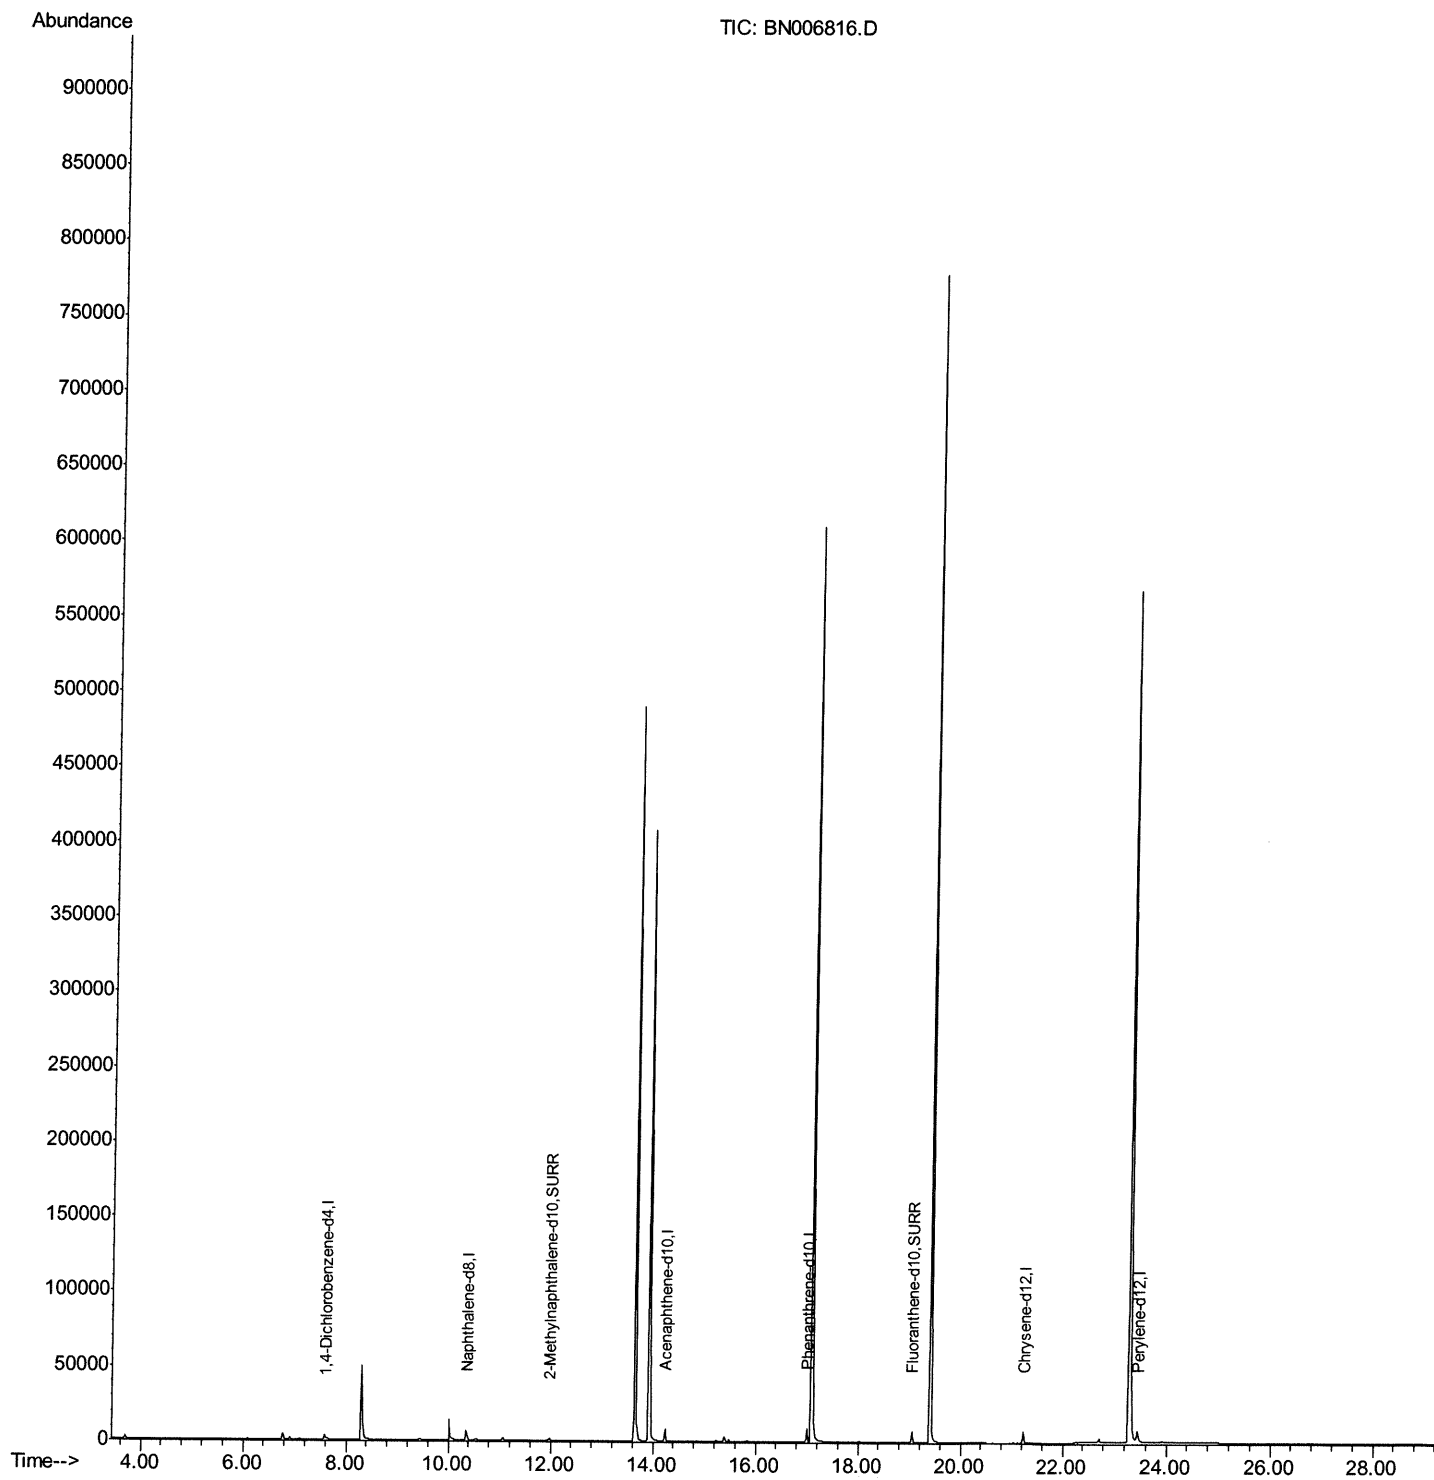

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
Data File : BN006816.D
Acq On : 12 Jul 2019 04:05
Operator : HP/JU
Sample : K3717-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF4A8

Manual Integrations
APPROVED

mohammad
7/12/2019 10:27:46 PM

Quant Time: Jul 12 08:27:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

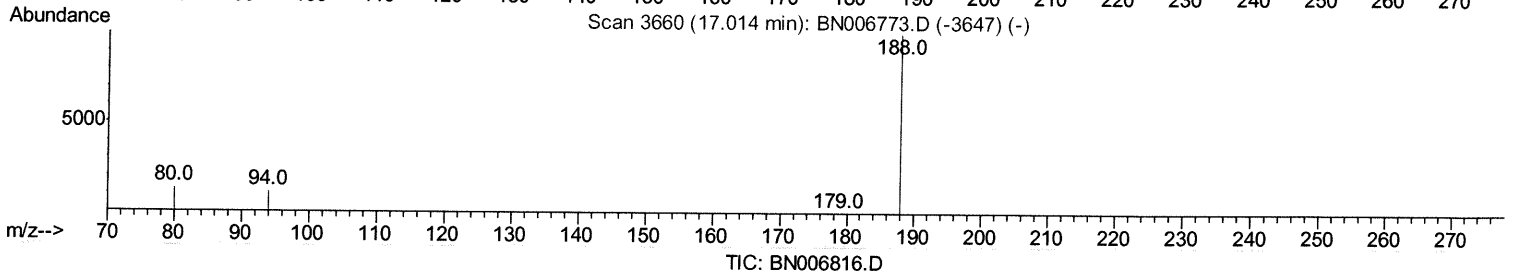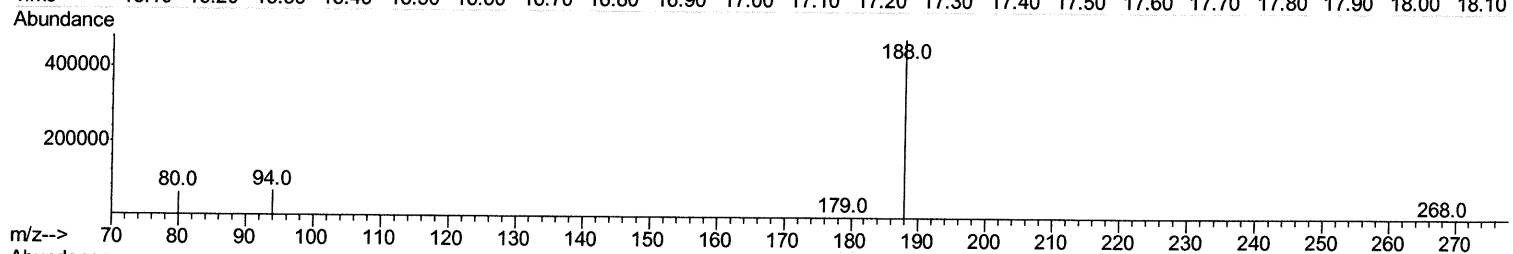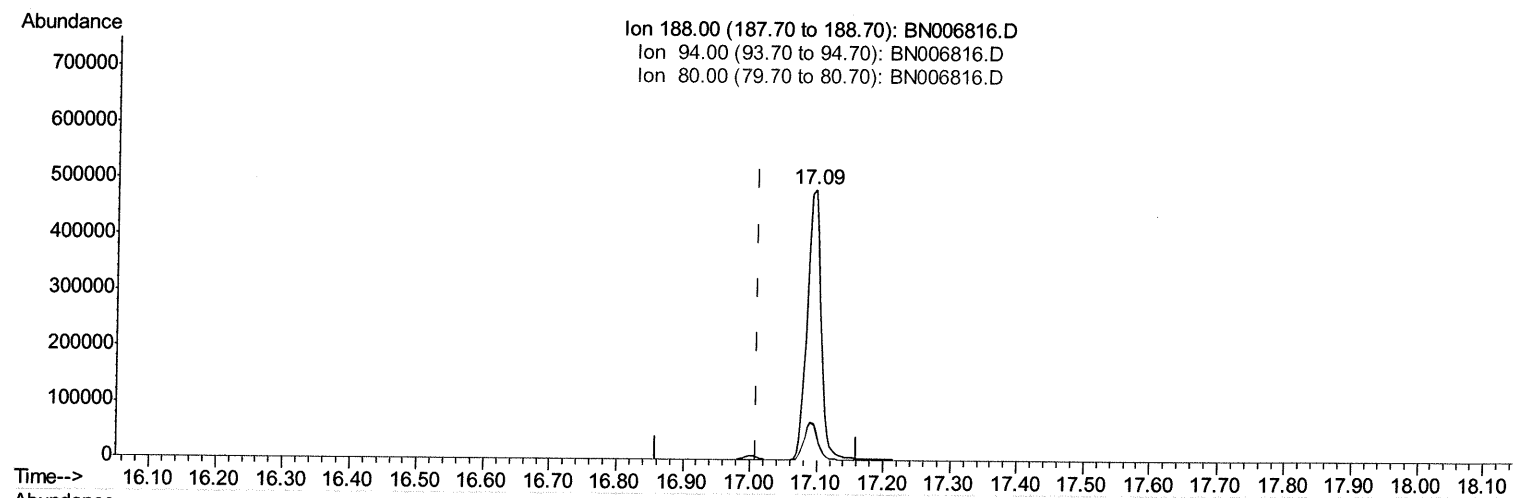

(10) Phenanthrene-d10 (I)

17.095min (+0.084) 0.40ng/ul

response 690833

Ion	Exp%	Act%
188.00	100	100
94.00	13.70	13.51
80.00	14.80	12.68
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006816.D
 Acq On : 12 Jul 2019 04:05
 Operator : HP/JU
 Sample : K3717-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF4A8

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:27:46 PM

Quant Time: Jul 12 08:27:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

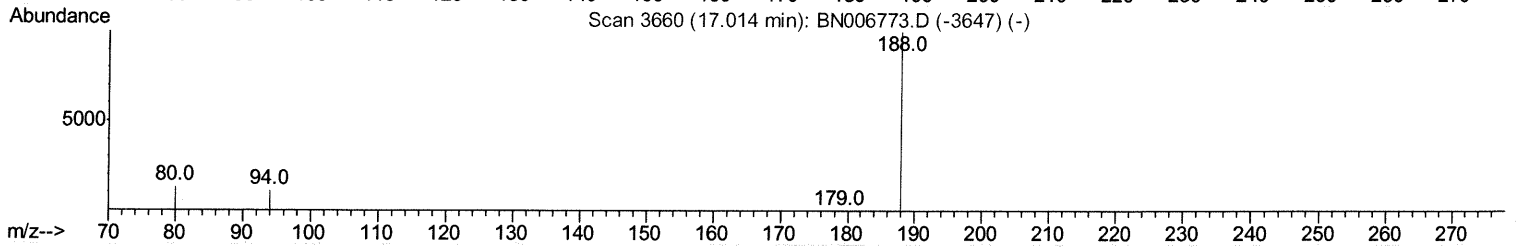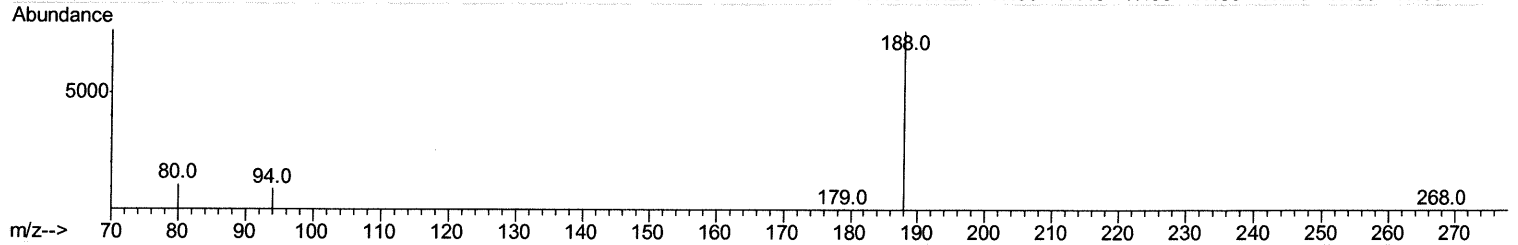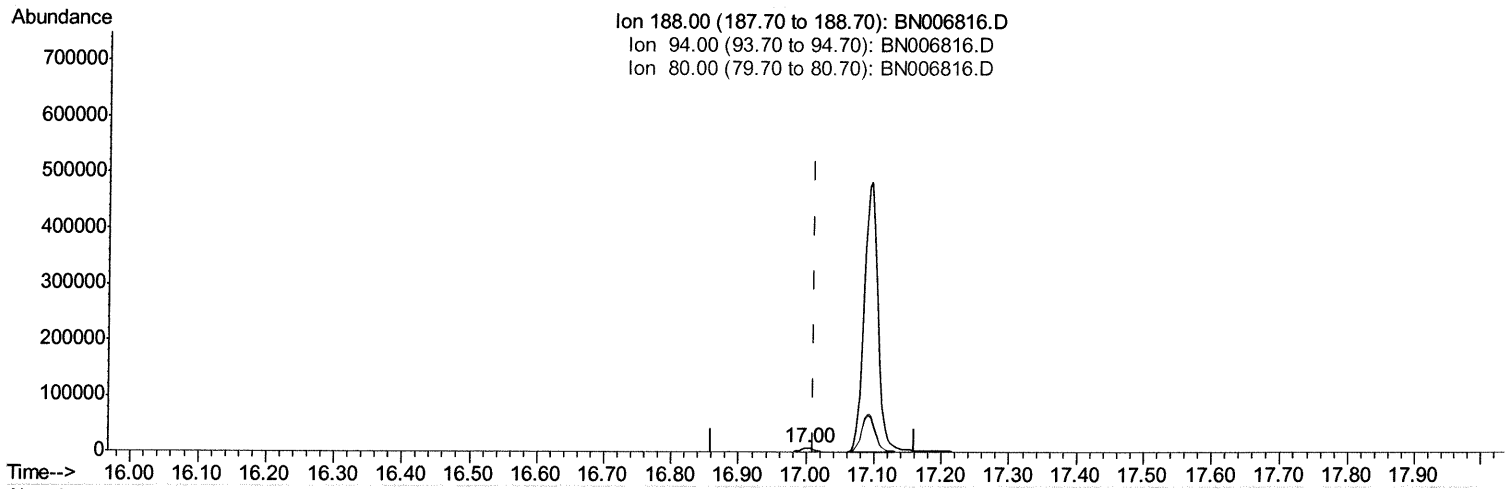

TIC: BN006816.D

(10) Phenanthrene-d10 (I)

17.002min (-0.008) 0.40ng/ul m *JU 07/12/19*

response 10423

Ion	Exp%	Act%
188.00	100	100
94.00	13.70	12.02
80.00	14.80	14.26
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
Data File : BN006816.D
Acq On : 12 Jul 2019 04:05
Operator : HP/JU
Sample : K3717-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF4A8

Manual Integrations
APPROVED

mohammad
7/12/2019 10:27:46 PM

Quant Time: Jul 12 08:27:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

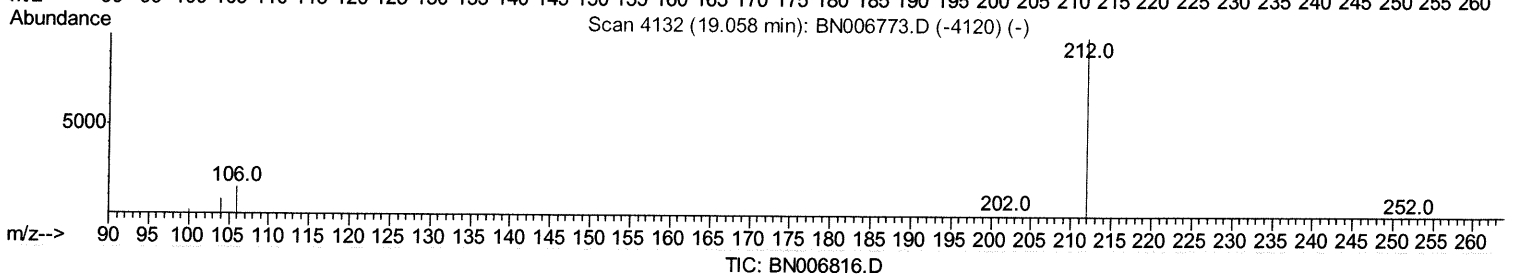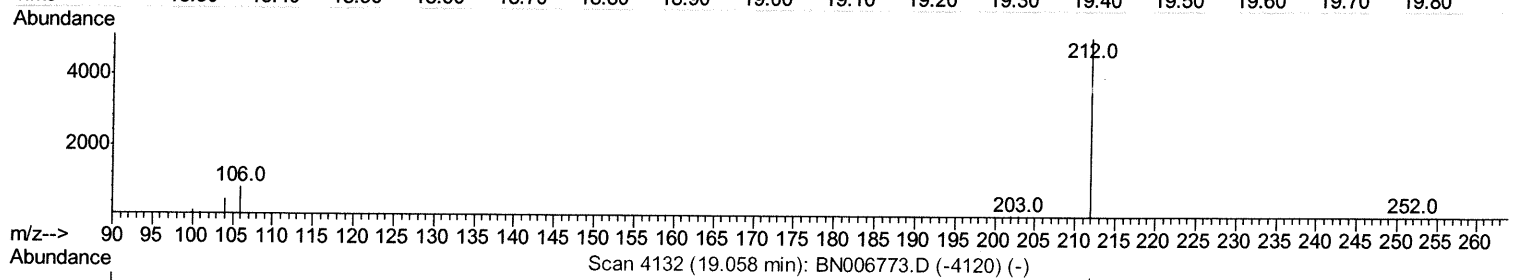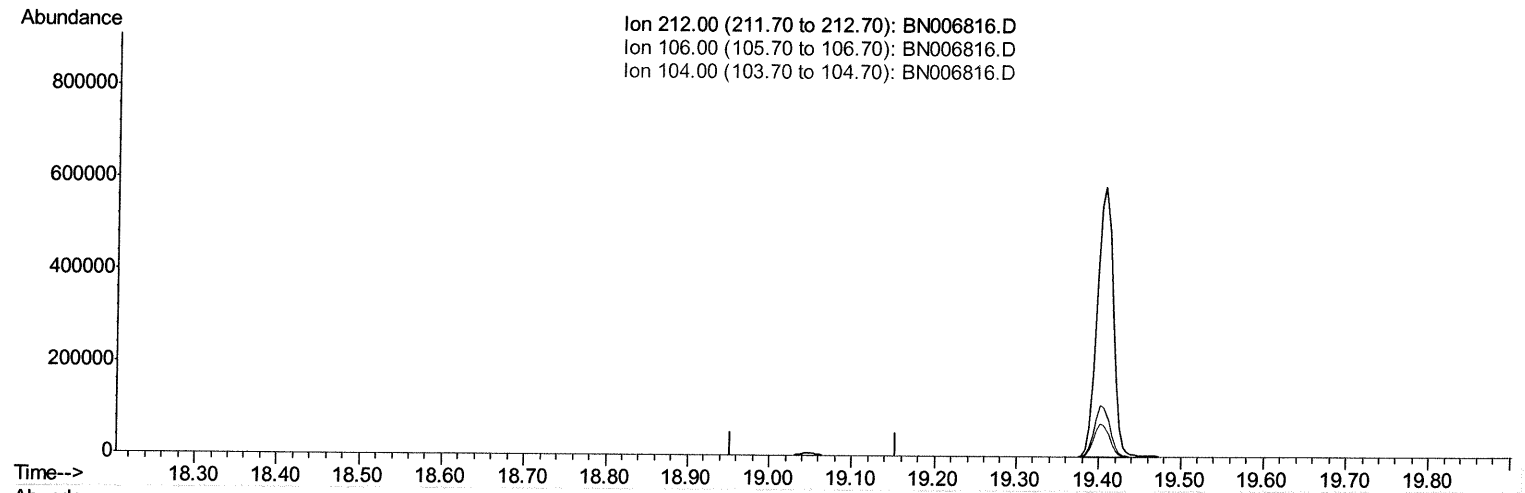

(14) Fluoranthene-d10 (SURR)

19.053min (-19.053) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	17.80	0.00#
104.00	9.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006816.D
 Acq On : 12 Jul 2019 04:05
 Operator : HP/JU
 Sample : K3717-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF4A8

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:27:46 PM

Quant Time: Jul 12 08:27:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

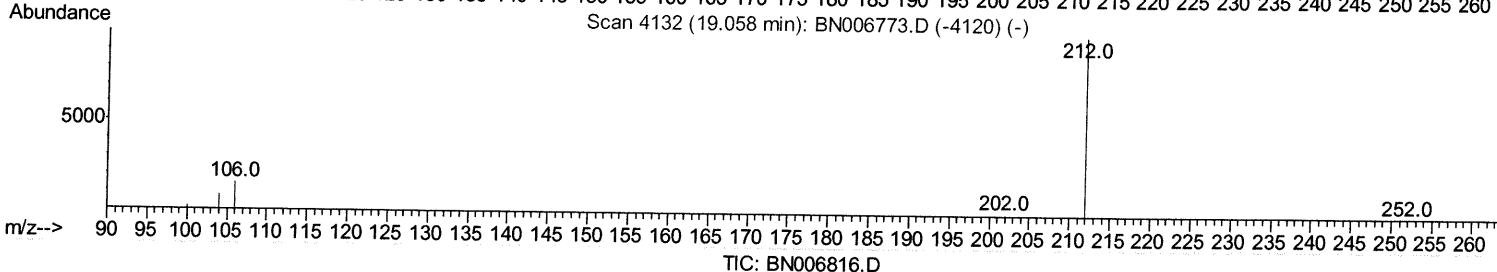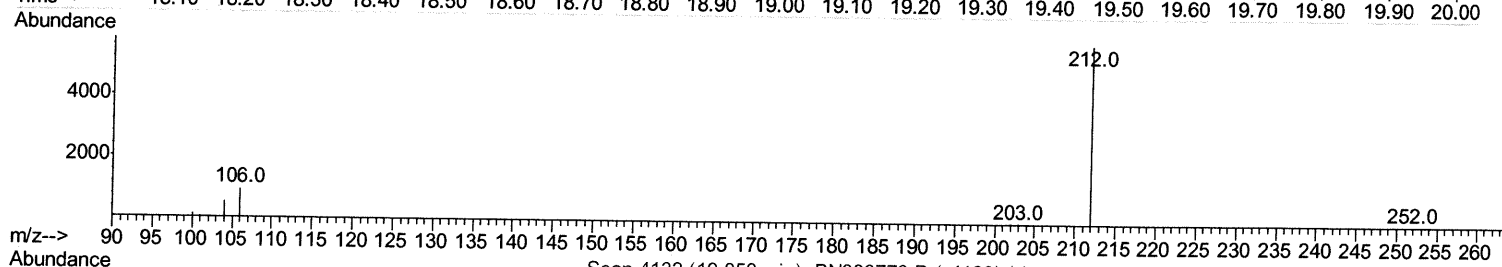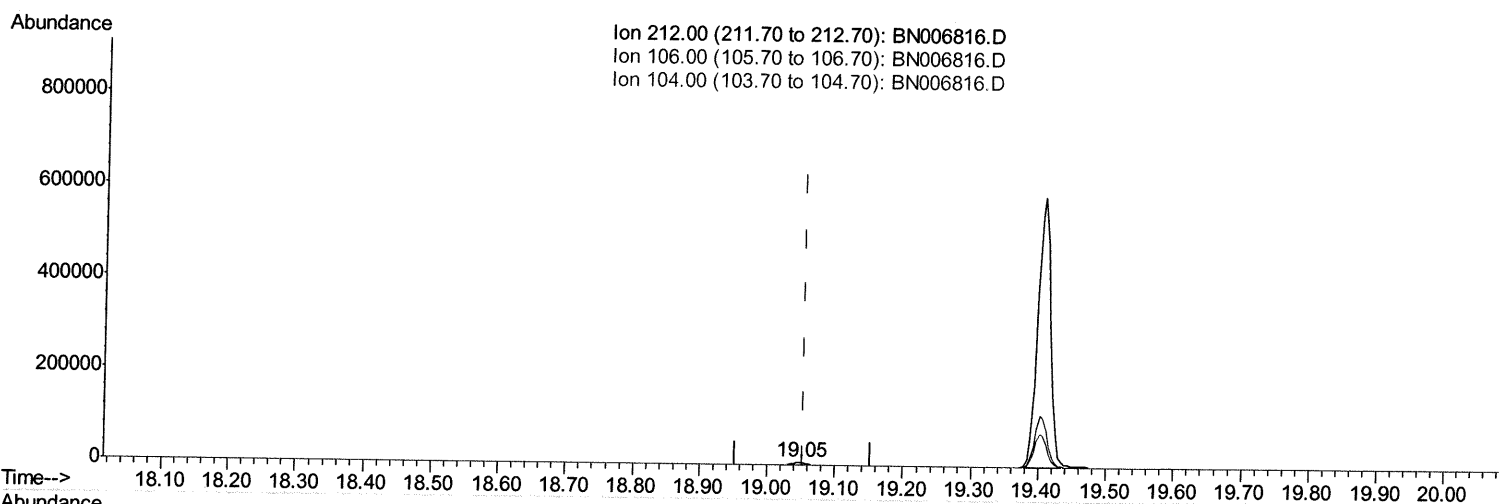

(14) Fluoranthene-d10 (SURR) *JU*
 19.048min (-0.005) 0.27ng/ul m *07/12/19*

response 8375

Ion	Exp%	Act%
212.00	100	100
106.00	17.80	0.00#
104.00	9.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006816.D
 Acq On : 12 Jul 2019 04:05
 Operator : HP/JU
 Sample : K3717-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF4A8

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:27:46 PM

Quant Time: Jul 12 08:27:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

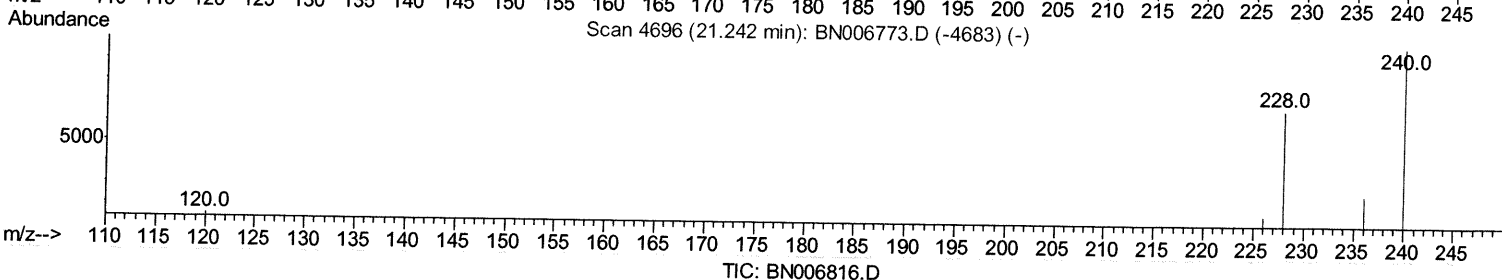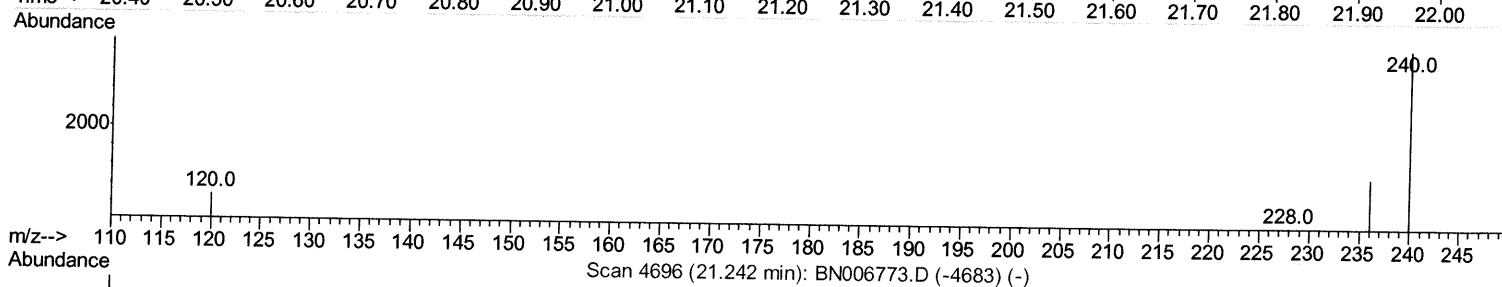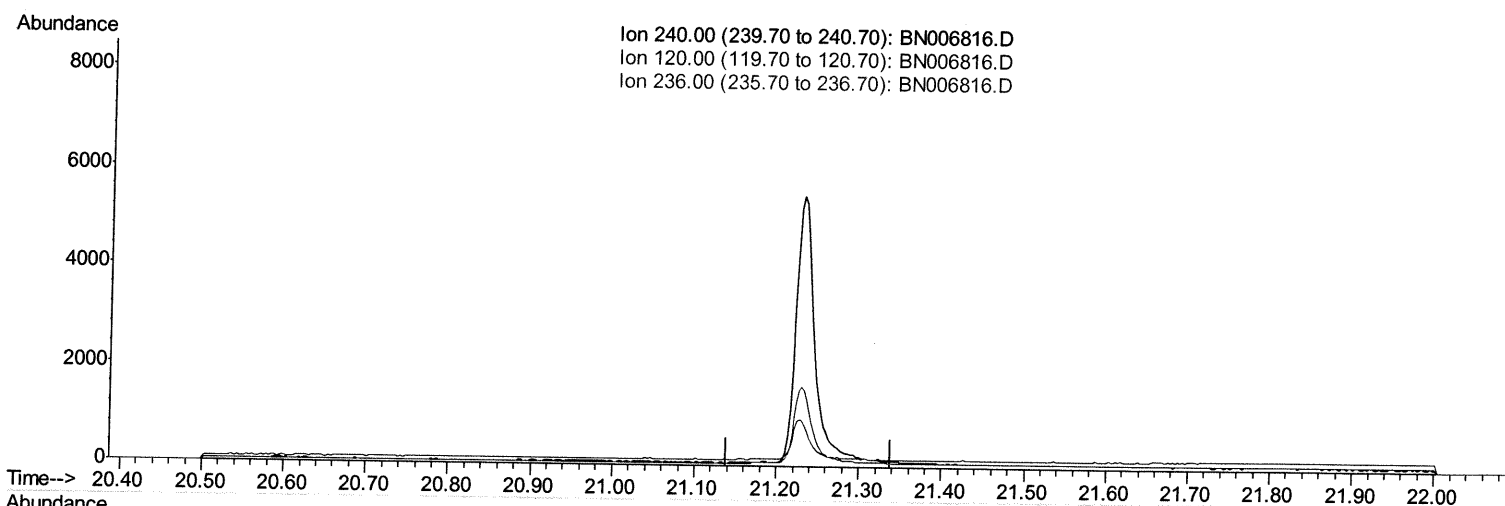

(16) Chrysene-d12 (I)

21.239min (-21.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.20	0.00#
236.00	30.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006816.D
 Acq On : 12 Jul 2019 04:05
 Operator : HP/JU
 Sample : K3717-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF4A8

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:27:46 PM

Quant Time: Jul 12 08:27:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

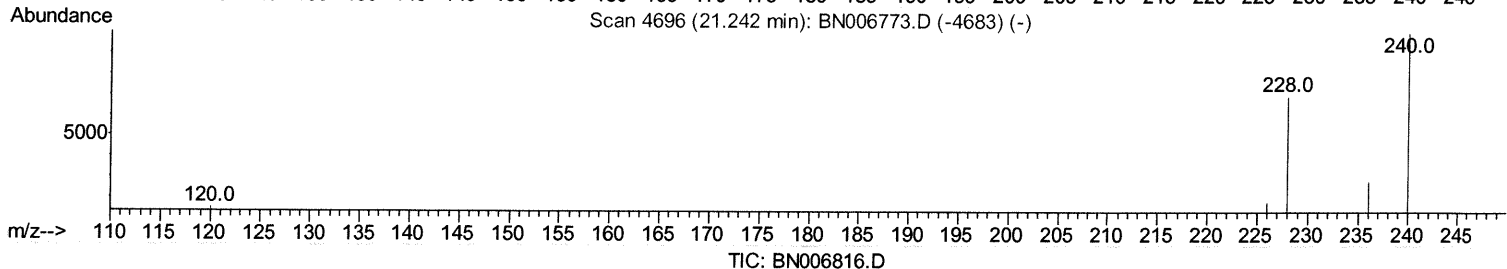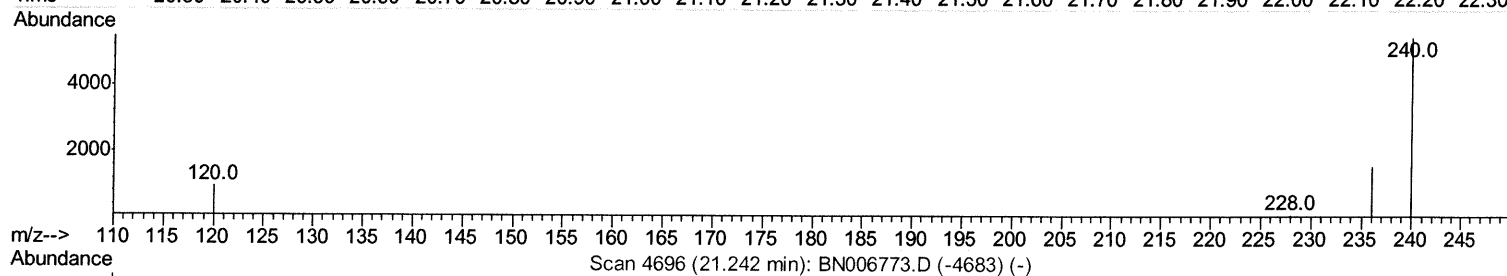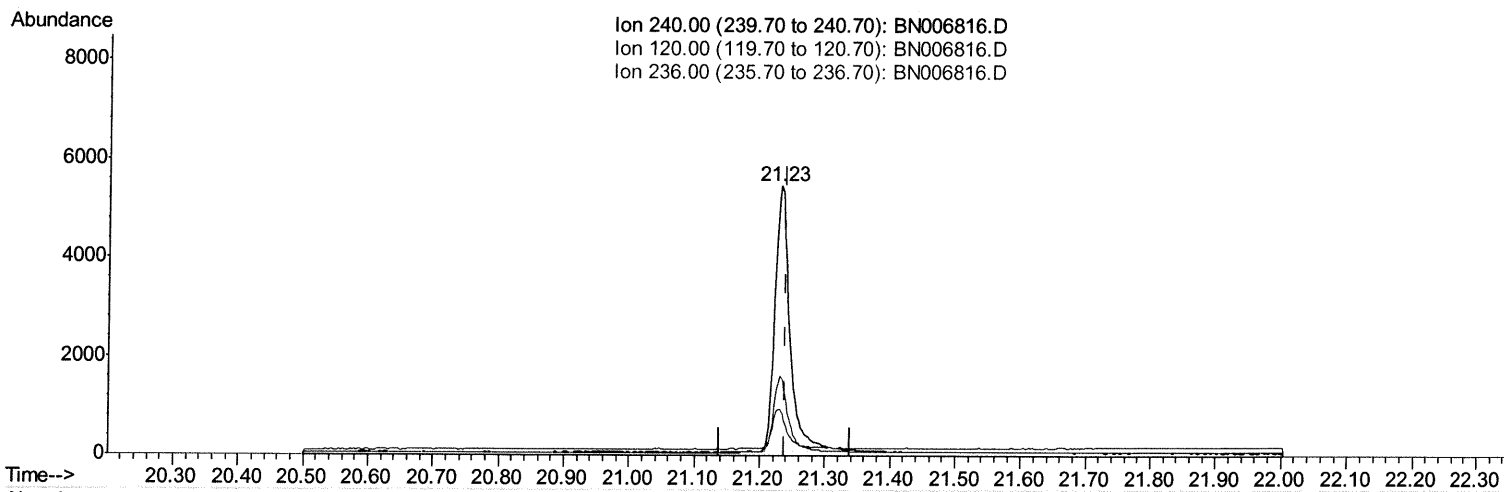

(16) Chrysene-d12 (I)

21.230min (-0.009) 0.40ng/ul m *JU 07/12/19*

response 8793

Ion	Exp%	Act%
240.00	100	100
120.00	20.20	17.44
236.00	30.00	29.44
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
Data File : BN006816.D
Acq On : 12 Jul 2019 04:05
Operator : HP/JU
Sample : K3717-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF4A8

Manual Integrations
APPROVED

mohammad
7/12/2019 10:27:46 PM

Quant Time: Jul 12 08:29:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

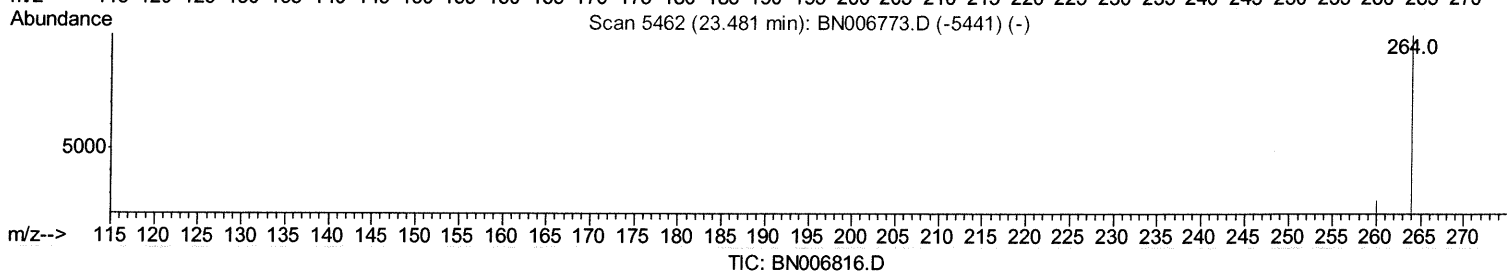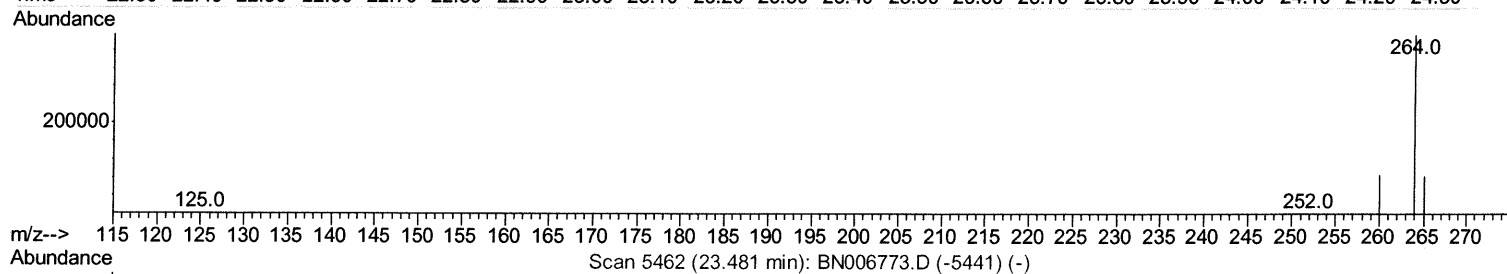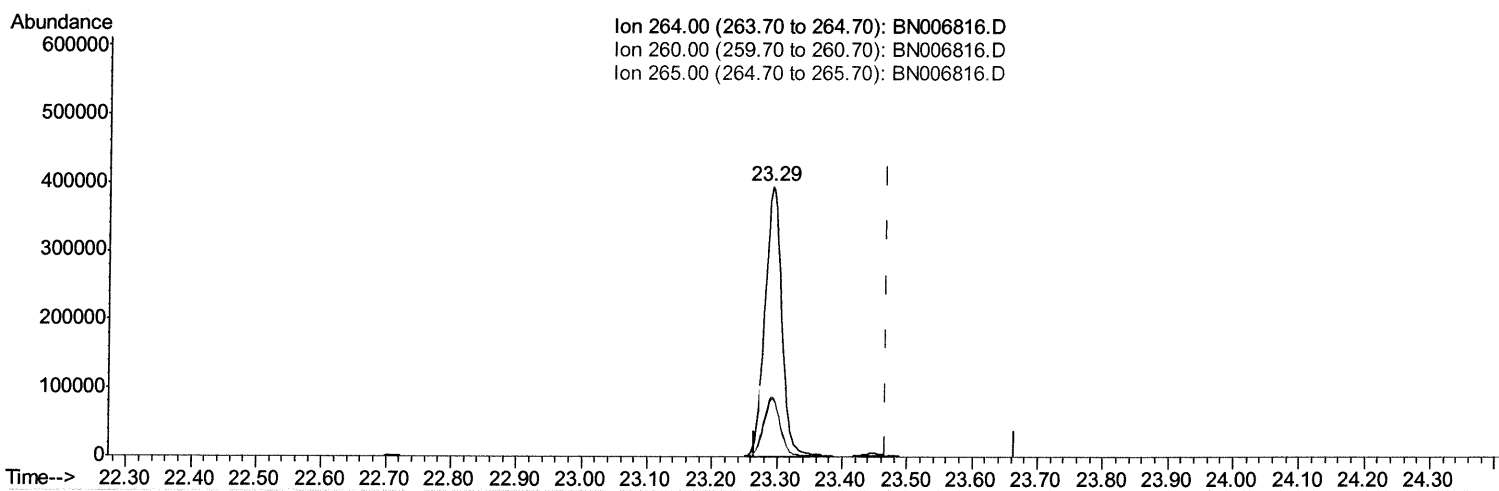

(20) Perylene-d12 (I)

23.291min (-0.175) 0.40ng/ul

response 664008

Ion	Exp%	Act%
264.00	100	100
260.00	27.80	22.38
265.00	36.10	21.29#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006816.D
 Acq On : 12 Jul 2019 04:05
 Operator : HP/JU
 Sample : K3717-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF4A8

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:27:46 PM

Quant Time: Jul 12 08:29:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

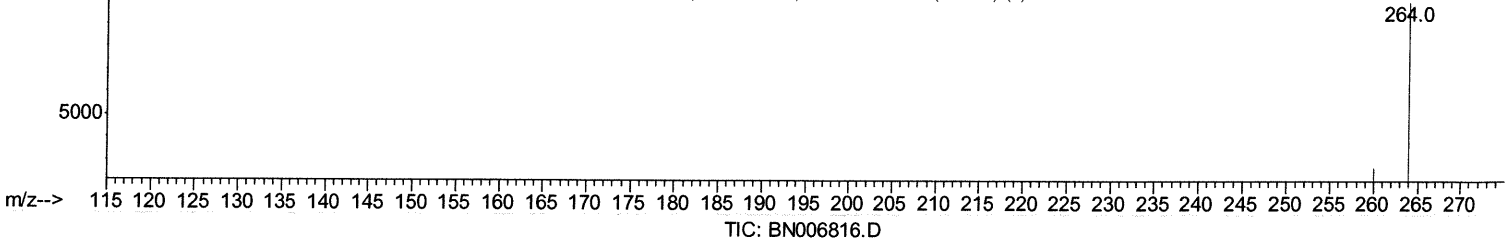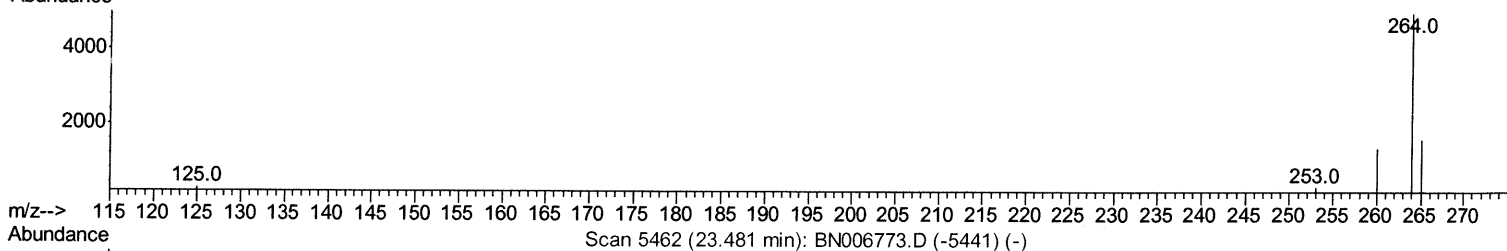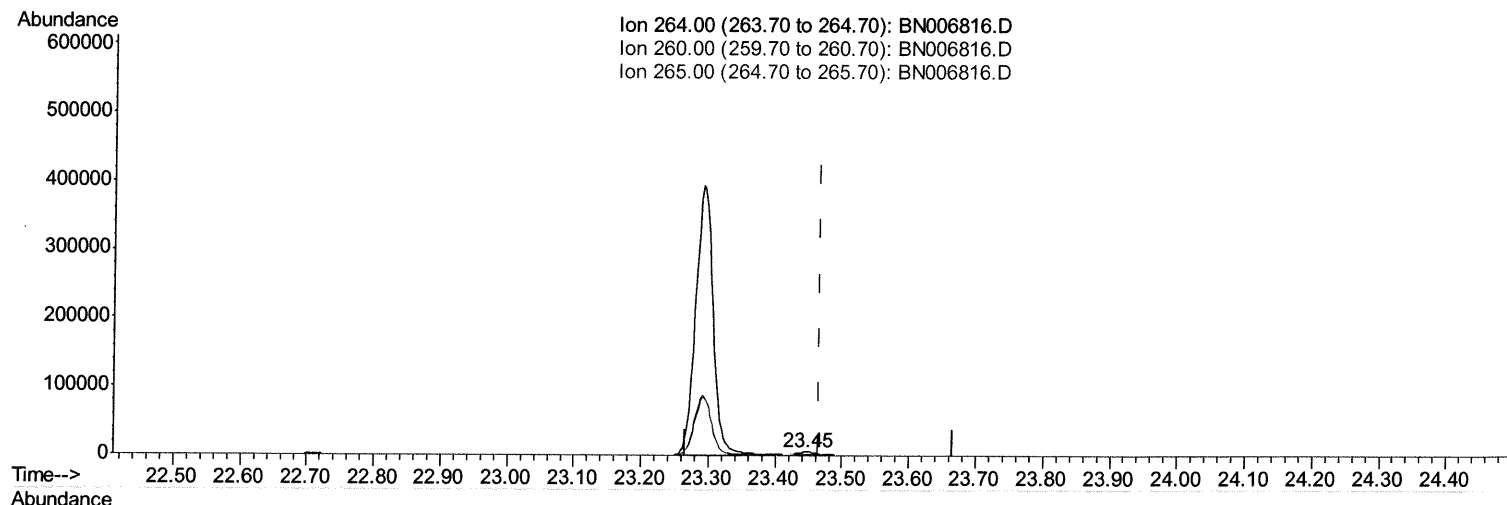

(20) Perylene-d12 (I)

23.446min (-0.021) 0.40ng/ul m ⁵⁰07/12/19

response 7908

Ion	Exp%	Act%
264.00	100	100
260.00	27.80	26.77
265.00	36.10	31.84
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006816.D
 Acq On : 12 Jul 2019 04:05
 Operator : HP/JU
 Sample : K3717-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF4A8

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:27:46 PM

Quant Time: Jul 12 08:30:15 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	2485	0.40	nq/ul	0.00
2) Naphthalene-d8	10.35	136	8907	0.40	nq/ul	-0.01
6) Acenaphthene-d10	14.24	164	4718	0.40	nq/ul	0.00
10) Phenanthrene-d10	17.00	188	10423m >	0.40	nq/ul	0.00
16) Chrysene-d12	21.23	240	8793m >	0.40	nq/ul	0.00
20) Perylene-d12	23.45	264	7908m >	0.40	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.97	152	2983	0.22	nq/ul	0.00
14) Fluoranthene-d10	19.05	212	8375m >	0.27	ng/ul	0.00

Target Compounds Ovalue

Ju 07/12/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed