


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
Data File : BN006830.D
Acq On : 12 Jul 2019 12:50
Operator : HP/JU
Sample : K3717-14
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF499

Manual Integrations
APPROVED

mohammad
7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:27:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

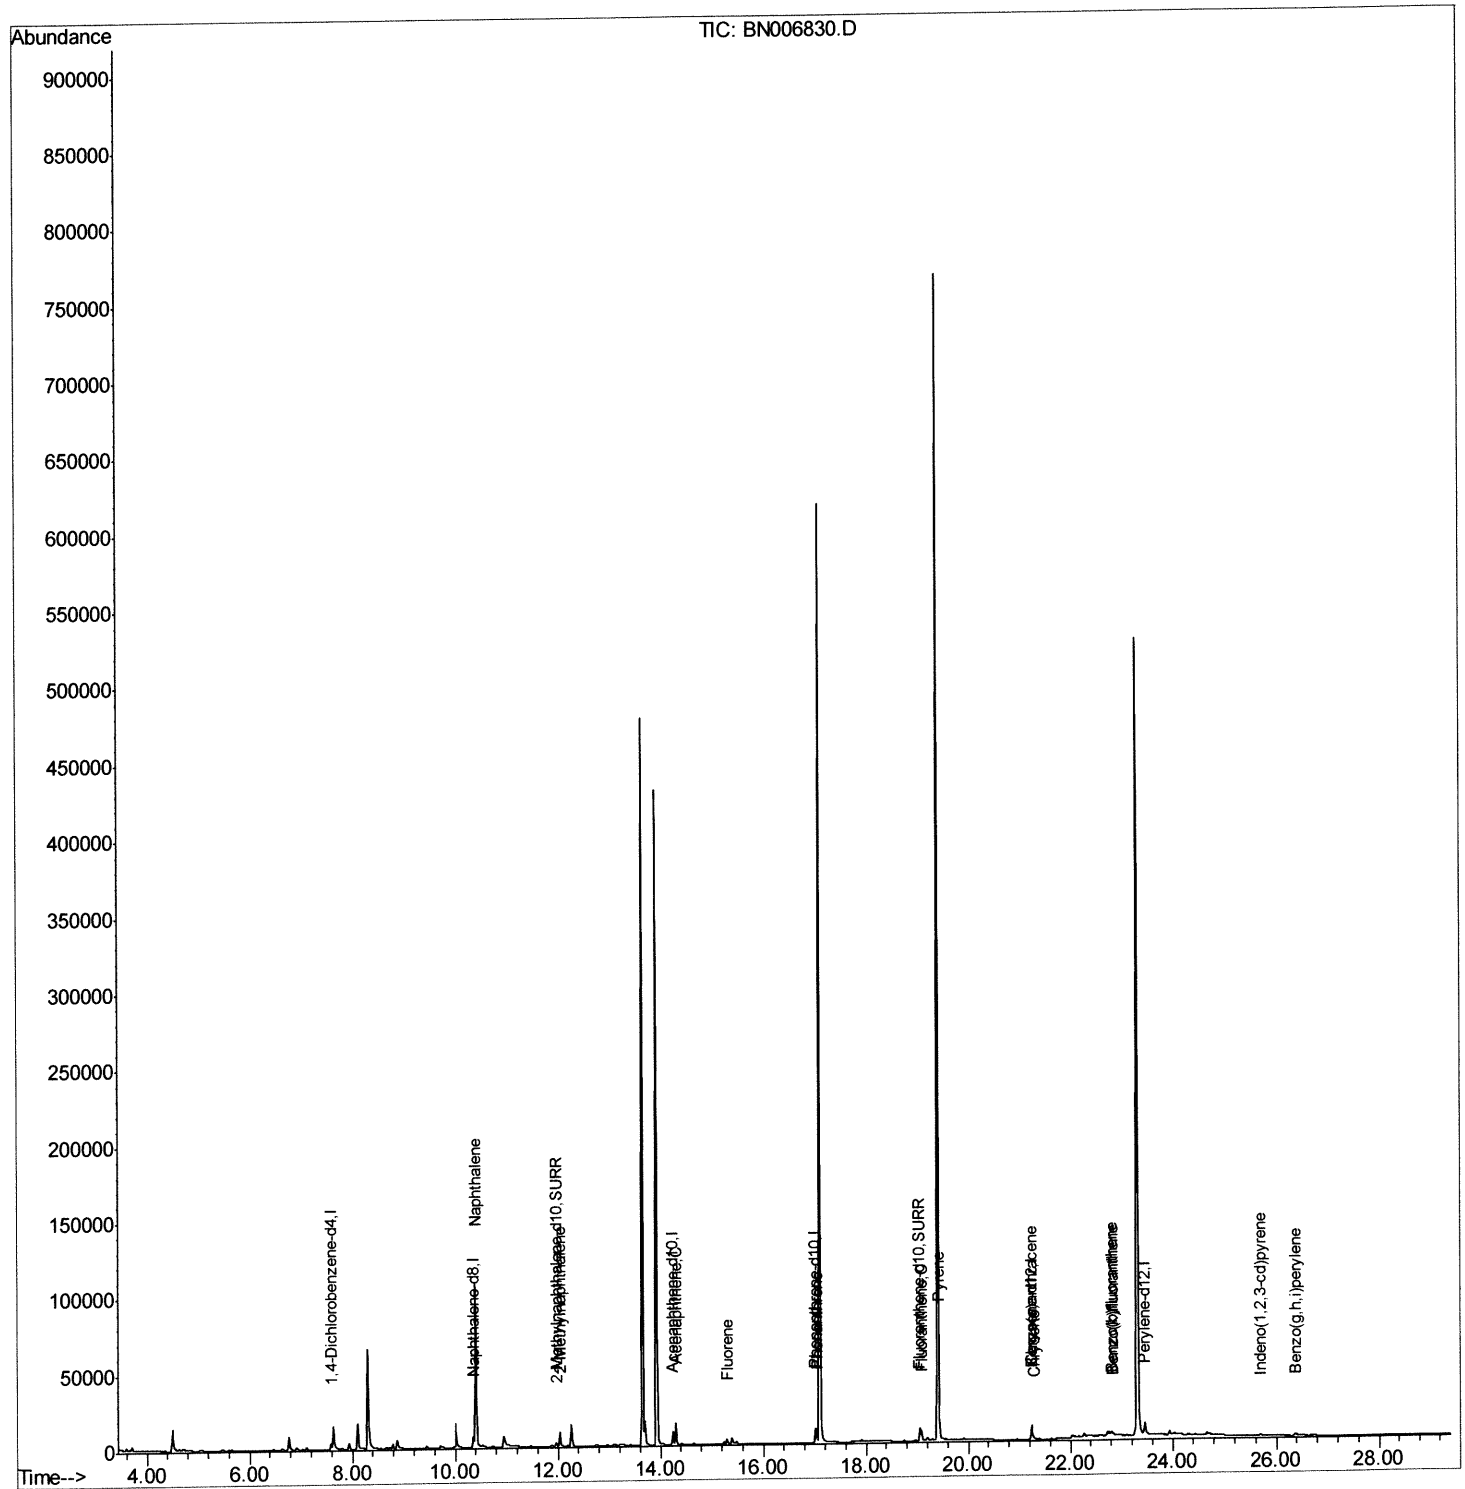

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
Data File : BN006830.D
Acq On : 12 Jul 2019 12:50
Operator : HP/JU
Sample : K3717-14
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF499

Manual Integrations
APPROVED

mohammad
7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:20:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

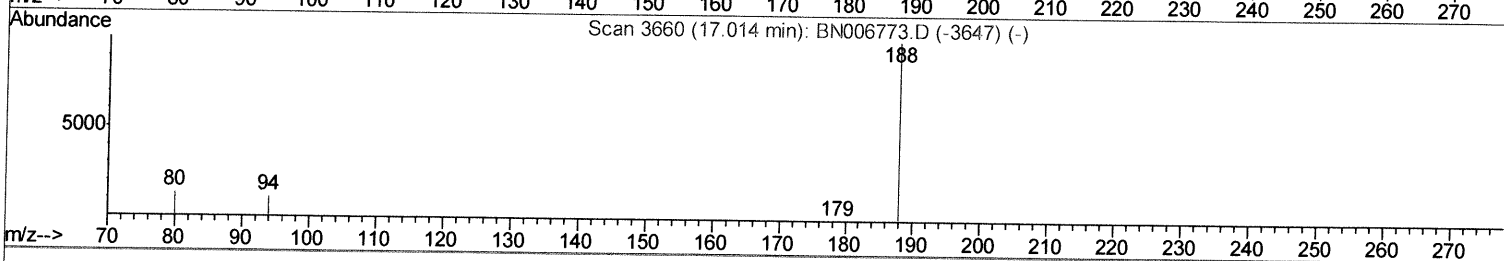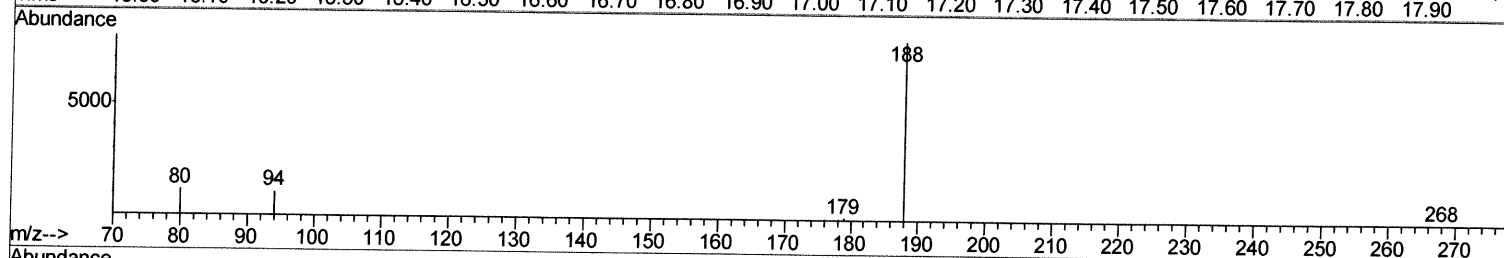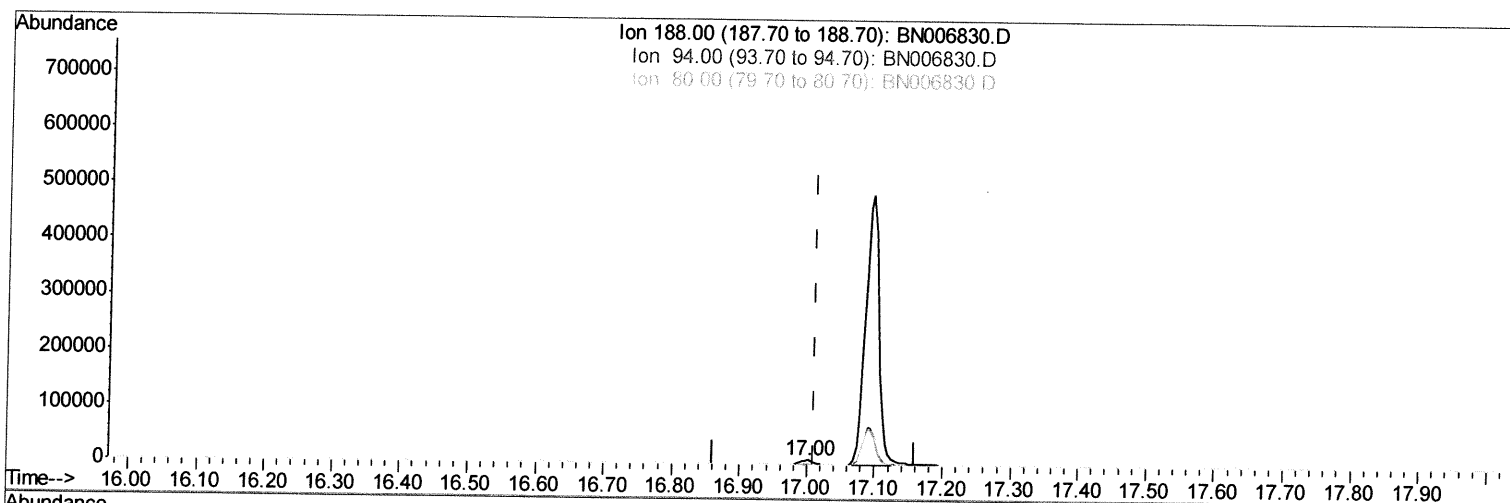

TIC: BN006830.D

(10) Phenanthrene-d10 (I)

17.002min (-0.009) 0.40ng/ul m *Jv 07/16/19*

response 11017

Ion	Exp%	Act%
188.00	100	100
94.00	13.70	13.58
80.00	14.80	14.90
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:20:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

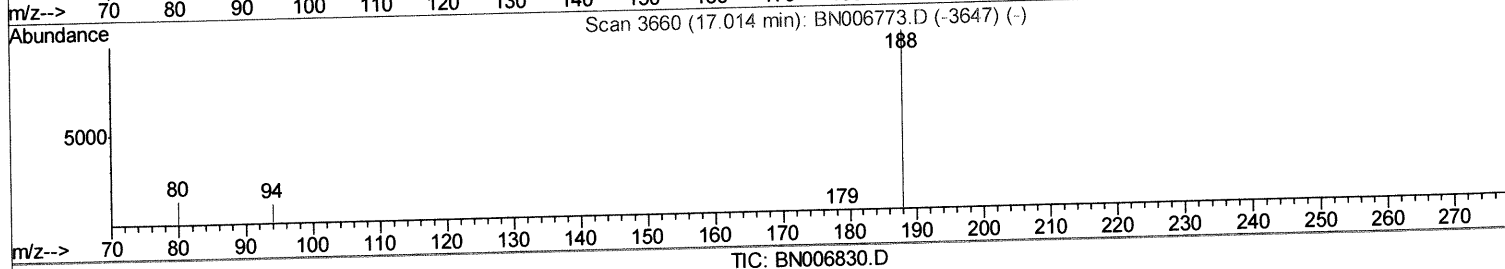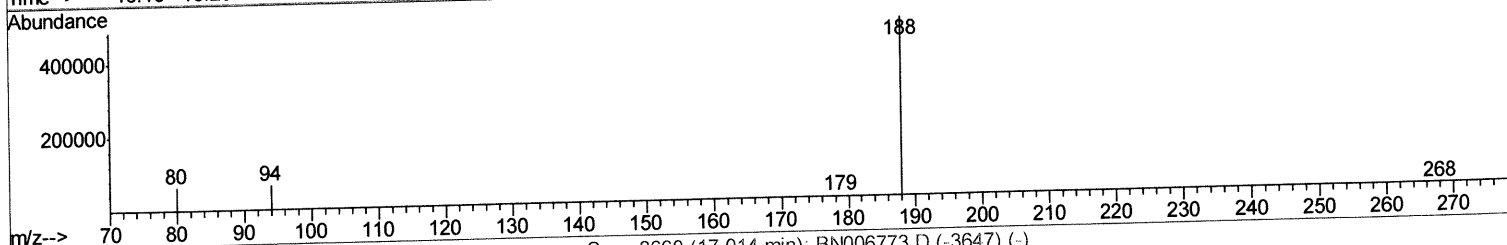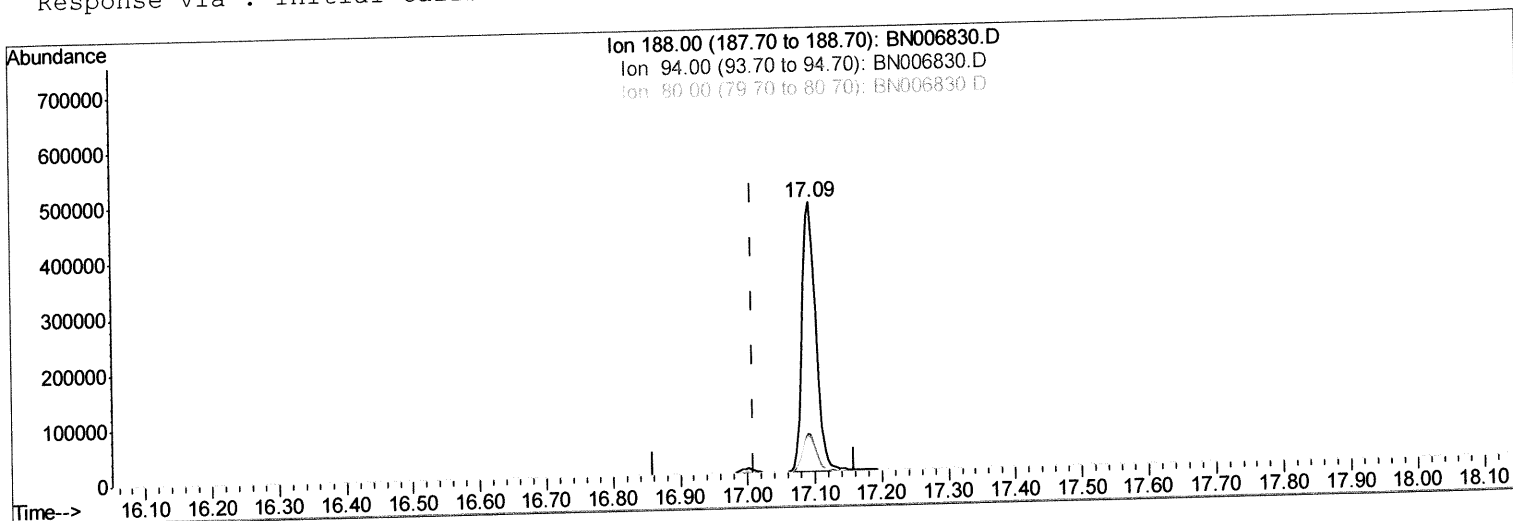

(10) Phenanthrene-d10 (I)

17.094min (+0.084) 0.40ng/ul

response 676948

Ion	Exp%	Act%
188.00	100	100
94.00	13.70	13.59
80.00	14.80	12.80
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
Data File : BN006830.D
Acq On : 12 Jul 2019 12:50
Operator : HP/JU
Sample : K3717-14
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF499

Manual Integrations
APPROVED

mohammad
7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:21:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

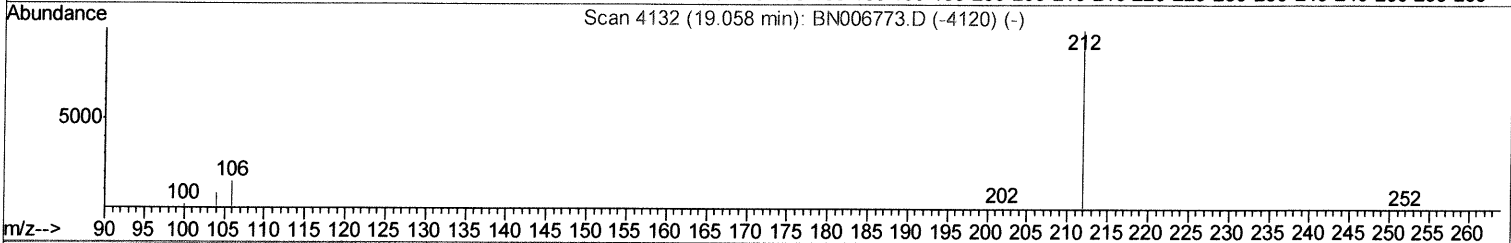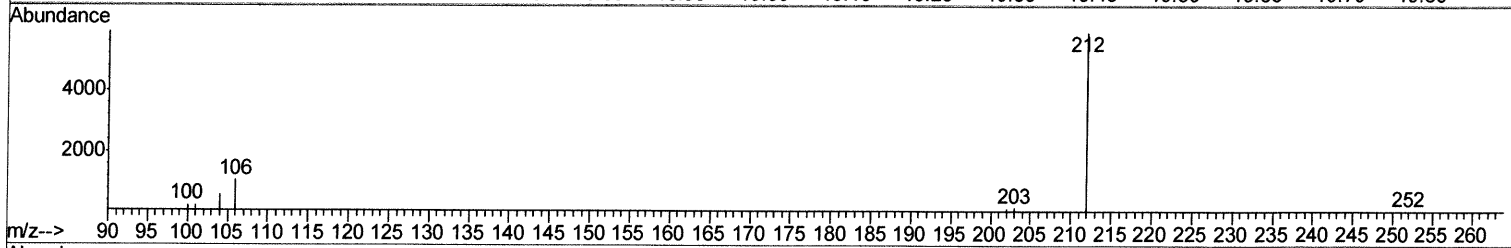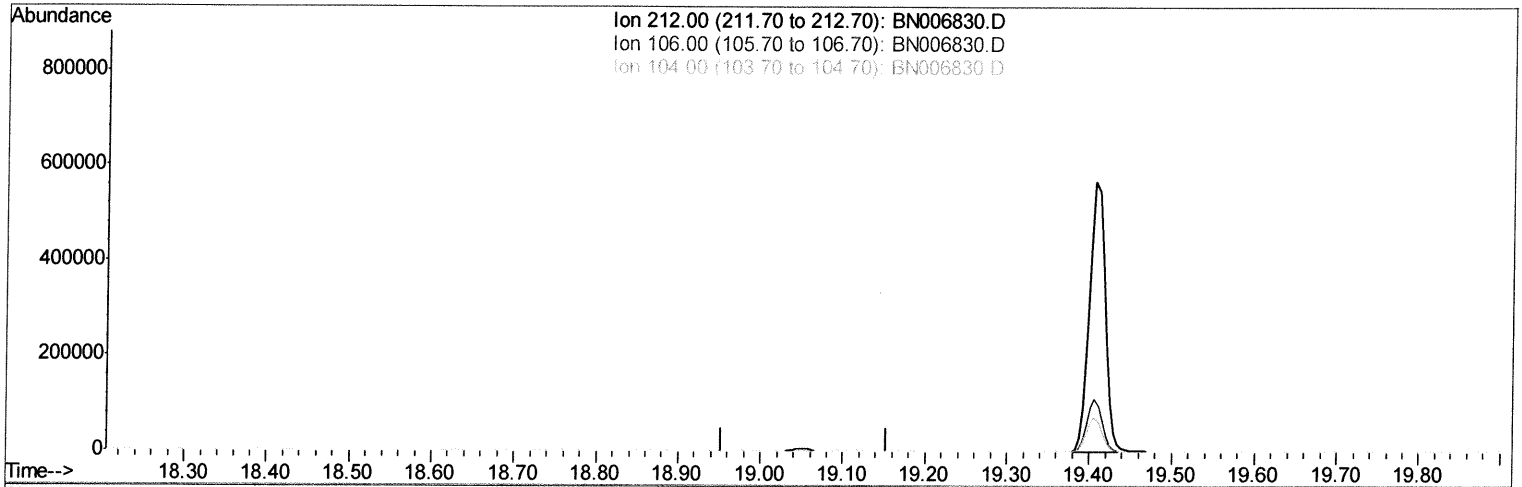

TIC: BN006830.D

(14) Fluoranthene-d10 (SURR)

19.053min (-19.053) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	17.80	0.00#
104.00	9.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
Data File : BN006830.D
Acq On : 12 Jul 2019 12:50
Operator : HP/JU
Sample : K3717-14
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF499

Manual Integrations
APPROVED

mohammad
7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:21:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

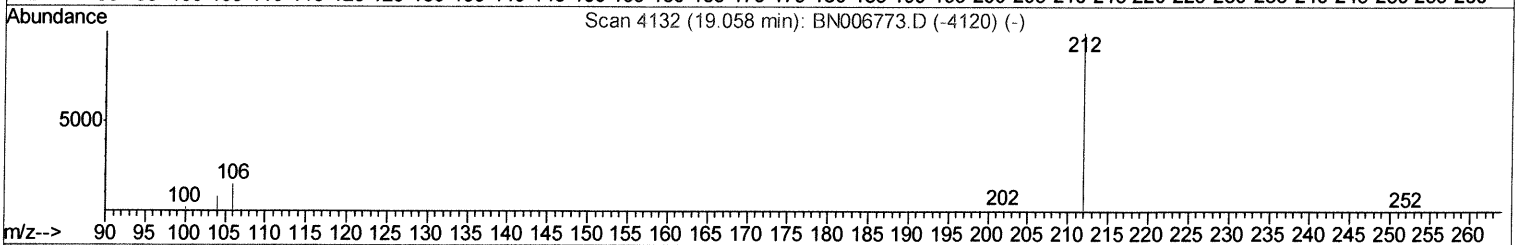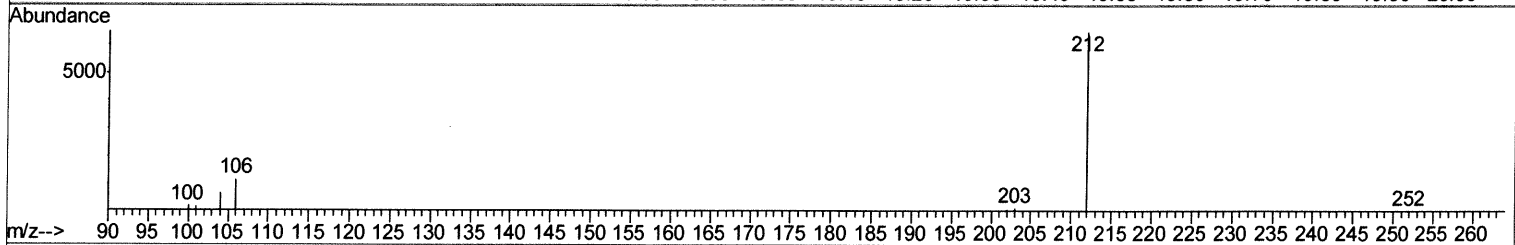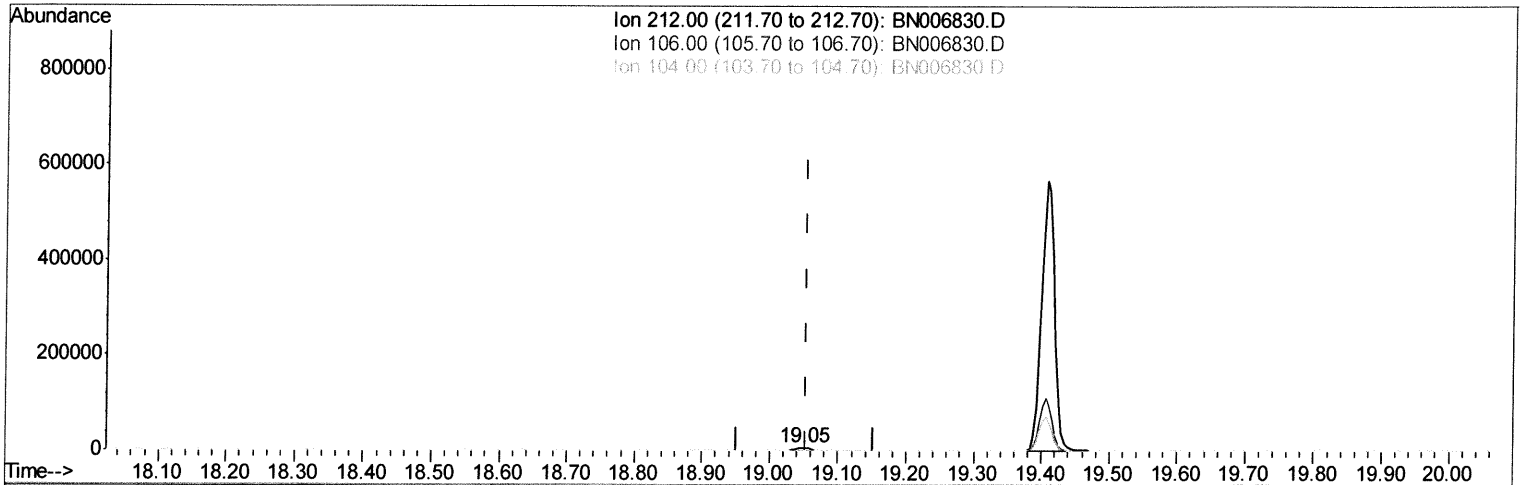

TIC: BN006830.D

(14) Fluoranthene-d10 (SURR)

19.048min (-0.005) 0.28ng/ul m

JU
07/16/19

response 9021

Ion	Exp%	Act%
212.00	100	100
106.00	17.80	0.00#
104.00	9.70	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:21:59 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

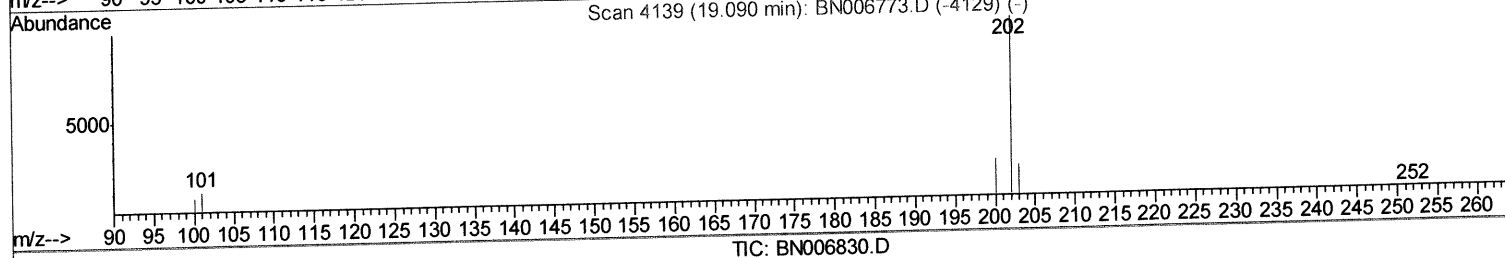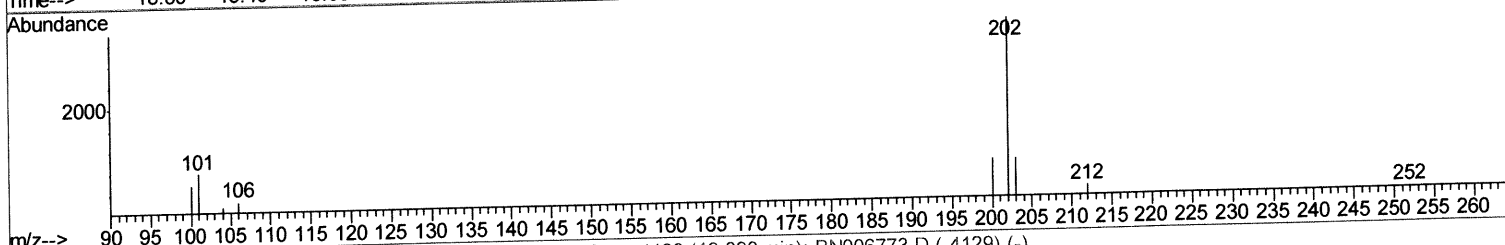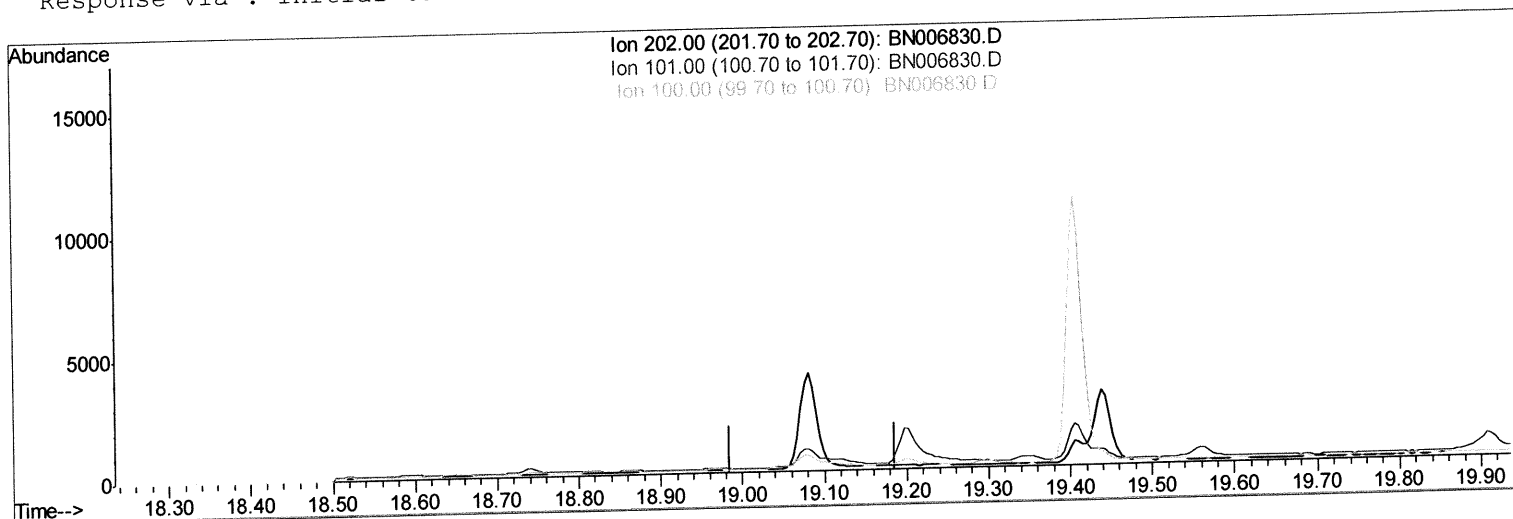

(15) Fluoranthene (C)

19.086min (-19.086) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	13.20	0.00
100.00	9.90	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:21:59 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

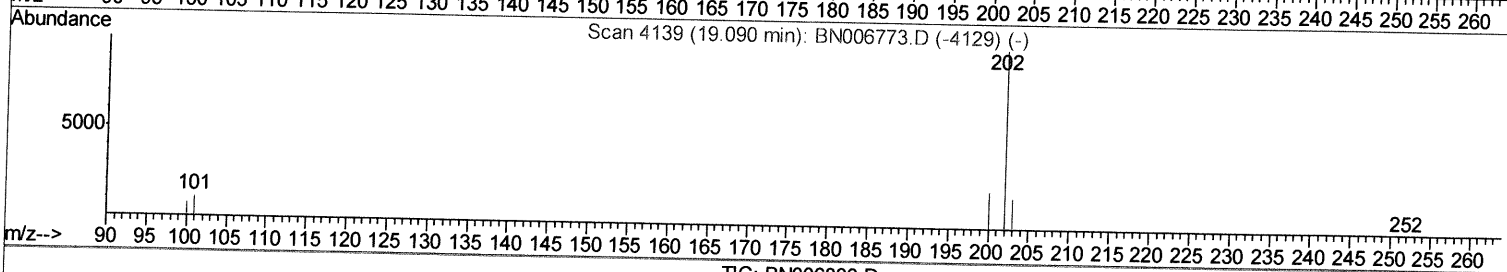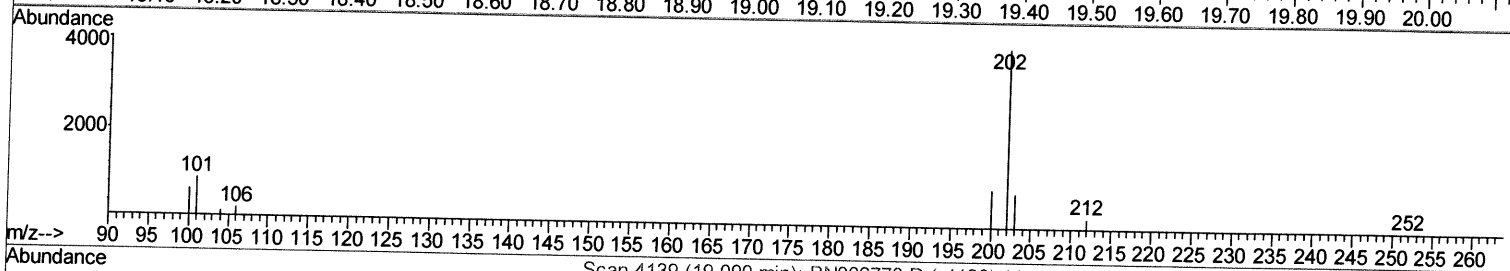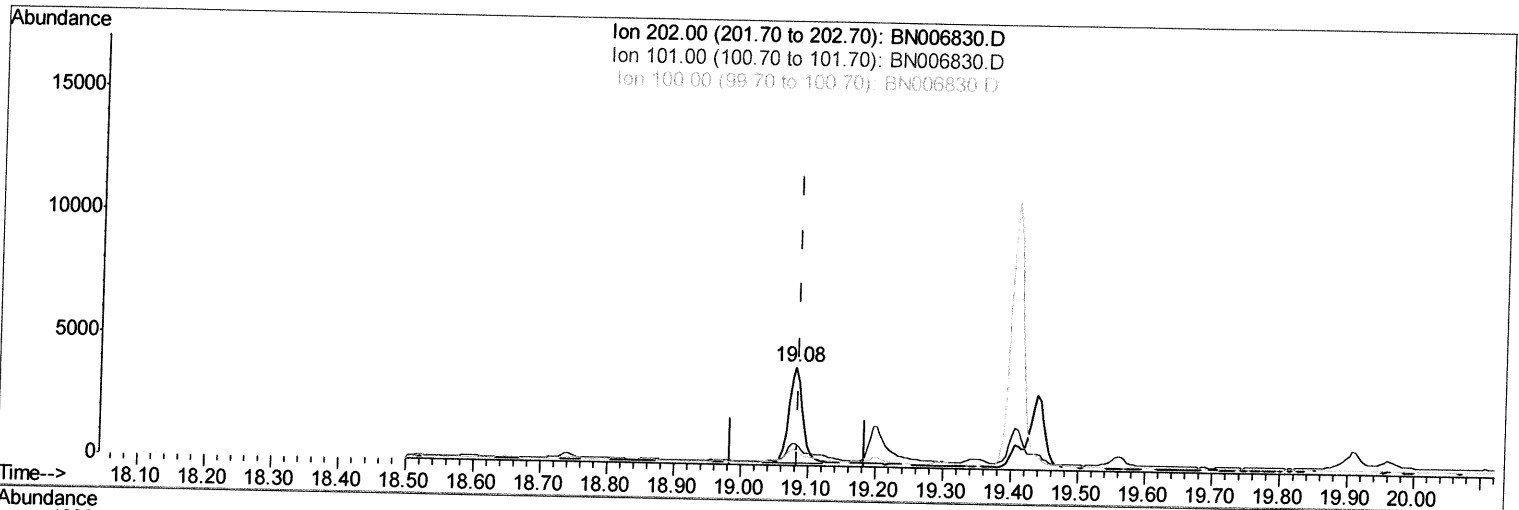

(15) Fluoranthene (C)

19.081min (-0.005) 0.13ng/ul m ^{JU} 07/16/19

response 5720

Ion	Exp%	Act%
202.00	100	100
101.00	13.20	22.41
100.00	9.90	16.32
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
Data File : BN006830.D
Acq On : 12 Jul 2019 12:50
Operator : HP/JU
Sample : K3717-14
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampled :
BF499

Manual Integrations
APPROVED

mohammad
7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:21:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

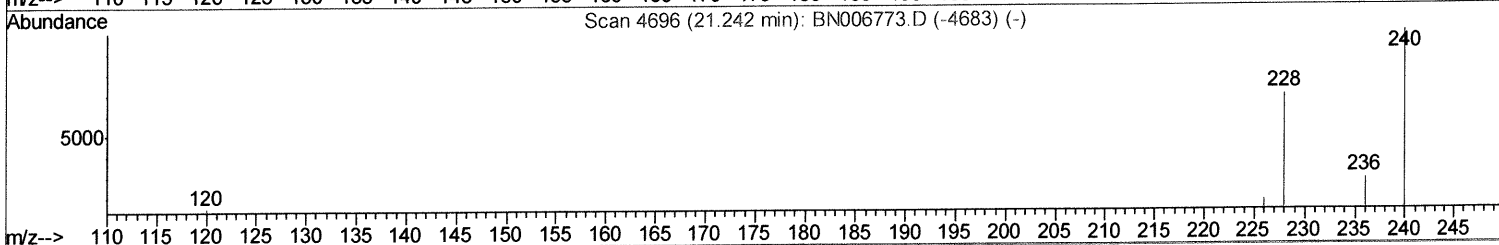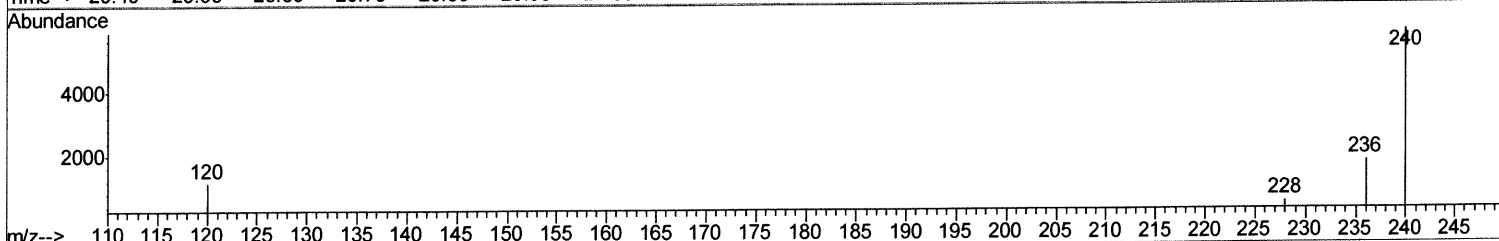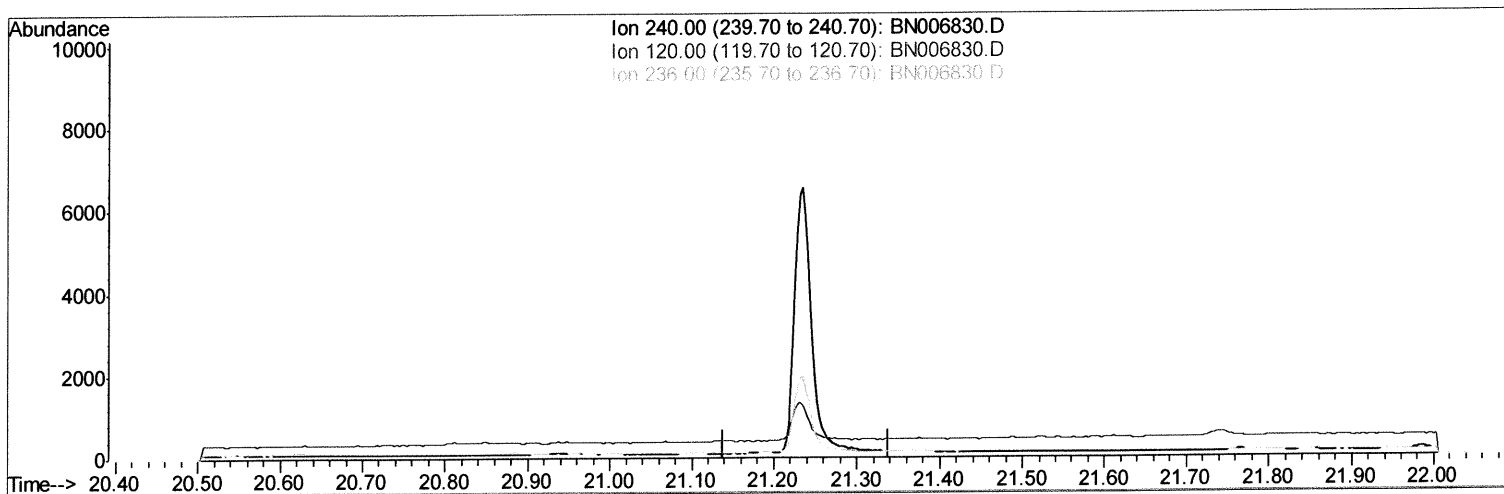

TIC: BN006830.D

(16) Chrysene-d12 (I)

21.239min (-21.239) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.20	0.00#
236.00	30.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
Data File : BN006830.D
Acq On : 12 Jul 2019 12:50
Operator : HP/JU
Sample : K3717-14
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF499

Manual Integrations
APPROVED

mohammad
7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:21:59 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

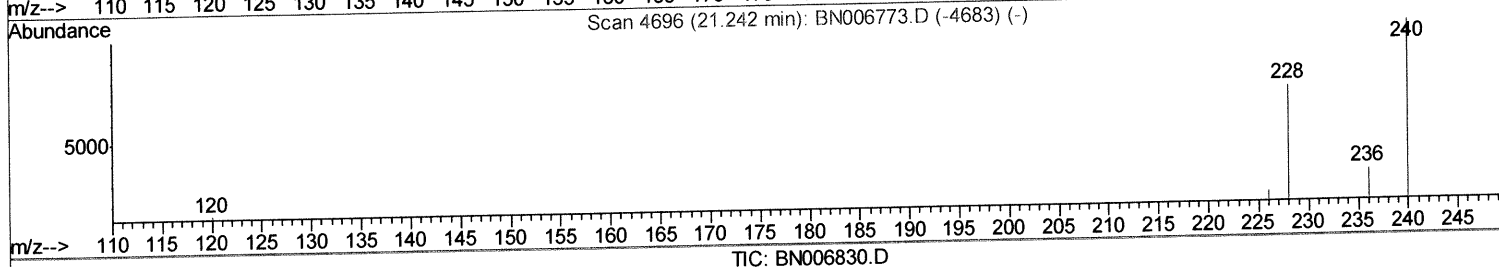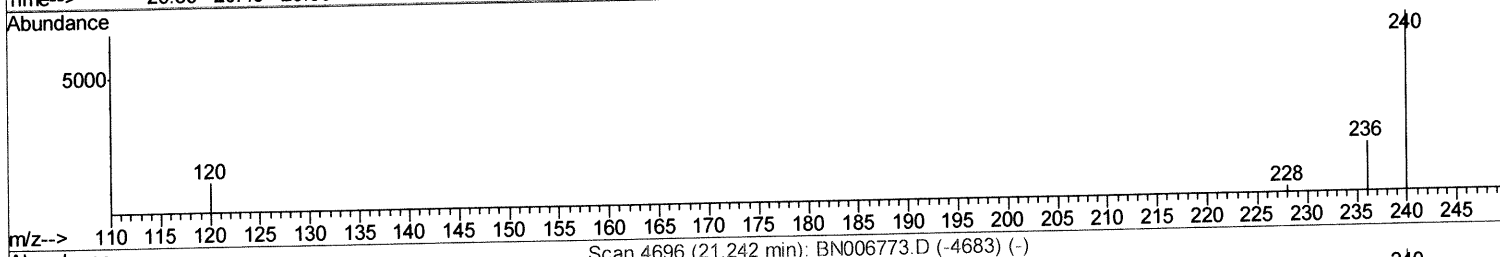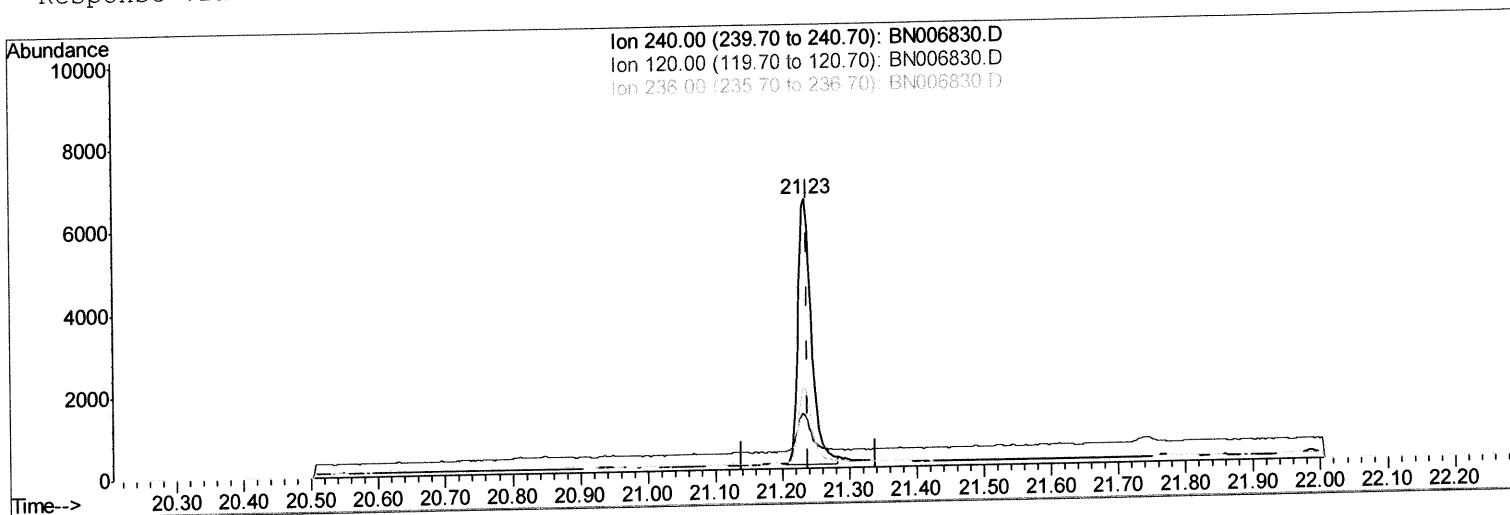

(16) Chrysene-d12 (I)

21.235min (-0.004) 0.40ng/ul m *JU 07/16/19*

response 9028

Ion	Exp%	Act%
240.00	100	100
120.00	20.20	19.65
236.00	30.00	30.05
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:23:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

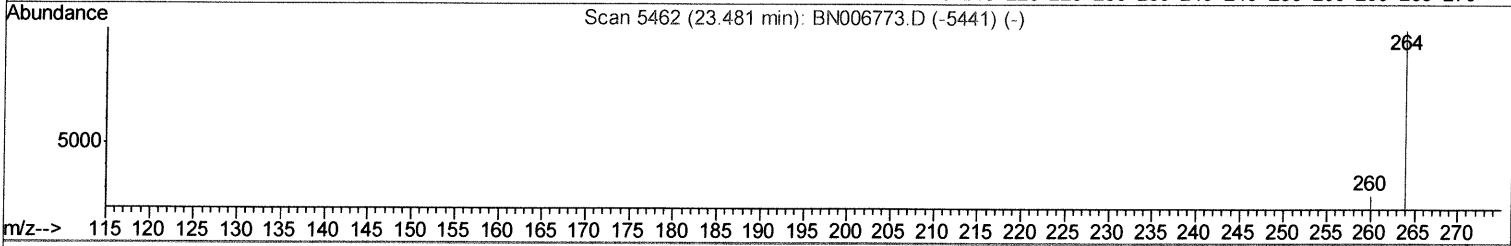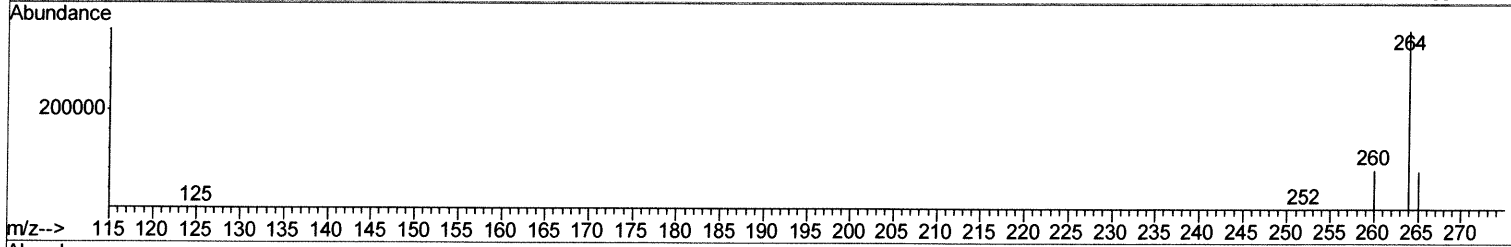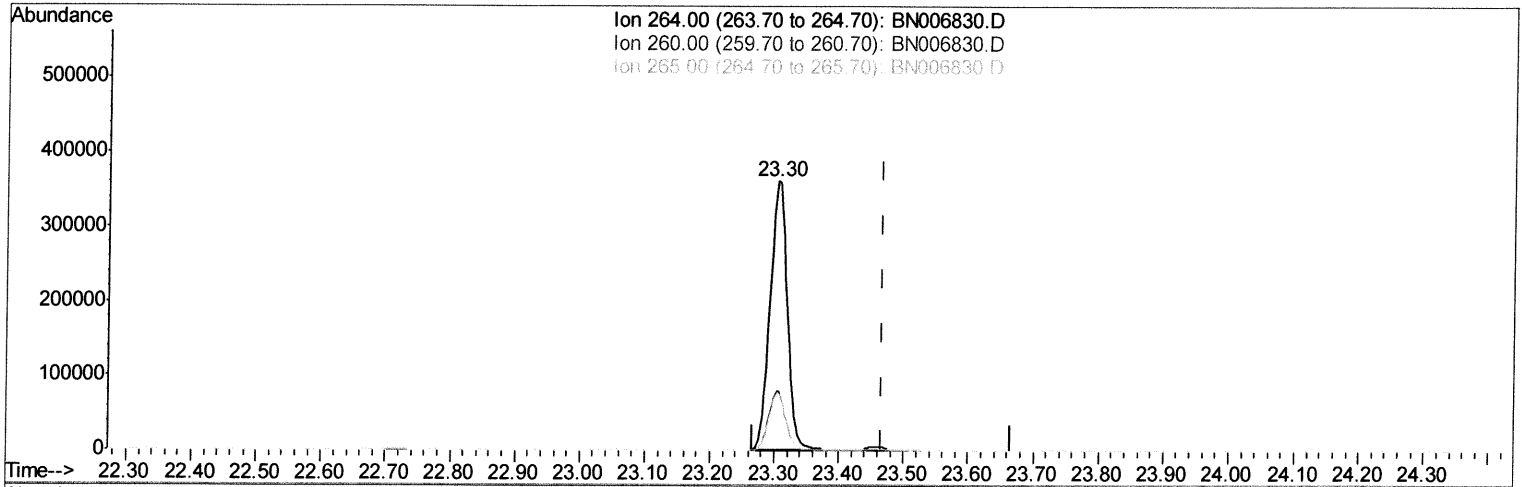

TIC: BN006830.D

(20) Perylene-d12 (I)

23.304min (-0.162) 0.40ng/ul

response 663318

Ion	Exp%	Act%
264.00	100	100
260.00	27.80	22.37
265.00	36.10	21.44#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:23:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

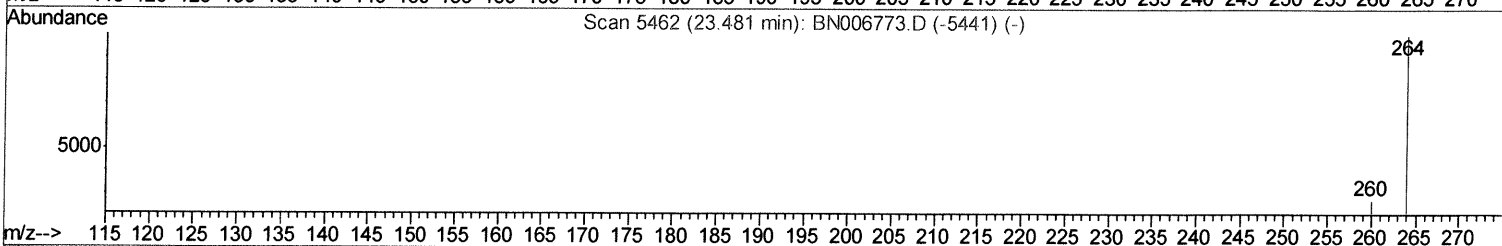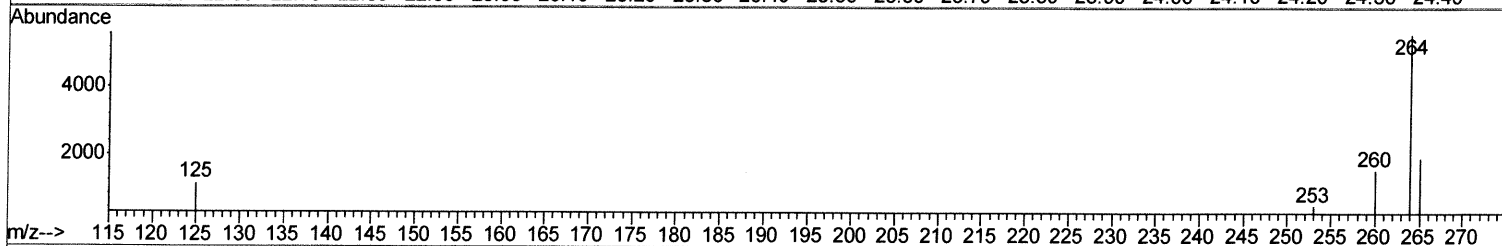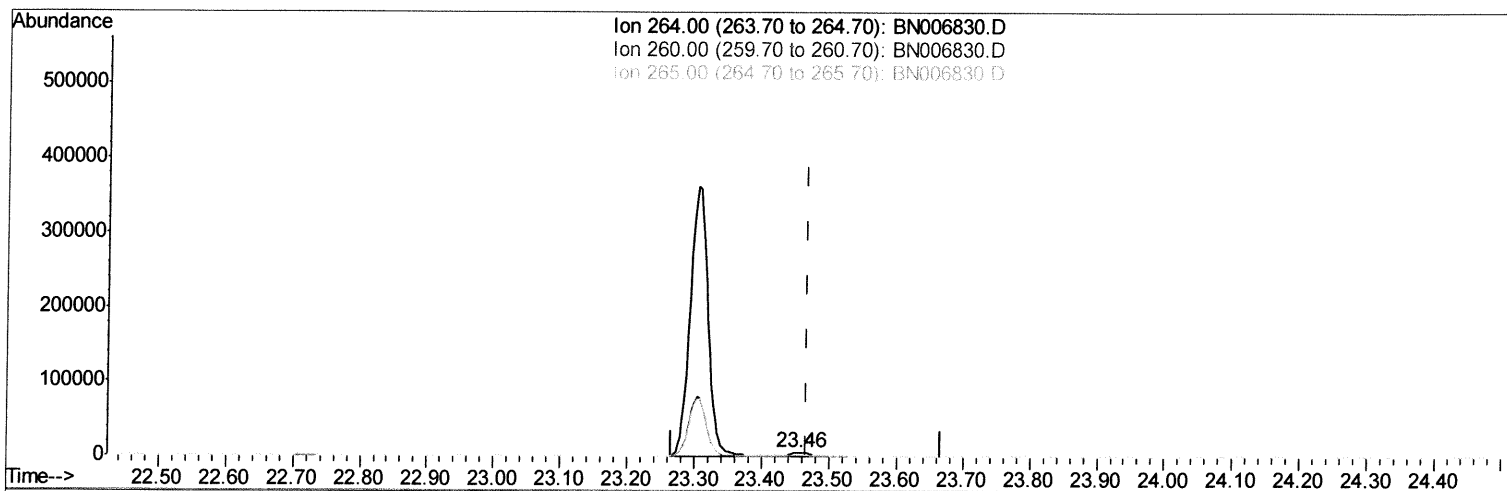

TIC: BN006830.D

(20) Perylene-d12 (I)

23.456min (-0.010) 0.40ng/ul m

JU
 07/16/19

response 8543

Ion	Exp%	Act%
264.00	100	100
260.00	27.80	27.43
265.00	36.10	33.86
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:23:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

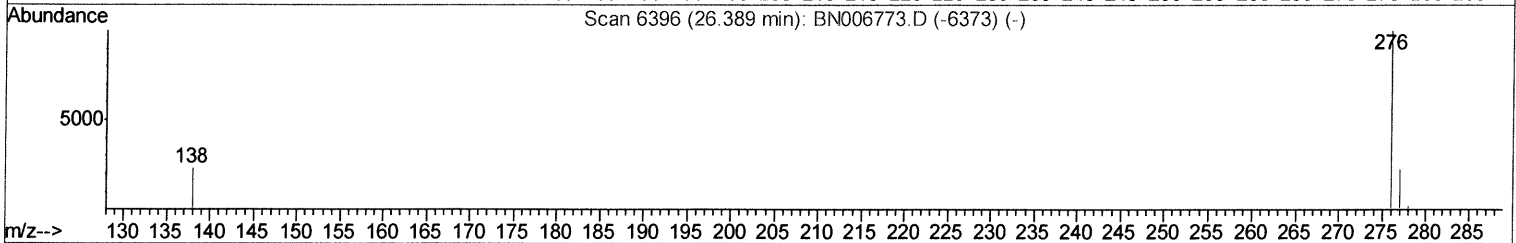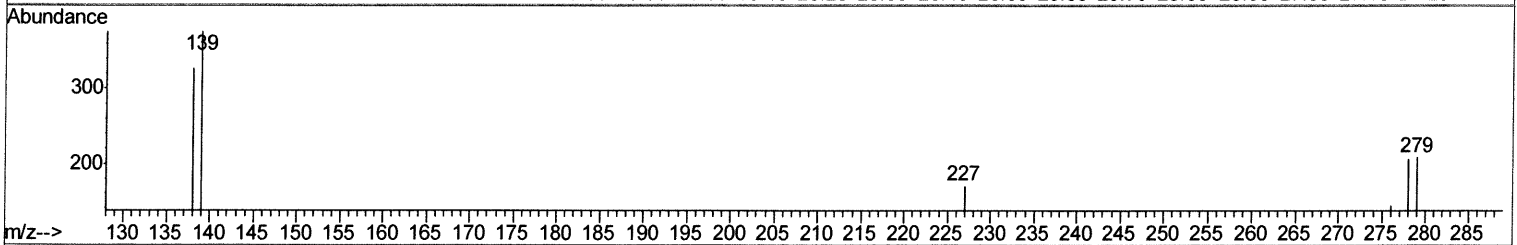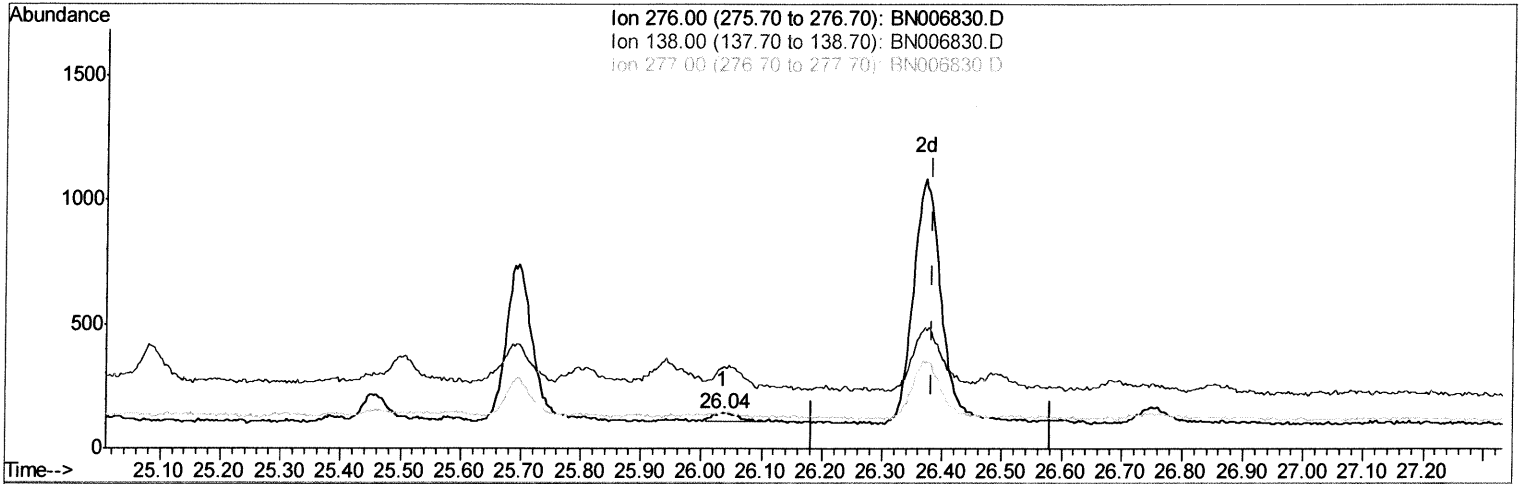

TIC: BN006830.D

(26) Benzo(g,h,i)perylene

26.035min (-0.347) 0.00ng/ul

response 102

Ion	Exp%	Act%
276.00	100	100
138.00	27.70	228.67#
277.00	24.40	95.80#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:23:53 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

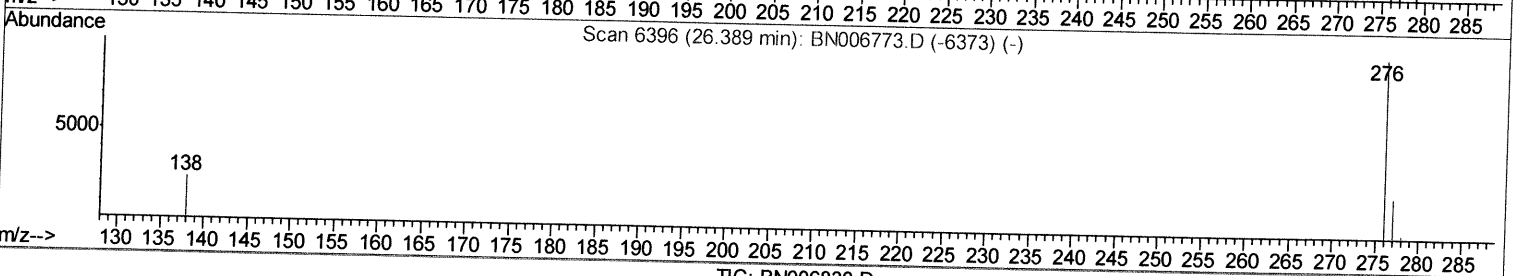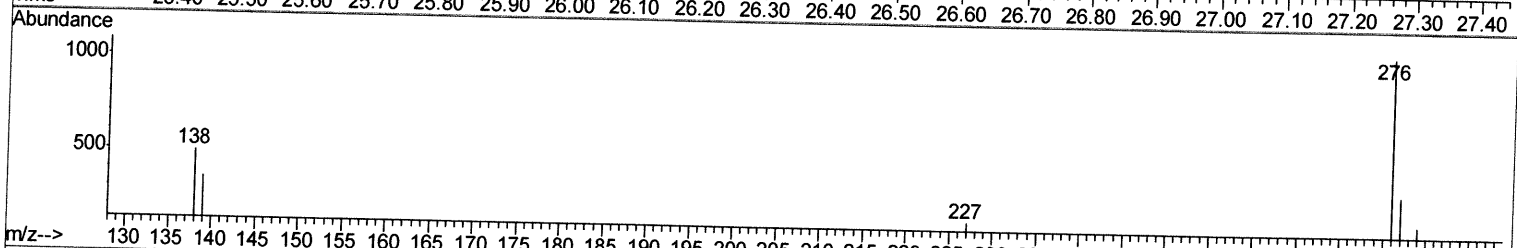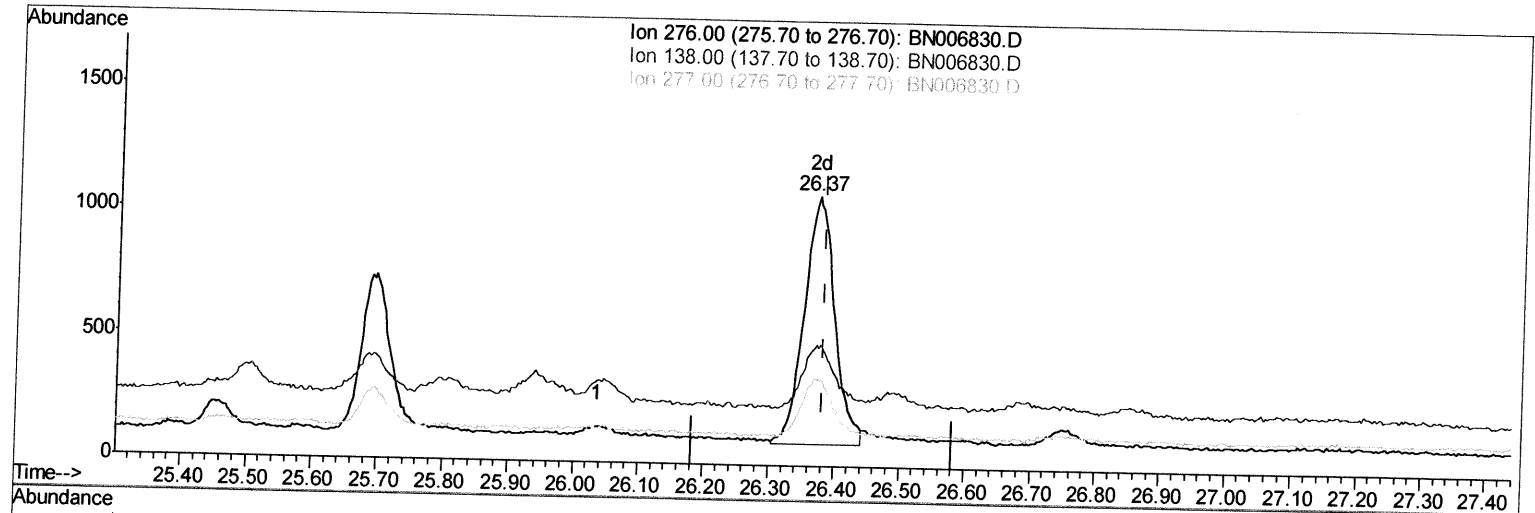

TIC: BN006830.D

(26) Benzo(g,h,i)perylene

26.371min (-0.012) 0.11ng/ul m *JU 07/16/19*

response 3244

Ion	Exp%	Act%
276.00	100	100
138.00	27.70	45.03#
277.00	24.40	31.95#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampled :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:24:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

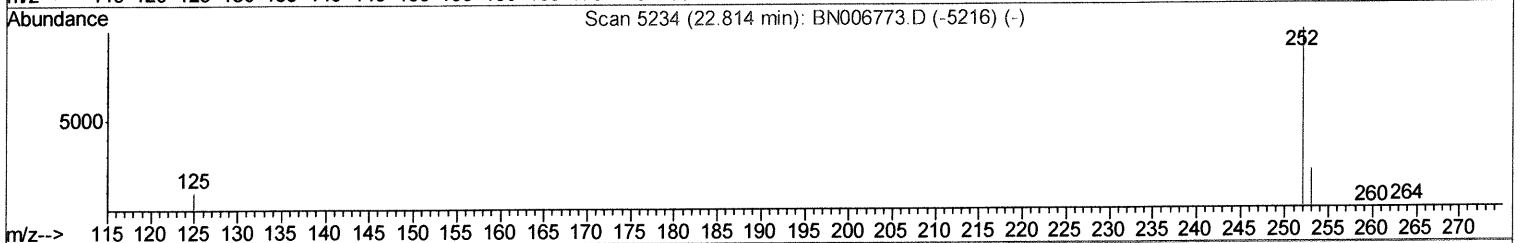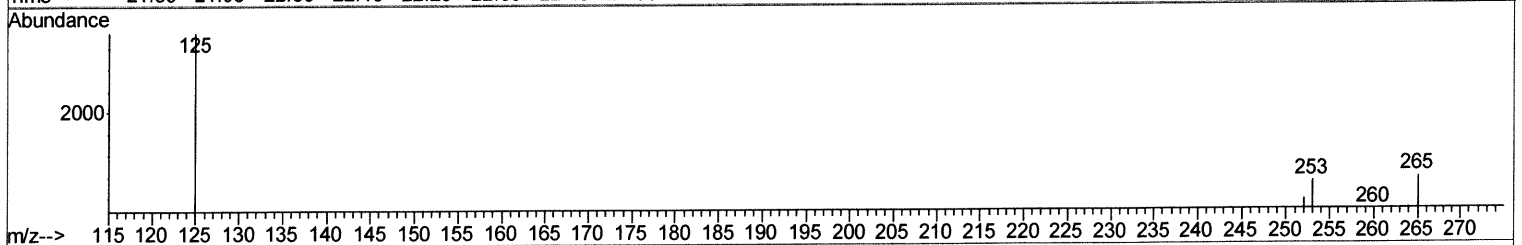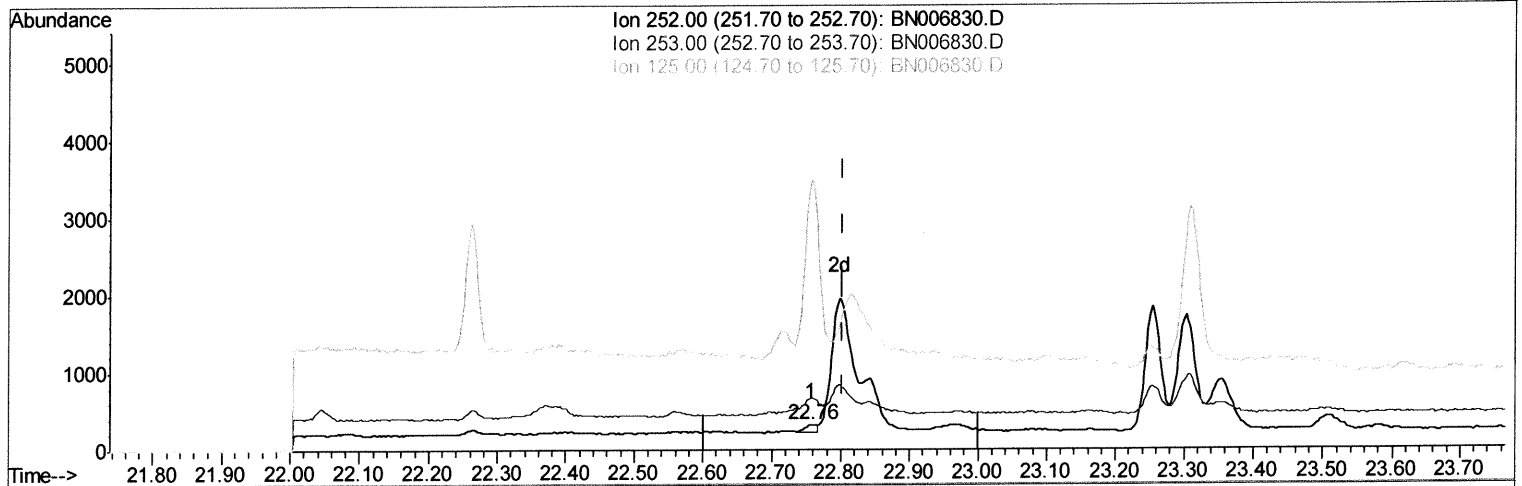

TIC: BN006830.D

(21) Benzo(b)fluoranthene
 22.757min (-0.045) 0.00ng/ul
 response 110

Ion	Exp%	Act%
252.00	100	100
253.00	23.90	207.45#
125.00	14.60	1083.23#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:24:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

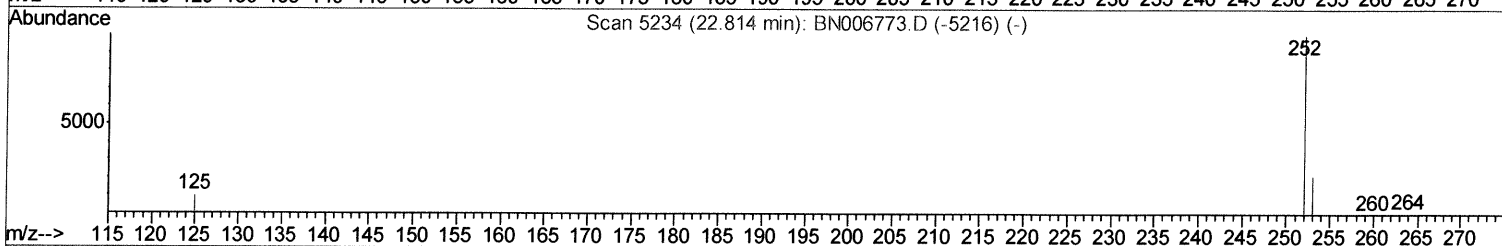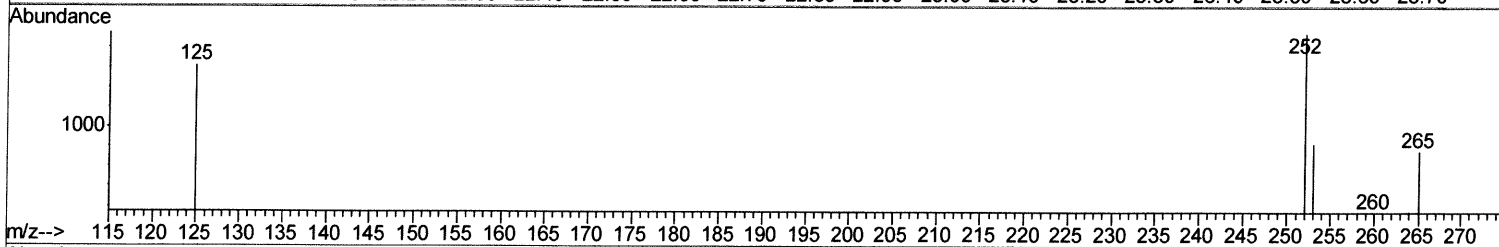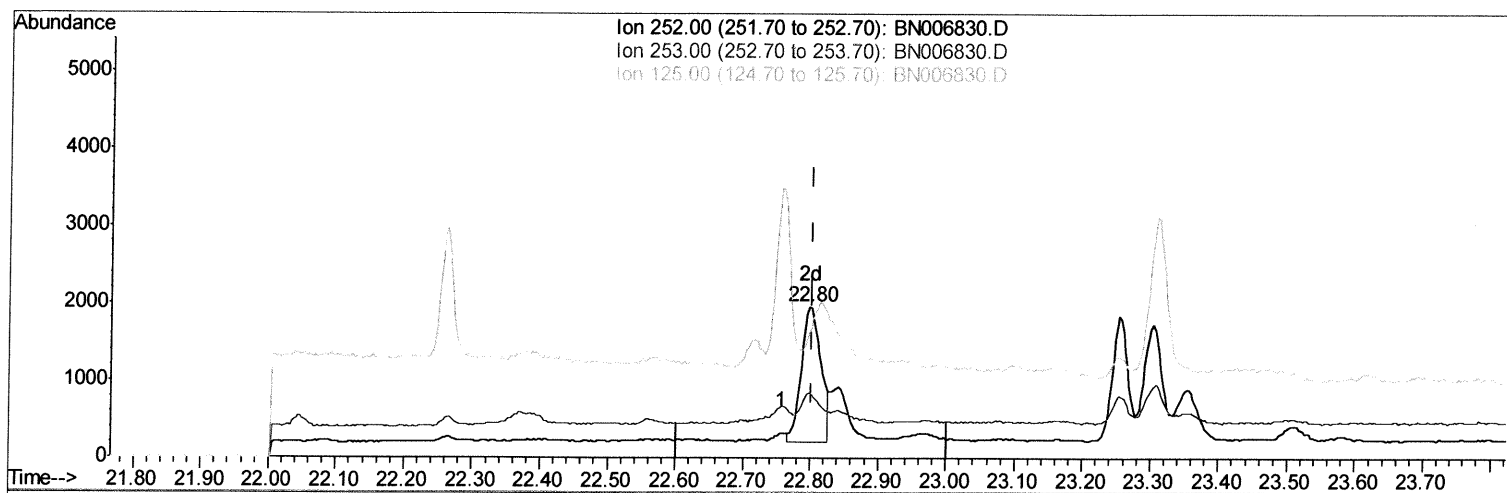

TIC: BN006830.D

(21) Benzo(b)fluoranthene

22.798min (-0.004) 0.10ng/ul m *JU 07/16/19*

response 3459

Ion	Exp%	Act%
252.00	100	100
253.00	23.90	43.14
125.00	14.60	82.65#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
Data File : BN006830.D
Acq On : 12 Jul 2019 12:50
Operator : HP/JU
Sample : K3717-14
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BF499

Manual Integrations
APPROVED

mohammad
7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:24:34 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

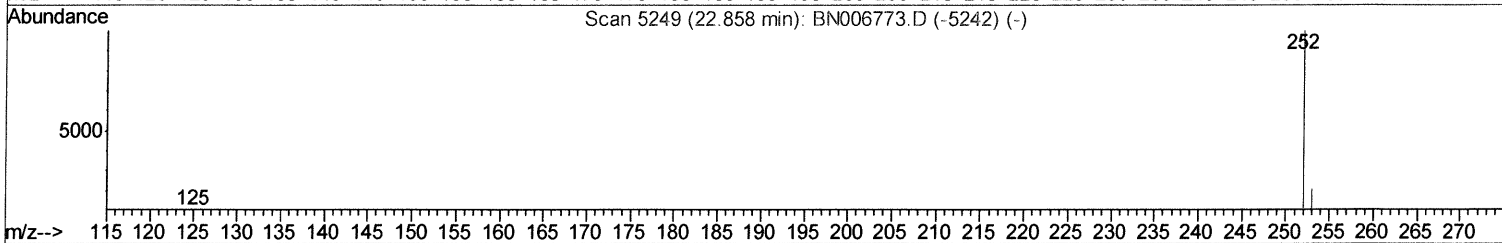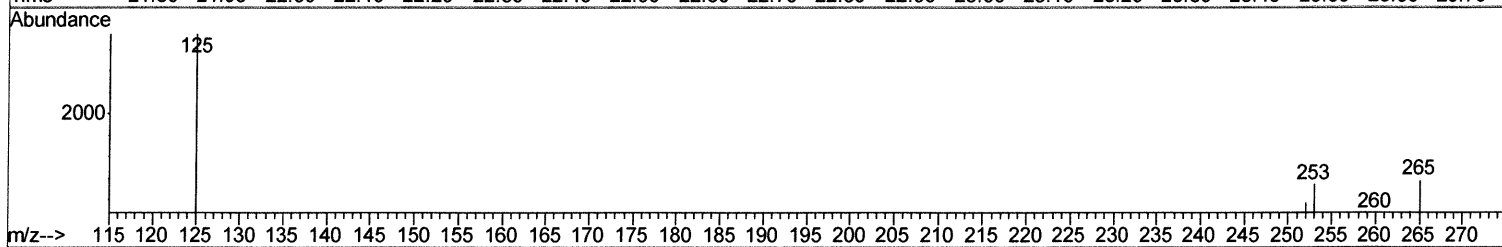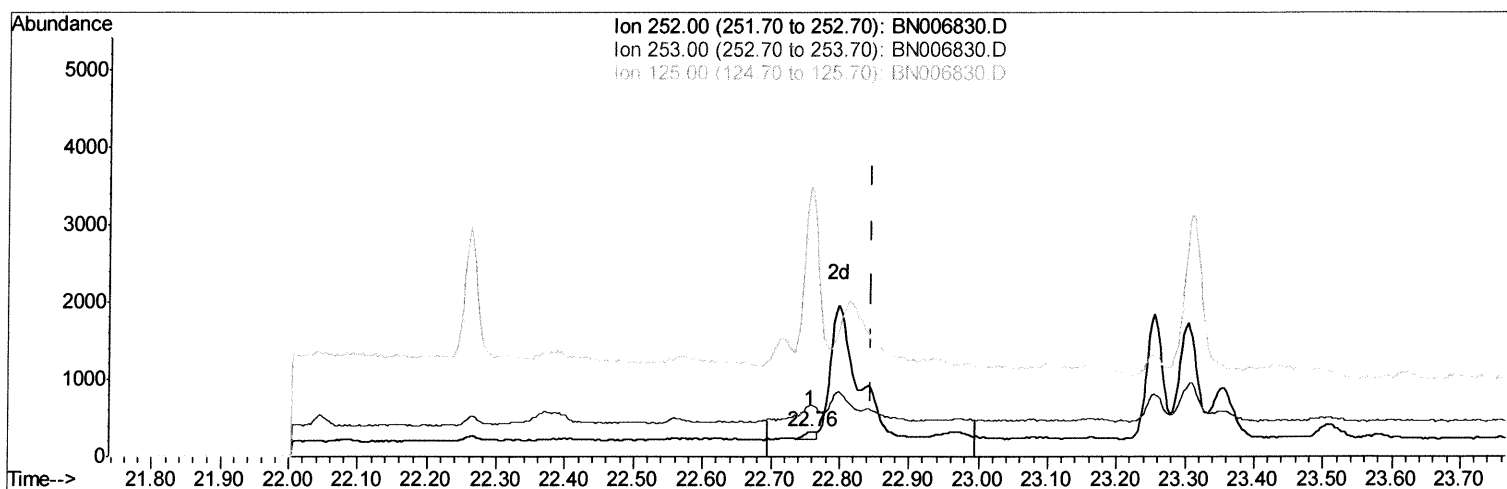

TIC: BN006830.D

(22) Benzo(k)fluoranthene

22.757min (-0.089) 0.00ng/ul

response 110

Ion	Exp%	Act%
252.00	100	100
253.00	24.00	207.45#
125.00	13.80	1083.23#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:24:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

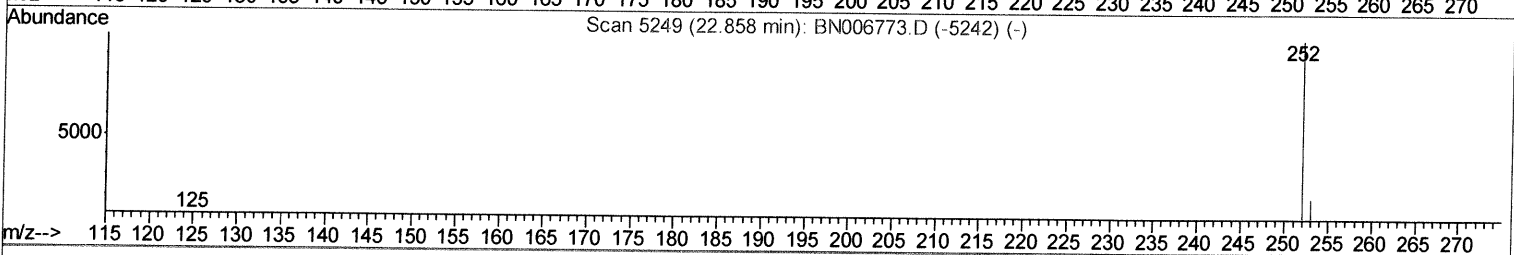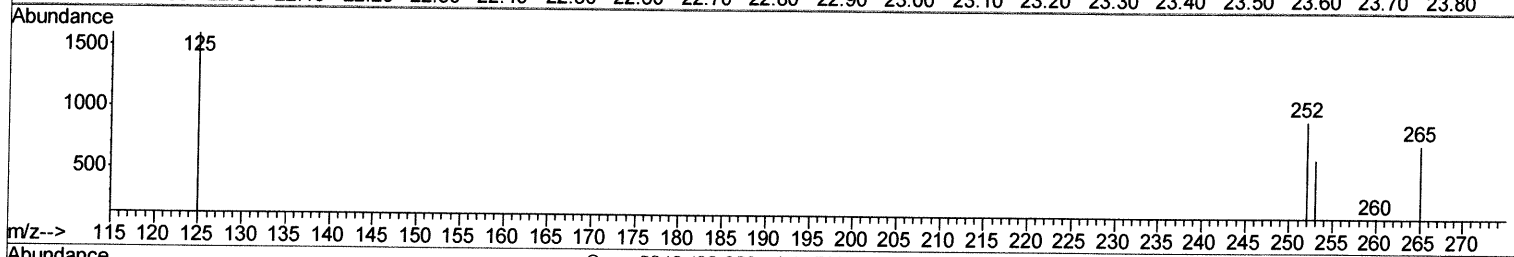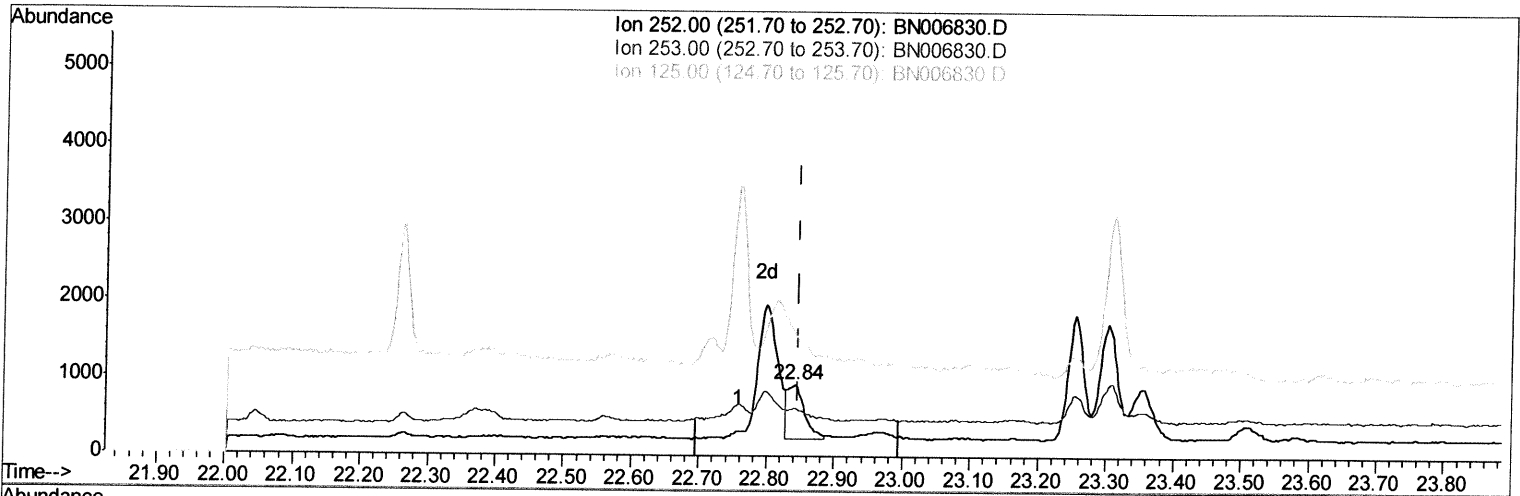

TIC: BN006830.D

(22) Benzo(k)fluoranthene

22.842min (-0.004) 0.03ng/ul m *JU* 07/16/19

response 1229

Ion	Exp%	Act%
252.00	100	100
253.00	24.00	66.31#
125.00	13.80	172.37#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:24:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

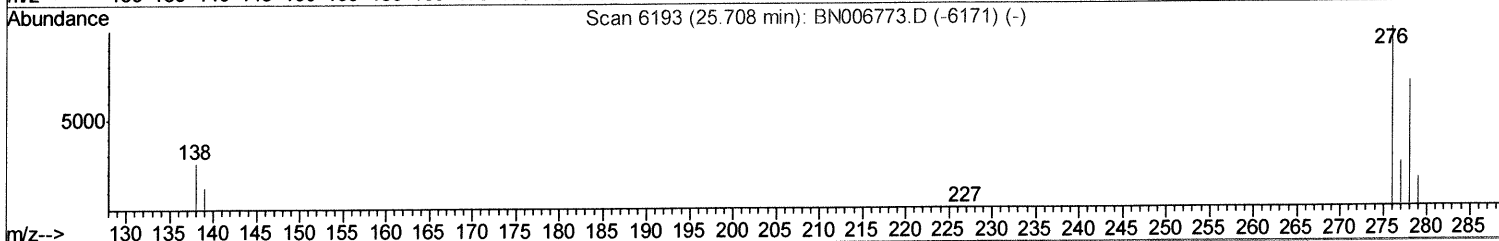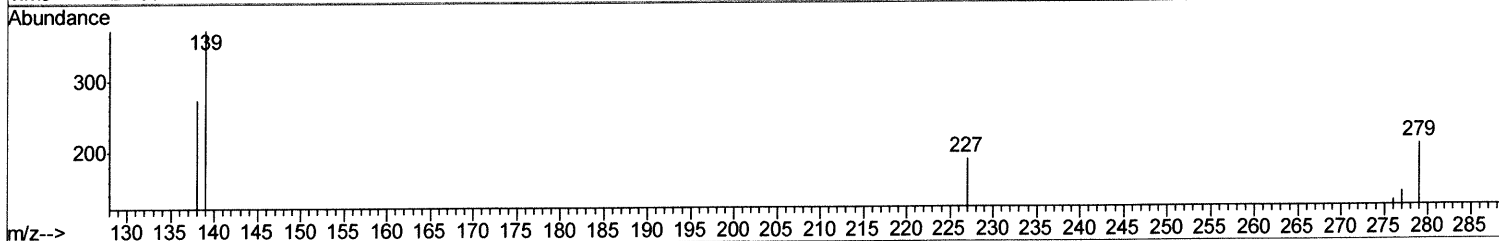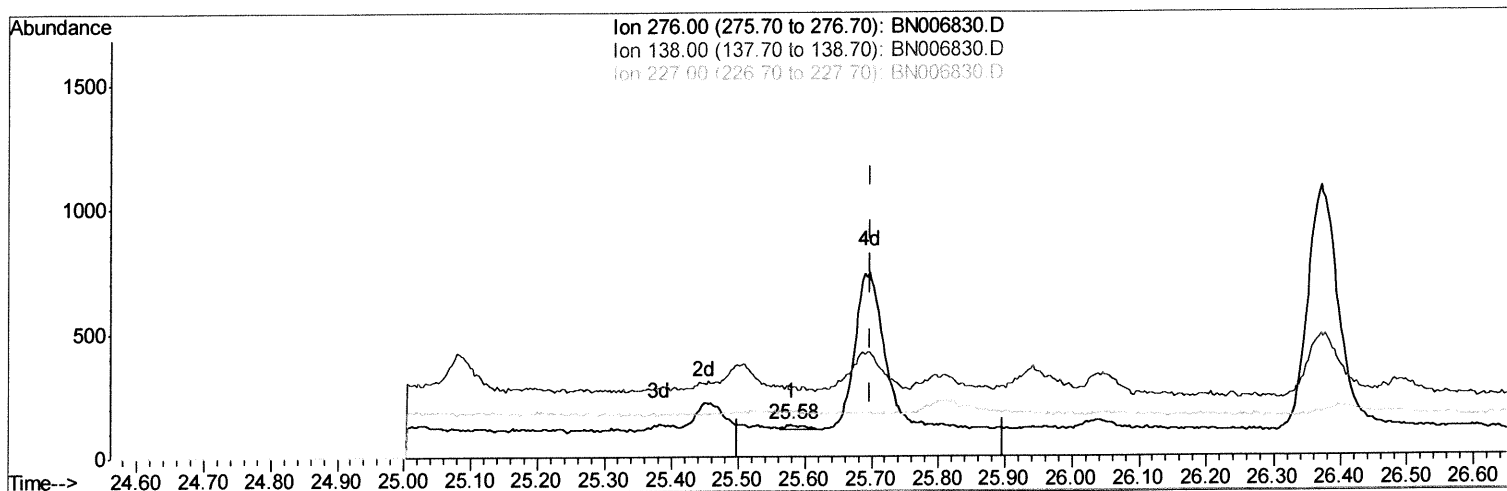

TIC: BN006830.D

(24) Indeno(1,2,3-cd)pyrene

25.579min (-0.119) 0.00ng/ul

response 42

Ion	Exp%	Act%
276.00	100	100
138.00	30.40	35.71
227.00	0.30	78.57#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:24:34 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration

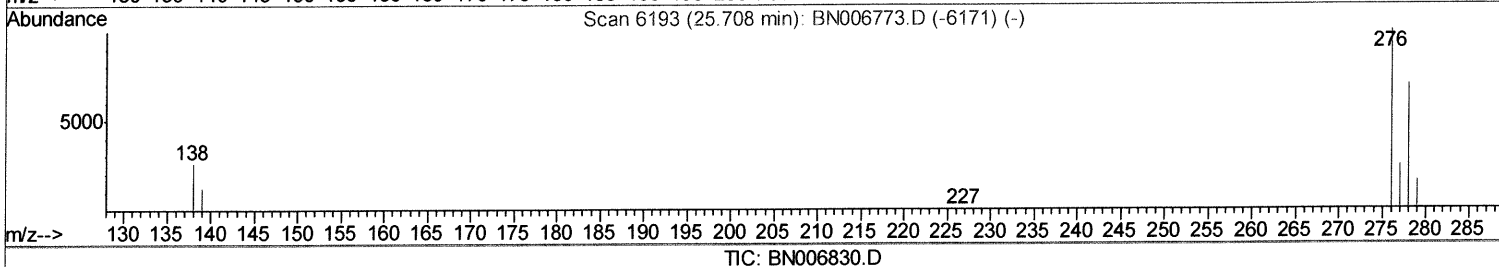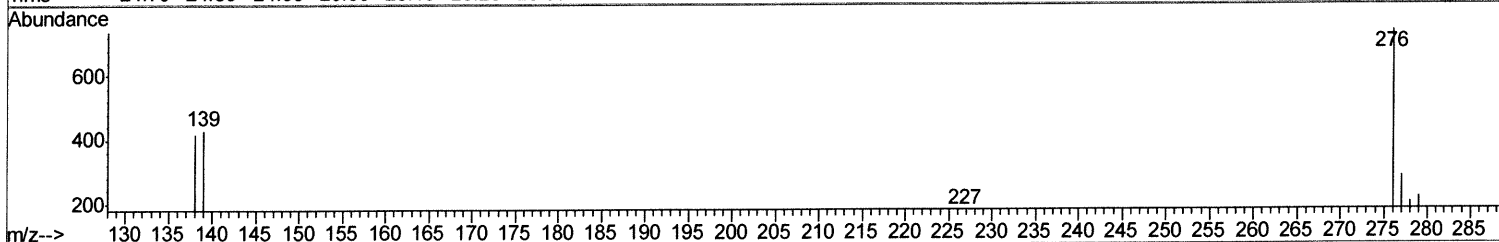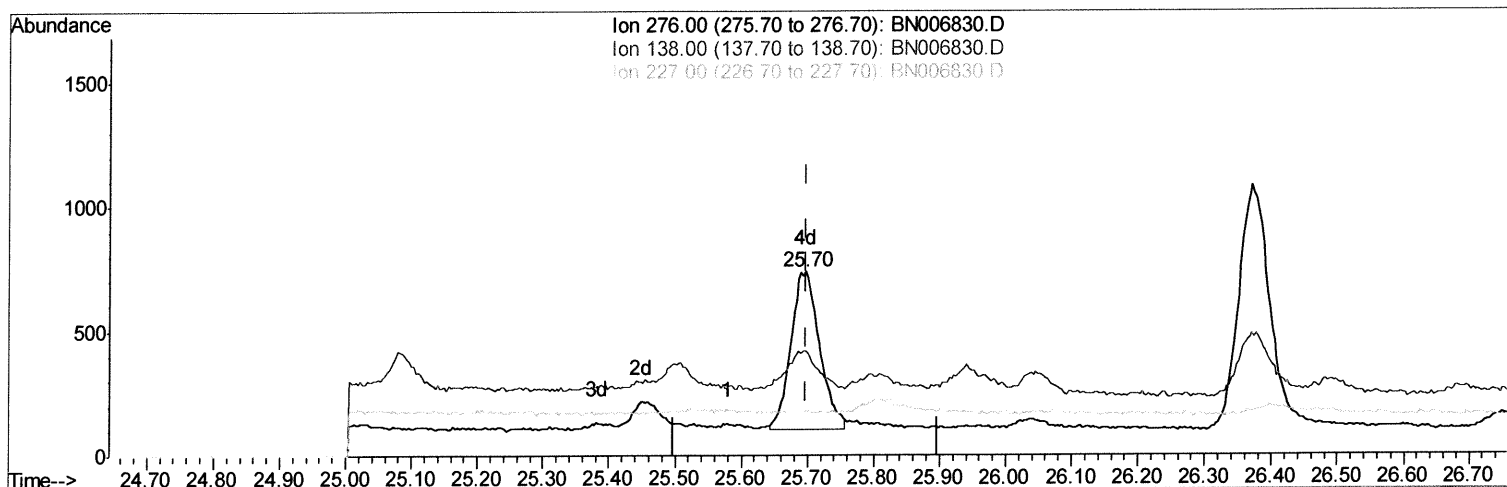

(24) Indeno(1,2,3-cd)pyrene

25.696min (-0.002) 0.06ng/ul m *JU 07/16/19*

response 1920

Ion	Exp%	Act%
276.00	100	100
138.00	30.40	0.78#
227.00	0.30	1.72#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071119\
 Data File : BN006830.D
 Acq On : 12 Jul 2019 12:50
 Operator : HP/JU
 Sample : K3717-14
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BF499

Manual Integrations
 APPROVED

mohammad
 7/12/2019 10:28:29 PM

Quant Time: Jul 12 15:27:07 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN062719.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Jul 12 06:39:20 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.58	152	2530	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	9368	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.24	164	4966	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	11017m>	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	9028m>	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	8543m>	0.40	ng/ul	-0.01

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.96	152	3444	0.24	ng/ul	-0.01
14) Fluoranthene-d10	19.05	212	9021m>	0.28	ng/ul	0.00

Target Compounds

					Qvalue
3) Naphthalene	10.40	128	148870	5.535	ng/ul 99
5) 2-Methylnaphthalene	12.03	142	6984	0.384	ng/ul 98
8) Acenaphthene	14.30	153	8394	0.425	ng/ul 100
9) Fluorene	15.30	166	2342	0.108	ng/ul# 98
12) Phenanthrene	17.04	178	8818	0.249	ng/ul 98
15) Fluoranthene	19.08	202	5720m>	0.131	ng/ul
17) Pyrene	19.44	202	4198	0.102	ng/ul# 84
18) Benzo(a)anthracene	21.22	228	881	0.024	ng/ul# 68
19) Chrysene	21.27	228	1761	0.043	ng/ul# 80
21) Benzo(b)fluoranthene	22.80	252	3459m>	0.099	ng/ul
22) Benzo(k)fluoranthene	22.84	252	1229m>	0.034	ng/ul
24) Indeno(1,2,3-cd)pyrene	25.70	276	1920m>	0.055	ng/ul
26) Benzo(g,h,i)perylene	26.37	276	3244m>	0.112	ng/ul

JU 07/16/19

(#) = qualifier out of range (m) = manual integration (+) = signals summed