

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
 Data File : BN006829.D
 Acq On : 12 Jul 2019 12:15
 Operator : HP/JU
 Sample : K3578-16
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 JLJG1

Quant Time: Jul 12 15:19:45 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 12 06:39:20 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	3251	0.40	ng/ul	0.00
2) Naphthalene-d8	10.36	136	12078	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.24	164	6420	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.00	188	13735	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	11519	0.40	ng/ul	0.00
20) Perylene-d12	23.46	264	13897	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.98	152	2017	0.11	ng/ul	0.00
14) Fluoranthene-d10	19.05	212	5514	0.14	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.04	178	923	0.021	ng/ul#	Ovalue 80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN071119\
Data File : BN006829.D
Acq On : 12 Jul 2019 12:15
Operator : HP/JU
Sample : K3578-16
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
JLJG1

Quant Time: Jul 12 15:19:45 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN062719.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 12 06:39:20 2019
Response via : Initial Calibration

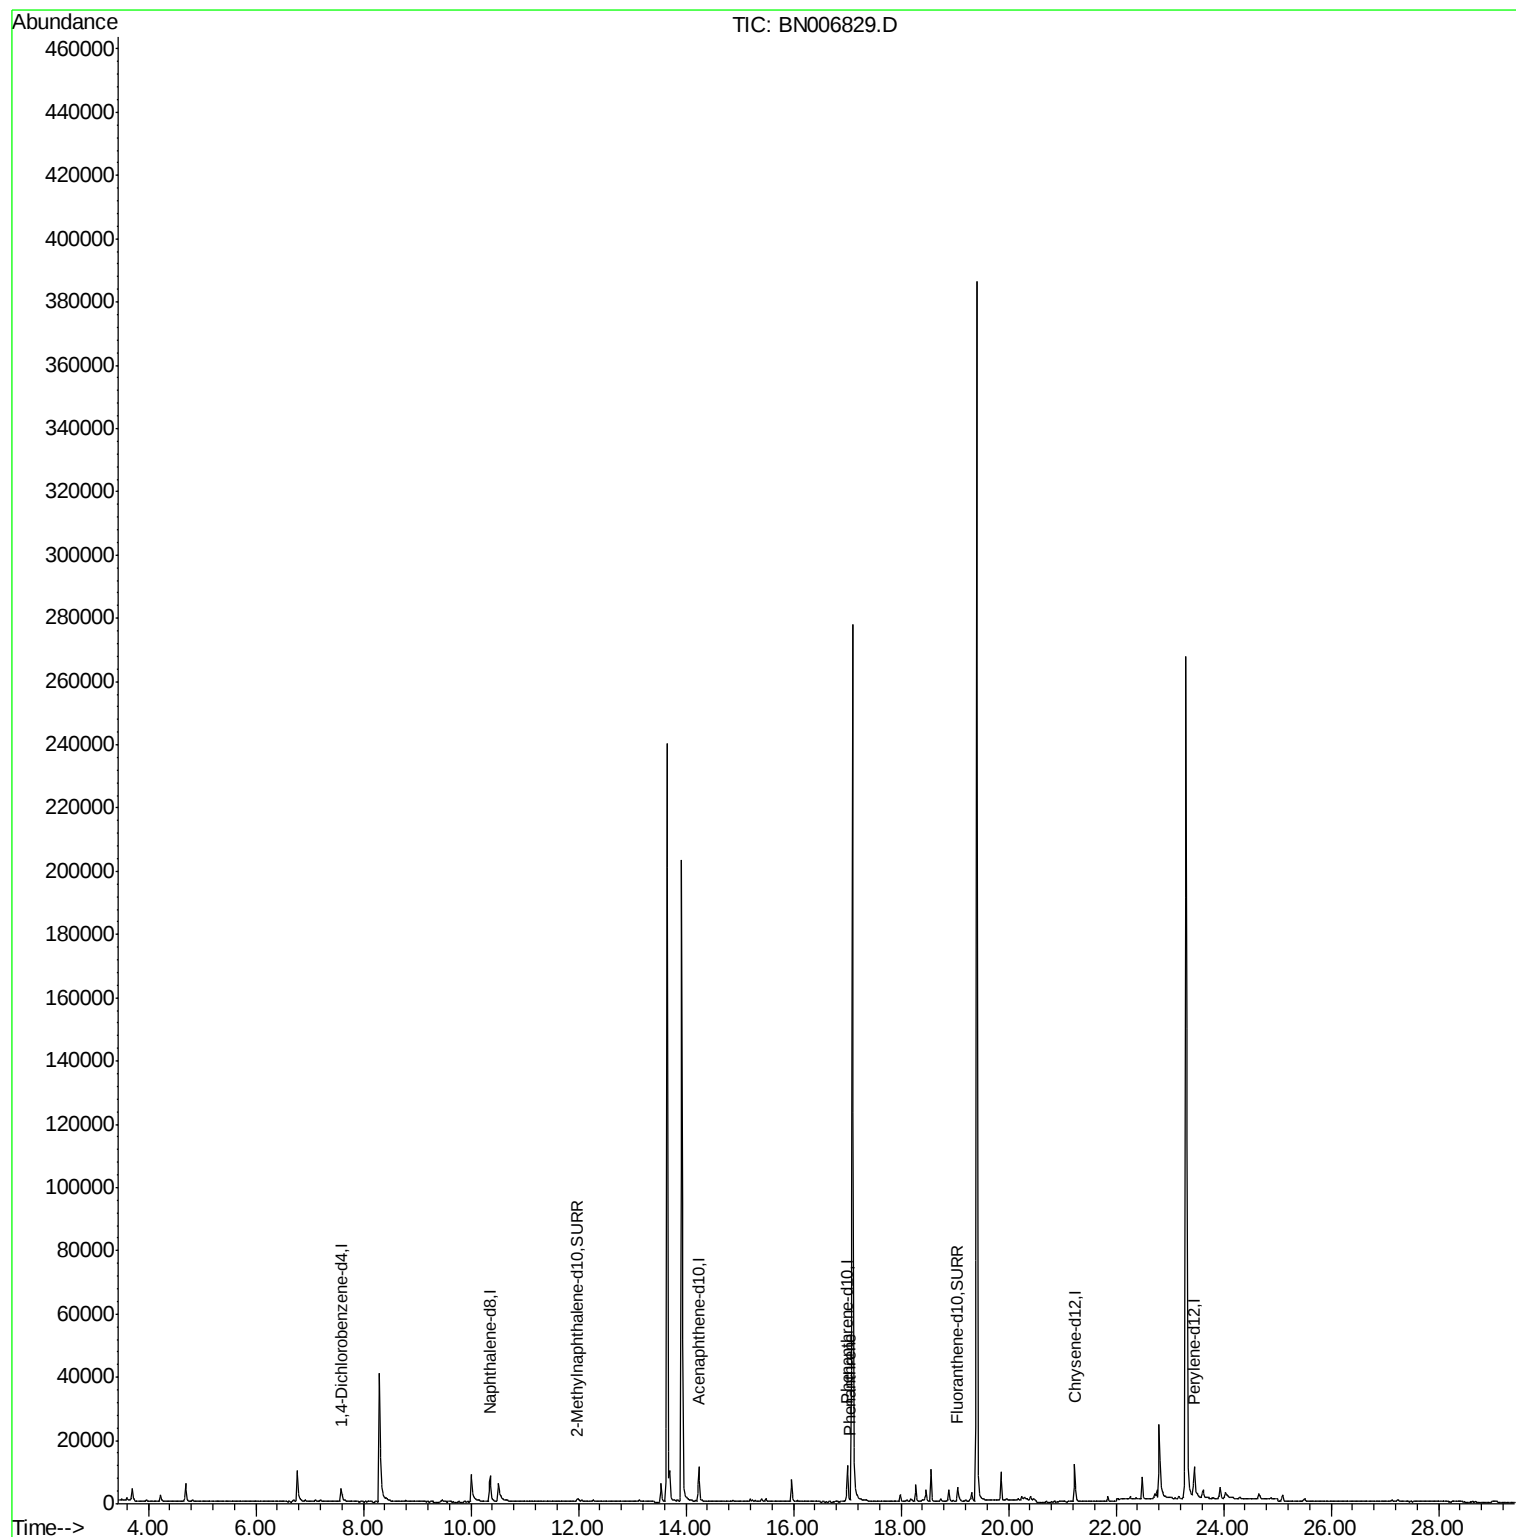

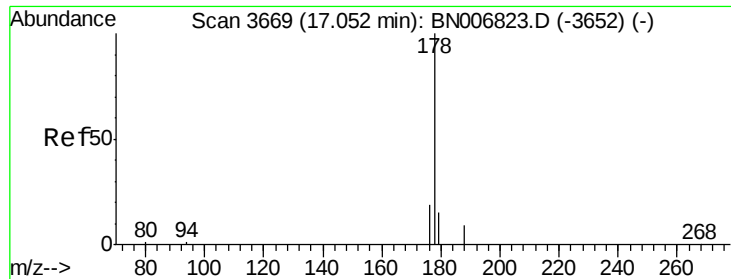

#12

Phenanthrene

Concen: 0.021 ng/ul

RT: 17.04 min Scan# 3667

Delta R.T. -0.01 min

Lab File: BN006829.D

Acq: 12 Jul 2019 12:15

Instrument :

BNA_N

ClientSampleId :

JLJG1

Tot Ion:178 Resp: 923

Ion Ratio Lower Upper

178 100

179 26.0 12.6 19.0#

176 27.6 15.8 23.8#

