

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071123\
 Data File : BN026464.D
 Acq On : 11 Jul 2023 15:54
 Operator : MA/JU
 Sample : PB1539963BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 12 02:12:32 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 15:51:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	6105	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.720	136	20488	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.557	164	11242	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.310	188	19411	0.400	ng/ul	-0.02
17) Chrysene-d12	21.521	240	11199	0.400	ng/ul	0.00
23) Perylene-d12	23.947	264	17457	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	33067	4.810	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.326	152	7736	0.245	ng/ul	0.00
18) Fluoranthene-d10	19.345	212	12288	0.288	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.708	202	2335	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.792	252	4530	0.070	ng/ul#	14


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071123\
Data File : BN026464.D
Acq On : 11 Jul 2023 15:54
Operator : MA/JU
Sample : PB1539963BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 12 02:12:32 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jul 09 15:51:14 2023
Response via : Initial Calibration

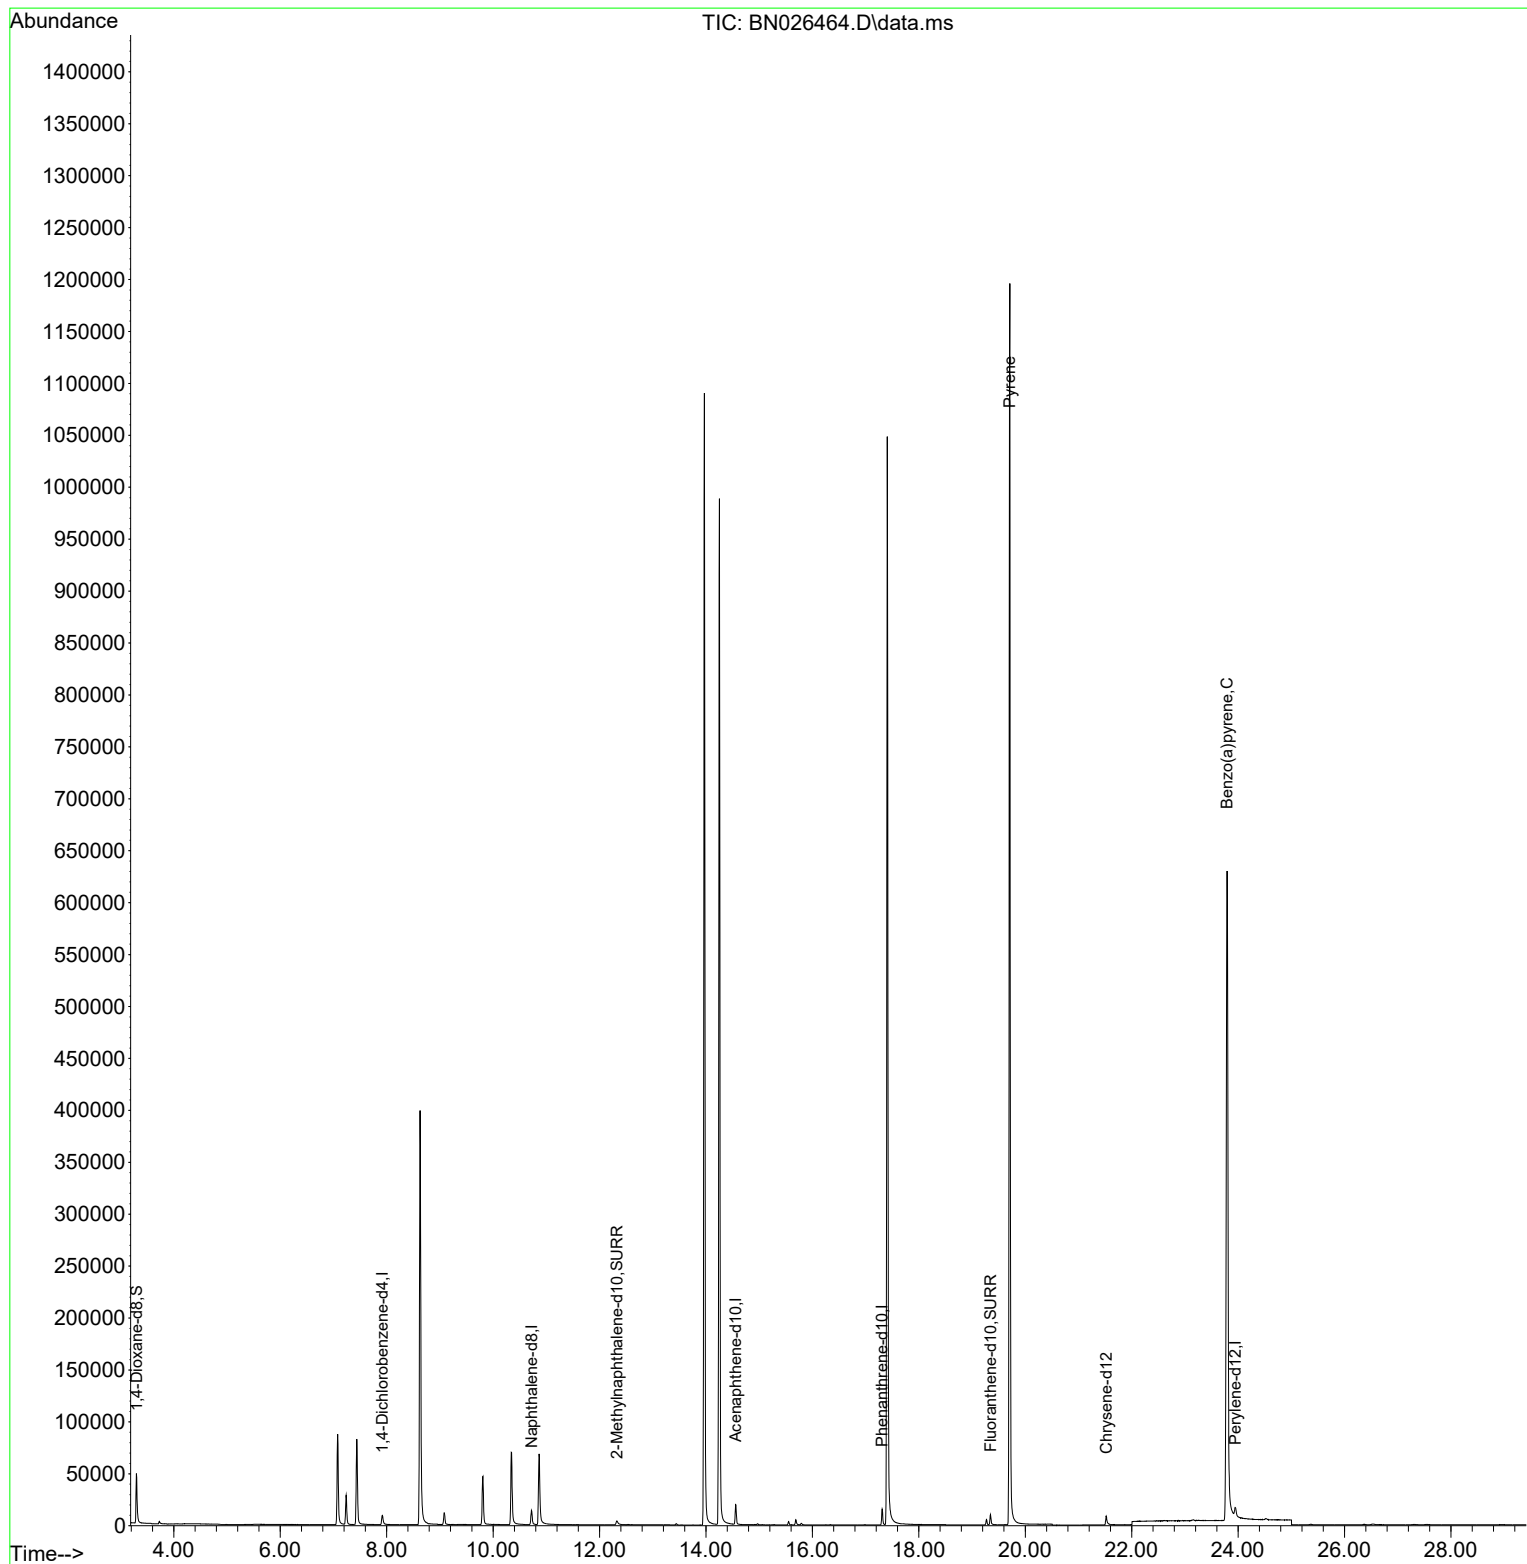

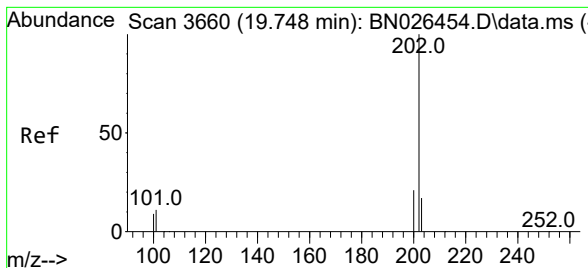

#20

Pyrene

Concen: 0.038 ng/ul

RT: 19.708 min Scan# 3

Delta R.T. -0.041 min


Lab File: BN026464.D

Acq: 11 Jul 2023 15:54

Instrument :

BNA_N

ClientSampleId :

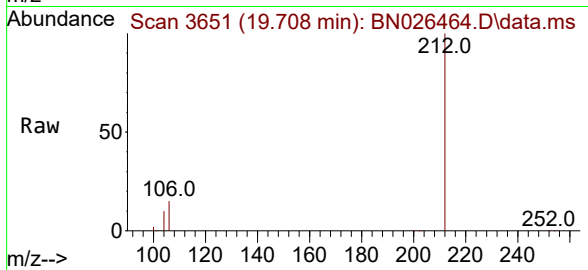




Tgt Ion:202 Resp: 2335

Ion Ratio Lower Upper

202 100

101 194.5 11.4 17.0#

100 1502.6 9.1 13.7#

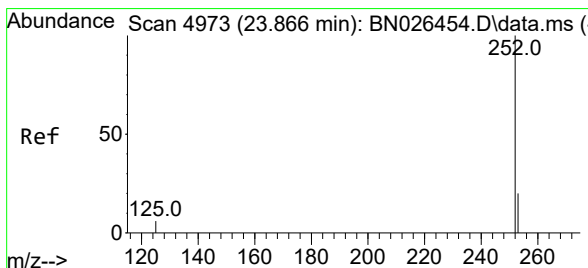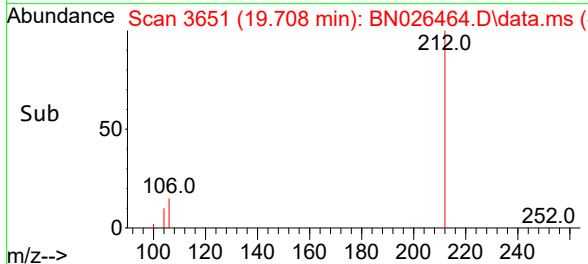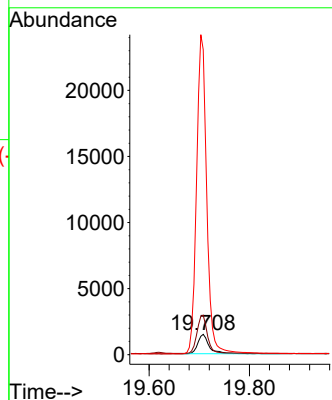

#26

Benzo(a)pyrene

Concen: 0.070 ng/ul

RT: 23.792 min Scan# 4947

Delta R.T. -0.078 min

Lab File: BN026464.D

Acq: 11 Jul 2023 15:54

Tgt Ion:252 Resp: 4530

Ion Ratio Lower Upper

252 100

253 61.2 26.0 39.0#

125 87.0 17.3 25.9#

