

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071123\
 Data File : BN026466.D
 Acq On : 11 Jul 2023 17:08
 Operator : MA/JU
 Sample : 03414-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Jul 12 02:12:48 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 15:51:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	4011	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.721	136	14135	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.561	164	8214	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.313	188	14778	0.400	ng/ul	-0.01
17) Chrysene-d12	21.523	240	8281	0.400	ng/ul	0.00
23) Perylene-d12	23.967	264	10382	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	13941	3.086	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.321	152	4330	0.199	ng/ul	-0.01
18) Fluoranthene-d10	19.345	212	7427	0.236	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.707	202	1565	0.034	ng/ul#	1
26) Benzo(a)pyrene	23.809	252	2217	0.058	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071123\
Data File : BN026466.D
Acq On : 11 Jul 2023 17:08
Operator : MA/JU
Sample : 03414-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Jul 12 02:12:48 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jul 09 15:51:14 2023
Response via : Initial Calibration

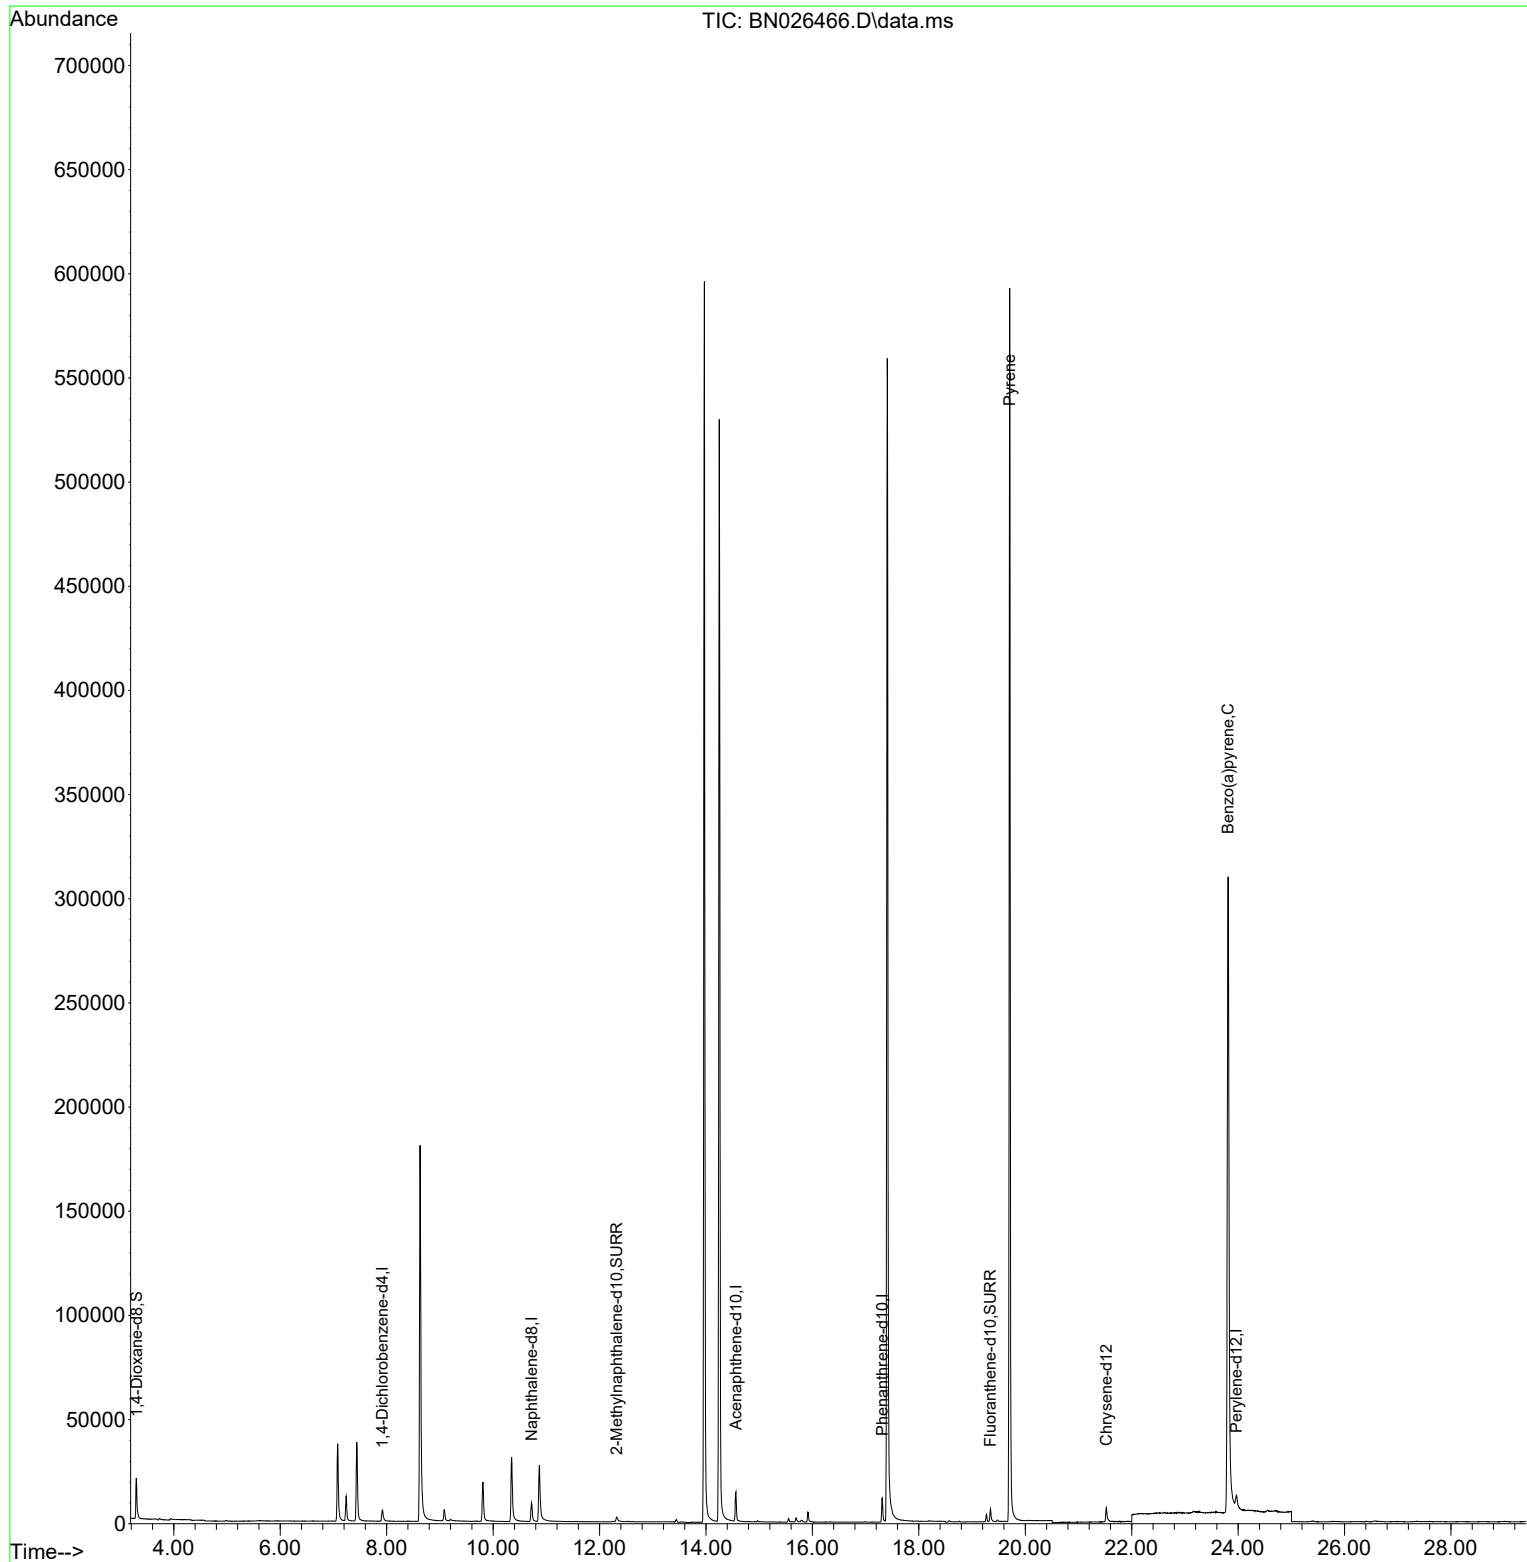

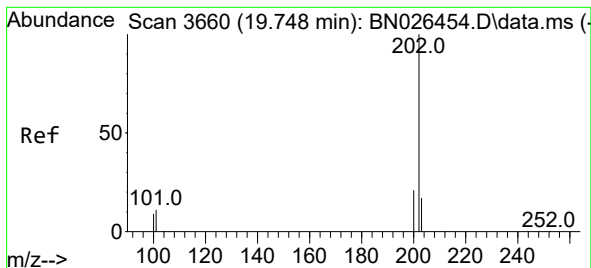

#20

Pyrene

Concen: 0.034 ng/ul

RT: 19.707 min Scan# 3

Delta R.T. -0.042 min


Lab File: BN026466.D

Acq: 11 Jul 2023 17:08

Instrument :

BNA_N

ClientSampleId :

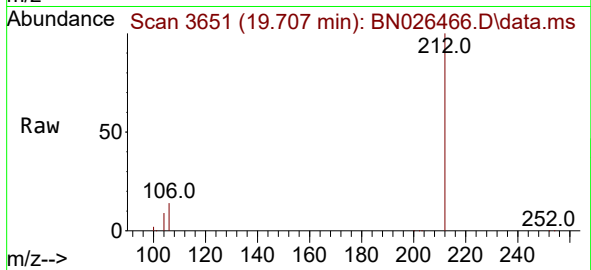




Tgt Ion:202 Resp: 1565

Ion Ratio Lower Upper

202 100

101 185.1 11.4 17.0#

100 1404.1 9.1 13.7#

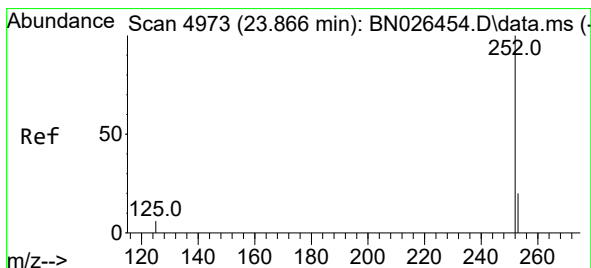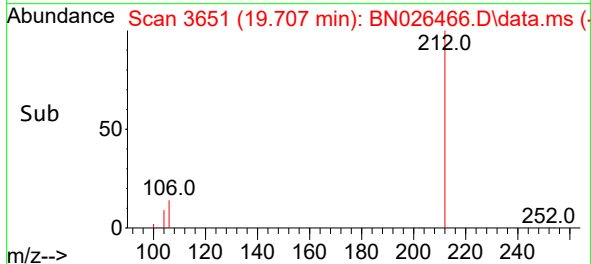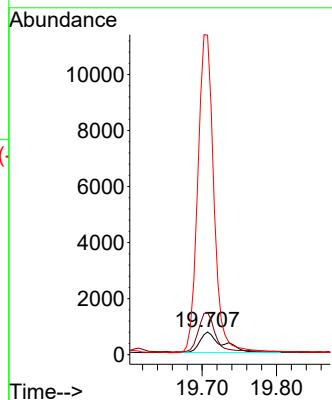

#26

Benzo(a)pyrene

Concen: 0.058 ng/ul

RT: 23.809 min Scan# 4953

Delta R.T. -0.061 min

Lab File: BN026466.D

Acq: 11 Jul 2023 17:08

Tgt Ion:252 Resp: 2217

Ion Ratio Lower Upper

252 100

253 79.3 26.0 39.0#

125 93.2 17.3 25.9#

