

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071123\
 Data File : BN026461.D
 Acq On : 11 Jul 2023 14:04
 Operator : MA/JU
 Sample : 03477-08
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 HOA46

Quant Time: Jul 12 02:12:03 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Jul 09 15:51:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.917	152	4718	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.721	136	15817	0.400	ng/ul	#-0.02
9) Acenaphthene-d10	14.561	164	8974	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	16400	0.400	ng/ul	-0.02
17) Chrysene-d12	21.514	240	10229	0.400	ng/ul	0.00
23) Perylene-d12	23.961	264	12106	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.297	96	31704	5.967	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.315	152	7167	0.295	ng/ul	-0.02
18) Fluoranthene-d10	19.340	212	13716	0.352	ng/ul	-0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.331	88	164545	29.166	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN071123\
Data File : BN026461.D
Acq On : 11 Jul 2023 14:04
Operator : MA/JU
Sample : 03477-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
HOA46

Quant Time: Jul 12 02:12:03 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN062223.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Jul 09 15:51:14 2023
Response via : Initial Calibration

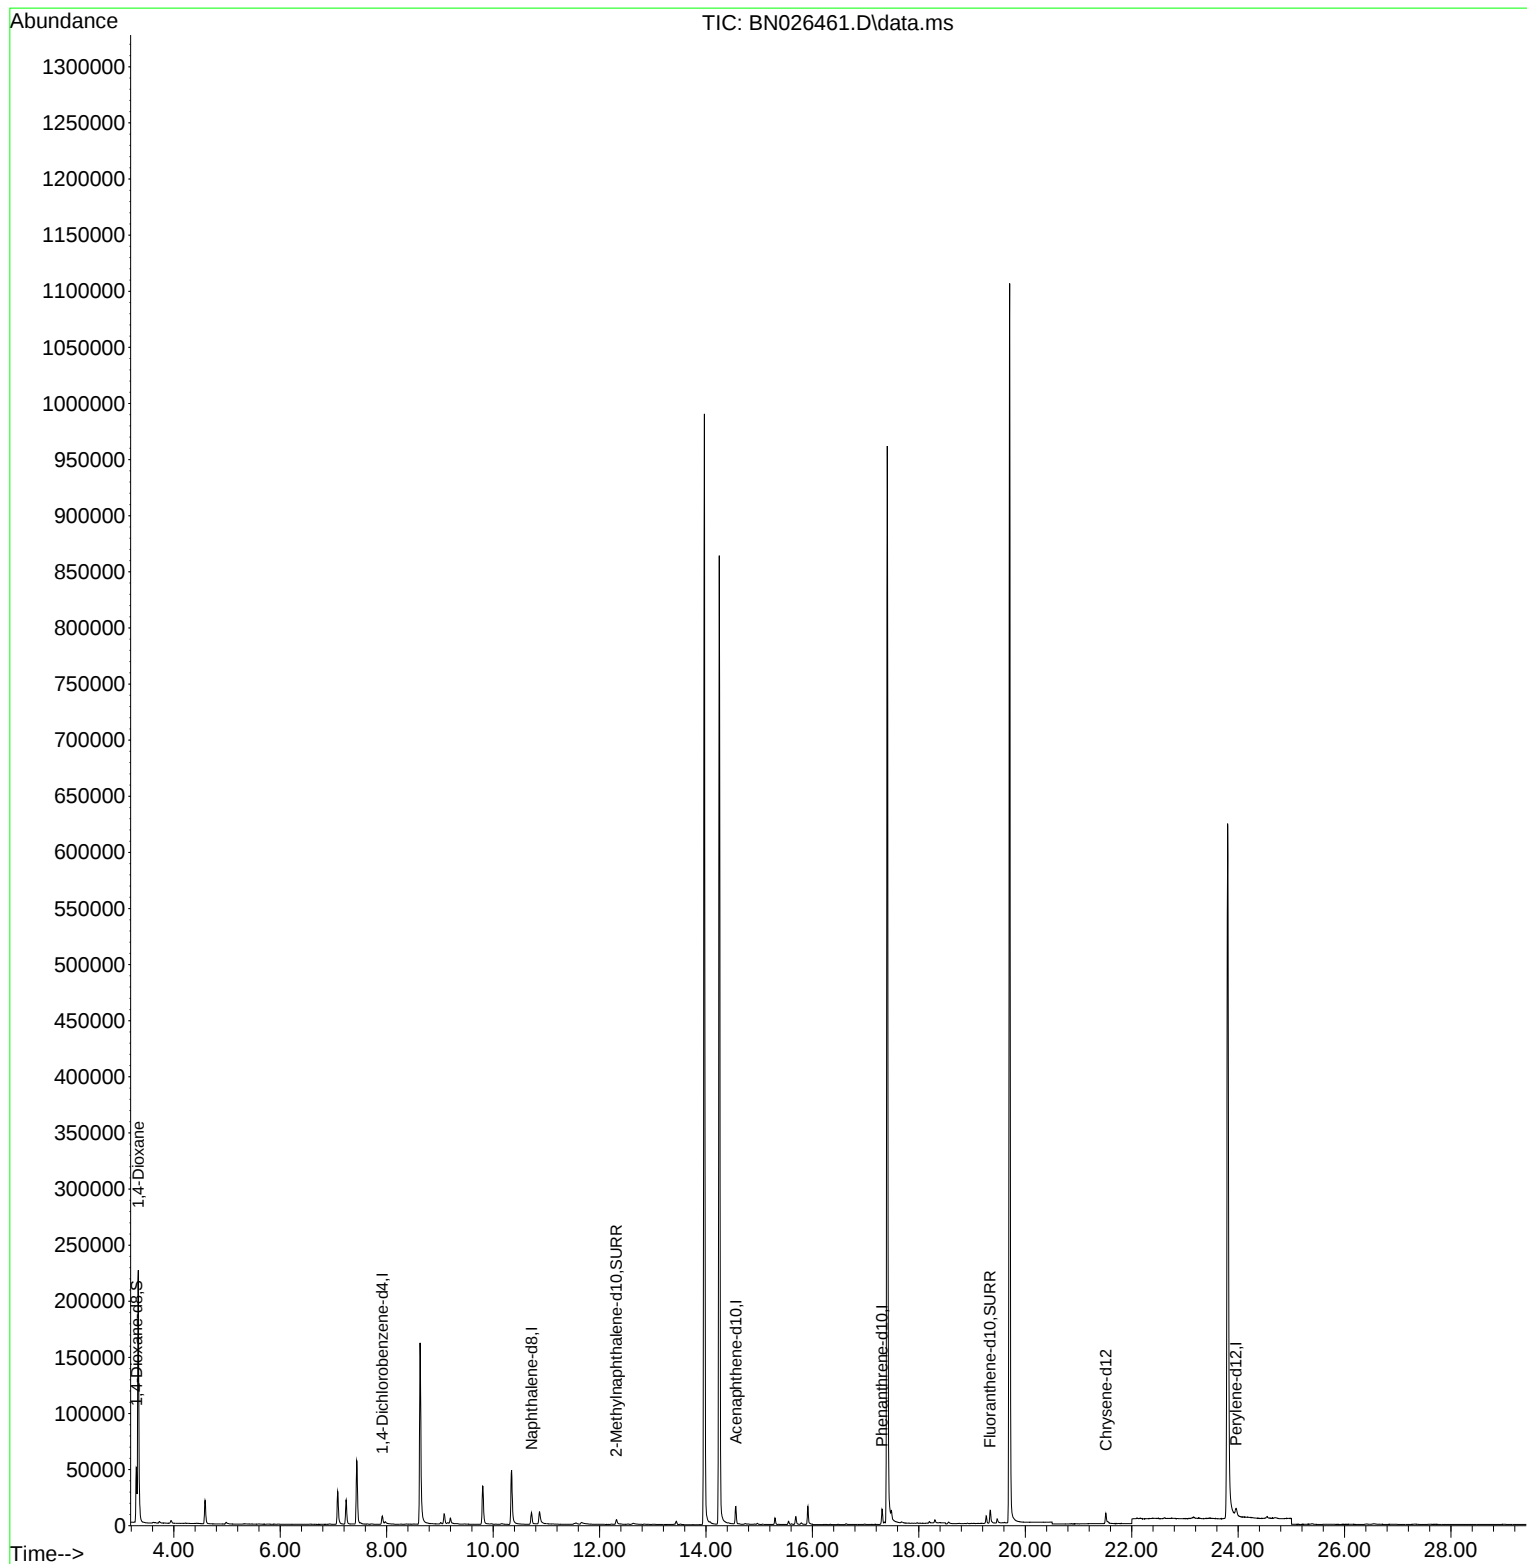

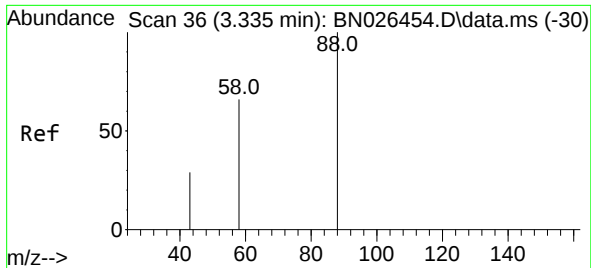

#2

1,4-Dioxane

Concen: 29.166 ng/ul

RT: 3.331 min Scan# 31

Delta R.T. -0.008 min

Lab File: BN026461.D


Acq: 11 Jul 2023 14:04

Instrument :

BNA_N

ClientSampleId :

HOA46

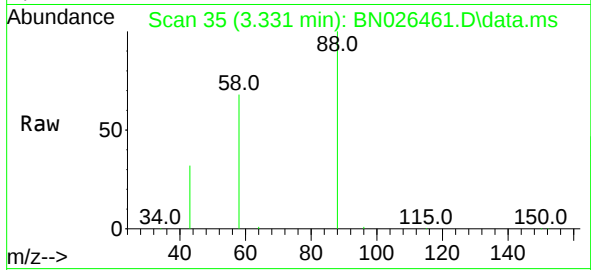

Tgt Ion: 88 Resp: 164545

Ion Ratio Lower Upper

88 100

43 31.5 29.5 44.3

58 67.6 37.4 56.2#

