


Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071221\
Data File : BN015494.D
Acq On : 12 Jul 2021 17:44
Operator : CG/JU
Sample : PB137523BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK523

Manual Integrations
APPROVED

mohammad
7/13/2021 1:44:04 PM

Quant Time: Jul 12 18:27:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 12 15:47:53 2021
Response via : Initial Calibration

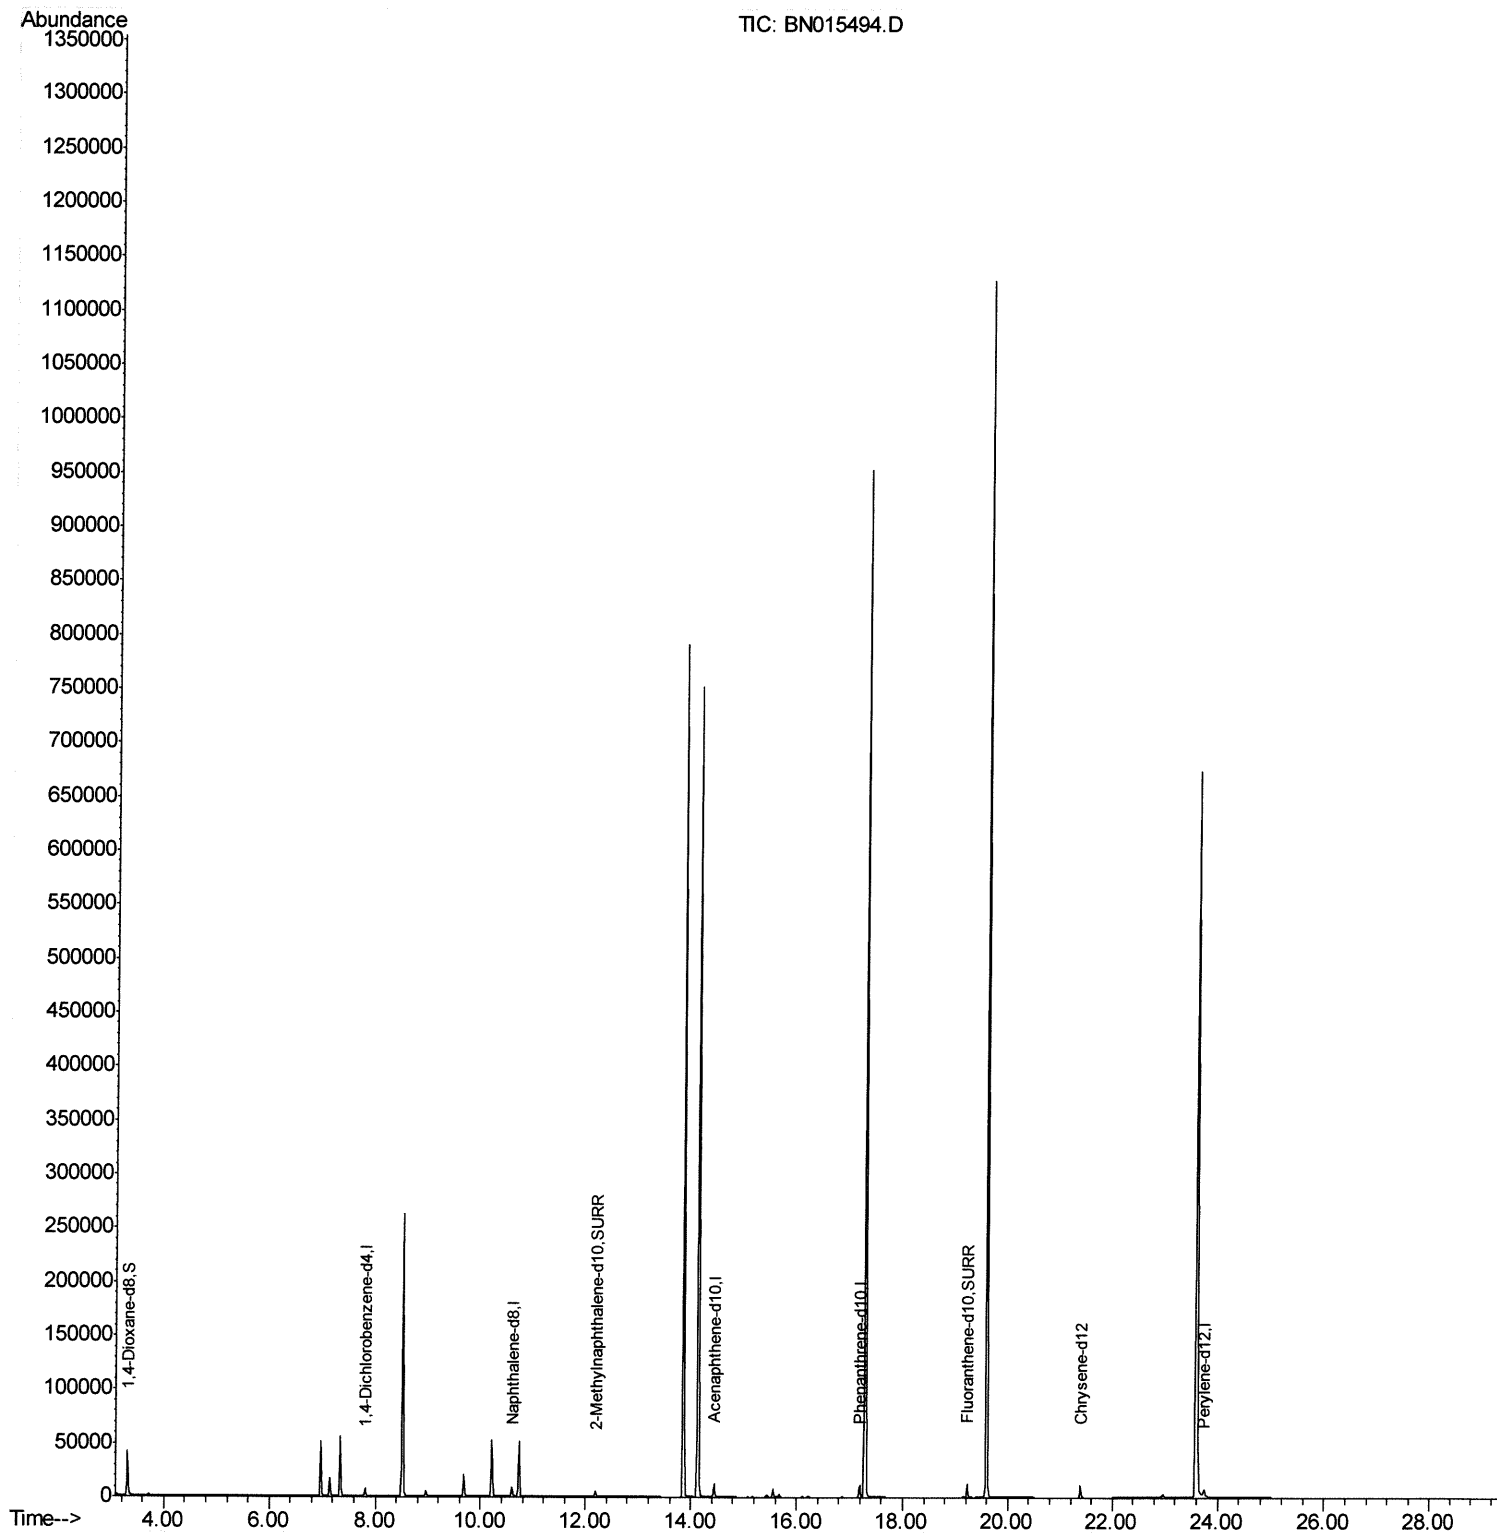



Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071221\
 Data File : BN015494.D
 Acq On : 12 Jul 2021 17:44
 Operator : CG/JU
 Sample : PB137523BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK523

Manual Integrations
 APPROVED

mohammad
 7/13/2021 1:44:04 PM

Quant Time: Jul 12 18:26:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 15:47:53 2021
 Response via : Initial Calibration

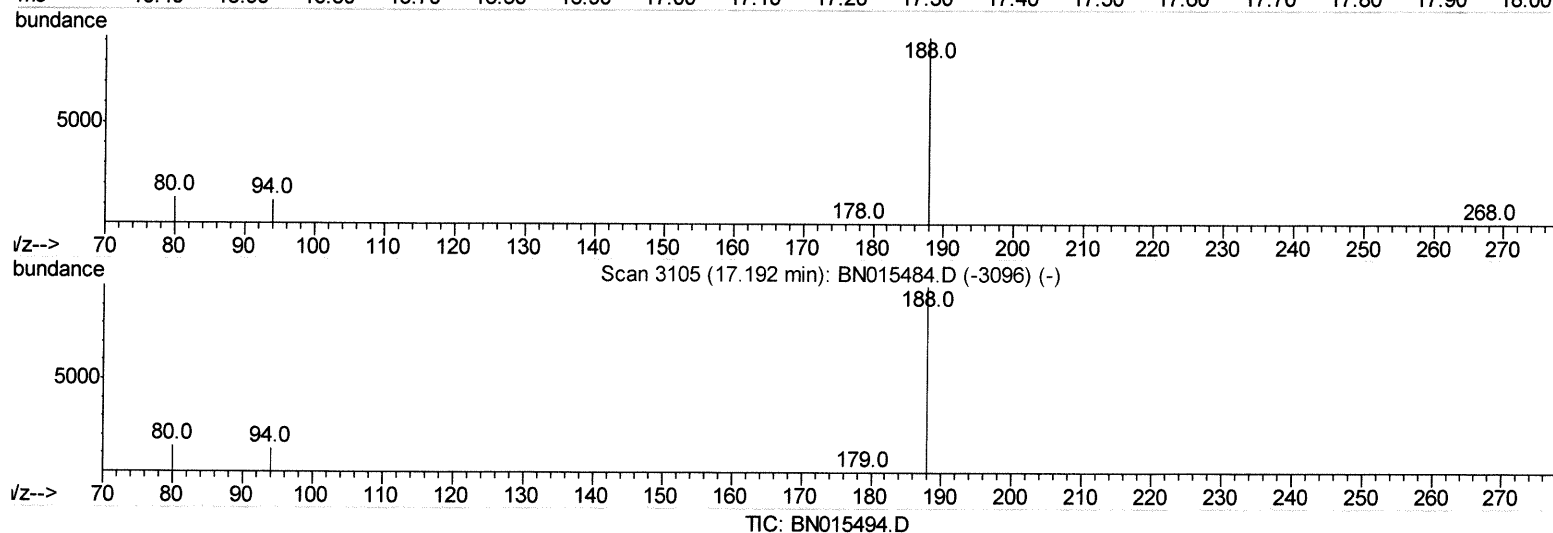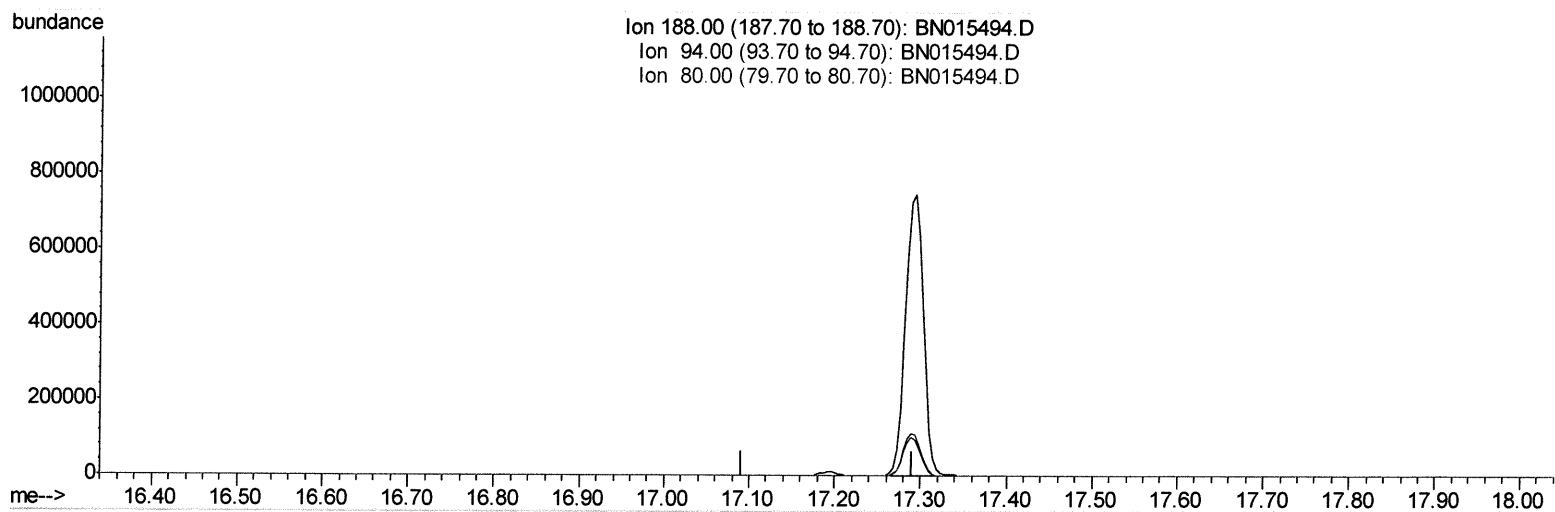

(13) Phenanthrene-d10 (I)

17.192min (-17.192) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	14.10	0.00#
80.00	14.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071221\
 Data File : BN015494.D
 Acq On : 12 Jul 2021 17:44
 Operator : CG/JU
 Sample : PB137523BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK523

Manual Integrations
 APPROVED

mohammad
 7/13/2021 1:44:04 PM

Quant Time: Jul 12 18:26:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 15:47:53 2021
 Response via : Initial Calibration

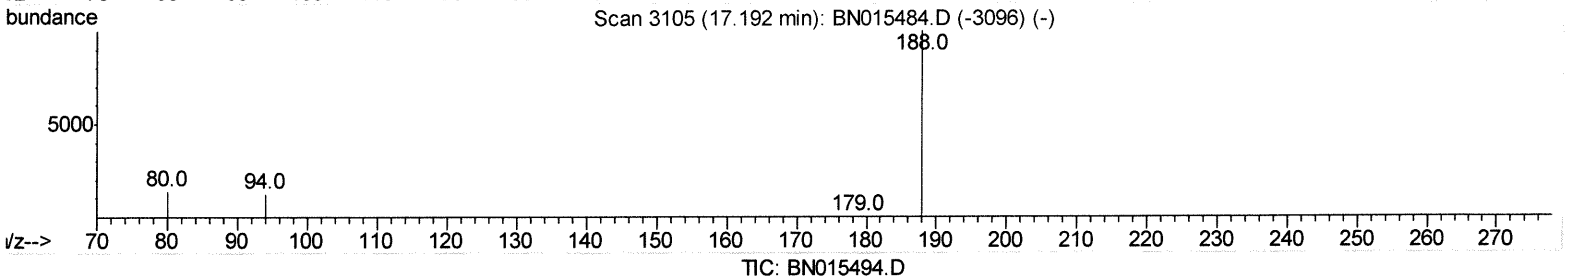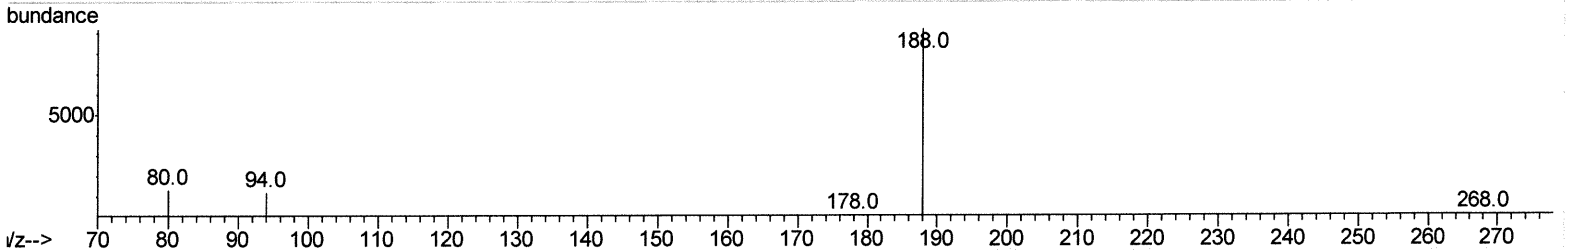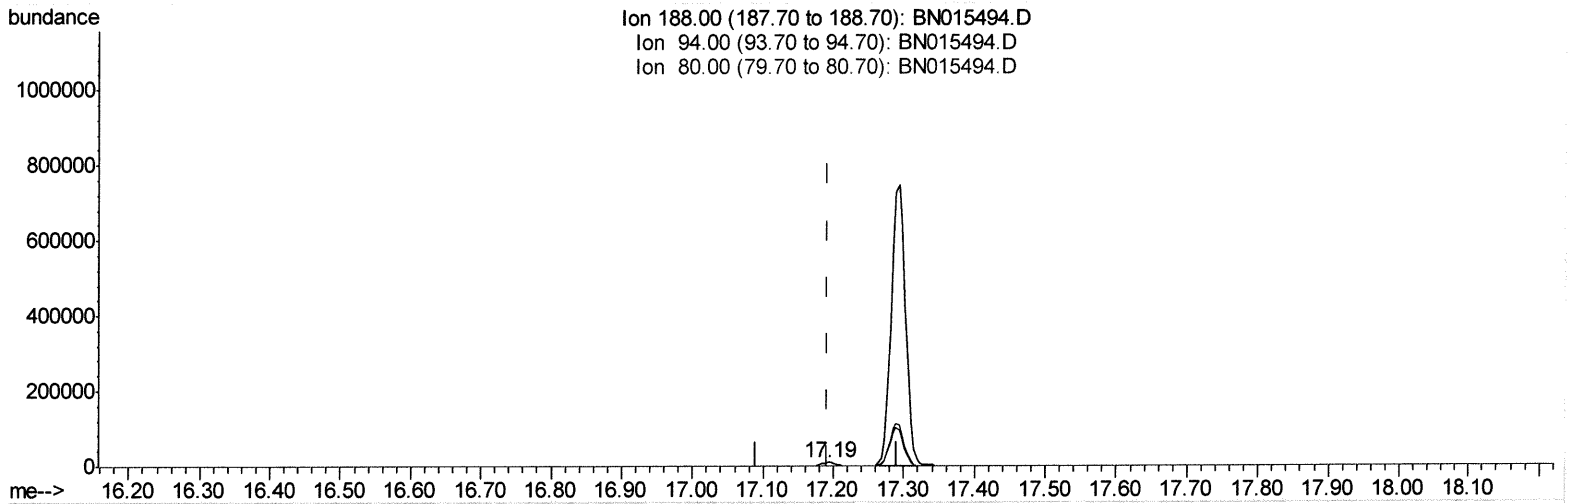

(13) Phenanthrene-d10 (I)

17.192min (+0.001) 0.40ng/ul m

response 13010

547/14/21

Ion	Exp%	Act%
188.00	100	100
94.00	14.10	13.03
80.00	14.40	14.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA N\Data\BN071221\
 Data File : BN015494.D
 Acq On : 12 Jul 2021 17:44
 Operator : CG/JU
 Sample : PB137523BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK523

Manual Integrations
 APPROVED

mohammad
 7/13/2021 1:44:04 PM

Quant Time: Jul 12 18:27:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SFAM-EPA-SIM-BN062121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 15:47:53 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	3448	0.40	ng/ul	0.00
4) Naphthalene-d8	10.59	136	12217	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.44	164	6846	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.19	188	13010m	0.40	ng/ul	0.00
17) Chrysene-d12	21.39	240	9789	0.40	ng/ul	0.00
23) Perylene-d12	23.74	264	10312	0.40	ng/ul	0.00

Jul 14/21

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	26967	6.94	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.19	152	6693	0.35	ng/ul	0.00
18) Fluoranthene-d10	19.23	212	12733	0.40	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed